


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090718\  
 Data File : BG036612.D  
 Acq On : 8 Sep 2018 1:28  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG082318.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Aug 31 13:03:20 2018

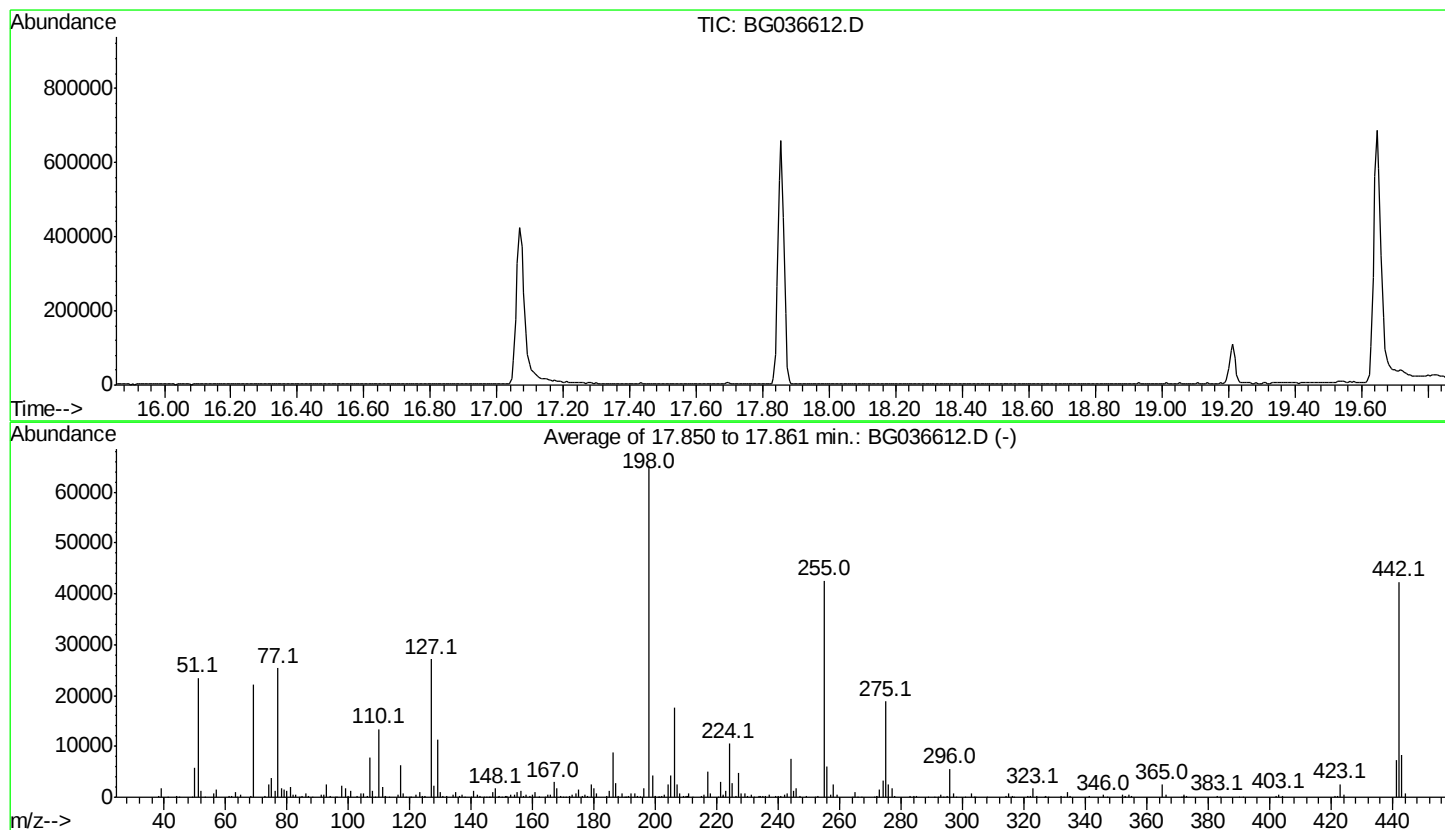

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 35.9         | 23432      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.9          | 196        | PASS                |
| 69             | 198             | 0.00            | 100             | 33.9         | 22121      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 41.6         | 27149      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 65221      | PASS                |
| 199            | 198             | 5               | 9               | 6.5          | 4236       | PASS                |
| 275            | 198             | 10              | 60              | 28.9         | 18880      | PASS                |
| 365            | 198             | 1               | 100             | 3.8          | 2480       | PASS                |
| 441            | 198             | 0.01            | 100             | 11.1         | 7255       | PASS                |
| 442            | 198             | 50              | 100             | 65.0         | 42373      | PASS                |
| 443            | 442             | 15              | 24              | 19.7         | 8350       | PASS                |