

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058923.D
 Acq On : 8 Sep 2023 18:40
 Operator : MA/JU
 Sample : PB155272BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058923.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.640	19	26	35	rVB5	11894	29054	1.20%	0.127%
2	4.075	94	100	116	rBV	162375	290485	11.99%	1.266%
3	4.210	121	123	126	rVB3	3290	3529	0.15%	0.015%
4	4.245	126	129	133	rBV2	2632	5031	0.21%	0.022%
5	4.727	210	211	214	rBV2	3565	3586	0.15%	0.016%
6	4.950	245	249	251	rBV2	2928	4359	0.18%	0.019%
7	5.397	321	325	327	rBV2	2713	3615	0.15%	0.016%
8	5.485	339	340	343	rVB	5390	4215	0.17%	0.018%
9	5.526	343	347	349	rBV	3387	5214	0.22%	0.023%
10	5.620	359	363	366	rVB	3122	4057	0.17%	0.018%
11	6.208	459	463	466	rBV	2382	4215	0.17%	0.018%
12	7.436	665	672	682	rVB	226040	401062	16.55%	1.747%
13	7.653	702	709	716	rBV	164500	282526	11.66%	1.231%
14	7.847	734	742	748	rBV	204157	353070	14.57%	1.538%
15	8.035	770	774	775	rVB	3774	4271	0.18%	0.019%
16	8.335	817	825	835	rBV3	197702	343656	14.18%	1.497%
17	8.799	901	904	907	rVB3	4261	5016	0.21%	0.022%
18	8.840	907	911	915	rBV	3423	5903	0.24%	0.026%
19	9.010	932	940	948	rBV2	296774	511351	21.10%	2.228%
20	9.463	1014	1017	1020	rBV2	2463	3572	0.15%	0.016%
21	9.527	1020	1028	1034	rVV2	214808	388035	16.01%	1.691%
22	9.768	1066	1069	1073	rBV2	2335	3372	0.14%	0.015%
23	9.874	1086	1087	1090	rVB	3593	3196	0.13%	0.014%
24	9.898	1090	1091	1094	rBV	3907	3598	0.15%	0.016%
25	10.244	1144	1150	1157	rBV	176656	310745	12.83%	1.354%
26	10.315	1159	1162	1166	rBV	2485	3797	0.16%	0.017%
27	10.767	1231	1239	1246	rBV	316875	573405	23.67%	2.498%
28	10.861	1252	1255	1258	rBV	2604	3155	0.13%	0.014%
29	11.032	1281	1284	1285	rBV	3660	3275	0.14%	0.014%
30	11.043	1285	1286	1292	rVB	3144	3379	0.14%	0.015%
31	11.178	1301	1309	1317	rVB	304420	562921	23.23%	2.453%
32	11.314	1324	1332	1342	rVB	329751	593174	24.48%	2.584%
33	12.171	1475	1478	1481	rBV	2125	3167	0.13%	0.014%
34	12.730	1569	1573	1574	rBV2	6802	7928	0.33%	0.035%
35	12.829	1588	1590	1592	rBV	2942	3175	0.13%	0.014%
36	12.953	1608	1611	1614	rBV	4129	4136	0.17%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058923.D
 Acq On : 8 Sep 2023 18:40
 Operator : MA/JU
 Sample : PB155272BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

37	13.129	1638	1641	1647	rBV	4658	10126	0.42%	0.044%
38	13.540	1708	1711	1713	rBV	3738	3789	0.16%	0.017%
39	13.799	1751	1755	1758	rBV5	14349	20674	0.85%	0.090%
40	14.151	1811	1815	1816	rBV5	2881	3163	0.13%	0.014%
41	14.304	1840	1841	1843	rBV5	3407	3245	0.13%	0.014%
42	14.357	1843	1850	1858	rVB	825832	1168824	48.24%	5.092%
43	14.522	1873	1878	1880	rBV	3499	4319	0.18%	0.019%
44	14.663	1894	1902	1910	rVB	764291	1214842	50.14%	5.293%
45	14.810	1925	1927	1930	rVB	3746	3409	0.14%	0.015%
46	14.956	1945	1952	1959	rVB	707740	1054427	43.52%	4.594%
47	15.021	1962	1963	1965	rBV	3922	3152	0.13%	0.014%
48	15.115	1972	1979	1989	rBV	370052	593017	24.47%	2.584%
49	15.356	2017	2020	2022	rVB2	3697	4217	0.17%	0.018%
50	15.579	2056	2058	2060	rBV	6099	4195	0.17%	0.018%
51	15.626	2063	2066	2070	rVB2	3577	4191	0.17%	0.018%
52	15.944	2114	2120	2128	rVB	1126109	1704868	70.36%	7.428%
53	16.043	2128	2137	2142	rBV	286603	412859	17.04%	1.799%
54	16.131	2150	2152	2155	rVB3	6134	5240	0.22%	0.023%
55	16.173	2155	2159	2161	rBV2	6671	10029	0.41%	0.044%
56	16.208	2164	2165	2168	rBV2	3986	3926	0.16%	0.017%
57	16.320	2183	2184	2187	rBV	4566	4564	0.19%	0.020%
58	16.713	2249	2251	2252	rBV2	5399	4581	0.19%	0.020%
59	16.778	2259	2262	2265	rBV2	2678	4142	0.17%	0.018%
60	17.025	2301	2304	2307	rBV3	3701	4752	0.20%	0.021%
61	17.277	2345	2347	2349	rVB2	5374	4039	0.17%	0.018%
62	17.295	2349	2350	2352	rBV	4799	4586	0.19%	0.020%
63	17.383	2362	2365	2368	rBV4	3529	3786	0.16%	0.016%
64	17.706	2413	2420	2427	rVB	1072485	1612803	66.56%	7.027%
65	17.806	2430	2437	2445	rVB	1422178	2131476	87.97%	9.287%
66	17.865	2445	2447	2448	rBV2	4629	3503	0.14%	0.015%
67	18.176	2498	2500	2502	rBV3	4706	3329	0.14%	0.015%
68	18.411	2538	2540	2541	rBV	5777	3502	0.14%	0.015%
69	18.728	2592	2594	2596	rBV3	5136	5732	0.24%	0.025%
70	19.181	2669	2671	2673	rBV3	4788	4004	0.17%	0.017%
71	19.645	2745	2750	2753	rBV5	18290	28549	1.18%	0.124%
72	19.704	2756	2760	2766	rVB	21413	32480	1.34%	0.142%
73	19.786	2772	2774	2775	rVB2	6016	3635	0.15%	0.016%
74	19.810	2775	2778	2780	rBV3	4977	5472	0.23%	0.024%
75	19.945	2799	2801	2803	rVB3	5158	3923	0.16%	0.017%
76	20.080	2817	2824	2830	rBV	1638004	2422957	100.00%	10.557%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058923.D
 Acq On : 8 Sep 2023 18:40
 Operator : MA/JU
 Sample : PB155272BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

77	21.090	2994	2996	3001	rBV5	6771	9143	0.38%	0.040%
78	21.437	3053	3055	3057	rBV2	7372	6485	0.27%	0.028%
79	22.030	3149	3156	3164	rBV2	874512	1575061	65.01%	6.862%
80	22.342	3206	3209	3211	rBV3	10194	10435	0.43%	0.045%
81	24.821	3629	3631	3633	rVB3	8227	4009	0.17%	0.017%
82	25.362	3712	3723	3737	rVB2	773847	2328738	96.11%	10.146%
83	25.609	3754	3765	3777	rBV2	534522	1712568	70.68%	7.461%
84	25.920	3817	3818	3819	rBV	7966	3322	0.14%	0.014%
85	26.466	3909	3911	3913	rBV3	7385	4660	0.19%	0.020%
86	27.195	4033	4035	4039	rBV4	7342	9607	0.40%	0.042%
87	28.358	4231	4233	4236	rBV4	6574	5504	0.23%	0.024%
88	28.682	4286	4288	4289	rBV2	7102	5235	0.22%	0.023%
89	31.132	4703	4705	4707	rBV3	8650	7037	0.29%	0.031%
90	31.331	4737	4739	4740	rBV2	8209	7827	0.32%	0.034%



Sum of corrected areas: 22952203

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058923.D
Acq On : 8 Sep 2023 18:40
Operator : MA/JU
Sample : PB155272BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK272

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

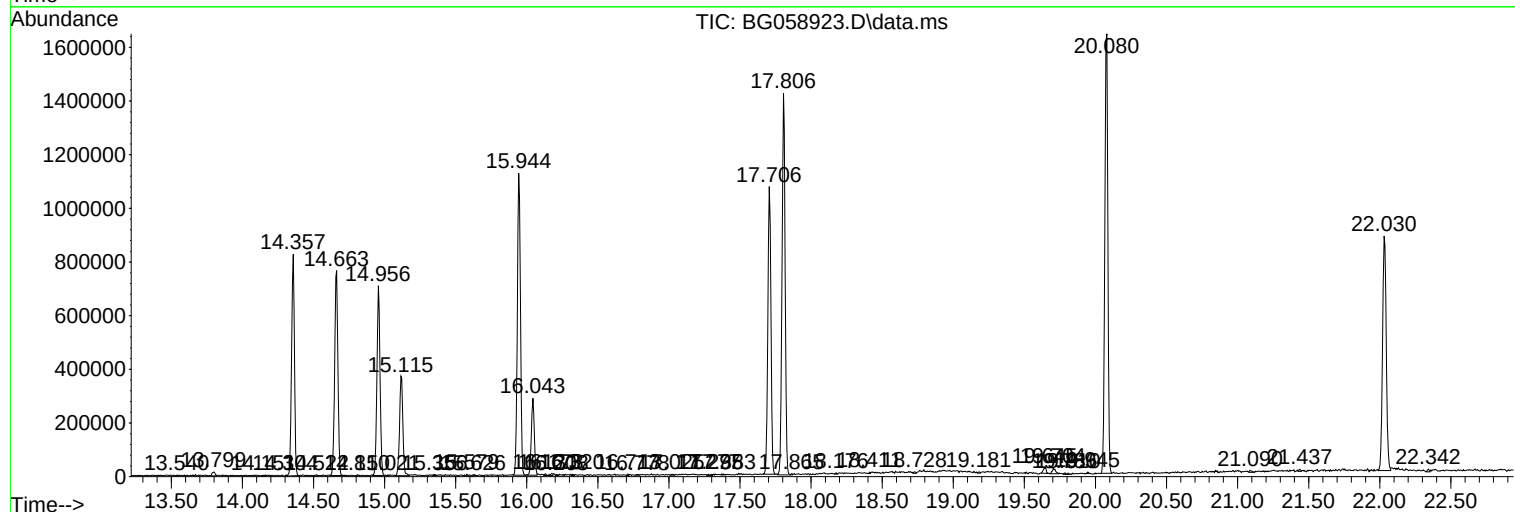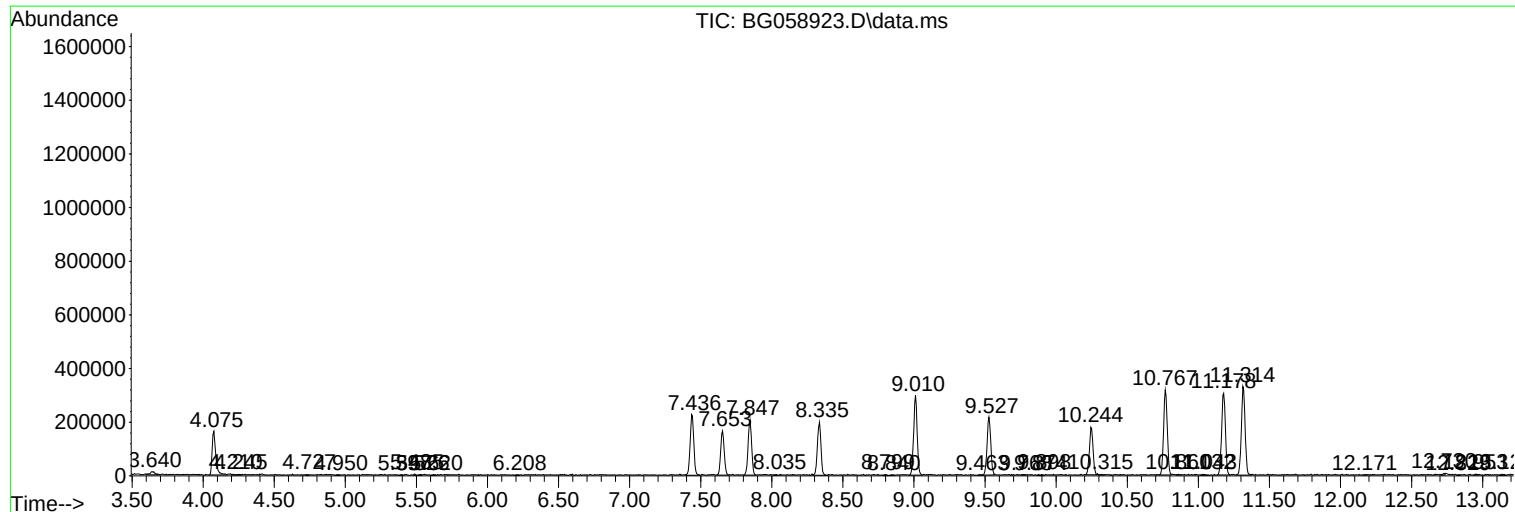

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058923.D
Acq On : 8 Sep 2023 18:40
Operator : MA/JU
Sample : PB155272BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK272

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058923.D
Acq On : 8 Sep 2023 18:40
Operator : MA/JU
Sample : PB155272BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK272

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc