

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058926.D
 Acq On : 8 Sep 2023 20:58
 Operator : MA/JU
 Sample : 04227-21
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBJ90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058926.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.562	8	12	15	rBV4	4889	7216	0.21%	0.025%
2	3.638	19	25	31	rBV5	10431	20670	0.61%	0.073%
3	4.073	95	99	105	rBV2	75214	127871	3.77%	0.450%
4	4.290	133	136	139	rVB4	7560	9953	0.29%	0.035%
5	4.948	243	248	254	rVB6	18480	32622	0.96%	0.115%
6	7.434	664	671	678	rBV	76781	135079	3.98%	0.476%
7	7.651	700	708	716	rBV	263335	422043	12.44%	1.487%
8	7.845	733	741	750	rBV	232137	407132	12.00%	1.434%
9	8.333	816	824	830	rBV	227643	397290	11.71%	1.399%
10	8.509	850	854	857	rBV	3674	4626	0.14%	0.016%
11	9.008	931	939	946	rBV2	225887	393042	11.58%	1.384%
12	9.525	1020	1027	1034	rBV	316063	566543	16.70%	1.996%
13	9.578	1034	1036	1041	rVB	3813	4888	0.14%	0.017%
14	9.754	1064	1066	1070	rVB	4027	4536	0.13%	0.016%
15	10.242	1142	1149	1156	rBV3	232767	426310	12.56%	1.502%
16	10.765	1231	1238	1249	rVB	434392	781058	23.02%	2.751%
17	11.100	1293	1295	1300	rBV	2654	4667	0.14%	0.016%
18	11.176	1300	1308	1316	rVV	356891	634987	18.71%	2.237%
19	11.311	1323	1331	1340	rBV	361180	677840	19.98%	2.388%
20	11.746	1404	1405	1411	rBV	3758	5579	0.16%	0.020%
21	11.969	1440	1443	1450	rVB2	5503	7572	0.22%	0.027%
22	12.733	1568	1573	1578	rVB2	12290	20860	0.61%	0.073%
23	13.803	1750	1755	1760	rVB2	14926	26243	0.77%	0.092%
24	14.355	1842	1849	1857	rBV	1164560	1695477	49.97%	5.972%
25	14.660	1894	1901	1912	rVB2	1167257	1809129	53.32%	6.373%
26	14.790	1920	1923	1930	rVB2	4761	7314	0.22%	0.026%
27	14.960	1945	1952	1960	rBV	695898	1127054	33.22%	3.970%
28	15.113	1971	1978	1984	rBV2	106119	168848	4.98%	0.595%
29	15.348	2015	2018	2020	rBV2	4668	6475	0.19%	0.023%
30	15.947	2111	2120	2131	rBV	1640711	2573201	75.84%	9.064%
31	16.047	2131	2137	2142	rVB	422591	618048	18.21%	2.177%
32	16.517	2211	2217	2219	rBV	6005	9655	0.28%	0.034%
33	16.588	2224	2229	2232	rVB	4593	8173	0.24%	0.029%
34	16.881	2277	2279	2282	rBV	3830	5391	0.16%	0.019%
35	17.022	2301	2303	2307	rBV	4388	4897	0.14%	0.017%
36	17.704	2411	2419	2428	rBV	1059414	1671522	49.26%	5.888%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058926.D
 Acq On : 8 Sep 2023 20:58
 Operator : MA/JU
 Sample : 04227-21
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBJ90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

37	17.810	2430	2437	2446	rVB	2024571	3139864	92.54%	11.060%
38	17.868	2446	2447	2452	rBV2	4592	5422	0.16%	0.019%
39	18.121	2486	2490	2494	rVB3	4461	7250	0.21%	0.026%
40	18.333	2522	2526	2528	rBV2	4529	6230	0.18%	0.022%
41	18.532	2556	2560	2565	rBV2	49323	61167	1.80%	0.215%
42	18.632	2575	2577	2581	rVB5	5838	6405	0.19%	0.023%
43	18.697	2585	2588	2591	rBV3	3628	4574	0.13%	0.016%
44	18.891	2620	2621	2624	rBV3	6498	6932	0.20%	0.024%
45	19.584	2735	2739	2743	rBV6	5815	7640	0.23%	0.027%
46	19.643	2743	2749	2754	rBV	34317	58107	1.71%	0.205%
47	19.707	2754	2760	2764	rVB	33691	53928	1.59%	0.190%
48	19.796	2772	2775	2781	rVB4	24233	30291	0.89%	0.107%
49	19.948	2797	2801	2805	rBV5	12220	15934	0.47%	0.056%
50	20.078	2816	2823	2831	rBV	2345611	3393081	100.00%	11.952%
51	20.683	2924	2926	2927	rBV2	7036	6052	0.18%	0.021%
52	21.593	3078	3081	3088	rVB6	23785	36676	1.08%	0.129%
53	22.034	3148	3156	3164	rBV	877193	1596007	47.04%	5.622%
54	22.187	3180	3182	3186	rBV4	10682	10347	0.30%	0.036%
55	23.538	3410	3412	3413	rVB2	9013	4486	0.13%	0.016%
56	23.615	3422	3425	3426	rBV3	13725	15396	0.45%	0.054%
57	24.878	3638	3640	3641	rVB2	8759	4804	0.14%	0.017%
58	25.366	3711	3723	3736	rVB2	1042547	3292792	97.04%	11.599%
59	25.618	3753	3766	3778	rVB3	532520	1736391	51.17%	6.116%
60	26.012	3831	3833	3835	rBV2	7693	5823	0.17%	0.021%
61	26.264	3874	3876	3879	rBV4	6430	5899	0.17%	0.021%
62	26.488	3913	3914	3917	rBV3	8376	8277	0.24%	0.029%
63	27.863	4146	4148	4149	rBV2	6468	5110	0.15%	0.018%
64	28.756	4298	4300	4303	rBV4	6678	7509	0.22%	0.026%
65	29.531	4430	4432	4433	rBV2	8773	5317	0.16%	0.019%
66	29.566	4436	4438	4439	rBV2	6083	4688	0.14%	0.017%
67	31.864	4827	4829	4830	rBV2	6434	4813	0.14%	0.017%
68	32.263	4895	4897	4900	rVB4	6091	4819	0.14%	0.017%
69	32.416	4922	4923	4927	rVB4	6332	5810	0.17%	0.020%
70	32.469	4930	4932	4934	rBV3	8709	7186	0.21%	0.025%




Sum of corrected areas: 28388838

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058926.D
Acq On : 8 Sep 2023 20:58
Operator : MA/JU
Sample : 04227-21
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJ90

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

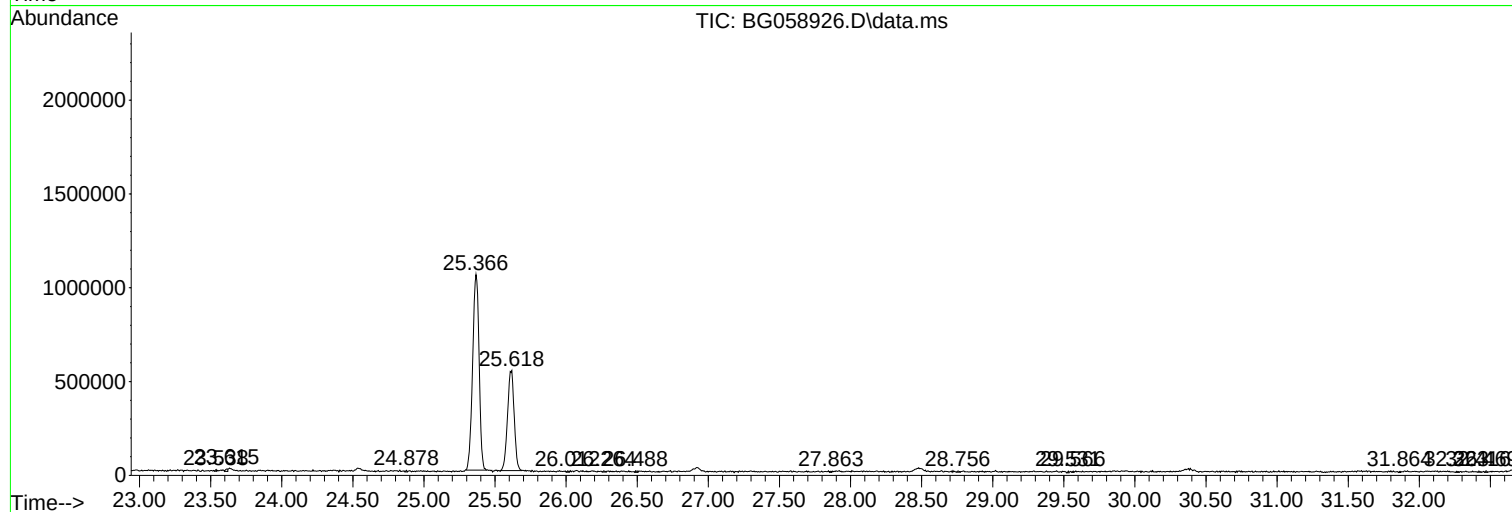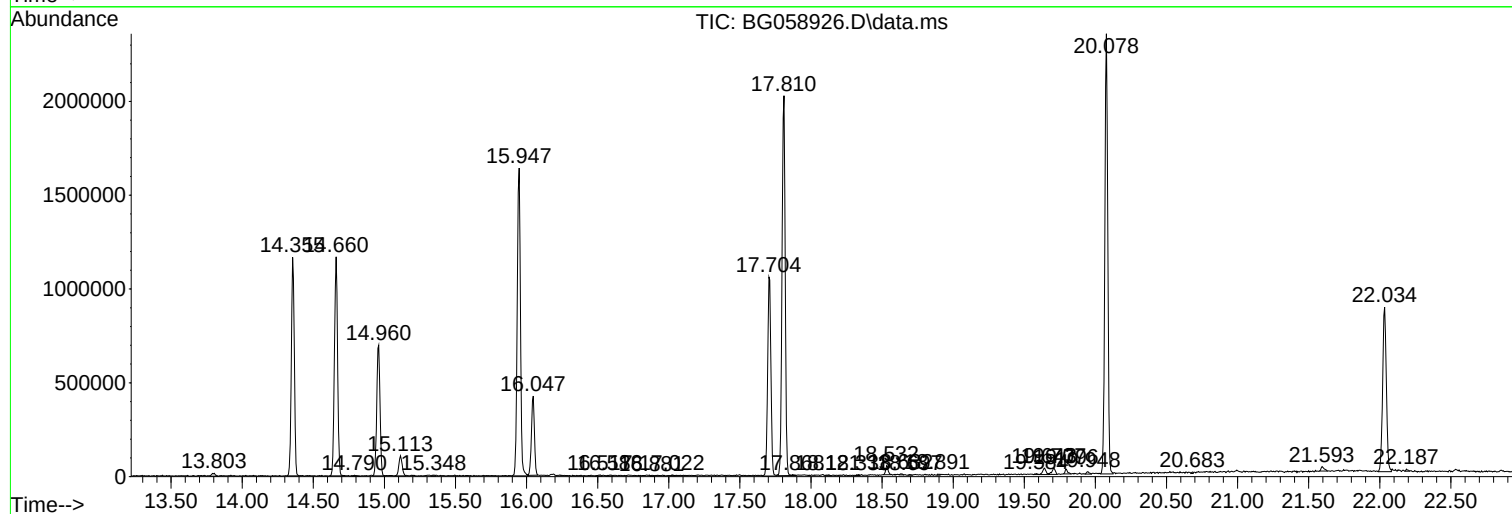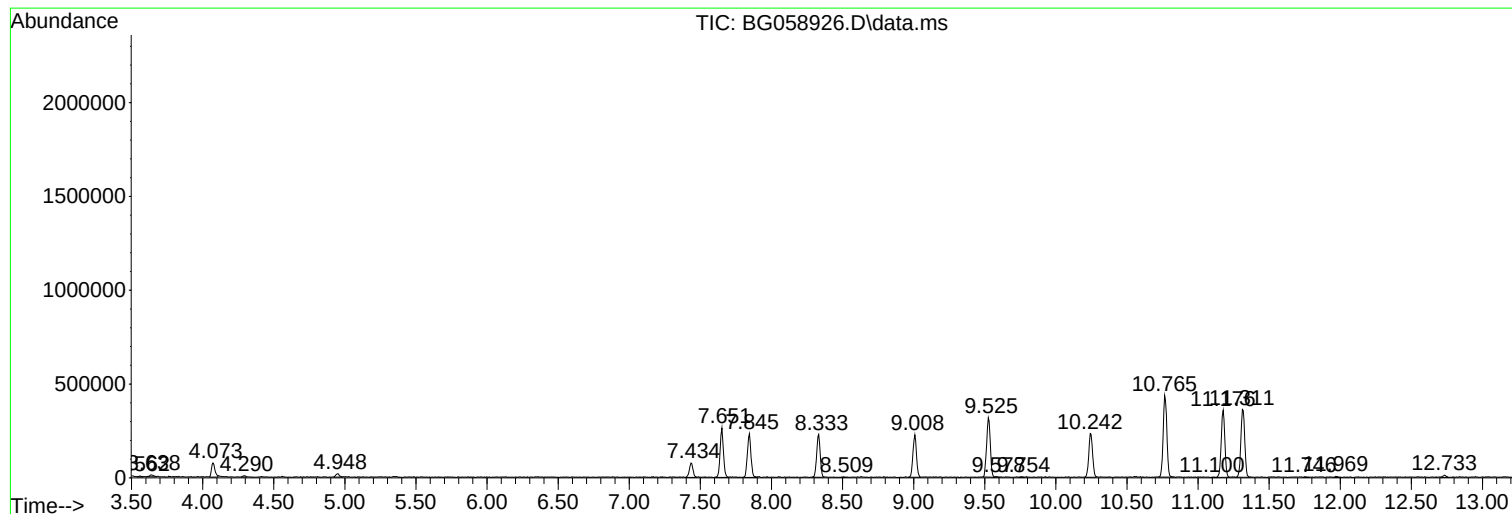

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058926.D
Acq On : 8 Sep 2023 20:58
Operator : MA/JU
Sample : 04227-21
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJ90

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058926.D
Acq On : 8 Sep 2023 20:58
Operator : MA/JU
Sample : 04227-21
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJ90

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc