

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058927.D
 Acq On : 8 Sep 2023 21:40
 Operator : MA/JU
 Sample : 04227-22
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBKF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.641	22	26	33	rVB3	11080	20216	0.62%	0.075%
2	4.075	95	100	108	rBV	63234	101083	3.09%	0.374%
3	4.416	154	158	163	rVB	15796	24079	0.73%	0.089%
4	4.951	244	249	255	rBV3	22962	37764	1.15%	0.140%
5	5.503	341	343	346	rBV3	2947	4282	0.13%	0.016%
6	5.903	405	411	412	rBV	4607	6531	0.20%	0.024%
7	6.243	466	469	473	rVB	3750	5553	0.17%	0.021%
8	6.302	475	479	483	rVB2	5087	6656	0.20%	0.025%
9	7.377	656	662	663	rBV	4792	4794	0.15%	0.018%
10	7.436	666	672	681	rVB2	64458	117058	3.57%	0.433%
11	7.653	701	709	717	rBV	242148	404814	12.36%	1.497%
12	7.742	720	724	725	rBV	5620	5815	0.18%	0.022%
13	7.841	734	741	750	rBV	221682	378633	11.56%	1.400%
14	8.165	793	796	801	rVB	2915	4398	0.13%	0.016%
15	8.329	817	824	833	rVB	229597	404441	12.35%	1.495%
16	8.535	855	859	862	rVB2	3305	5048	0.15%	0.019%
17	8.629	869	875	877	rVB2	4443	6282	0.19%	0.023%
18	9.005	933	939	947	rVB2	200586	332581	10.15%	1.230%
19	9.322	989	993	996	rBV2	3041	4234	0.13%	0.016%
20	9.528	1021	1028	1035	rBV	311675	529965	16.18%	1.960%
21	9.757	1061	1067	1070	rBV3	13298	22120	0.68%	0.082%
22	10.245	1142	1150	1158	rBV2	223529	409514	12.50%	1.514%
23	10.333	1162	1165	1168	rVB2	4086	5452	0.17%	0.020%
24	10.485	1187	1191	1193	rBV	3336	5169	0.16%	0.019%
25	10.767	1231	1239	1246	rBV	401899	707716	21.60%	2.617%
26	11.173	1301	1308	1316	rBV	330104	612602	18.70%	2.265%
27	11.314	1324	1332	1340	rBV	364710	672254	20.52%	2.486%
28	11.384	1342	1344	1348	rVB	3867	5674	0.17%	0.021%
29	11.719	1397	1401	1405	rBV	3234	4955	0.15%	0.018%
30	12.248	1486	1491	1495	rBV3	17511	26931	0.82%	0.100%
31	12.730	1568	1573	1579	rVB3	11001	19592	0.60%	0.072%
32	12.977	1612	1615	1617	rBV	4874	5915	0.18%	0.022%
33	13.793	1750	1754	1759	rVB4	9564	14531	0.44%	0.054%
34	13.975	1779	1785	1791	rVB2	23357	36304	1.11%	0.134%
35	14.216	1822	1826	1831	rBV4	7250	11895	0.36%	0.044%
36	14.357	1843	1850	1856	rVB	983916	1469599	44.86%	5.434%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058927.D
 Acq On : 8 Sep 2023 21:40
 Operator : MA/JU
 Sample : 04227-22
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBKF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

37	14.469	1866	1869	1872	rVB	3564	4551	0.14%	0.017%
38	14.657	1894	1901	1910	rVB	1001540	1594705	48.68%	5.897%
39	14.892	1936	1941	1944	rBV	2645	4477	0.14%	0.017%
40	14.957	1945	1952	1958	rVB	683338	1065271	32.52%	3.939%
41	15.109	1972	1978	1986	rBV	88055	135820	4.15%	0.502%
42	15.303	2008	2011	2016	rVB4	3593	4353	0.13%	0.016%
43	15.497	2041	2044	2047	rBV	3236	4524	0.14%	0.017%
44	15.944	2112	2120	2127	rVB	1456476	2196115	67.03%	8.120%
45	16.044	2130	2137	2145	rVB	373210	553239	16.89%	2.046%
46	16.179	2156	2160	2165	rBV3	7298	10165	0.31%	0.038%
47	16.473	2208	2210	2215	rVB3	3706	4687	0.14%	0.017%
48	16.931	2285	2288	2291	rBV	3011	4463	0.14%	0.017%
49	17.706	2411	2420	2427	rBV	1074197	1667361	50.89%	6.165%
50	17.806	2430	2437	2445	rBV2	1851340	2768203	84.50%	10.236%
51	18.035	2472	2476	2480	rBV3	4770	9920	0.30%	0.037%
52	18.347	2527	2529	2532	rVB	5021	5107	0.16%	0.019%
53	18.529	2553	2560	2566	rBV4	56753	89135	2.72%	0.330%
54	18.823	2602	2610	2611	rBV3	7396	14370	0.44%	0.053%
55	18.870	2617	2618	2622	rVB3	6798	6713	0.20%	0.025%
56	18.899	2622	2623	2626	rBV3	5557	5477	0.17%	0.020%
57	19.052	2645	2649	2650	rBV4	6664	5337	0.16%	0.020%
58	19.263	2683	2685	2688	rBV3	5059	4343	0.13%	0.016%
59	19.399	2705	2708	2709	rBV	7584	7961	0.24%	0.029%
60	19.639	2744	2749	2753	rBV3	29227	44396	1.36%	0.164%
61	19.704	2755	2760	2765	rVB	31175	49724	1.52%	0.184%
62	19.792	2771	2775	2779	rBV4	21941	32647	1.00%	0.121%
63	19.880	2788	2790	2793	rVB3	5776	5942	0.18%	0.022%
64	19.939	2797	2800	2808	rVB5	13275	22782	0.70%	0.084%
65	20.074	2817	2823	2833	rVB	2198433	3110472	94.94%	11.501%
66	20.709	2930	2931	2933	rBV2	6764	4653	0.14%	0.017%
67	20.997	2978	2980	2982	rBV3	9588	6367	0.19%	0.024%
68	21.155	3005	3007	3008	rBV2	5998	4700	0.14%	0.017%
69	21.285	3027	3029	3034	rBV6	8526	11346	0.35%	0.042%
70	21.596	3079	3082	3086	rBV5	41158	54893	1.68%	0.203%
71	22.031	3149	3156	3165	rBV	946355	1671621	51.02%	6.181%
72	22.654	3261	3262	3263	rVB	14458	5096	0.16%	0.019%
73	22.665	3263	3264	3269	rBV5	10093	16093	0.49%	0.060%
74	23.500	3404	3406	3408	rBV3	9725	7577	0.23%	0.028%
75	23.599	3421	3423	3424	rBV2	7131	6002	0.18%	0.022%
76	23.840	3460	3464	3465	rBV4	10842	13973	0.43%	0.052%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058927.D
 Acq On : 8 Sep 2023 21:40
 Operator : MA/JU
 Sample : 04227-22
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBKF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

77	24.222	3527	3529	3532	rBV4	7383	7856	0.24%	0.029%
78	24.516	3577	3579	3580	rBV2	10765	7682	0.23%	0.028%
79	24.675	3604	3606	3608	rVB3	7468	4931	0.15%	0.018%
80	24.857	3635	3637	3641	rBV5	8389	10721	0.33%	0.040%
81	25.362	3711	3723	3738	rVB2	1083433	3276100	100.00%	12.114%
82	25.609	3753	3765	3776	rBV2	602210	1897554	57.92%	7.016%
83	25.850	3804	3806	3807	rBV2	7215	4237	0.13%	0.016%
84	25.973	3825	3827	3829	rBV3	7768	5903	0.18%	0.022%
85	26.555	3925	3926	3930	rBV2	9464	8139	0.25%	0.030%
86	26.896	3980	3984	3985	rBV4	18897	19968	0.61%	0.074%
87	27.971	4165	4167	4170	rBV4	7693	5183	0.16%	0.019%
88	28.118	4190	4192	4195	rBV2	7052	6243	0.19%	0.023%
89	28.470	4246	4252	4265	rVB2	21524	71644	2.19%	0.265%
90	28.629	4277	4279	4281	rBV3	7097	6596	0.20%	0.024%
91	28.652	4281	4283	4284	rVB2	8057	4234	0.13%	0.016%
92	30.339	4564	4570	4571	rBV5	15811	19860	0.61%	0.073%
93	30.591	4611	4613	4615	rBV3	6099	6279	0.19%	0.023%
94	31.249	4723	4725	4727	rBV3	6712	5433	0.17%	0.020%
95	31.537	4772	4774	4776	rBV3	8983	6755	0.21%	0.025%




Sum of corrected areas: 27044349

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058927.D
Acq On : 8 Sep 2023 21:40
Operator : MA/JU
Sample : 04227-22
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBKF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

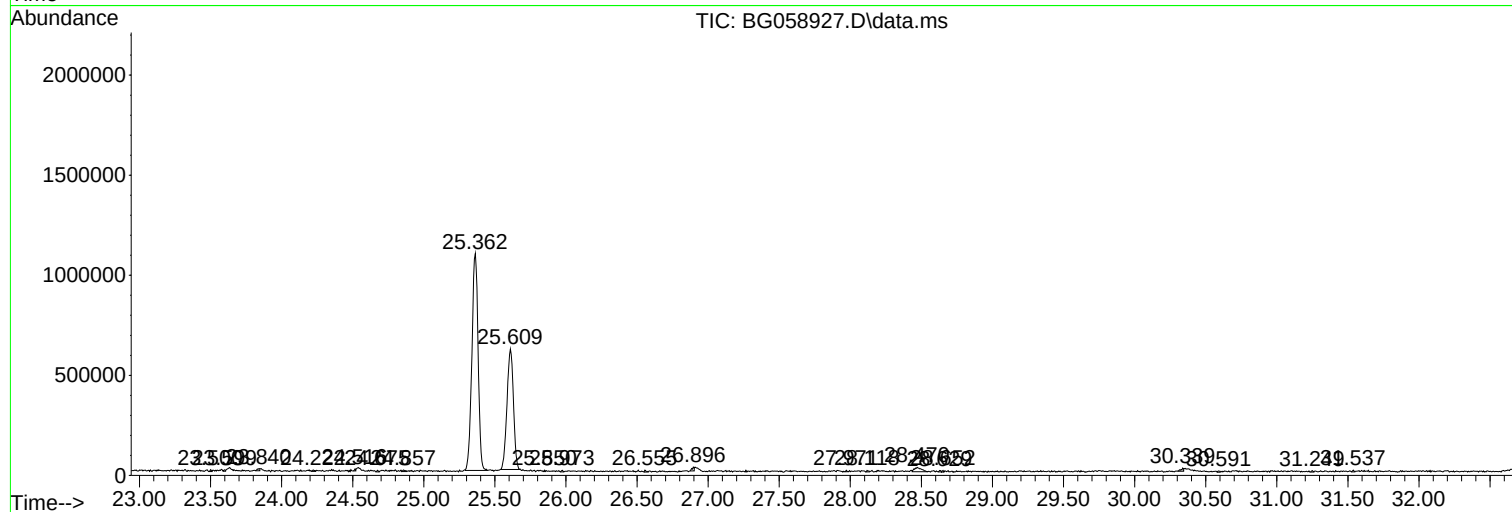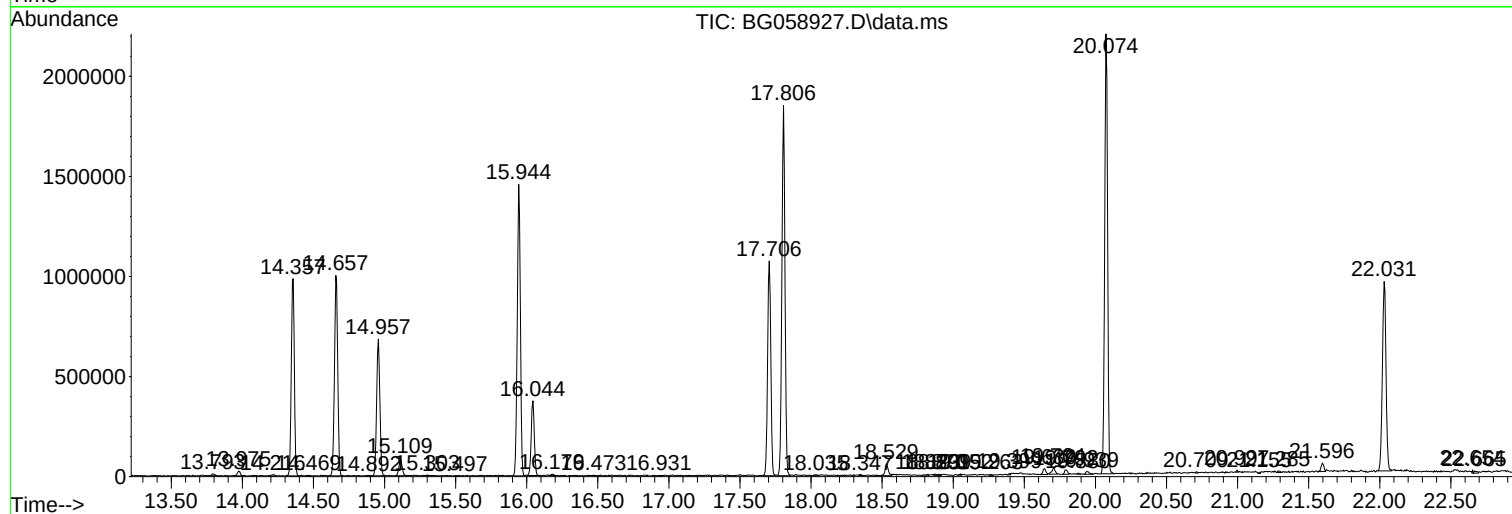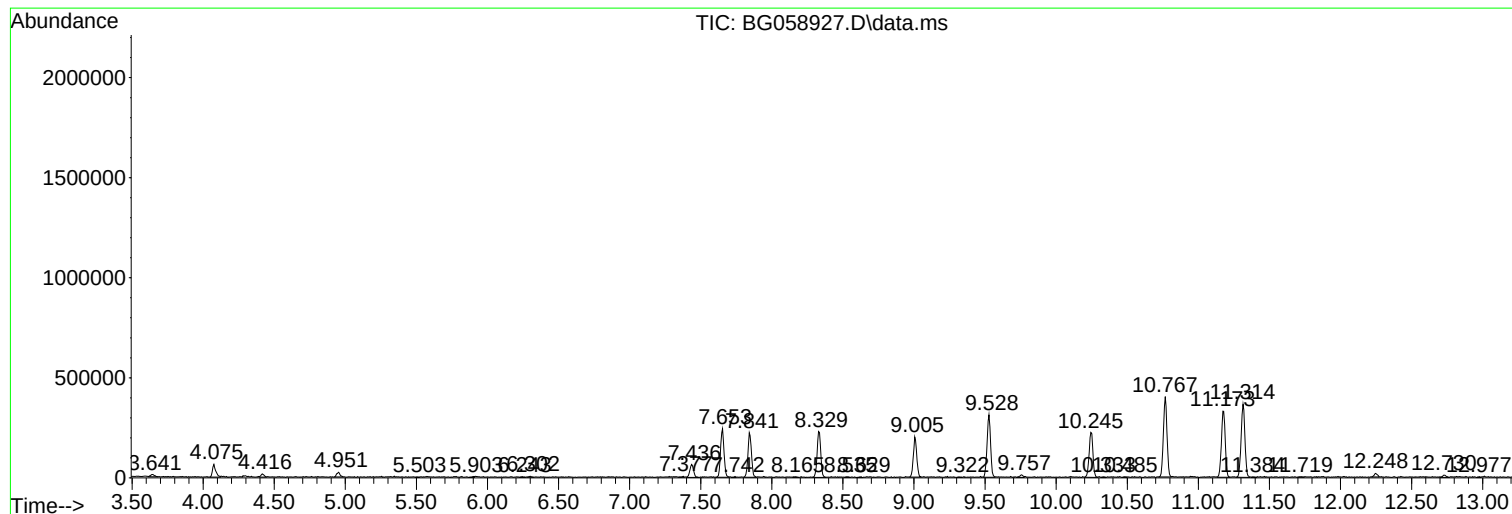

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058927.D
Acq On : 8 Sep 2023 21:40
Operator : MA/JU
Sample : 04227-22
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBKF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058927.D
Acq On : 8 Sep 2023 21:40
Operator : MA/JU
Sample : 04227-22
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBKF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc