

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058939.D
 Acq On : 9 Sep 2023 6:41
 Operator : MA/JU
 Sample : PB155303BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK303

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058939.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.642	20	26	33	rVB5	13030	26325	1.07%	0.110%
2	4.029	90	92	94	rBV2	119580	43630	1.77%	0.183%
3	4.070	94	99	109	rVV	135076	259923	10.55%	1.090%
4	4.300	136	138	141	rVB3	5781	3847	0.16%	0.016%
5	4.347	141	146	147	rBV3	3570	4697	0.19%	0.020%
6	4.429	156	160	161	rVB4	3798	4723	0.19%	0.020%
7	5.022	258	261	263	rBV2	3408	4240	0.17%	0.018%
8	5.152	282	283	288	rBV	3250	4594	0.19%	0.019%
9	5.275	301	304	307	rBV2	4309	5804	0.24%	0.024%
10	5.351	316	317	321	rBV	3241	3960	0.16%	0.017%
11	5.763	384	387	389	rBV3	3112	4487	0.18%	0.019%
12	6.045	431	435	438	rVV	2867	4419	0.18%	0.019%
13	6.944	582	588	592	rBV	2984	5423	0.22%	0.023%
14	7.437	665	672	679	rVB	241311	418711	16.99%	1.756%
15	7.555	690	692	697	rVB	3536	4909	0.20%	0.021%
16	7.649	700	708	716	rVV	177051	300566	12.20%	1.260%
17	7.843	735	741	750	rVB2	207702	371300	15.07%	1.557%
18	8.025	769	772	777	rVB3	2671	4531	0.18%	0.019%
19	8.330	818	824	833	rVB	213868	369245	14.98%	1.548%
20	8.448	841	844	846	rBV	3020	3688	0.15%	0.015%
21	9.006	932	939	948	rBV2	312478	532568	21.61%	2.233%
22	9.082	950	952	955	rVB	5022	4574	0.19%	0.019%
23	9.123	955	959	961	rBV	3754	5353	0.22%	0.022%
24	9.159	961	965	967	rVB	4584	6188	0.25%	0.026%
25	9.188	967	970	971	rBV	3503	3927	0.16%	0.016%
26	9.353	997	998	1003	rBV	5911	6778	0.28%	0.028%
27	9.523	1020	1027	1034	rVB	209884	381971	15.50%	1.602%
28	9.811	1073	1076	1080	rBV	2695	3789	0.15%	0.016%
29	10.246	1143	1150	1158	rVB	188768	339676	13.78%	1.424%
30	10.363	1167	1170	1173	rBV	3969	6793	0.28%	0.028%
31	10.398	1173	1176	1179	rVB	4977	7020	0.28%	0.029%
32	10.445	1183	1184	1187	rBV	4198	4505	0.18%	0.019%
33	10.639	1214	1217	1218	rBV	3503	3764	0.15%	0.016%
34	10.769	1230	1239	1246	rBV	329222	585587	23.76%	2.455%
35	10.868	1253	1256	1259	rBV	2368	3689	0.15%	0.015%
36	11.174	1300	1308	1316	rVV	321276	599006	24.31%	2.512%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058939.D
 Acq On : 9 Sep 2023 6:41
 Operator : MA/JU
 Sample : PB155303BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK303

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

37	11.315	1325	1332	1339	rVB	297929	539820	21.90%	2.264%
38	11.667	1389	1392	1394	rBV	3770	3656	0.15%	0.015%
39	11.838	1418	1421	1423	rBV	3957	4298	0.17%	0.018%
40	11.944	1438	1439	1442	rVB	5403	4062	0.16%	0.017%
41	12.608	1550	1552	1555	rBV	3293	3857	0.16%	0.016%
42	12.725	1568	1572	1573	rBV2	7692	10437	0.42%	0.044%
43	13.395	1683	1686	1690	rBV	3357	5840	0.24%	0.024%
44	13.794	1749	1754	1757	rBV2	12946	22223	0.90%	0.093%
45	14.353	1842	1849	1856	rBV2	823752	1160814	47.10%	4.867%
46	14.405	1856	1858	1862	rVB	2838	4082	0.17%	0.017%
47	14.529	1876	1879	1881	rBV	3786	4992	0.20%	0.021%
48	14.658	1893	1901	1909	rBV	753202	1218544	49.45%	5.110%
49	14.752	1914	1917	1920	rBV	3099	4987	0.20%	0.021%
50	14.799	1923	1925	1930	rBV	3457	4442	0.18%	0.019%
51	14.952	1943	1951	1959	rBV	711833	1119960	45.45%	4.696%
52	15.116	1972	1979	1987	rBV	386450	593789	24.09%	2.490%
53	15.193	1990	1992	1995	rVB3	6545	5608	0.23%	0.024%
54	15.228	1995	1998	2000	rBV	3764	4334	0.18%	0.018%
55	15.786	2090	2093	2094	rBV	3316	3785	0.15%	0.016%
56	15.851	2100	2104	2106	rVB	3431	3899	0.16%	0.016%
57	15.880	2106	2109	2111	rBV	3287	4210	0.17%	0.018%
58	15.939	2113	2119	2127	rVB	1100978	1718993	69.75%	7.208%
59	16.039	2129	2136	2142	rVV	310662	457820	18.58%	1.920%
60	16.115	2147	2149	2152	rVB	4621	4529	0.18%	0.019%
61	16.174	2156	2159	2160	rBV	7948	8505	0.35%	0.036%
62	16.450	2202	2206	2207	rVB	3979	4103	0.17%	0.017%
63	16.697	2246	2248	2251	rBV2	3123	3994	0.16%	0.017%
64	17.002	2296	2300	2304	rVB2	4442	6219	0.25%	0.026%
65	17.237	2339	2340	2342	rBV2	4930	3646	0.15%	0.015%
66	17.472	2379	2380	2386	rBV2	5634	6582	0.27%	0.028%
67	17.578	2395	2398	2399	rBV2	4395	3629	0.15%	0.015%
68	17.702	2413	2419	2428	rBV	1147961	1781133	72.27%	7.469%
69	17.801	2429	2436	2447	rVB2	1461030	2230057	90.49%	9.351%
70	17.878	2447	2449	2452	rBV	4450	6240	0.25%	0.026%
71	18.460	2547	2548	2553	rVB2	3907	4249	0.17%	0.018%
72	18.524	2557	2559	2560	rBV2	4617	4140	0.17%	0.017%
73	18.671	2582	2584	2587	rBV	4654	4219	0.17%	0.018%
74	19.570	2735	2737	2739	rVB	6140	4469	0.18%	0.019%
75	19.640	2744	2749	2754	rBV6	24101	36533	1.48%	0.153%
76	19.705	2754	2760	2765	rBV3	21298	39771	1.61%	0.167%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058939.D
 Acq On : 9 Sep 2023 6:41
 Operator : MA/JU
 Sample : PB155303BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK303

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

77	19.887	2787	2791	2793	rVB3	5918	5448	0.22%	0.023%
78	19.934	2797	2799	2803	rVB3	7906	9452	0.38%	0.040%
79	20.075	2816	2823	2833	rVB	1627072	2464411	100.00%	10.334%
80	20.246	2850	2852	2855	rVB4	5880	3813	0.15%	0.016%
81	20.757	2935	2939	2941	rBV2	6409	8150	0.33%	0.034%
82	20.986	2976	2978	2982	rBV4	8965	11935	0.48%	0.050%
83	21.086	2993	2995	2996	rBV2	5583	3891	0.16%	0.016%
84	21.291	3028	3030	3034	rVB3	7704	6807	0.28%	0.029%
85	21.579	3076	3079	3081	rBV3	11508	10407	0.42%	0.044%
86	22.032	3148	3156	3166	rVB	933666	1684989	68.37%	7.065%
87	22.478	3230	3232	3233	rVB2	8596	4314	0.18%	0.018%
88	24.605	3592	3594	3595	rBV2	8746	5657	0.23%	0.024%
89	25.351	3709	3721	3732	rBV2	761033	2325700	94.37%	9.752%
90	25.604	3754	3764	3777	rVB	595678	1837484	74.56%	7.705%
91	26.621	3935	3937	3940	rBV4	9652	10338	0.42%	0.043%
92	27.995	4169	4171	4172	rBV2	7487	4029	0.16%	0.017%
93	28.753	4298	4300	4302	rBV3	6845	4658	0.19%	0.020%
94	28.988	4338	4340	4342	rBV3	6610	6409	0.26%	0.027%
95	29.629	4447	4449	4451	rBV3	7763	6476	0.26%	0.027%
96	30.416	4581	4583	4585	rVB3	8677	3810	0.15%	0.016%
97	31.562	4776	4778	4780	rBV3	9653	9960	0.40%	0.042%
98	31.955	4843	4845	4846	rBV	6694	5266	0.21%	0.022%
99	31.973	4846	4848	4851	rVV4	8798	10006	0.41%	0.042%
100	32.243	4893	4894	4895	rBV	8282	4424	0.18%	0.019%




Sum of corrected areas: 23848514

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058939.D
Acq On : 9 Sep 2023 6:41
Operator : MA/JU
Sample : PB155303BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK303

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

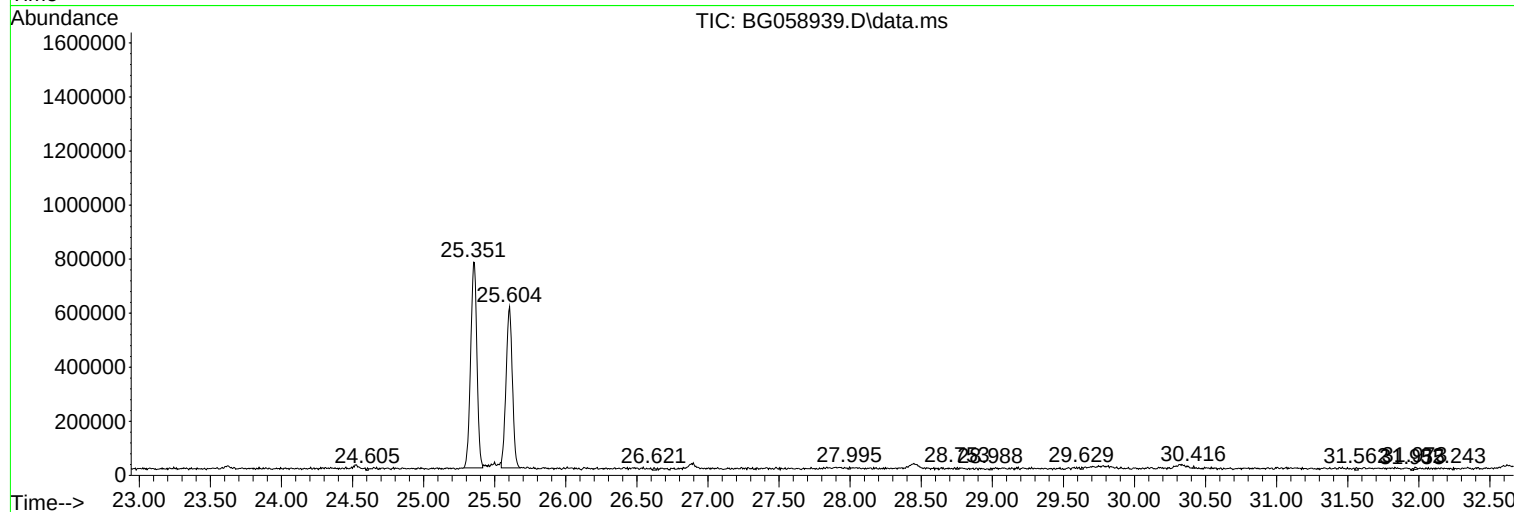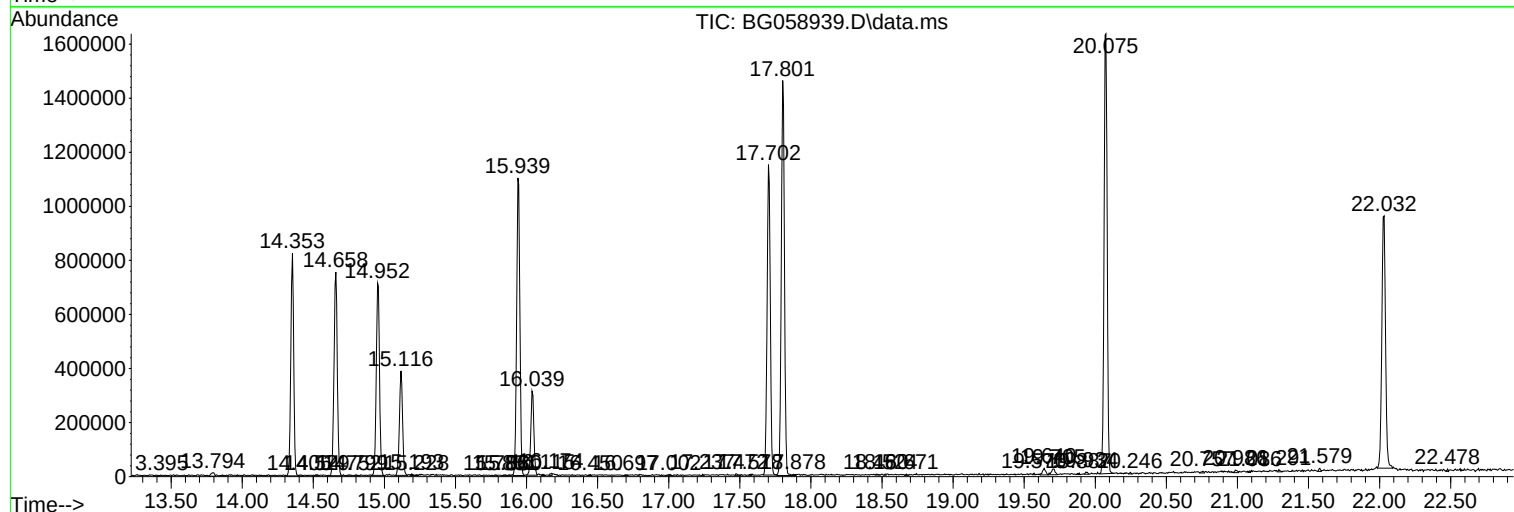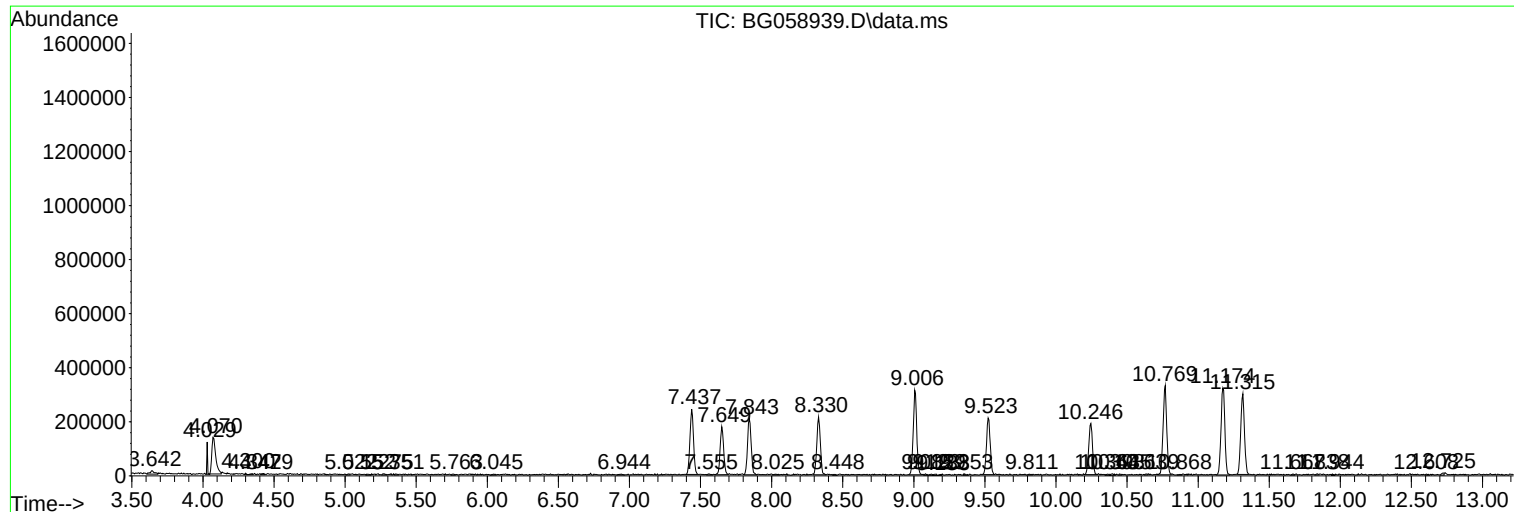

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058939.D
Acq On : 9 Sep 2023 6:41
Operator : MA/JU
Sample : PB155303BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK303

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058939.D
Acq On : 9 Sep 2023 6:41
Operator : MA/JU
Sample : PB155303BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK303

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc