

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058940.D
 Acq On : 9 Sep 2023 7:22
 Operator : MA/JU
 Sample : PB155306BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK306

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058940.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.647	21	27	29	rBV5	14210	20770	0.78%	0.080%
2	3.700	34	36	39	rBV3	4109	4235	0.16%	0.016%
3	3.918	72	73	77	rVB2	4526	4558	0.17%	0.018%
4	3.982	81	84	86	rBV	4093	5176	0.20%	0.020%
5	4.012	86	89	91	rVB	3616	4570	0.17%	0.018%
6	4.070	94	99	112	rBV	184607	346392	13.08%	1.338%
7	4.634	192	195	197	rBV2	3215	3705	0.14%	0.014%
8	5.527	346	347	350	rVB	5590	4733	0.18%	0.018%
9	6.544	519	520	524	rVB	4668	4257	0.16%	0.016%
10	7.020	600	601	609	rVB	2931	5515	0.21%	0.021%
11	7.143	619	622	628	rVB2	2395	4355	0.16%	0.017%
12	7.325	650	653	656	rBV2	4298	6081	0.23%	0.023%
13	7.437	666	672	681	rVB	291484	510718	19.28%	1.972%
14	7.578	693	696	700	rBV3	3463	4461	0.17%	0.017%
15	7.648	702	708	715	rVV	213607	356123	13.44%	1.375%
16	7.695	715	716	724	rVB	2642	4124	0.16%	0.016%
17	7.842	733	741	751	rBV	253192	451836	17.06%	1.745%
18	8.089	781	783	786	rVB	4215	4614	0.17%	0.018%
19	8.330	815	824	832	rBV	241690	420411	15.87%	1.624%
20	9.006	931	939	947	rBV	362408	639527	24.14%	2.470%
21	9.270	980	984	988	rVB	2972	3736	0.14%	0.014%
22	9.523	1020	1027	1035	rVB	265709	474344	17.91%	1.832%
23	9.652	1048	1049	1054	rVB	4022	5284	0.20%	0.020%
24	9.699	1054	1057	1058	rBV	4292	4697	0.18%	0.018%
25	10.245	1143	1150	1158	rVB2	220423	401130	15.14%	1.549%
26	10.422	1175	1180	1184	rBV	2674	4866	0.18%	0.019%
27	10.762	1231	1238	1247	rBV	376100	684141	25.83%	2.642%
28	11.109	1295	1297	1301	rBV	3264	4789	0.18%	0.018%
29	11.174	1301	1308	1316	rVB	358643	650388	24.55%	2.512%
30	11.315	1322	1332	1340	rBV2	342622	650341	24.55%	2.512%
31	11.444	1352	1354	1357	rVB2	4596	3832	0.14%	0.015%
32	11.661	1387	1391	1392	rBV2	5363	4762	0.18%	0.018%
33	11.685	1392	1395	1398	rBV2	3665	4304	0.16%	0.017%
34	11.744	1400	1405	1407	rBV2	2550	3873	0.15%	0.015%
35	11.938	1435	1438	1442	rVB2	2866	3923	0.15%	0.015%
36	12.043	1454	1456	1458	rBV	4989	4474	0.17%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058940.D
 Acq On : 9 Sep 2023 7:22
 Operator : MA/JU
 Sample : PB155306BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK306

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

37	12.643	1557	1558	1563	rVB2	3861	4387	0.17%	0.017%
38	12.690	1563	1566	1569	rBV2	3507	3996	0.15%	0.015%
39	12.725	1569	1572	1577	rVB3	8274	12798	0.48%	0.049%
40	13.030	1622	1624	1626	rVB3	5424	3793	0.14%	0.015%

41	13.072	1626	1631	1633	rBV3	2917	4020	0.15%	0.016%
42	13.377	1681	1683	1687	rBV	3437	4518	0.17%	0.017%
43	13.794	1748	1754	1762	rBV3	13949	25725	0.97%	0.099%
44	13.965	1781	1783	1786	rVB	4012	4625	0.17%	0.018%
45	14.223	1825	1827	1829	rBV	4351	4199	0.16%	0.016%

46	14.352	1841	1849	1856	rBV	916343	1324098	49.98%	5.113%
47	14.546	1878	1882	1887	rBV	2919	5169	0.20%	0.020%
48	14.658	1892	1901	1907	rBV	856828	1386971	52.36%	5.356%
49	14.952	1940	1951	1958	rBV	721009	1161078	43.83%	4.484%
50	15.116	1970	1979	1988	rBV	414224	646652	24.41%	2.497%

51	15.228	1996	1998	2000	rVB2	4466	4006	0.15%	0.015%
52	15.939	2113	2119	2127	rVB	1252617	1940385	73.25%	7.493%
53	16.039	2130	2136	2145	rVV	349395	510749	19.28%	1.972%
54	16.121	2148	2150	2153	rVB2	4560	5124	0.19%	0.020%
55	16.180	2156	2160	2164	rVB4	4180	6291	0.24%	0.024%

56	16.262	2171	2174	2175	rVB4	6083	4005	0.15%	0.015%
57	16.567	2225	2226	2230	rBV	4119	4676	0.18%	0.018%
58	16.714	2250	2251	2254	rBV3	4841	4273	0.16%	0.017%
59	17.184	2328	2331	2334	rBV3	3313	4412	0.17%	0.017%
60	17.361	2359	2361	2364	rBV2	3573	4872	0.18%	0.019%

61	17.701	2412	2419	2428	rBV	1136236	1779836	67.19%	6.873%
62	17.801	2429	2436	2443	rVV	1504204	2356105	88.94%	9.099%
63	17.866	2446	2447	2450	rBV2	4706	4117	0.16%	0.016%
64	17.895	2450	2452	2456	rVB3	5796	3759	0.14%	0.015%
65	17.989	2466	2468	2471	rBV	4518	4878	0.18%	0.019%

66	18.077	2480	2483	2488	rVB2	4258	7594	0.29%	0.029%
67	18.653	2579	2581	2583	rBV2	3874	3888	0.15%	0.015%
68	18.730	2592	2594	2598	rVB2	4661	5804	0.22%	0.022%
69	18.782	2598	2603	2605	rBV	4461	6662	0.25%	0.026%
70	18.918	2622	2626	2628	rBV	4120	6428	0.24%	0.025%

71	19.223	2675	2678	2680	rBV2	4394	4360	0.16%	0.017%
72	19.276	2684	2687	2690	rVV2	3440	4498	0.17%	0.017%
73	19.305	2690	2692	2695	rVB3	5817	4271	0.16%	0.016%
74	19.429	2711	2713	2716	rBV2	5503	5184	0.20%	0.020%
75	19.482	2719	2722	2723	rBV3	5105	5051	0.19%	0.020%

76	19.576	2737	2738	2741	rVB2	4366	4165	0.16%	0.016%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058940.D
 Acq On : 9 Sep 2023 7:22
 Operator : MA/JU
 Sample : PB155306BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK306

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

77	19.640	2743	2749	2753	rBV3	23861	41342	1.56%	0.160%
78	19.705	2755	2760	2764	rVB3	23153	36095	1.36%	0.139%
79	19.864	2786	2787	2791	rVB3	4815	4355	0.16%	0.017%
80	19.893	2791	2792	2794	rBV2	5938	4507	0.17%	0.017%
81	19.963	2803	2804	2807	rVB2	7842	4808	0.18%	0.019%
82	20.075	2816	2823	2829	rBV	1838014	2649123	100.00%	10.231%
83	20.586	2908	2910	2912	rBV2	4813	3745	0.14%	0.014%
84	20.745	2935	2937	2941	rBV5	3764	4767	0.18%	0.018%
85	21.144	3003	3005	3006	rBV2	5122	4283	0.16%	0.017%
86	21.644	3089	3090	3091	rBV	10359	3906	0.15%	0.015%
87	22.026	3148	3155	3162	rBV2	990630	1660545	62.68%	6.413%
88	22.367	3211	3213	3214	rBV2	7793	4471	0.17%	0.017%
89	23.119	3339	3341	3343	rVB2	7420	4122	0.16%	0.016%
90	23.195	3353	3354	3357	rVB3	7862	4945	0.19%	0.019%
91	24.270	3535	3537	3538	rBV2	7956	4346	0.16%	0.017%
92	25.010	3661	3663	3665	rBV2	6617	5026	0.19%	0.019%
93	25.351	3709	3721	3733	rBV2	851527	2553681	96.40%	9.862%
94	25.604	3752	3764	3776	rVB2	583239	1863088	70.33%	7.195%
95	26.609	3933	3935	3937	rBV3	7194	4835	0.18%	0.019%
96	27.384	4066	4067	4069	rBV	8836	5794	0.22%	0.022%
97	29.347	4399	4401	4402	rBV	8779	5295	0.20%	0.020%
98	29.364	4402	4404	4406	rVV3	6246	4425	0.17%	0.017%
99	31.544	4773	4775	4778	rBV4	7016	5726	0.22%	0.022%
100	32.513	4938	4940	4942	rBV3	9061	8612	0.33%	0.033%




Sum of corrected areas: 25894309

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058940.D
Acq On : 9 Sep 2023 7:22
Operator : MA/JU
Sample : PB155306BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

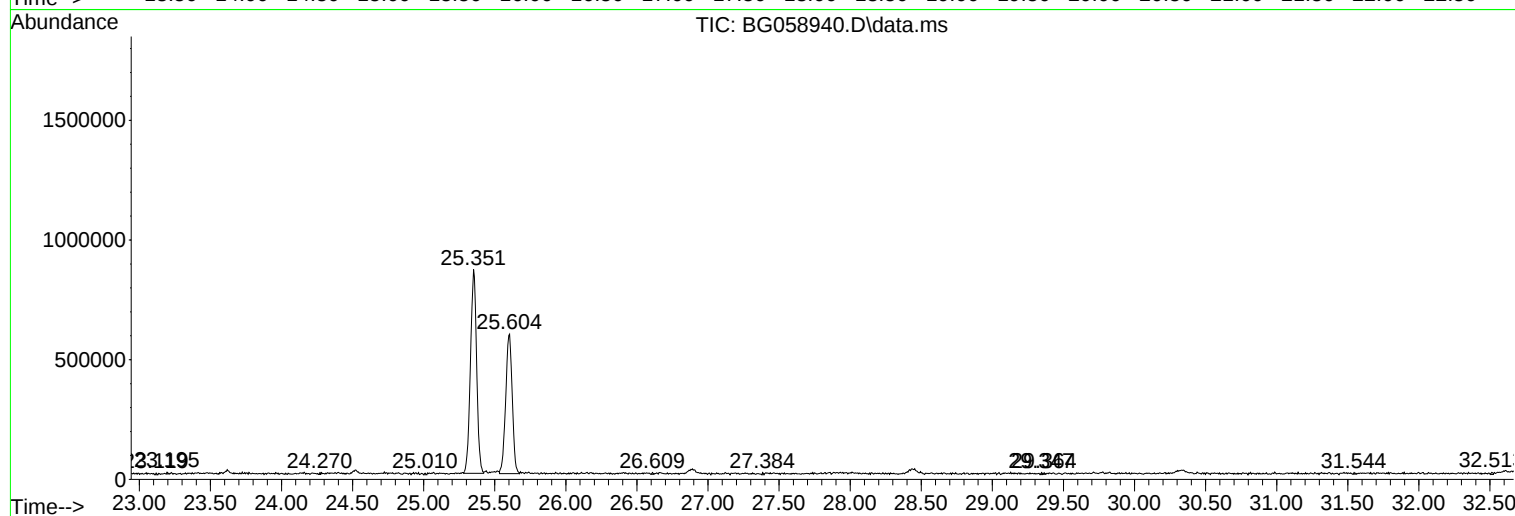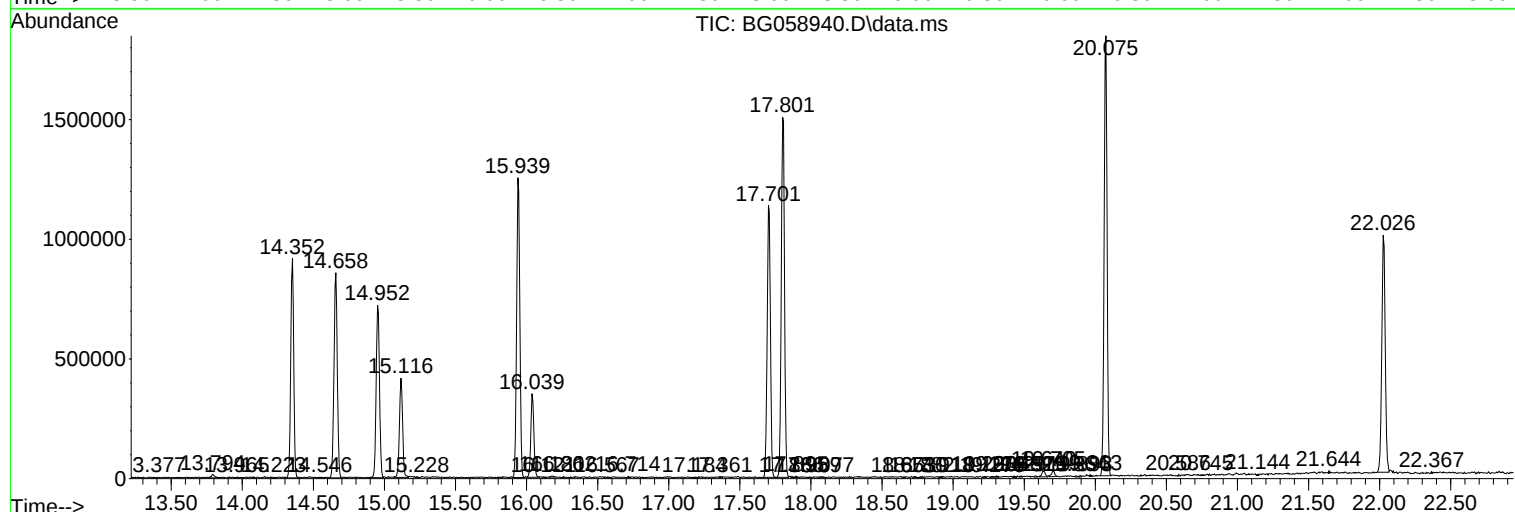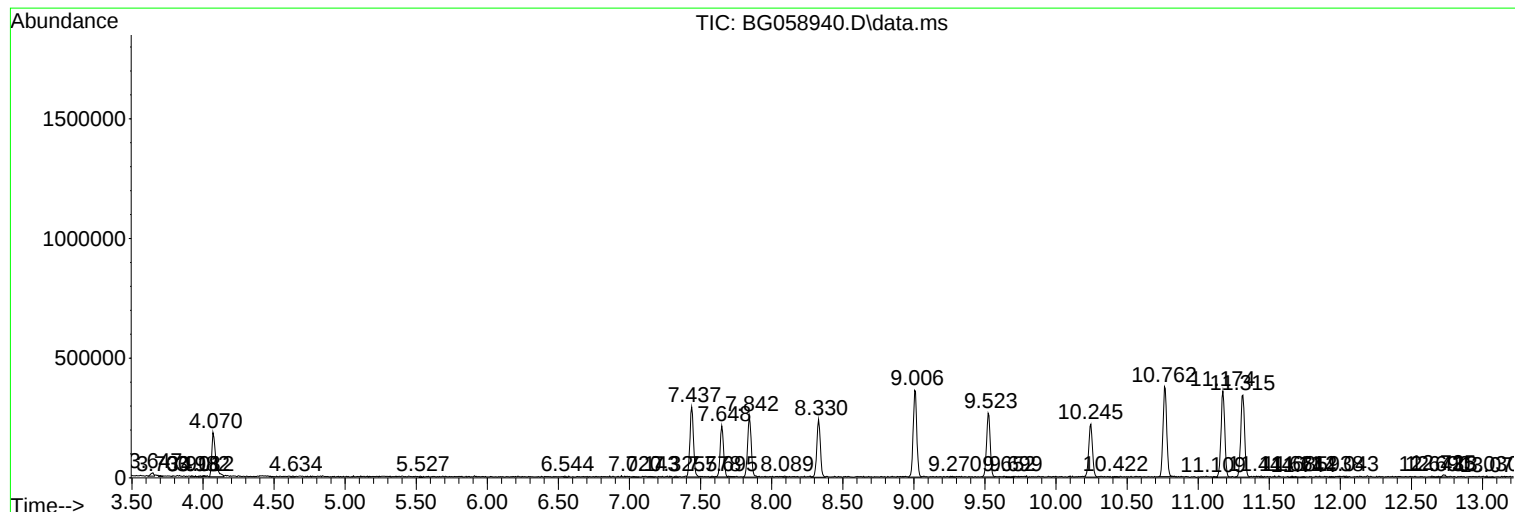

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058940.D
Acq On : 9 Sep 2023 7:22
Operator : MA/JU
Sample : PB155306BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058940.D
Acq On : 9 Sep 2023 7:22
Operator : MA/JU
Sample : PB155306BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc