

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058942.D
 Acq On : 9 Sep 2023 8:44
 Operator : MA/JU
 Sample : 04230-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BH493

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.724	37	40	43	rBV4	3828	5910	0.17%	0.022%
2	4.076	96	100	107	rBV2	43647	88702	2.56%	0.337%
3	4.276	129	134	135	rBV3	5795	6934	0.20%	0.026%
4	4.294	135	137	141	rVB3	8553	9243	0.27%	0.035%
5	4.405	154	156	159	rBV2	4691	5319	0.15%	0.020%
6	4.687	201	204	208	rVB3	3633	5393	0.16%	0.020%
7	4.787	219	221	224	rBV2	4526	4997	0.14%	0.019%
8	4.858	230	233	237	rVB5	3157	5493	0.16%	0.021%
9	5.345	311	316	319	rBV2	2709	6196	0.18%	0.024%
10	6.526	513	517	520	rBV2	3346	4724	0.14%	0.018%
11	7.437	664	672	677	rBV	66432	118454	3.42%	0.450%
12	7.649	700	708	718	rBV	221484	390910	11.29%	1.485%
13	7.842	733	741	752	rVB2	204571	376223	10.87%	1.429%
14	7.966	759	762	765	rBV2	6679	7476	0.22%	0.028%
15	8.107	782	786	788	rBV2	5105	6979	0.20%	0.027%
16	8.148	790	793	796	rBV	3687	4876	0.14%	0.019%
17	8.330	816	824	831	rBV	204324	367237	10.61%	1.395%
18	8.935	924	927	930	rBV	5278	5698	0.16%	0.022%
19	9.012	932	940	946	rBV	186420	339248	9.80%	1.289%
20	9.188	967	970	974	rBV	5529	7213	0.21%	0.027%
21	9.523	1020	1027	1035	rBV2	265507	492617	14.23%	1.872%
22	9.752	1062	1066	1070	rVB	6059	7008	0.20%	0.027%
23	10.163	1134	1136	1141	rBV	3319	6262	0.18%	0.024%
24	10.246	1141	1150	1158	rVV2	221050	415633	12.00%	1.579%
25	10.768	1231	1239	1247	rVB2	374326	676476	19.54%	2.570%
26	11.015	1277	1281	1282	rBV2	4028	5103	0.15%	0.019%
27	11.174	1300	1308	1317	rBV	314044	576634	16.65%	2.191%
28	11.315	1322	1332	1339	rBV	322135	596358	17.22%	2.266%
29	11.550	1370	1372	1376	rVB	5125	5848	0.17%	0.022%
30	11.650	1388	1389	1394	rVB2	4520	4773	0.14%	0.018%
31	12.043	1453	1456	1457	rBV2	5803	5118	0.15%	0.019%
32	12.566	1543	1545	1548	rBV2	4267	5382	0.16%	0.020%
33	12.725	1568	1572	1578	rVB4	11347	20948	0.60%	0.080%
34	12.825	1587	1589	1591	rBV	6218	5028	0.15%	0.019%
35	13.007	1618	1620	1623	rBV	4290	5304	0.15%	0.020%
36	13.501	1700	1704	1705	rVB2	6359	4852	0.14%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
 Data File : BG058942.D
 Acq On : 9 Sep 2023 8:44
 Operator : MA/JU
 Sample : 04230-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BH493

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
 Title : SVOA CALIBRATION

37	13.788	1751	1753	1762	rVB4	6814	13527	0.39%	0.051%
38	14.352	1840	1849	1855	rBV	997266	1420609	41.03%	5.397%
39	14.658	1894	1901	1909	rBV	982583	1532227	44.25%	5.821%
40	14.793	1921	1924	1929	rBV	3533	4685	0.14%	0.018%
41	14.899	1933	1942	1945	rBV2	8983	19153	0.55%	0.073%
42	14.952	1945	1951	1958	rVB2	636985	1016750	29.36%	3.863%
43	15.110	1972	1978	1985	rBV2	102879	163270	4.72%	0.620%
44	15.939	2111	2119	2128	rBV	1415176	2217763	64.05%	8.426%
45	16.039	2128	2136	2143	rVB	414477	611441	17.66%	2.323%
46	16.174	2156	2159	2161	rBV4	7012	6574	0.19%	0.025%
47	16.274	2175	2176	2180	rVB	4824	5027	0.15%	0.019%
48	16.309	2180	2182	2188	rBV	3823	6474	0.19%	0.025%
49	16.726	2250	2253	2255	rBV2	3632	4710	0.14%	0.018%
50	17.126	2318	2321	2323	rBV2	4365	4718	0.14%	0.018%
51	17.261	2341	2344	2347	rBV	3330	5167	0.15%	0.020%
52	17.372	2360	2363	2367	rVB	4844	6151	0.18%	0.023%
53	17.484	2380	2382	2387	rBV3	6550	9429	0.27%	0.036%
54	17.701	2412	2419	2427	rBV	1093087	1674570	48.36%	6.362%
55	17.801	2428	2436	2443	rBV2	1818518	2850892	82.33%	10.831%
56	18.301	2518	2521	2524	rBV2	4953	7356	0.21%	0.028%
57	18.530	2555	2560	2564	rBV3	49630	67195	1.94%	0.255%
58	18.918	2624	2626	2629	rVB3	5595	6001	0.17%	0.023%
59	18.947	2629	2631	2634	rBV3	5356	5607	0.16%	0.021%
60	19.082	2651	2654	2657	rVB4	6704	7339	0.21%	0.028%
61	19.511	2724	2727	2728	rBV2	5131	5170	0.15%	0.020%
62	19.558	2733	2735	2738	rBV3	4667	5778	0.17%	0.022%
63	19.593	2739	2741	2744	rVV2	7113	8337	0.24%	0.032%
64	19.640	2744	2749	2754	rVV3	31756	49290	1.42%	0.187%
65	19.705	2754	2760	2764	rVB2	32411	51070	1.47%	0.194%
66	19.787	2770	2774	2782	rBV5	30745	47289	1.37%	0.180%
67	19.940	2796	2800	2802	rBV4	12200	12873	0.37%	0.049%
68	20.075	2816	2823	2829	rBV	2451431	3462613	100.00%	13.156%
69	20.692	2924	2928	2929	rBV3	5736	7870	0.23%	0.030%
70	21.479	3060	3062	3064	rBV3	6783	6151	0.18%	0.023%
71	21.591	3078	3081	3086	rVB6	16444	24800	0.72%	0.094%
72	22.026	3148	3155	3163	rBV	911606	1610089	46.50%	6.117%
73	24.723	3612	3614	3615	rBV	7974	6545	0.19%	0.025%
74	25.357	3710	3722	3735	rVB2	953360	2972286	85.84%	11.293%
75	25.604	3754	3764	3777	rVB2	549580	1720357	49.68%	6.536%
76	26.767	3960	3962	3963	rBV2	7921	6910	0.20%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058942.D
Acq On : 9 Sep 2023 8:44
Operator : MA/JU
Sample : 04230-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH493

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Title : SVOA CALIBRATION

77	27.643	4109	4111	4112	rBV2	7737	5652	0.16%	0.021%
78	28.260	4214	4216	4218	rBV3	8948	6525	0.19%	0.025%
79	29.141	4364	4366	4367	rBV2	7213	5661	0.16%	0.022%
80	30.669	4624	4626	4627	rBV2	7252	5539	0.16%	0.021%
81	31.039	4687	4689	4692	rBV4	7440	8436	0.24%	0.032%
82	31.609	4782	4786	4787	rBV4	8398	10366	0.30%	0.039%
83	31.797	4816	4818	4820	rBV3	6560	5525	0.16%	0.021%
84	31.891	4832	4834	4837	rBV4	8173	8252	0.24%	0.031%




Sum of corrected areas: 26320588

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058942.D
Acq On : 9 Sep 2023 8:44
Operator : MA/JU
Sample : 04230-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH493

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

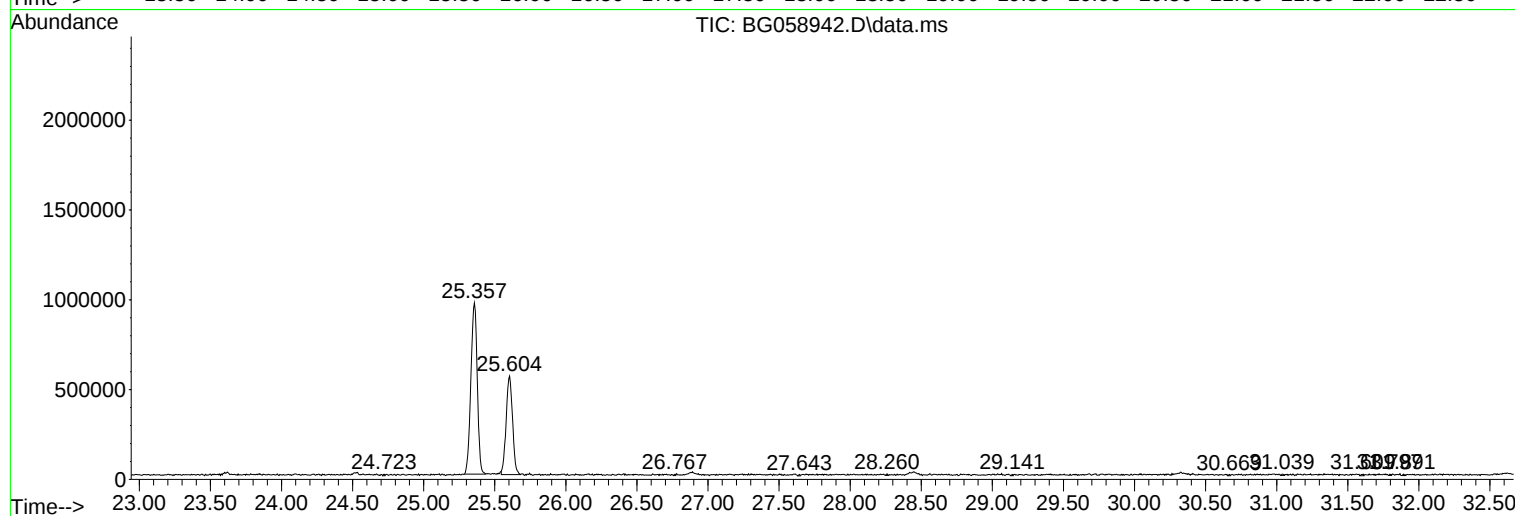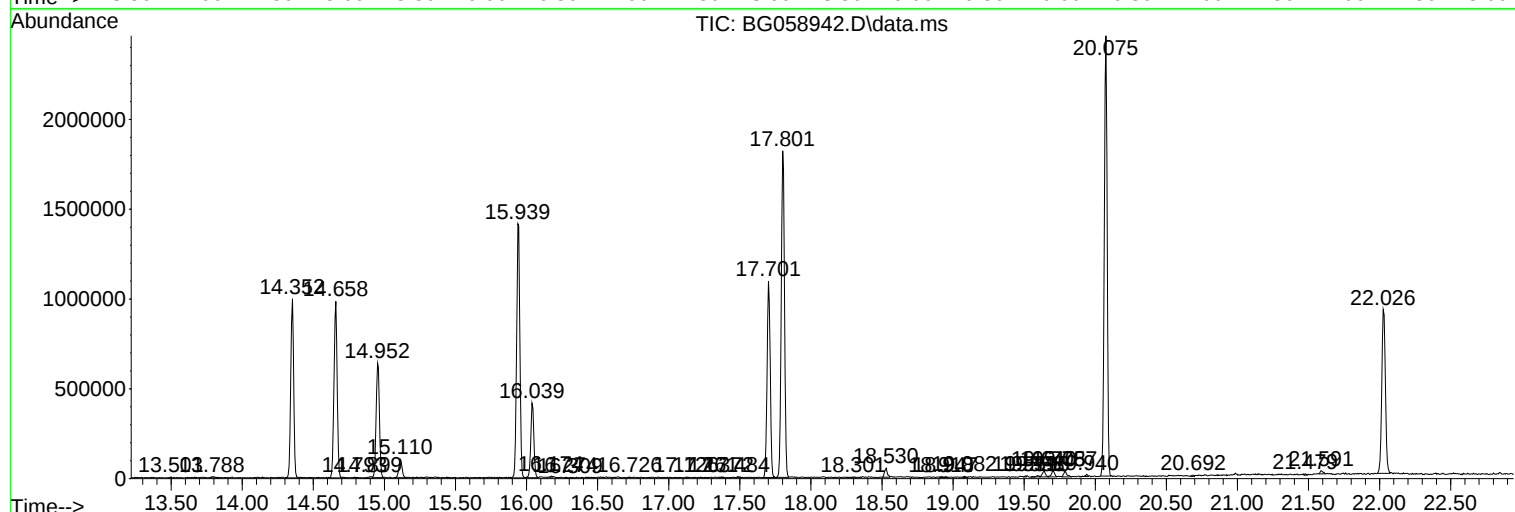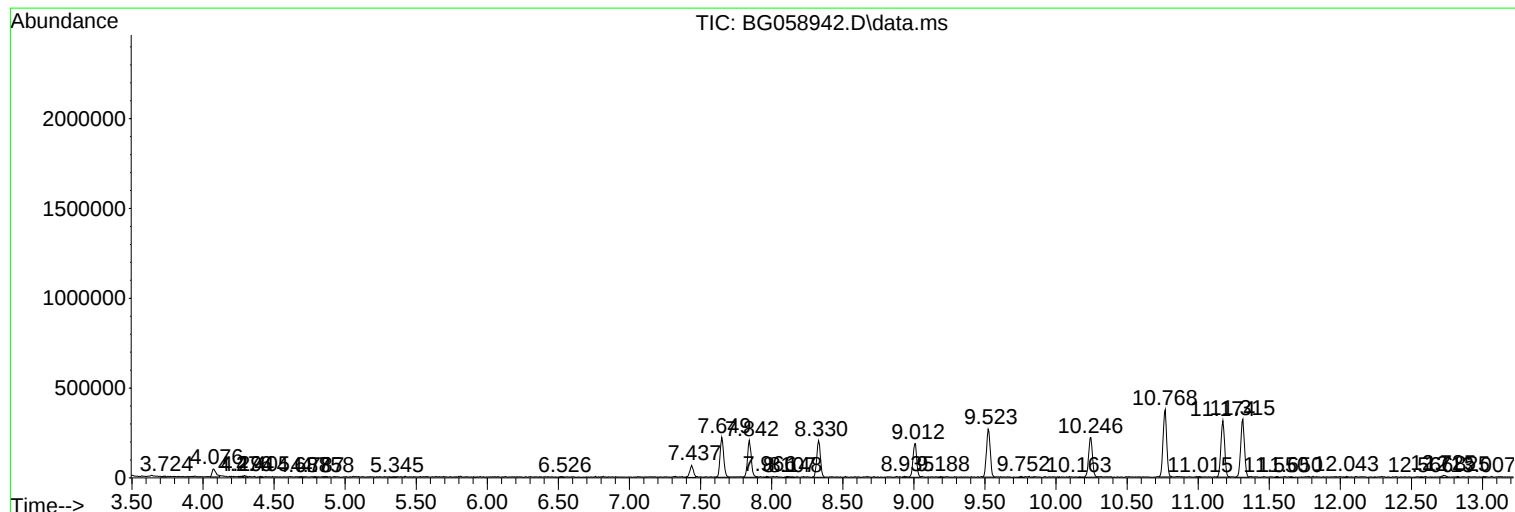

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058942.D
Acq On : 9 Sep 2023 8:44
Operator : MA/JU
Sample : 04230-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH493

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090823\
Data File : BG058942.D
Acq On : 9 Sep 2023 8:44
Operator : MA/JU
Sample : 04230-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH493

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc