
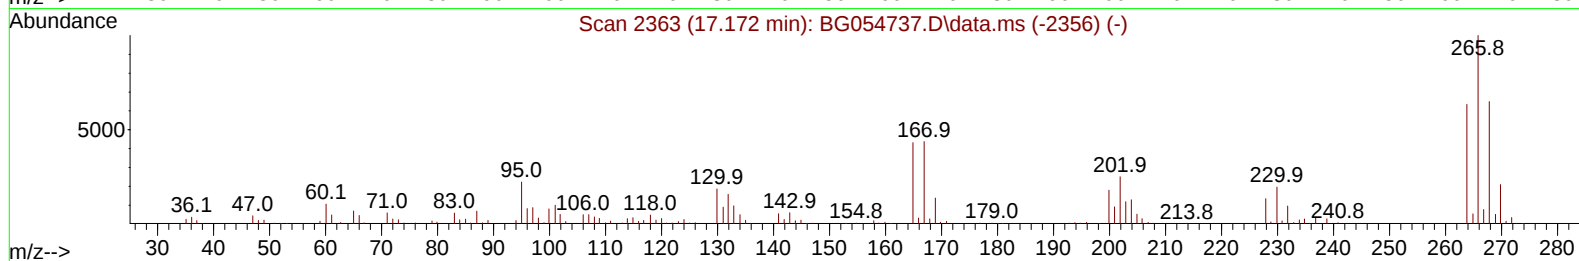
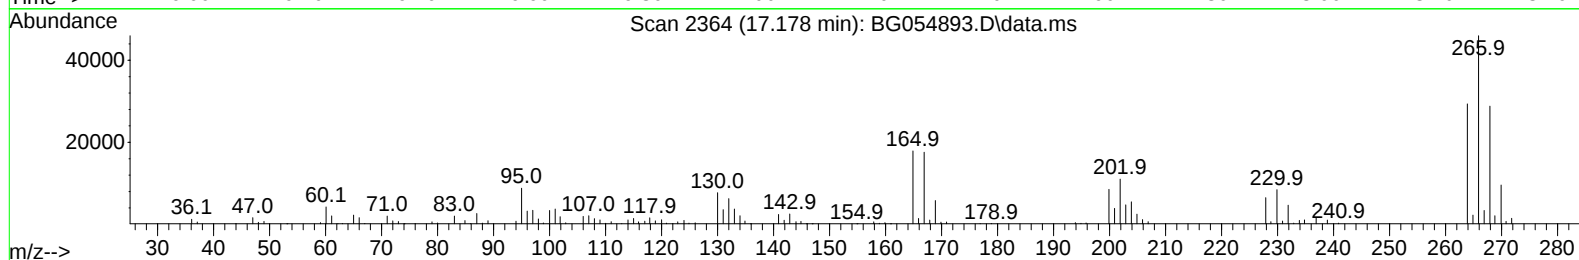


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090922\
Data File : BG054893.D
Acq On : 9 Sep 2022 11:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 04:41:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 01:53:42 2022
Response via : Initial Calibration

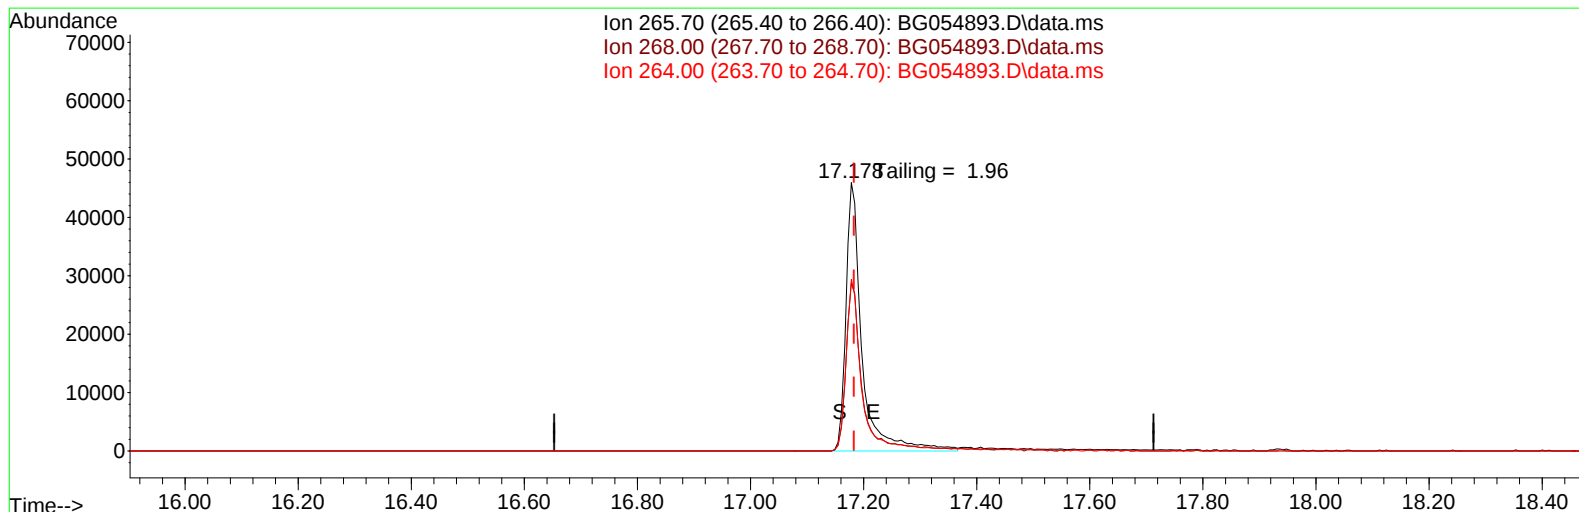

TIC: BG054893.D\data.ms

(70) Pentachlorophenol (C)




17.178min (-0.004) 25683.55 ng

response 91285

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.65
264.00	61.70	63.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090922\
Data File : BG054893.D
Acq On : 9 Sep 2022 11:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 04:41:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 01:53:42 2022
Response via : Initial Calibration

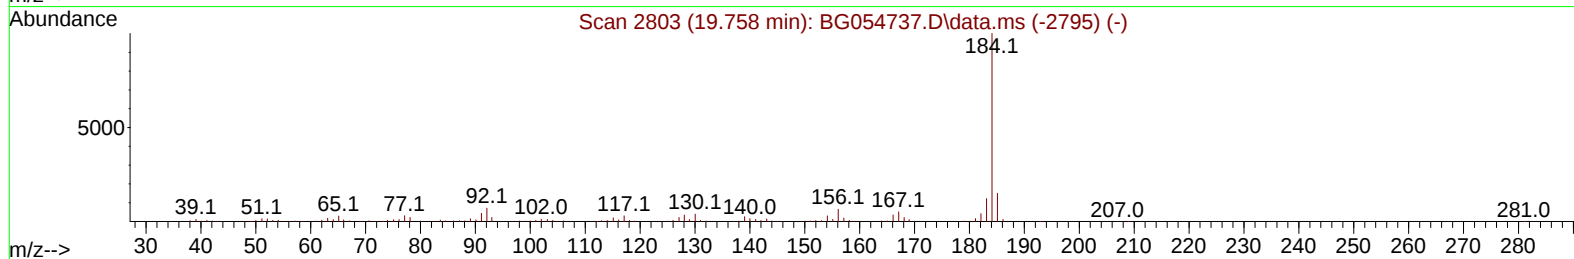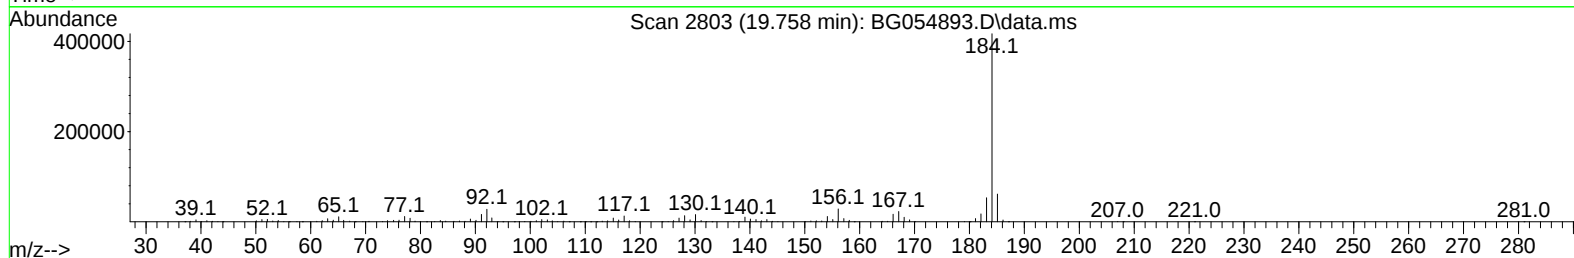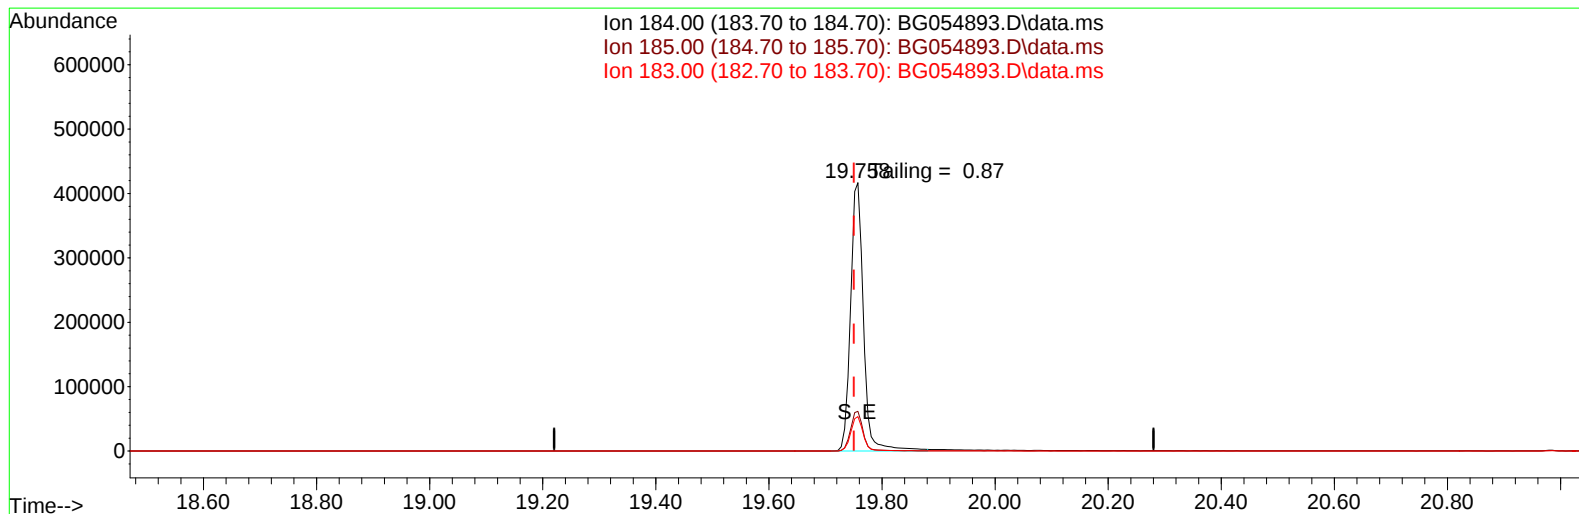

TIC: BG054893.D\data.ms

(77) Benzidine**19.758min (+ 0.007) 73694.95 ng****response 673548**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.80
183.00	12.30	12.81
0.00	0.00	0.00