

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090922\
 Data File : BG054907.D
 Acq On : 9 Sep 2022 21:57
 Operator : CG/JU
 Sample : N4538-07 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MBD-SB-1-2-0-5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054907.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.203	320	326	333	rVB2	6534	10296	1.60%	0.219%
2	5.685	402	408	419	rVB	110646	181979	28.28%	3.870%
3	7.300	676	683	694	rBV	114455	203226	31.59%	4.321%
4	8.140	820	826	837	rVB	150395	263521	40.96%	5.604%
5	9.316	1019	1026	1036	rBV	65108	123878	19.25%	2.634%
6	10.972	1300	1308	1320	rBV	210835	392372	60.99%	8.344%
7	13.399	1712	1721	1736	rBV	224250	341614	53.10%	7.264%
8	13.652	1758	1764	1769	rVB2	6736	10287	1.60%	0.219%
9	14.780	1949	1956	1965	rBV	346326	548252	85.21%	11.658%
10	16.266	2204	2209	2219	rBV	116401	191039	29.69%	4.062%
11	17.524	2416	2423	2430	rBV	390862	619154	96.23%	13.166%
12	19.321	2727	2729	2733	rVB4	12102	13695	2.13%	0.291%
13	19.457	2748	2752	2754	rBV5	7936	12023	1.87%	0.256%
14	19.574	2768	2772	2777	rBV	17147	31468	4.89%	0.669%
15	19.933	2831	2833	2841	rVB	18085	26671	4.15%	0.567%
16	20.121	2860	2865	2871	rBV	343165	452492	70.33%	9.622%
17	21.819	3148	3154	3161	rBV	375257	643383	100.00%	13.681%
18	25.197	3721	3729	3742	rVB3	199166	637330	99.06%	13.552%




Sum of corrected areas: 4702680

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090922\
Data File : BG054907.D
Acq On : 9 Sep 2022 21:57
Operator : CG/JU
Sample : N4538-07 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MBD-SB-1-2-0-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

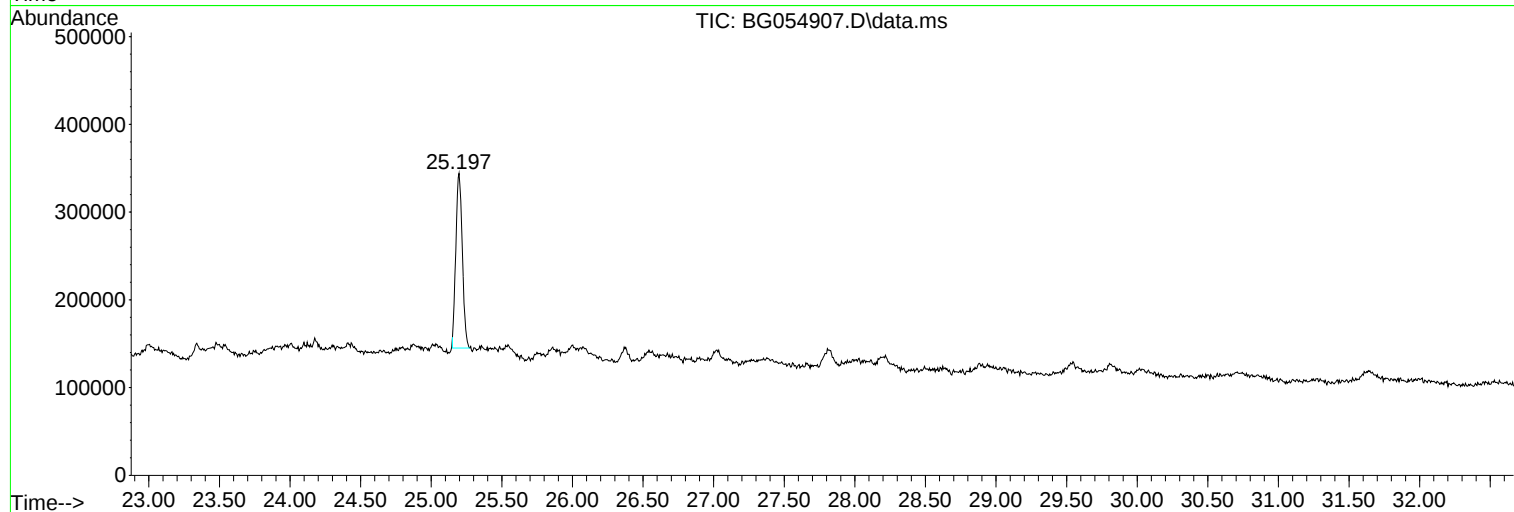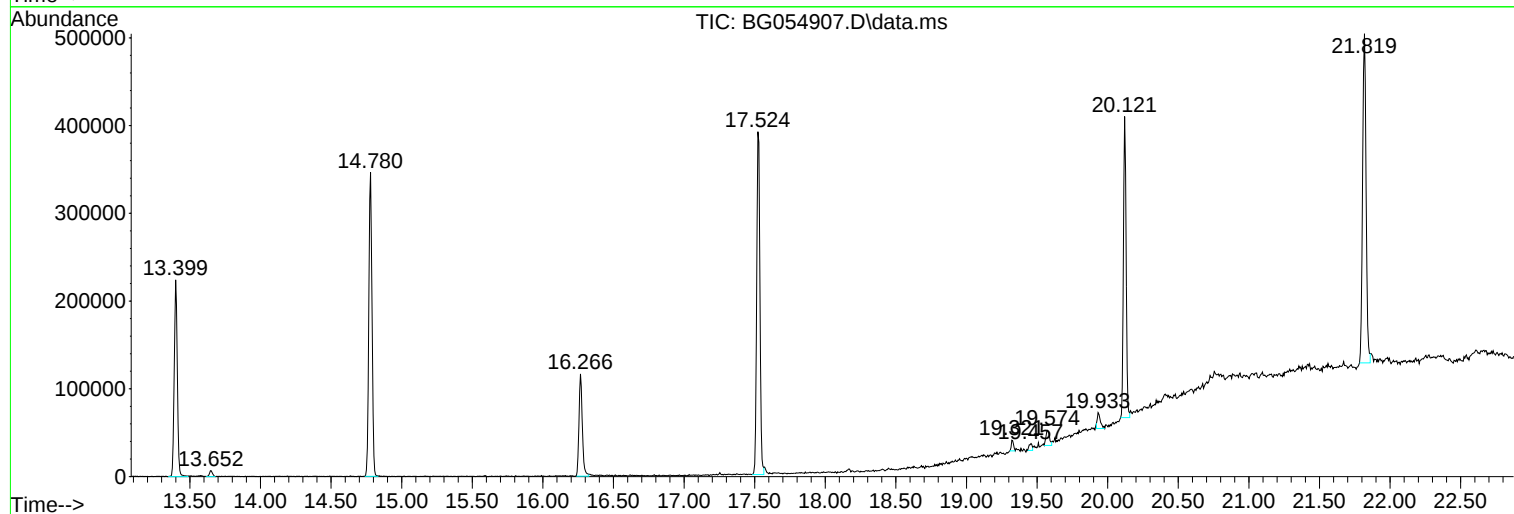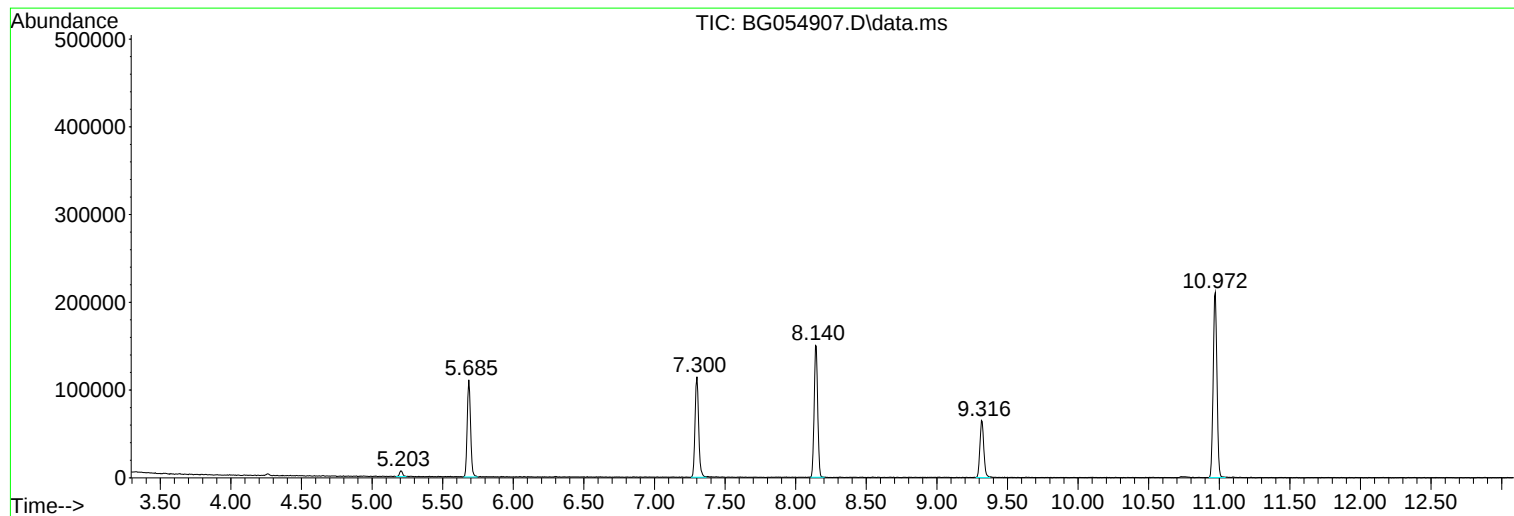

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090922\
Data File : BG054907.D
Acq On : 9 Sep 2022 21:57
Operator : CG/JU
Sample : N4538-07 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MBD-SB-1-2-0-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090922\
Data File : BG054907.D
Acq On : 9 Sep 2022 21:57
Operator : CG/JU
Sample : N4538-07 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MBD-SB-1-2-0-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------