


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090922\
 Data File : BG054893.D
 Acq On : 9 Sep 2022 11:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 10 01:53:42 2022

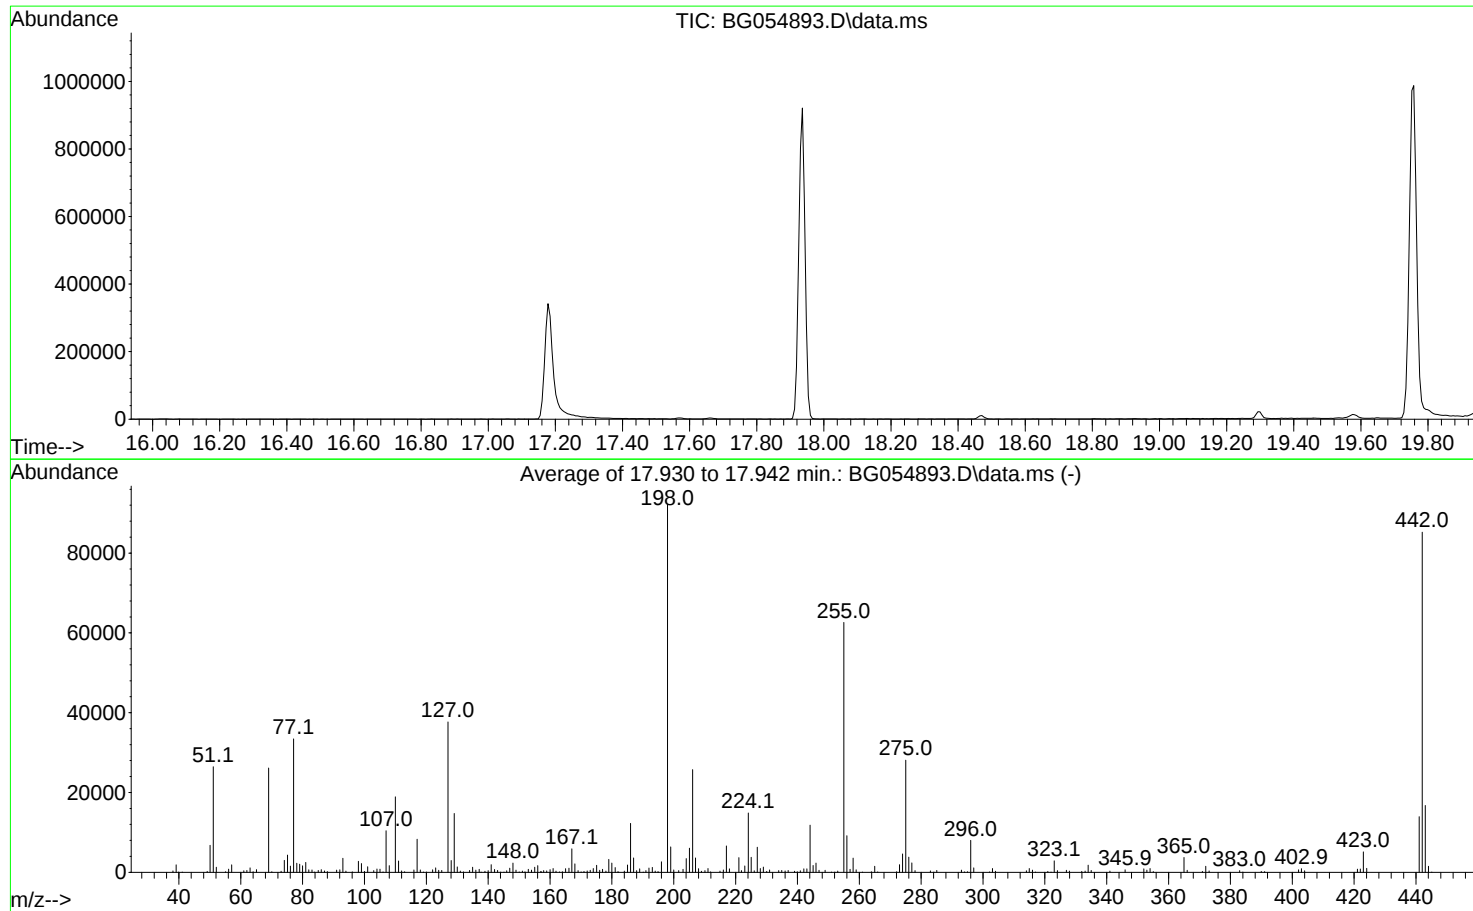




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	26448	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.3	26112	PASS
70	69	0.00	2	0.5	132	PASS
127	198	10	80	40.9	37680	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	92200	PASS
199	198	5	9	6.9	6378	PASS
275	198	10	60	30.5	28083	PASS
365	198	1	100	4.0	3698	PASS
441	198	0.01	100	15.1	13955	PASS
442	442	50	100	100.0	85237	PASS
443	442	15	24	19.6	16735	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090922\
Data File : BG054893.D
Acq On : 9 Sep 2022 11:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 10 04:41:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 01:53:42 2022
Response via : Initial Calibration

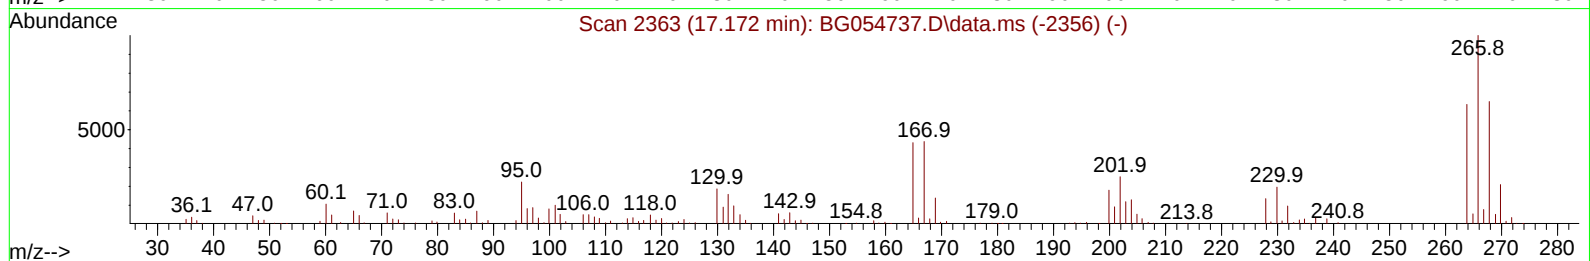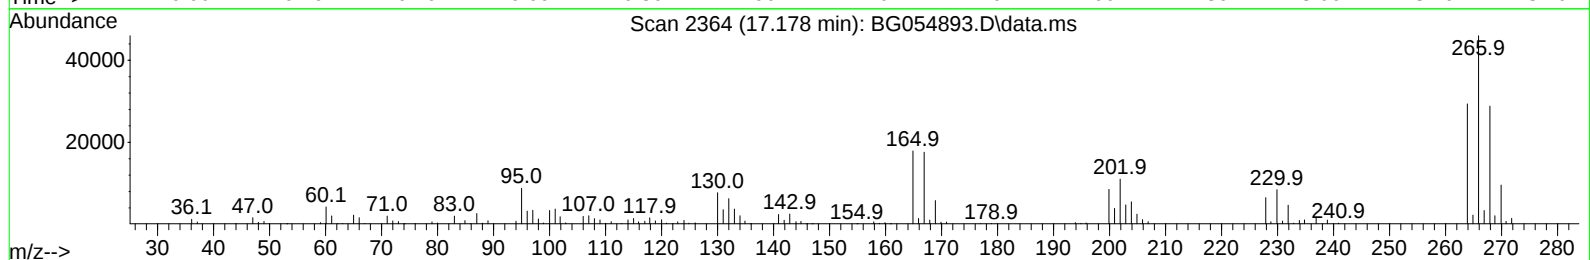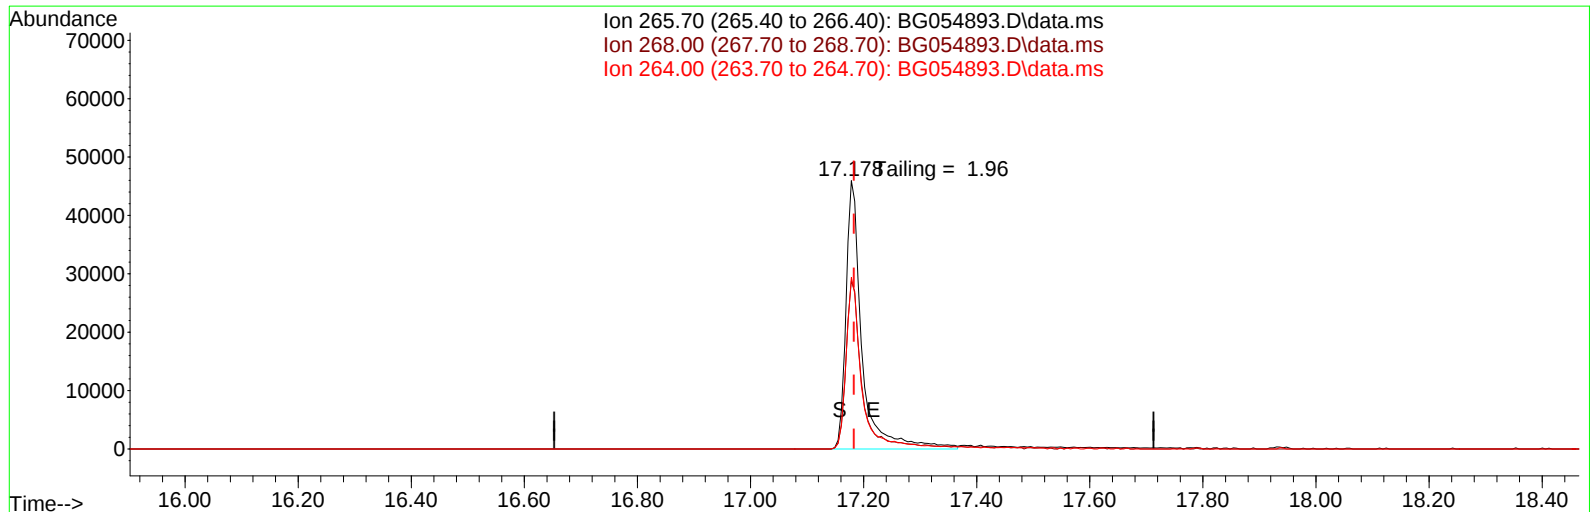

TIC: BG054893.D\data.ms

(70) Pentachlorophenol (C)

17.178min (-0.004) 25683.55 ng




response 91285

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.65
264.00	61.70	63.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090922\
Data File : BG054893.D
Acq On : 9 Sep 2022 11:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 10 04:41:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 01:53:42 2022
Response via : Initial Calibration

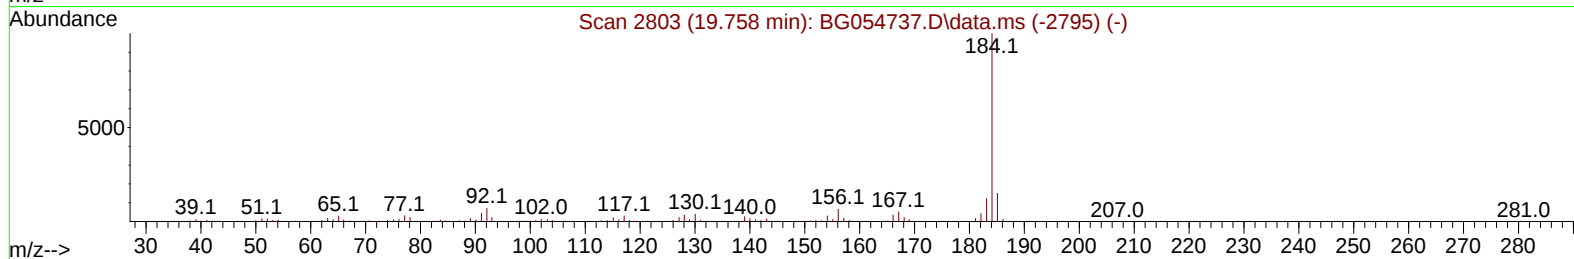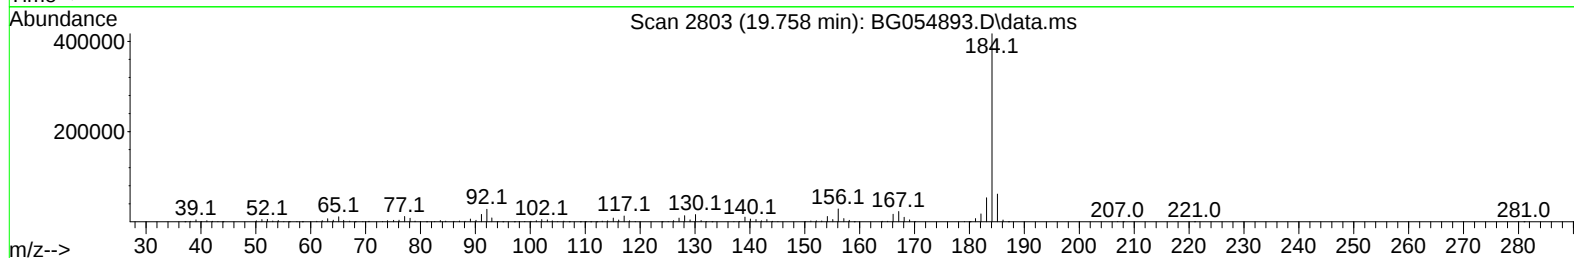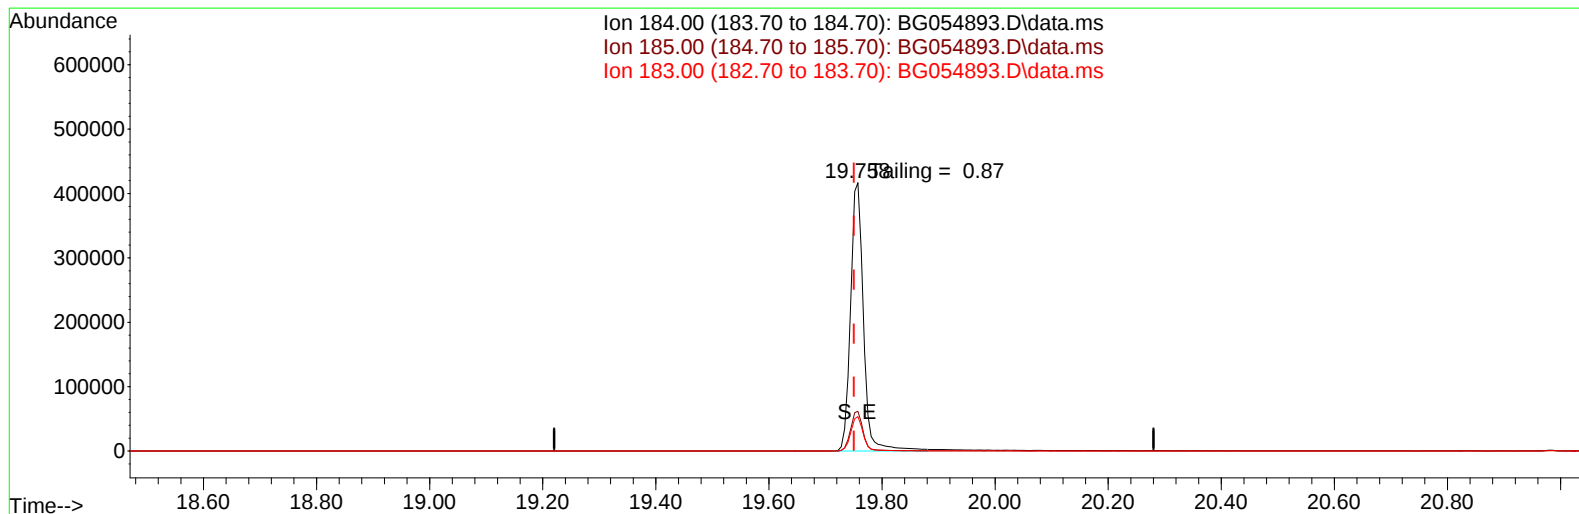

TIC: BG054893.D\data.ms

(77) Benzidine

19.758min (+ 0.007) 73694.95 ng

response 673548

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.80
183.00	12.30	12.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/9/2022	BNA_G	BG054893.D
Compound Name	Response	Retention Time
DDT	322215	20.985
DDD	10171	20.539
DDE	911	20.028
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11082	333297	3.32

Instrument :
BNA_G
ClientSampleId :
DFTPP