

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
 Data File : BG058980.D
 Acq On : 11 Sep 2023 12:43
 Operator : MA/JU
 Sample : 04195-14
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBY84

Quant Time: Sep 12 00:49:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 11 00:07:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.323	152	73702	20.000	ng/ul	0.00
20) Naphthalene-d8	11.172	136	353475	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.950	164	266798	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.700	188	688108	20.000	ng/ul	# 0.00
79) Chrysene-d12	22.018	240	677556	20.000	ng/ul	0.00
88) Perylene-d12	25.591	264	777014	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.640	96	2933	1.691	ng/uL	0.00
4) Pyridine-d5	4.057	84	124	0.023	ng/ul	-0.01
7) Phenol-d5	7.430	99	66620	8.964	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.641	67	38668	8.873	ng/ul	0.00
11) 2-Chlorophenol-d4	7.841	132	43203	9.064	ng/ul	0.00
15) 4-Methylphenol-d8	9.004	113	39837	6.938	ng/ul	0.00
21) Nitrobenzene-d5	9.521	128	22768	8.880	ng/ul	0.00
24) 2-Nitrophenol-d4	10.238	143	26343	9.364	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.761	165	50623	8.466	ng/ul	0.00
31) 4-Chloroaniline-d4	11.307	131	54916	6.830	ng/ul	0.00
46) Dimethylphthalate-d6	14.345	166	180151	8.705	ng/ul	0.00
49) Acenaphthylene-d8	14.651	160	195458	8.481	ng/ul	0.00
54) 4-Nitrophenol-d4	15.115	143	25864	7.524	ng/ul	0.00
60) Fluorene-d10	15.937	176	162364	8.840	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.037	200	22059	6.531	ng/ul	0.00
73) Anthracene-d10	17.794	188	267949	8.772	ng/ul	0.00
81) Pyrene-d10	20.068	212	350166	9.756	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.332	264	346153	9.088	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	9.163	105	21220	2.229	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
Data File : BG058980.D
Acq On : 11 Sep 2023 12:43
Operator : MA/JU
Sample : 04195-14
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YBY84

Quant Time: Sep 12 00:49:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 11 00:07:05 2023
Response via : Initial Calibration

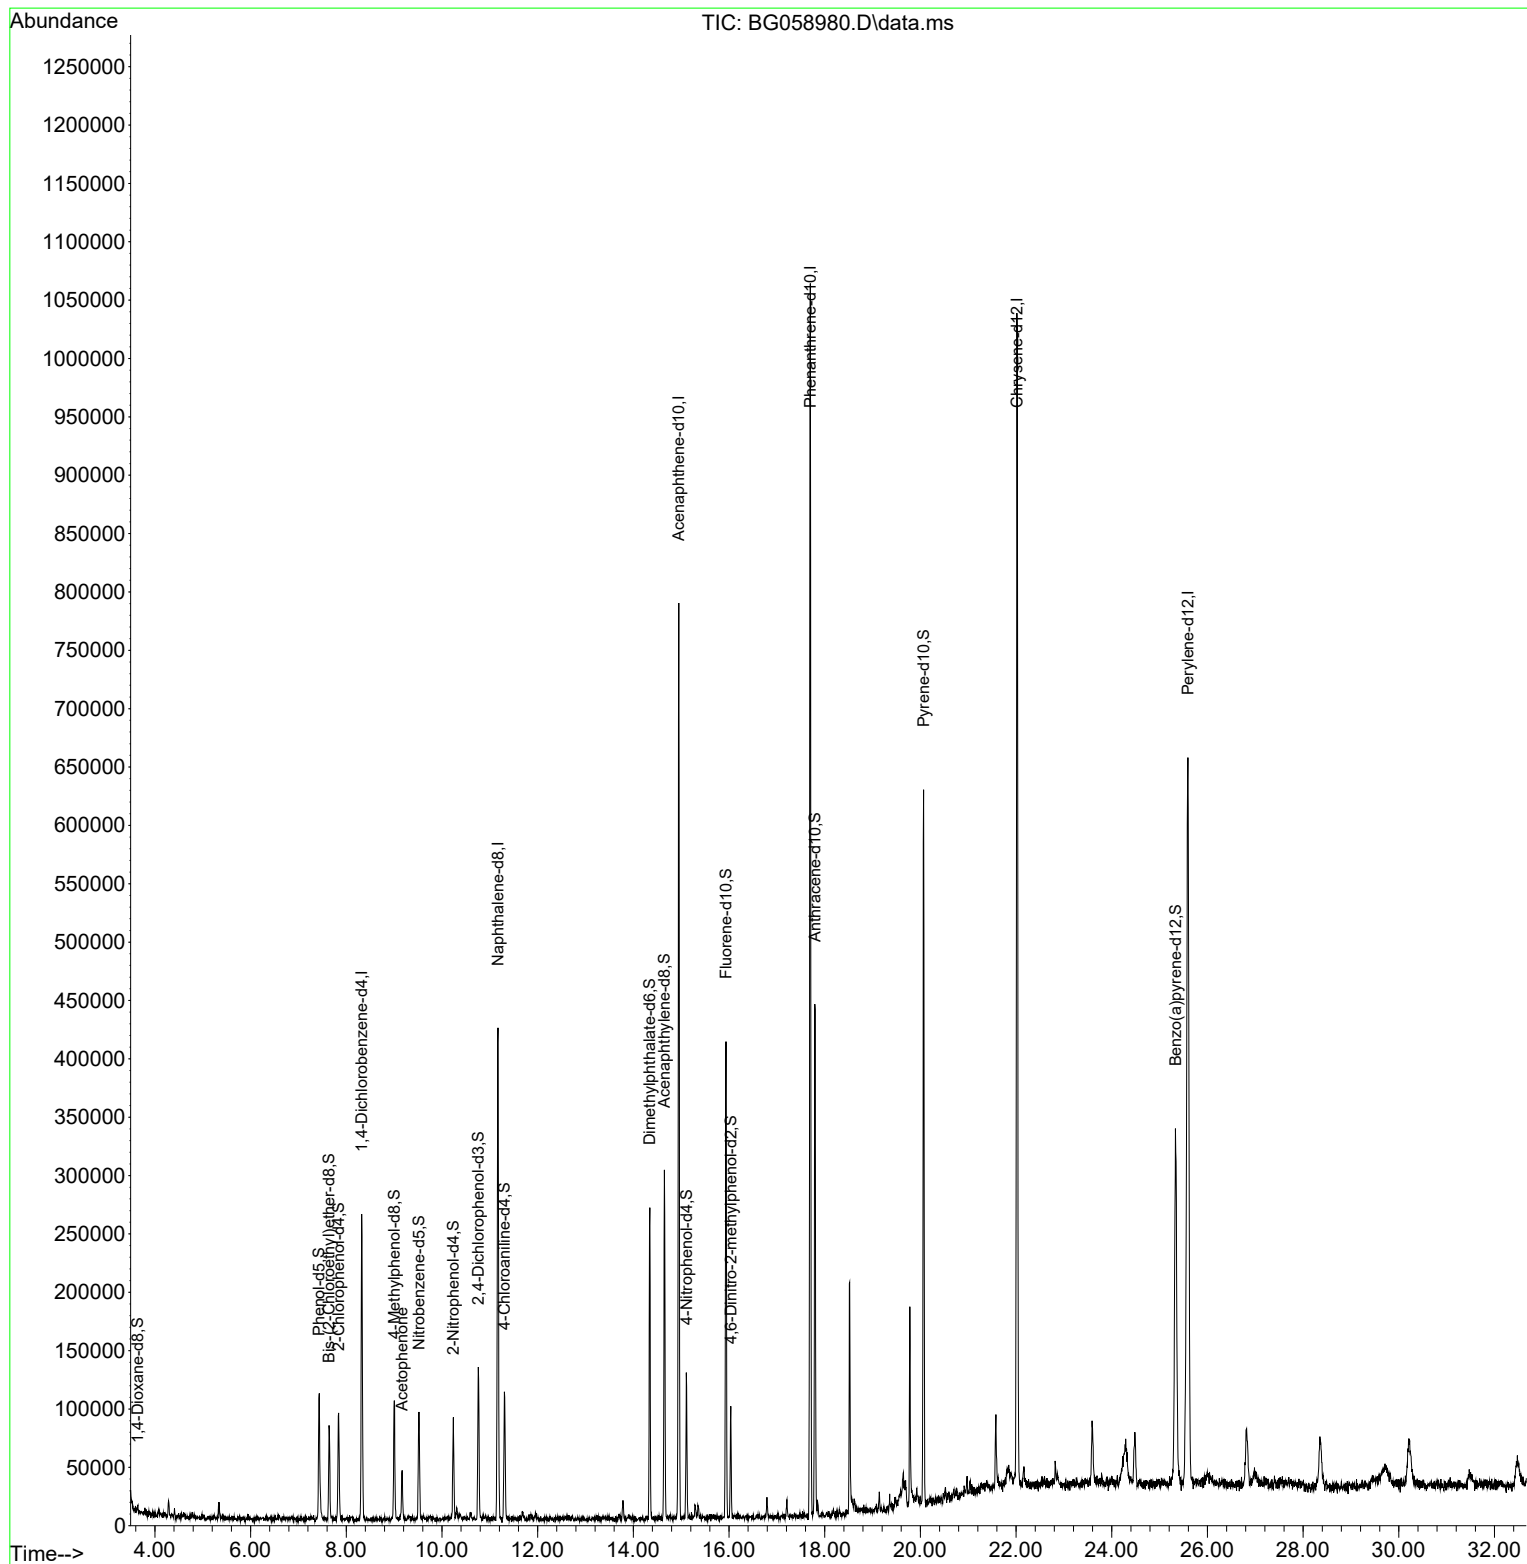

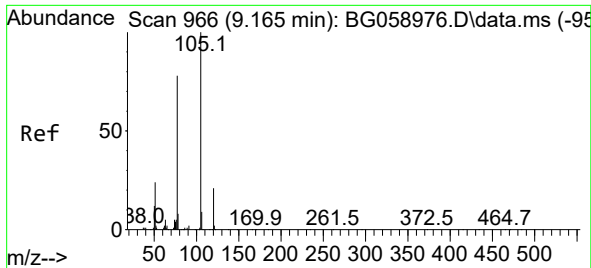

#16
 Acetophenone
 Concen: 2.229 ng/ul
 RT: 9.163 min Scan# 90
 Delta R.T. -0.007 min
 Lab File: BG058980.D
 Acq: 11 Sep 2023 12:43

Instrument :
 BNA_G
 ClientSampleId :
 YBY84

Tgt Ion:	105	Resp:	21220
Ion Ratio	Lower	Upper	
105	100		
77	80.0	67.3	100.9
51	31.3	19.3	28.9#

