

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
 Data File : BG058965.D
 Acq On : 11 Sep 2023 1:44
 Operator : MA/JU
 Sample : 04247-09
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBKB6

Quant Time: Sep 11 02:18:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 11 00:07:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.320	152	57487	20.000	ng/u1	0.00
20) Naphthalene-d8	11.170	136	283432	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.948	164	216253	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.697	188	563071	20.000	ng/u1	# 0.00
79) Chrysene-d12	22.022	240	574886	20.000	ng/u1	0.00
88) Perylene-d12	25.582	264	665811	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.643	96	6754	4.994	ng/uL	0.00
4) Pyridine-d5	4.072	84	40376	9.429	ng/u1	0.00
7) Phenol-d5	7.427	99	45887	7.916	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.644	67	119522	35.161	ng/u1	0.00
11) 2-Chlorophenol-d4	7.838	132	103258	27.773	ng/u1	0.00
15) 4-Methylphenol-d8	8.996	113	76628	17.109	ng/u1	0.00
21) Nitrobenzene-d5	9.519	128	69006	33.565	ng/u1	0.00
24) 2-Nitrophenol-d4	10.241	143	76539	33.929	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.759	165	135855	28.336	ng/u1	0.00
31) 4-Chloroaniline-d4	11.305	131	179157	27.788	ng/u1	0.00
46) Dimethylphthalate-d6	14.348	166	524394	31.261	ng/u1	0.00
49) Acenaphthylene-d8	14.654	160	557473	29.844	ng/u1	0.00
54) 4-Nitrophenol-d4	15.106	143	20958	7.522	ng/u1	0.00
60) Fluorene-d10	15.935	176	481058	32.315	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	16.041	200	84268	30.488	ng/u1	0.00
73) Anthracene-d10	17.797	188	852288	34.097	ng/u1	0.00
81) Pyrene-d10	20.065	212	1036927	34.050	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.336	264	1122707	34.399	ng/u1	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.392	107	12280	2.201	ng/u1#	Qvalue 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
Data File : BG058965.D
Acq On : 11 Sep 2023 1:44
Operator : MA/JU
Sample : 04247-09
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBKB6

Quant Time: Sep 11 02:18:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 11 00:07:05 2023
Response via : Initial Calibration

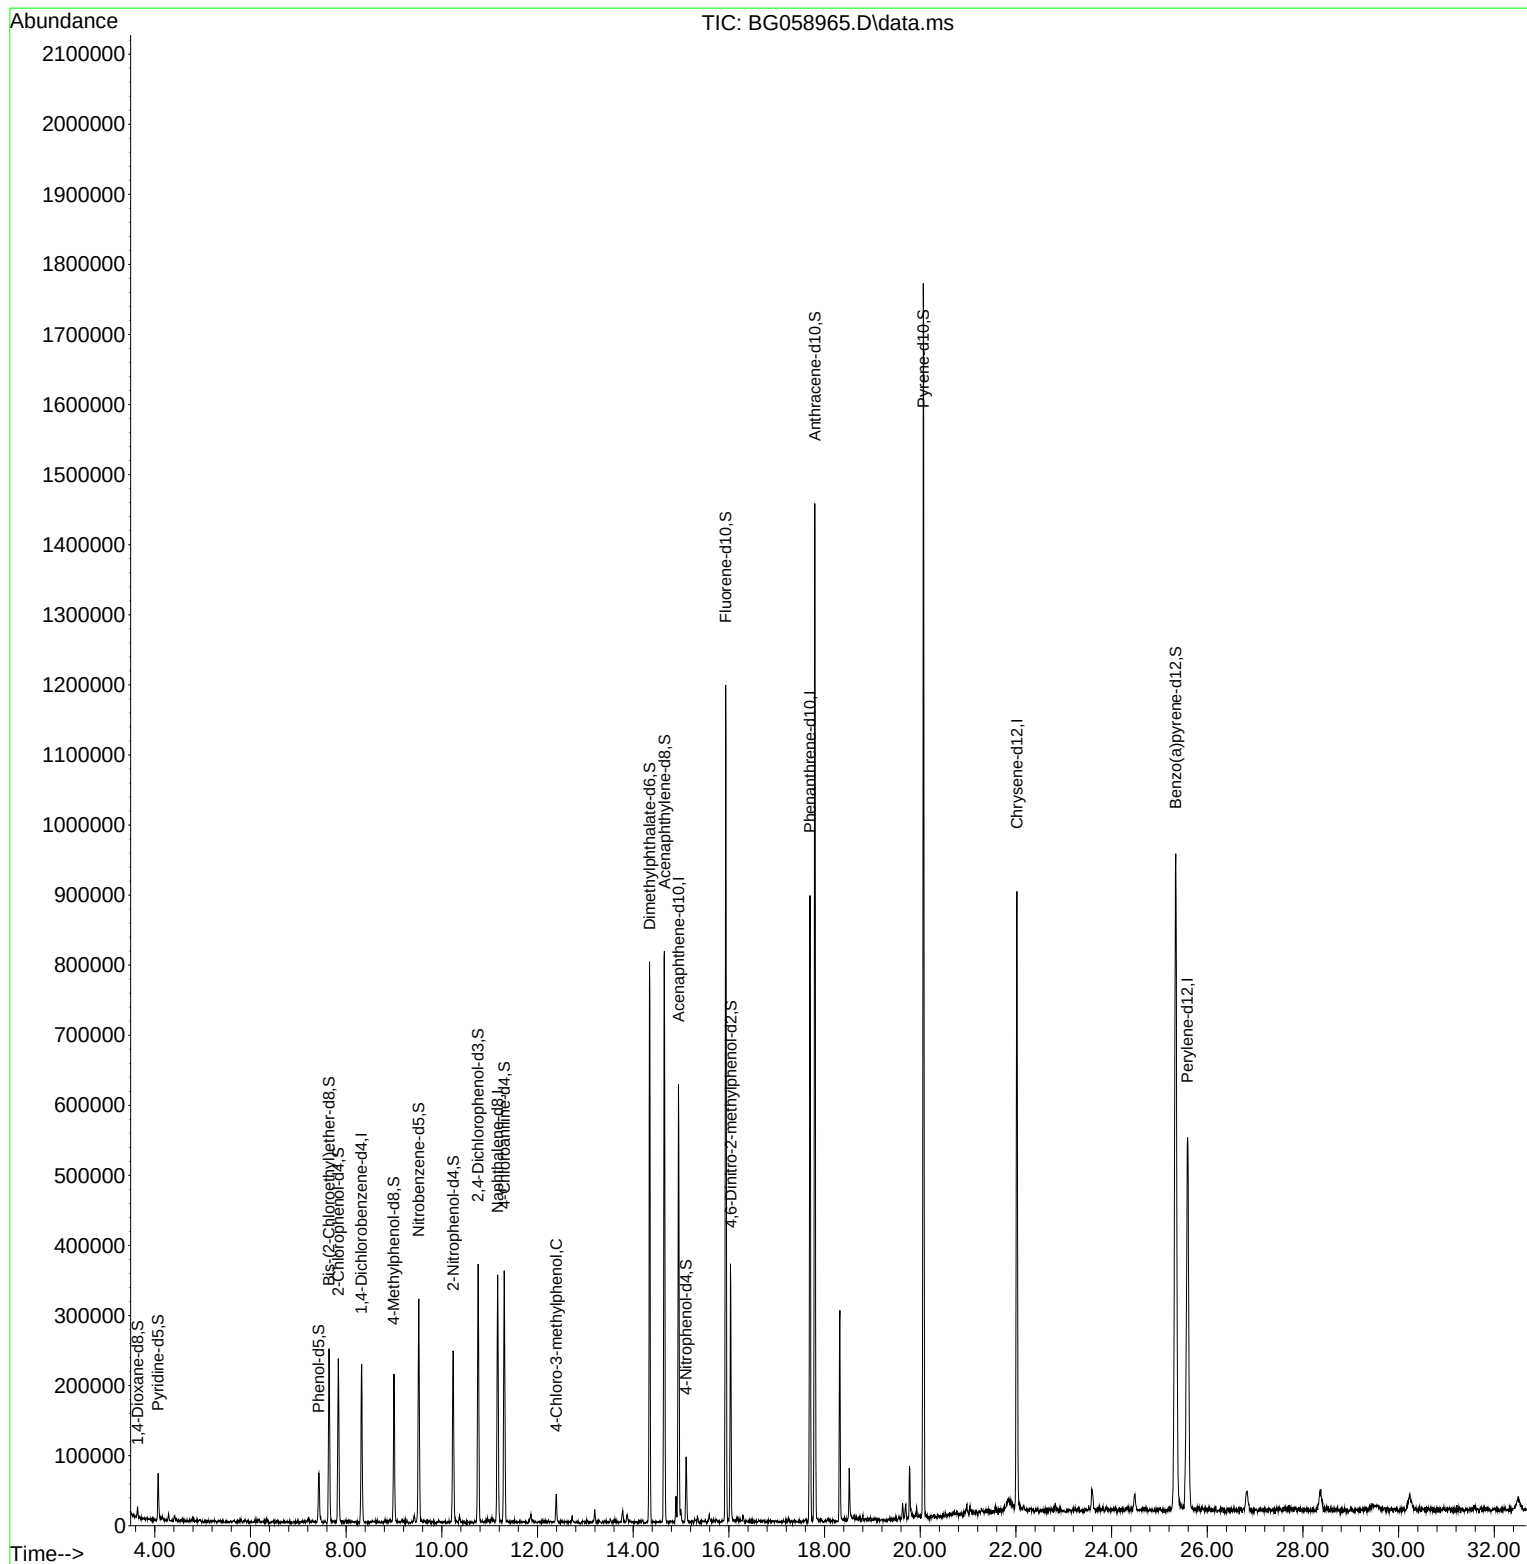

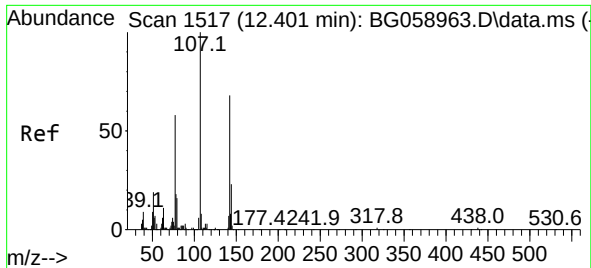

#35
4-Chloro-3-methylphenol
Concen: 2.201 ng/ul
RT: 12.392 min Scan# 11
Delta R.T. -0.010 min
Lab File: BG058965.D
Acq: 11 Sep 2023 1:44

Instrument :
BNA_G
ClientSampleId :
BBKB6

Tgt Ion:107 Resp: 12280
Ion Ratio Lower Upper
107 100
144 22.1 20.2 30.2
142 79.6 51.6 77.4#

