

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
 Data File : BG058977.D
 Acq On : 11 Sep 2023 10:40
 Operator : MA/JU
 Sample : PB155328BL
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK328

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058977.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.529	5	7	11	rBV4	7877	5769	0.24%	0.025%
2	3.640	22	26	32	rVV	18390	30859	1.26%	0.135%
3	3.681	32	33	38	rVB5	5953	6377	0.26%	0.028%
4	4.069	94	99	112	rBV	222179	360767	14.78%	1.575%
5	4.222	124	125	128	rVB3	4766	4219	0.17%	0.018%
6	4.251	128	130	134	rVV2	3405	3935	0.16%	0.017%
7	4.281	134	135	139	rVB3	5721	4703	0.19%	0.021%
8	4.404	152	156	159	rBV2	6963	9165	0.38%	0.040%
9	4.610	186	191	194	rBV3	4093	6916	0.28%	0.030%
10	4.680	201	203	206	rVB2	3756	4084	0.17%	0.018%
11	5.009	255	259	262	rBV3	5025	6201	0.25%	0.027%
12	5.708	374	378	379	rBV2	3733	3729	0.15%	0.016%
13	5.967	419	422	425	rBV2	4059	3858	0.16%	0.017%
14	6.930	585	586	590	rBV3	4675	5682	0.23%	0.025%
15	7.230	634	637	640	rBV2	3674	5421	0.22%	0.024%
16	7.324	650	653	655	rBV2	3376	3815	0.16%	0.017%
17	7.436	663	672	681	rBV	276706	490477	20.10%	2.141%
18	7.641	701	707	715	rBV	216828	375732	15.40%	1.640%
19	7.841	732	741	752	rVB	238163	448492	18.38%	1.958%
20	8.141	789	792	796	rBV2	4553	5010	0.21%	0.022%
21	8.323	817	823	832	rVB	202265	366996	15.04%	1.602%
22	8.775	893	900	901	rBV	3340	5058	0.21%	0.022%
23	8.822	905	908	912	rVB	3430	3980	0.16%	0.017%
24	8.916	921	924	927	rVB3	4770	5357	0.22%	0.023%
25	9.004	932	939	949	rVB	372640	634177	25.98%	2.768%
26	9.521	1019	1027	1034	rBV	269650	501528	20.55%	2.189%
27	9.662	1046	1051	1052	rBV	4292	5732	0.23%	0.025%
28	10.039	1112	1115	1122	rVB2	4011	6261	0.26%	0.027%
29	10.180	1135	1139	1141	rVB	5578	6609	0.27%	0.029%
30	10.238	1141	1149	1158	rBV2	229448	433402	17.76%	1.892%
31	10.761	1230	1238	1248	rVV	362218	663233	27.18%	2.895%
32	11.173	1297	1308	1316	rBV	333555	611825	25.07%	2.671%
33	11.308	1324	1331	1340	rBV	382871	669549	27.43%	2.923%
34	11.872	1421	1427	1428	rVB	4800	7642	0.31%	0.033%
35	11.889	1428	1430	1435	rBV	2689	3891	0.16%	0.017%
36	12.113	1464	1468	1470	rBV	3206	4547	0.19%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
 Data File : BG058977.D
 Acq On : 11 Sep 2023 10:40
 Operator : MA/JU
 Sample : PB155328BL
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK328

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

37	12.171	1475	1478	1482	rVV	2884	4301	0.18%	0.019%
38	12.265	1491	1494	1497	rBV	4680	4979	0.20%	0.022%
39	12.594	1548	1550	1553	rVB	4653	3918	0.16%	0.017%
40	12.730	1567	1573	1576	rBV3	8267	12477	0.51%	0.054%

41	12.959	1609	1612	1613	rVB3	4679	3979	0.16%	0.017%
42	13.111	1636	1638	1642	rBV	4247	6959	0.29%	0.030%
43	13.781	1749	1752	1758	rVB2	17842	26201	1.07%	0.114%
44	14.093	1803	1805	1808	rBV	2777	3738	0.15%	0.016%
45	14.292	1837	1839	1841	rBV	3892	4569	0.19%	0.020%

46	14.345	1841	1848	1854	rVB	758307	1092467	44.76%	4.769%
47	14.651	1891	1900	1912	rBV2	758210	1260105	51.63%	5.501%
48	14.739	1912	1915	1916	rVB2	4859	3960	0.16%	0.017%
49	14.950	1944	1951	1960	rVB2	569135	915903	37.53%	3.998%
50	15.039	1963	1966	1969	rVB2	3274	4701	0.19%	0.021%

51	15.115	1972	1979	1987	rBV	382171	622579	25.51%	2.718%
52	15.168	1987	1988	1991	rVV3	7465	4919	0.20%	0.021%
53	15.197	1991	1993	1998	rVB4	4472	5745	0.24%	0.025%
54	15.603	2060	2062	2066	rBV	5299	6558	0.27%	0.029%
55	15.938	2112	2119	2126	rBV	1114542	1629460	66.77%	7.113%

56	16.037	2130	2136	2142	rVV	317513	468914	19.21%	2.047%
57	16.173	2157	2159	2163	rVB3	7544	8733	0.36%	0.038%
58	16.419	2197	2201	2202	rBV2	4315	4449	0.18%	0.019%
59	16.584	2227	2229	2232	rVB	4806	4530	0.19%	0.020%
60	16.613	2232	2234	2236	rBV2	3945	3765	0.15%	0.016%

61	16.766	2257	2260	2263	rBV2	4561	4363	0.18%	0.019%
62	17.136	2321	2323	2326	rVB	4042	3787	0.16%	0.017%
63	17.236	2338	2340	2343	rVB3	6514	5734	0.23%	0.025%
64	17.359	2357	2361	2363	rBV	4163	6122	0.25%	0.027%
65	17.489	2381	2383	2389	rVB6	3943	5601	0.23%	0.024%

66	17.600	2397	2402	2403	rVB2	3652	4694	0.19%	0.020%
67	17.630	2405	2407	2409	rVV	6023	3793	0.16%	0.017%
68	17.700	2412	2419	2426	rVV	816656	1263366	51.76%	5.515%
69	17.800	2429	2436	2443	rBV	1207750	1905509	78.08%	8.318%
70	17.976	2462	2466	2469	rBV2	2172	4039	0.17%	0.018%

71	18.276	2515	2517	2519	rBV2	3466	3710	0.15%	0.016%
72	18.352	2528	2530	2536	rVB3	4946	5557	0.23%	0.024%
73	18.499	2552	2555	2557	rBV	3424	4525	0.19%	0.020%
74	18.805	2604	2607	2608	rBV2	5362	4528	0.19%	0.020%
75	19.069	2651	2652	2656	rBV3	5528	5512	0.23%	0.024%

76	19.357	2698	2701	2703	rBV3	3468	3848	0.16%	0.017%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
 Data File : BG058977.D
 Acq On : 11 Sep 2023 10:40
 Operator : MA/JU
 Sample : PB155328BL
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK328

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

77	19.469	2718	2720	2724	rVB3	3335	3895	0.16%	0.017%
78	19.633	2744	2748	2752	rVV4	21501	30472	1.25%	0.133%
79	19.698	2756	2759	2768	rVB2	19577	33276	1.36%	0.145%
80	19.997	2808	2810	2814	rBV5	2922	3925	0.16%	0.017%
81	20.068	2816	2822	2829	rVV	1550454	2229585	91.35%	9.733%
82	20.379	2873	2875	2877	rBV3	6055	4122	0.17%	0.018%
83	20.438	2881	2885	2886	rBV2	4794	5151	0.21%	0.022%
84	20.573	2906	2908	2911	rVB3	6245	5702	0.23%	0.025%
85	20.679	2924	2926	2929	rBV3	6039	7557	0.31%	0.033%
86	20.973	2974	2976	2978	rVB3	10201	5398	0.22%	0.024%
87	21.425	3052	3053	3055	rBV2	7131	3878	0.16%	0.017%
88	21.784	3113	3114	3117	rBV3	9069	6781	0.28%	0.030%
89	21.960	3142	3144	3145	rBV2	8611	4102	0.17%	0.018%
90	22.019	3147	3154	3163	rVV2	796354	1430080	58.60%	6.243%
91	22.818	3288	3290	3292	rBV3	11495	11948	0.49%	0.052%
92	23.587	3415	3421	3423	rBV5	20660	37813	1.55%	0.165%
93	25.338	3708	3719	3731	rBV	787064	2440587	100.00%	10.654%
94	25.591	3751	3762	3772	rVB2	484379	1528598	62.63%	6.673%
95	26.396	3897	3899	3902	rBV4	6674	6931	0.28%	0.030%
96	26.989	3998	4000	4002	rVB3	10326	8322	0.34%	0.036%
97	27.107	4018	4020	4025	rBV6	9366	10456	0.43%	0.046%
98	27.218	4036	4039	4042	rBV5	10792	16057	0.66%	0.070%
99	31.719	4803	4805	4806	rBV2	8175	5991	0.25%	0.026%
100	32.318	4906	4907	4910	rBV2	11047	8900	0.36%	0.039%




Sum of corrected areas: 22907122

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
Data File : BG058977.D
Acq On : 11 Sep 2023 10:40
Operator : MA/JU
Sample : PB155328BL
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK328

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

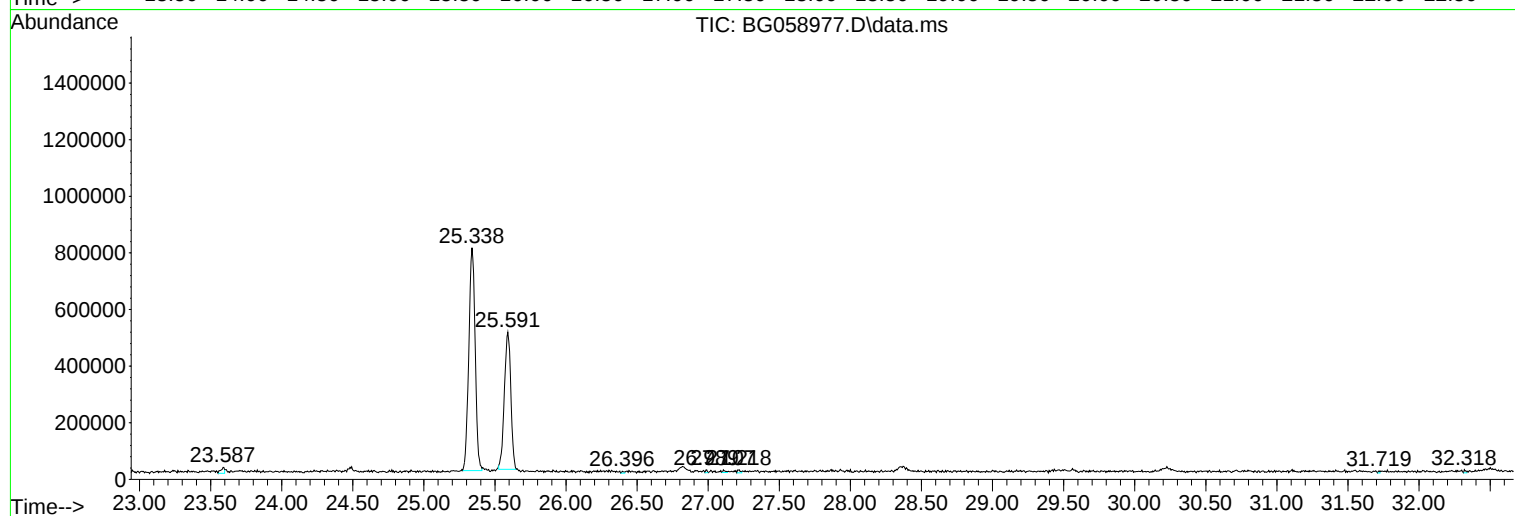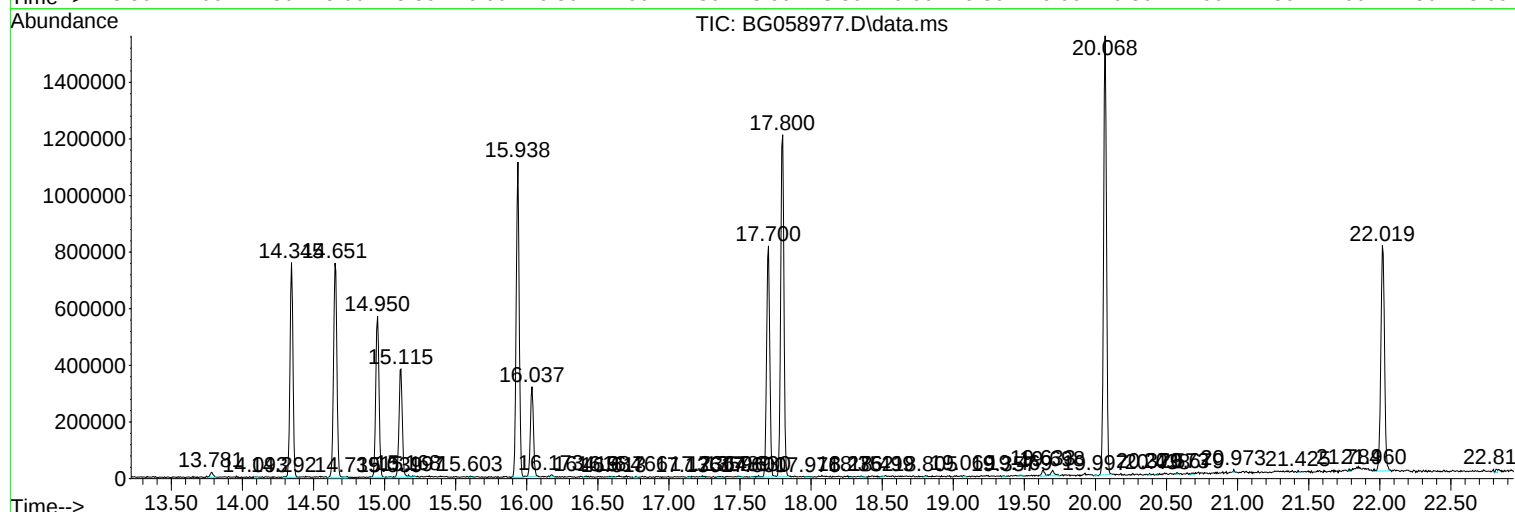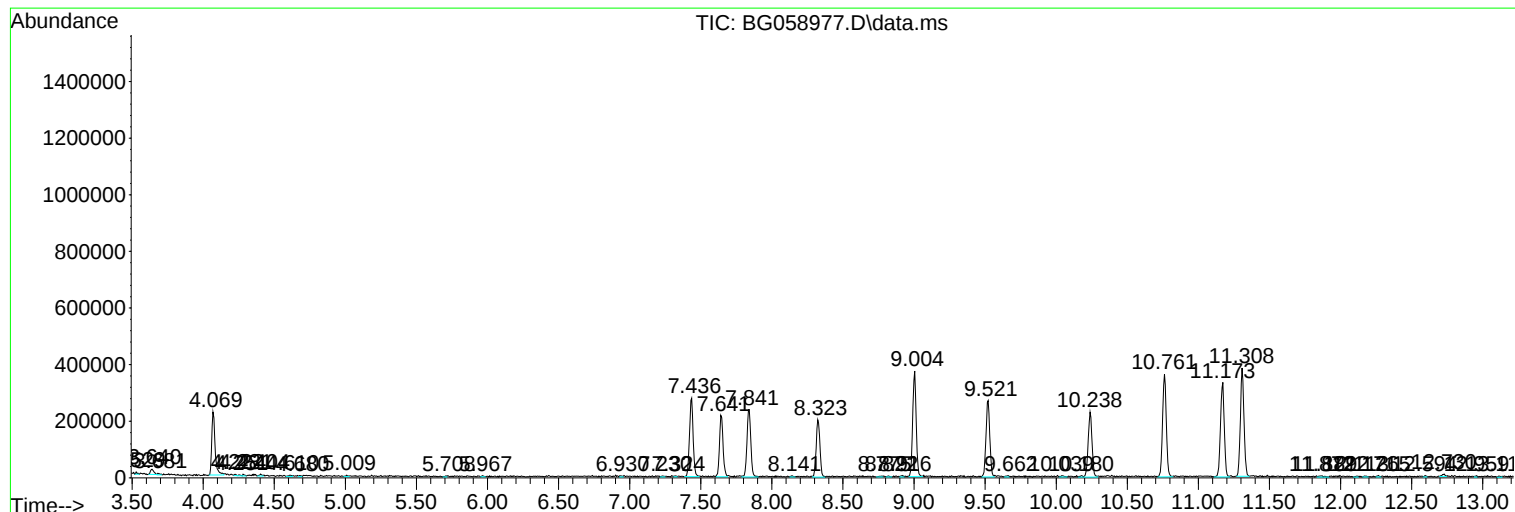

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
Data File : BG058977.D
Acq On : 11 Sep 2023 10:40
Operator : MA/JU
Sample : PB155328BL
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK328

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
Data File : BG058977.D
Acq On : 11 Sep 2023 10:40
Operator : MA/JU
Sample : PB155328BL
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK328

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc