

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
 Data File : BG058991.D
 Acq On : 11 Sep 2023 20:57
 Operator : MA/JU
 Sample : PB155374BL
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK374

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058991.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.578	13	15	21	rVB4	5953	8674	0.29%	0.031%
2	3.637	21	25	31	rBV3	23018	36414	1.24%	0.131%
3	4.066	93	98	111	rBV	272077	463120	15.74%	1.672%
4	4.412	154	157	161	rVB4	6200	8262	0.28%	0.030%
5	5.147	281	282	285	rBV2	4228	5354	0.18%	0.019%
6	5.346	313	316	317	rBV2	5298	5351	0.18%	0.019%
7	5.476	334	338	340	rBV2	3154	4325	0.15%	0.016%
8	6.216	460	464	469	rVB2	4004	6462	0.22%	0.023%
9	6.263	469	472	476	rBV2	3160	4595	0.16%	0.017%
10	6.504	510	513	515	rVB2	6907	6020	0.20%	0.022%
11	6.527	515	517	519	rBV3	5902	5255	0.18%	0.019%
12	7.432	664	671	681	rBV	356336	623043	21.17%	2.249%
13	7.550	688	691	692	rBV2	5413	5252	0.18%	0.019%
14	7.644	700	707	715	rVB	271007	470107	15.97%	1.697%
15	7.838	732	740	750	rBV	317359	585413	19.89%	2.113%
16	8.143	790	792	795	rVB	4061	5120	0.17%	0.018%
17	8.325	816	823	830	rBV	193836	341652	11.61%	1.233%
18	8.478	846	849	851	rVB	4132	4151	0.14%	0.015%
19	8.725	889	891	894	rVB	6049	4820	0.16%	0.017%
20	8.754	894	896	898	rBV	4757	4507	0.15%	0.016%
21	8.901	917	921	923	rVB2	5452	6304	0.21%	0.023%
22	9.001	931	938	946	rBV	470543	816538	27.74%	2.947%
23	9.336	994	995	998	rBV	6219	5553	0.19%	0.020%
24	9.518	1018	1026	1035	rBV	353369	626041	21.27%	2.260%
25	9.976	1103	1104	1108	rBV2	3684	5075	0.17%	0.018%
26	10.153	1130	1134	1138	rBV2	4121	6309	0.21%	0.023%
27	10.235	1141	1148	1160	rVB2	298067	541377	18.39%	1.954%
28	10.352	1165	1168	1170	rBV2	7481	5357	0.18%	0.019%
29	10.435	1178	1182	1187	rBV2	5460	9071	0.31%	0.033%
30	10.558	1201	1203	1205	rBV2	5434	4929	0.17%	0.018%
31	10.605	1209	1211	1214	rVB	5383	5015	0.17%	0.018%
32	10.758	1229	1237	1245	rBV	462529	865509	29.41%	3.124%
33	11.010	1277	1280	1282	rBV2	5328	5665	0.19%	0.020%
34	11.069	1288	1290	1293	rVB2	5284	5374	0.18%	0.019%
35	11.169	1299	1307	1315	rBV	343548	621422	21.11%	2.243%
36	11.251	1318	1321	1322	rBV	4296	4878	0.17%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
 Data File : BG058991.D
 Acq On : 11 Sep 2023 20:57
 Operator : MA/JU
 Sample : PB155374BL
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK374

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

37	11.304	1323	1330	1339	rVB	448981	831294	28.25%	3.001%
38	11.463	1353	1357	1358	rBV	3342	4232	0.14%	0.015%
39	11.504	1361	1364	1367	rBV	3019	4458	0.15%	0.016%
40	11.857	1419	1424	1427	rBV3	4249	5872	0.20%	0.021%
41	12.074	1459	1461	1464	rVB	5634	4367	0.15%	0.016%
42	12.274	1490	1495	1497	rBV3	4137	6949	0.24%	0.025%
43	12.303	1497	1500	1502	rBV2	3849	4408	0.15%	0.016%
44	12.450	1522	1525	1528	rVB	3331	4593	0.16%	0.017%
45	12.679	1562	1564	1567	rVB	5193	4213	0.14%	0.015%
46	12.720	1567	1571	1577	rBV2	13511	19738	0.67%	0.071%
47	12.808	1583	1586	1587	rVB	5354	5259	0.18%	0.019%
48	12.820	1587	1588	1590	rBV	5675	4657	0.16%	0.017%
49	12.949	1606	1610	1613	rBV2	5292	8017	0.27%	0.029%
50	13.020	1621	1622	1627	rVB	5888	8220	0.28%	0.030%
51	13.067	1627	1630	1631	rBV	6717	5269	0.18%	0.019%
52	13.625	1719	1725	1728	rBV	4571	6818	0.23%	0.025%
53	13.784	1747	1752	1757	rVB4	15529	20731	0.70%	0.075%
54	14.342	1840	1847	1855	rBV	966564	1420384	48.26%	5.127%
55	14.653	1893	1900	1906	rVB2	987379	1612272	54.78%	5.820%
56	14.947	1943	1950	1957	rVB	635611	1005050	34.15%	3.628%
57	15.035	1960	1965	1967	rBV2	3703	5511	0.19%	0.020%
58	15.112	1968	1978	1984	rBV	530069	793786	26.97%	2.865%
59	15.276	2003	2006	2008	rBV2	5164	5747	0.20%	0.021%
60	15.329	2013	2015	2019	rVB2	4664	5041	0.17%	0.018%
61	15.411	2026	2029	2032	rBV3	4204	4459	0.15%	0.016%
62	15.934	2112	2118	2124	rBV	1397423	2111850	71.76%	7.623%
63	16.034	2129	2135	2144	rVB	426065	626488	21.29%	2.261%
64	16.163	2154	2157	2162	rBV3	9527	15162	0.52%	0.055%
65	16.281	2176	2177	2180	rBV	4519	4523	0.15%	0.016%
66	16.716	2250	2251	2255	rBV2	5346	5641	0.19%	0.020%
67	17.021	2301	2303	2307	rBV2	4337	5170	0.18%	0.019%
68	17.186	2328	2331	2334	rBV2	3504	4704	0.16%	0.017%
69	17.591	2398	2400	2402	rVB	5092	4399	0.15%	0.016%
70	17.656	2407	2411	2412	rVV2	4757	4656	0.16%	0.017%
71	17.697	2412	2418	2424	rVV	893616	1403661	47.69%	5.067%
72	17.797	2428	2435	2443	rVB	1575390	2414943	82.05%	8.717%
73	18.173	2496	2499	2502	rVB4	4481	4954	0.17%	0.018%
74	18.249	2510	2512	2515	rVB3	7141	4718	0.16%	0.017%
75	18.402	2535	2538	2540	rBV3	5577	6151	0.21%	0.022%
76	18.825	2609	2610	2612	rBV2	5620	4167	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
 Data File : BG058991.D
 Acq On : 11 Sep 2023 20:57
 Operator : MA/JU
 Sample : PB155374BL
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK374

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

77	19.060	2646	2650	2654	rVB4	6077	8953	0.30%	0.032%
78	19.224	2676	2678	2680	rBV2	7251	4608	0.16%	0.017%
79	19.506	2724	2726	2728	rBV3	4362	4141	0.14%	0.015%
80	19.630	2742	2747	2751	rBV3	27222	40201	1.37%	0.145%
81	19.694	2755	2758	2764	rVB2	27600	39866	1.35%	0.144%
82	19.847	2782	2784	2786	rVB3	7400	4810	0.16%	0.017%
83	19.924	2795	2797	2800	rVB4	10692	6978	0.24%	0.025%
84	20.065	2814	2821	2829	rBV	1946766	2830339	96.17%	10.217%
85	20.358	2869	2871	2874	rVB3	5718	5448	0.19%	0.020%
86	20.388	2874	2876	2878	rBV3	6934	5557	0.19%	0.020%
87	20.705	2928	2930	2934	rVB4	9380	5834	0.20%	0.021%
88	20.916	2964	2966	2968	rBV	7089	4562	0.16%	0.016%
89	20.969	2972	2975	2981	rVB7	16391	25731	0.87%	0.093%
90	21.451	3055	3057	3058	rBV2	7581	5063	0.17%	0.018%
91	22.015	3147	3153	3164	rVB2	835184	1491288	50.67%	5.383%
92	23.155	3345	3347	3348	rBV2	11026	7284	0.25%	0.026%
93	23.584	3414	3420	3426	rBV10	25789	60958	2.07%	0.220%
94	25.335	3706	3718	3730	rVB2	934151	2943111	100.00%	10.624%
95	25.582	3748	3760	3771	rVB	515597	1611574	54.76%	5.817%
96	30.159	4537	4539	4540	rBV2	13235	7880	0.27%	0.028%
97	30.805	4648	4649	4651	rBV2	11233	7136	0.24%	0.026%
98	31.022	4684	4686	4687	rBV2	9454	5288	0.18%	0.019%
99	31.575	4778	4780	4782	rBV3	10540	10729	0.36%	0.039%
100	32.033	4856	4858	4861	rBV4	8266	11092	0.38%	0.040%




Sum of corrected areas: 27703277

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
Data File : BG058991.D
Acq On : 11 Sep 2023 20:57
Operator : MA/JU
Sample : PB155374BL
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK374

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

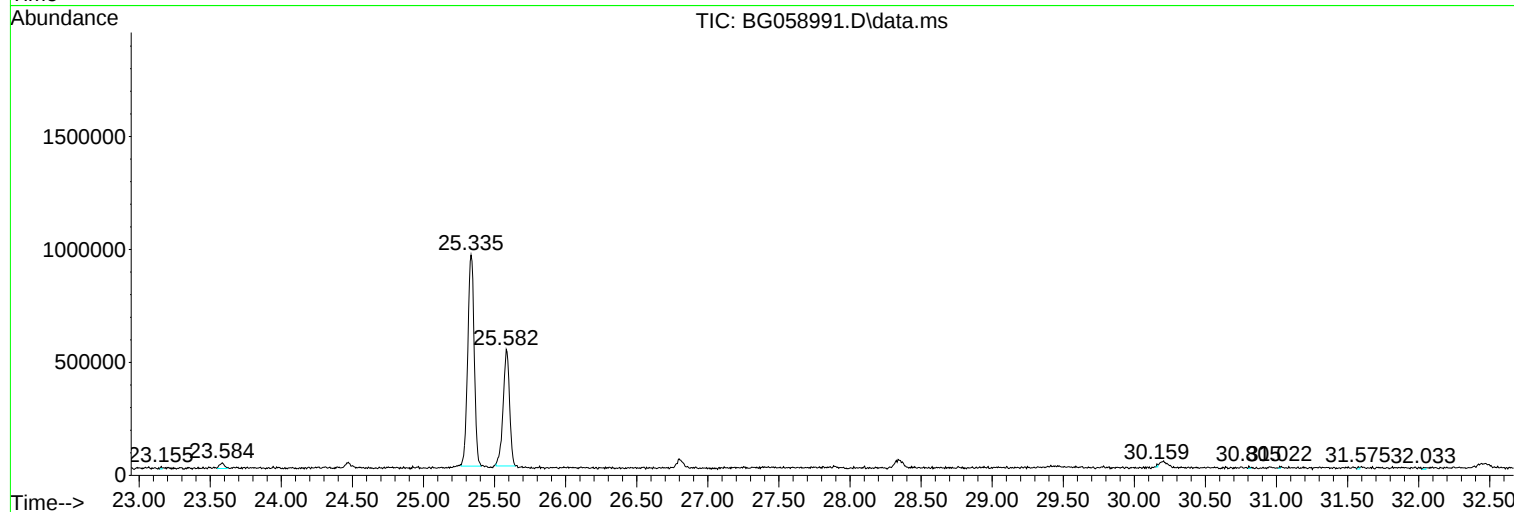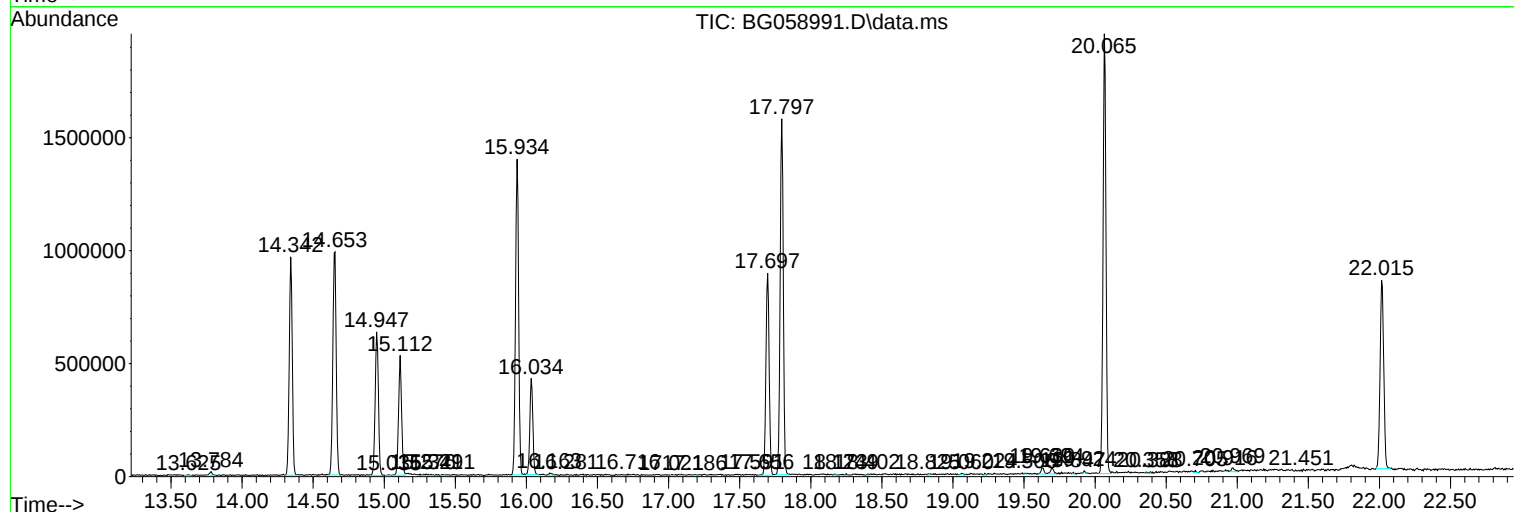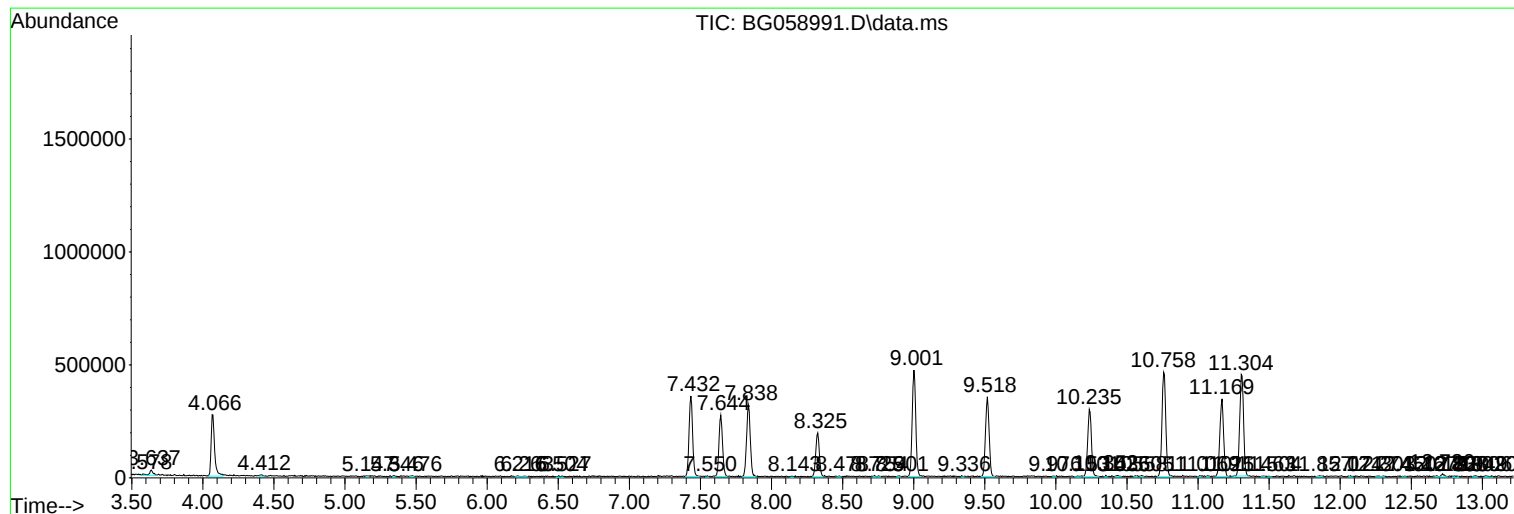

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
Data File : BG058991.D
Acq On : 11 Sep 2023 20:57
Operator : MA/JU
Sample : PB155374BL
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK374

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091023\
Data File : BG058991.D
Acq On : 11 Sep 2023 20:57
Operator : MA/JU
Sample : PB155374BL
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK374

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc