


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091218\
 Data File : BG036673.D
 Acq On : 12 Sep 2018 15:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 31 13:03:20 2018

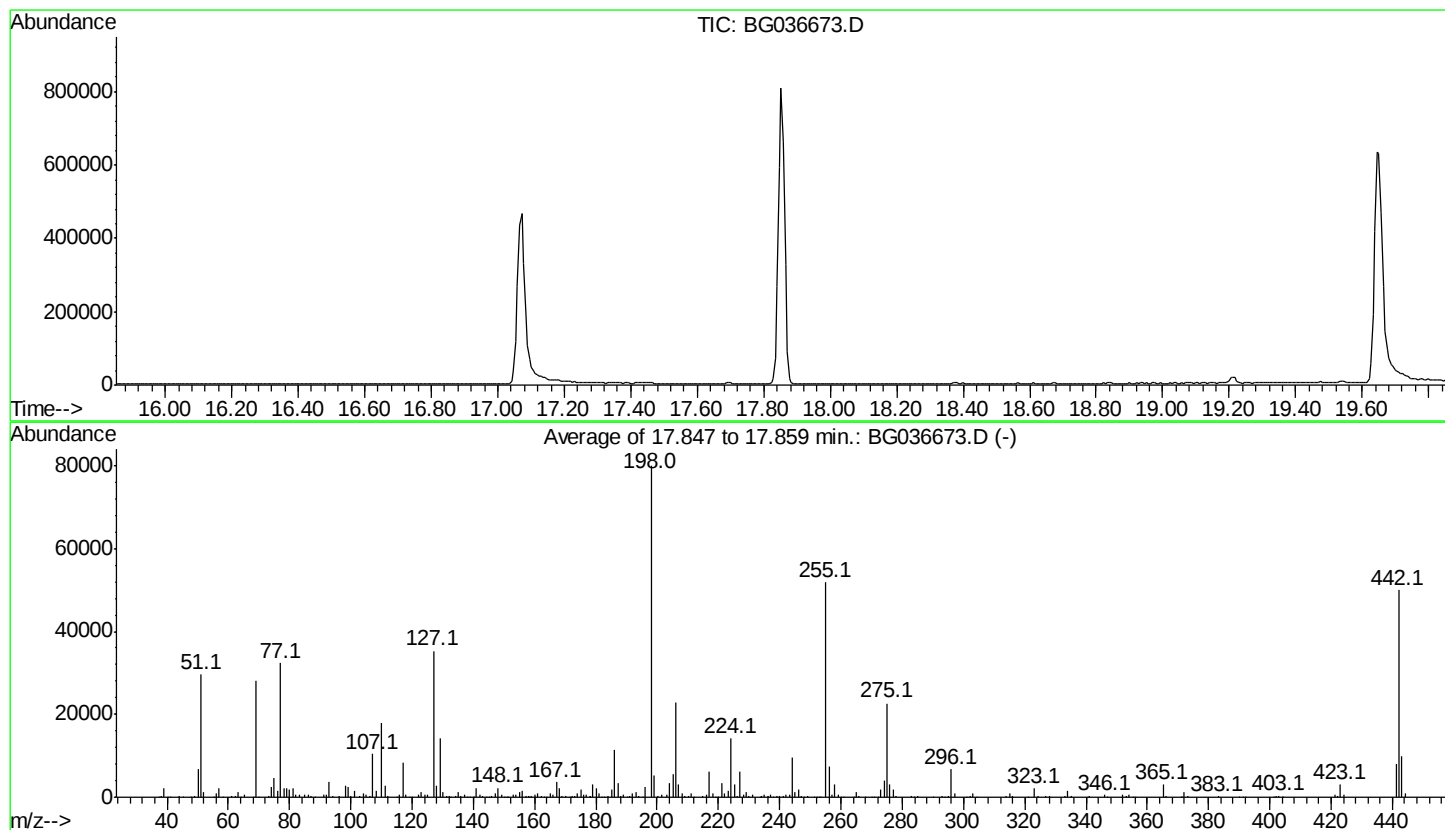

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	29544	PASS
68	69	0.00	2	0.5	137	PASS
69	198	0.00	100	35.0	28026	PASS
70	69	0.00	2	0.4	107	PASS
127	198	10	80	44.2	35352	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80000	PASS
199	198	5	9	6.8	5412	PASS
275	198	10	60	28.4	22690	PASS
365	198	1	100	3.8	3074	PASS
441	198	0.01	100	9.9	7937	PASS
442	198	50	100	62.4	49896	PASS
443	442	15	24	19.9	9917	PASS