


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091218\  
 Data File : BG036673.D  
 Acq On : 12 Sep 2018 15:11  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG082318.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Aug 31 13:03:20 2018

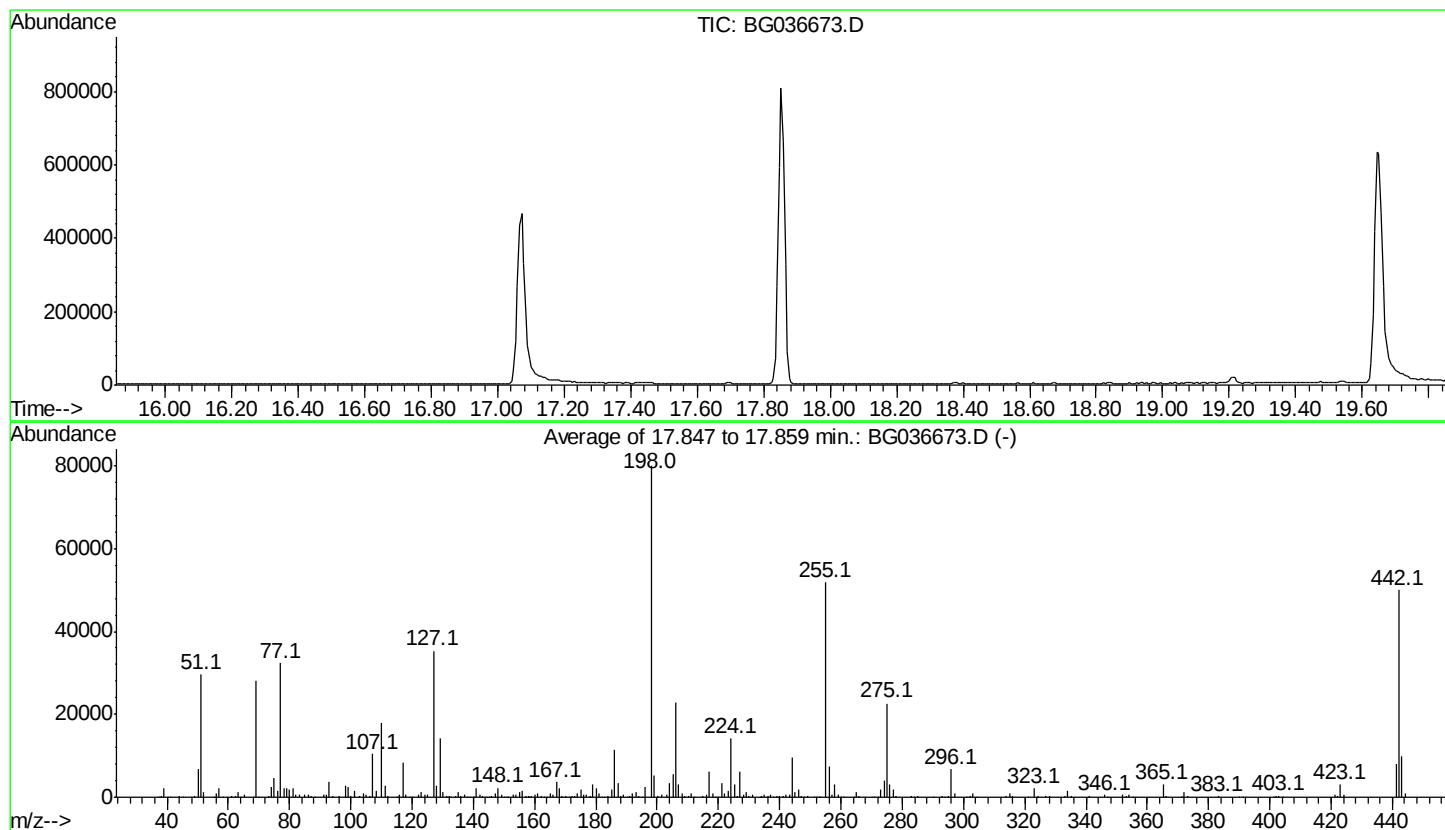

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 36.9      | 29544   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.5       | 137     | PASS             |
| 69          | 198          | 0.00         | 100          | 35.0      | 28026   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.4       | 107     | PASS             |
| 127         | 198          | 10           | 80           | 44.2      | 35352   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 80000   | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 5412    | PASS             |
| 275         | 198          | 10           | 60           | 28.4      | 22690   | PASS             |
| 365         | 198          | 1            | 100          | 3.8       | 3074    | PASS             |
| 441         | 198          | 0.01         | 100          | 9.9       | 7937    | PASS             |
| 442         | 198          | 50           | 100          | 62.4      | 49896   | PASS             |
| 443         | 442          | 15           | 24           | 19.9      | 9917    | PASS             |