

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091223\
 Data File : BG059013.D
 Acq On : 12 Sep 2023 16:34
 Operator : MA/JU
 Sample : 04358-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059013.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.069	98	99	103	rBV4	6031	7882	0.31%	0.096%
2	4.163	113	115	119	rBV5	6810	9563	0.38%	0.116%
3	4.486	167	170	173	rBV5	6321	7334	0.29%	0.089%
4	4.704	205	207	209	rVB3	6590	6434	0.26%	0.078%
5	4.898	239	240	243	rVB2	10242	6522	0.26%	0.079%
6	5.221	294	295	298	rBV3	9203	10086	0.40%	0.122%
7	5.297	306	308	314	rBV5	5158	9245	0.37%	0.112%
8	5.474	336	338	342	rBV4	7744	8804	0.35%	0.107%
9	5.820	395	397	399	rVB3	9107	7888	0.31%	0.096%
10	6.032	430	433	436	rBV3	8865	11937	0.48%	0.145%
11	6.096	442	444	449	rBV2	4979	6681	0.27%	0.081%
12	6.255	469	471	473	rBV	6096	6891	0.27%	0.084%
13	6.884	575	578	581	rBV4	5732	6650	0.26%	0.081%
14	6.960	590	591	594	rBV3	8668	6945	0.28%	0.084%
15	7.078	607	611	613	rBV4	6738	8704	0.35%	0.106%
16	7.254	640	641	644	rBV2	5718	6618	0.26%	0.080%
17	7.653	708	709	712	rBV3	6955	6540	0.26%	0.079%
18	7.882	745	748	749	rVB3	8746	6744	0.27%	0.082%
19	8.311	814	821	828	rVB	358759	602396	23.99%	7.311%
20	8.593	865	869	871	rBV2	7458	7497	0.30%	0.091%
21	9.069	947	950	951	rVB2	9216	7139	0.28%	0.087%
22	9.269	981	984	988	rBV5	6750	8119	0.32%	0.099%
23	10.056	1116	1118	1120	rVB2	9136	7766	0.31%	0.094%
24	10.192	1139	1141	1143	rBV4	6800	7025	0.28%	0.085%
25	10.579	1204	1207	1208	rBV3	8996	7080	0.28%	0.086%
26	10.697	1226	1227	1230	rBV3	8341	6628	0.26%	0.080%
27	10.908	1260	1263	1265	rBV3	7301	8884	0.35%	0.108%
28	11.155	1298	1305	1312	rVB	505471	922151	36.72%	11.192%
29	11.596	1377	1380	1383	rBV3	7007	8692	0.35%	0.105%
30	11.625	1383	1385	1387	rVB3	8262	6692	0.27%	0.081%
31	11.643	1387	1388	1391	rBV2	5688	7091	0.28%	0.086%
32	11.702	1394	1398	1400	rVB3	11198	11708	0.47%	0.142%
33	11.749	1402	1406	1407	rVB2	6468	6846	0.27%	0.083%
34	11.766	1407	1409	1414	rBV5	8238	9108	0.36%	0.111%
35	11.878	1426	1428	1430	rVB2	9546	6530	0.26%	0.079%
36	12.271	1491	1495	1497	rBV4	8512	9741	0.39%	0.118%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091223\
 Data File : BG059013.D
 Acq On : 12 Sep 2023 16:34
 Operator : MA/JU
 Sample : 04358-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

37	12.289	1497	1498	1501	rVB3	10331	6806	0.27%	0.083%
38	12.336	1501	1506	1509	rBV4	9901	17229	0.69%	0.209%
39	12.389	1513	1515	1518	rBV4	7650	6776	0.27%	0.082%
40	12.489	1528	1532	1534	rBV2	5587	9420	0.38%	0.114%
41	12.606	1550	1552	1555	rVB3	5788	7551	0.30%	0.092%
42	12.800	1582	1585	1587	rVB3	8265	8104	0.32%	0.098%
43	13.505	1703	1705	1708	rBV2	7565	10210	0.41%	0.124%
44	13.652	1727	1730	1732	rVB4	7119	7578	0.30%	0.092%
45	13.729	1741	1743	1745	rBV3	8984	12313	0.49%	0.149%
46	13.776	1747	1751	1754	rVB5	15343	25783	1.03%	0.313%
47	13.875	1765	1768	1769	rBV2	9231	7794	0.31%	0.095%
48	14.016	1789	1792	1793	rBV2	6698	7139	0.28%	0.087%
49	14.146	1811	1814	1817	rBV4	7390	9164	0.36%	0.111%
50	14.234	1828	1829	1840	rBV7	4083	9191	0.37%	0.112%
51	14.381	1852	1854	1857	rBV2	7454	8304	0.33%	0.101%
52	14.445	1862	1865	1867	rBV3	12389	12536	0.50%	0.152%
53	14.651	1897	1900	1903	rBV4	7283	9151	0.36%	0.111%
54	14.939	1942	1949	1955	rBV	936570	1451485	57.79%	17.616%
55	15.456	2035	2037	2038	rBV2	9832	7318	0.29%	0.089%
56	15.738	2084	2085	2090	rBV4	8726	13654	0.54%	0.166%
57	16.314	2180	2183	2184	rBV2	7688	9063	0.36%	0.110%
58	16.472	2207	2210	2213	rBV4	7081	9878	0.39%	0.120%
59	17.107	2314	2318	2319	rBV4	5684	7440	0.30%	0.090%
60	17.377	2363	2364	2369	rBV4	8136	8779	0.35%	0.107%
61	17.430	2371	2373	2374	rBV2	9239	7233	0.29%	0.088%
62	17.689	2410	2417	2425	rVB	1451127	2245728	89.42%	27.255%
63	22.007	3147	3152	3159	rVB	1512025	2511437	100.00%	30.480%




Sum of corrected areas: 8239625

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091223\
Data File : BG059013.D
Acq On : 12 Sep 2023 16:34
Operator : MA/JU
Sample : 04358-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

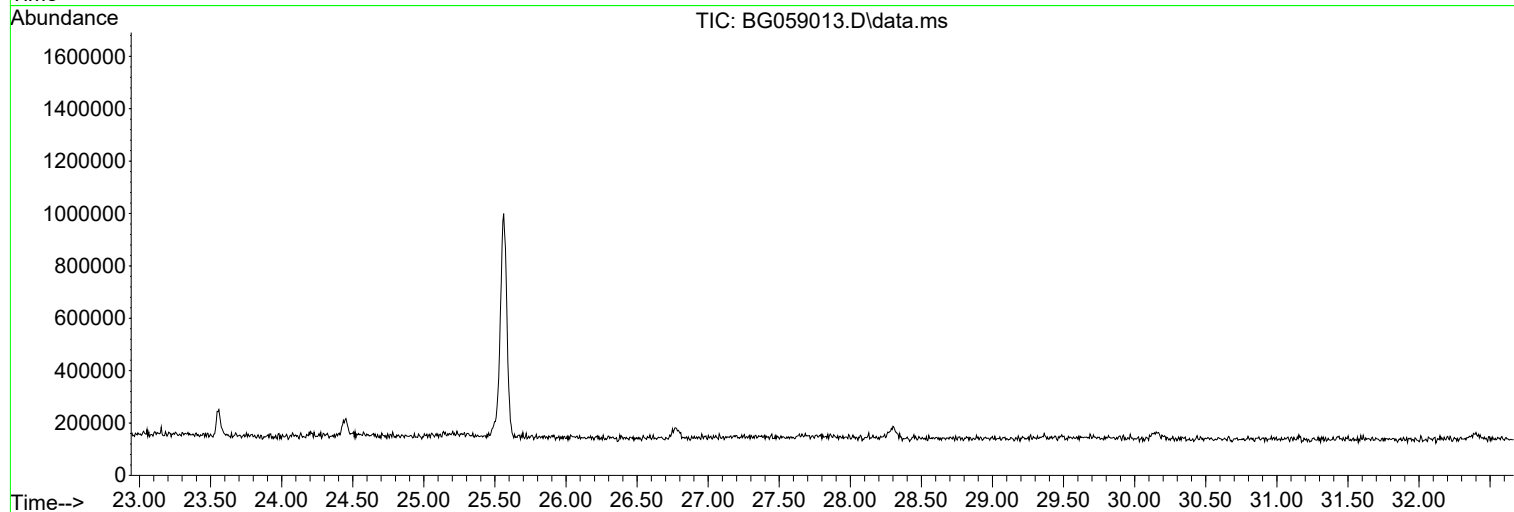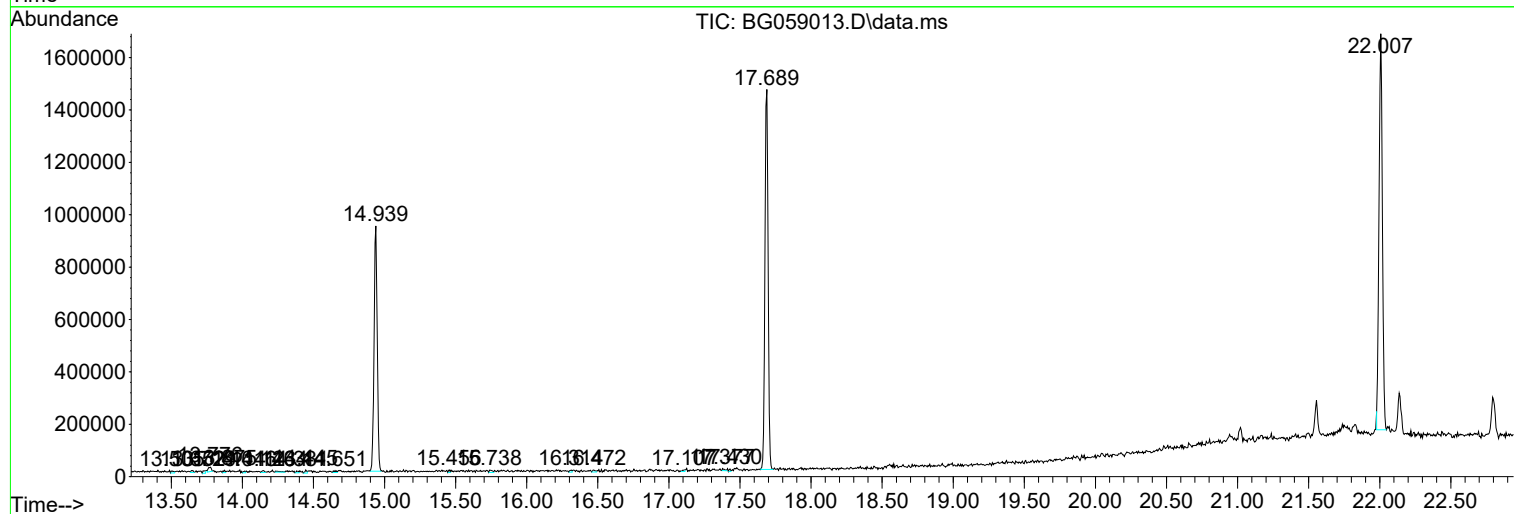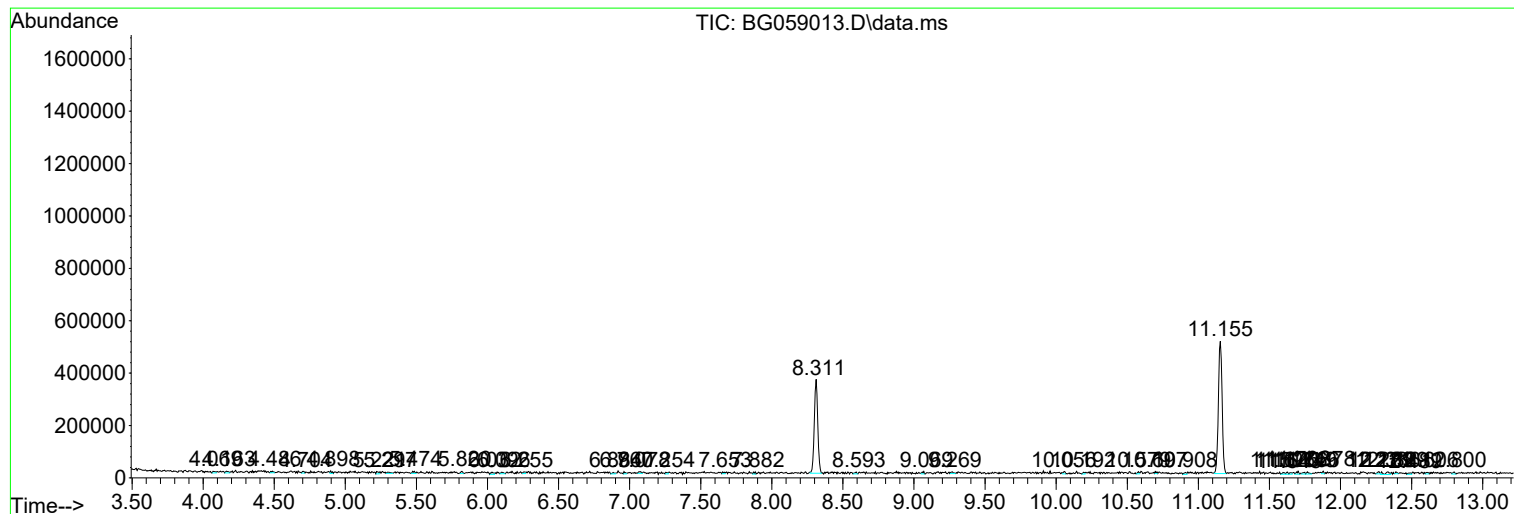

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091223\
Data File : BG059013.D
Acq On : 12 Sep 2023 16:34
Operator : MA/JU
Sample : 04358-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091223\
Data File : BG059013.D
Acq On : 12 Sep 2023 16:34
Operator : MA/JU
Sample : 04358-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc