

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091223\
 Data File : BG059025.D
 Acq On : 13 Sep 2023 1:31
 Operator : MA/JU
 Sample : PB155220BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059025.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.628	20	24	31	rBV6	28293	55616	1.78%	0.162%
2	4.057	93	97	106	rBV	377258	618795	19.84%	1.807%
3	4.439	159	162	164	rBV4	8658	9613	0.31%	0.028%
4	4.563	181	183	186	rVB3	9805	11377	0.36%	0.033%
5	4.598	186	189	192	rBV2	6636	9185	0.29%	0.027%
6	4.892	238	239	242	rBV3	8824	8182	0.26%	0.024%
7	4.974	250	253	254	rBV3	9697	8063	0.26%	0.024%
8	5.150	281	283	284	rBV	11977	8051	0.26%	0.024%
9	5.655	367	369	370	rBV2	10210	7530	0.24%	0.022%
10	5.685	372	374	377	rVB2	9698	8880	0.28%	0.026%
11	5.708	377	378	380	rBV	6985	6280	0.20%	0.018%
12	6.167	454	456	459	rBV3	6441	7692	0.25%	0.022%
13	6.261	468	472	474	rBV3	7634	9594	0.31%	0.028%
14	6.290	474	477	482	rVB4	8171	9821	0.31%	0.029%
15	6.631	533	535	539	rVB4	8100	7584	0.24%	0.022%
16	6.684	541	544	546	rVB2	9034	8401	0.27%	0.025%
17	6.830	566	569	572	rBV4	9249	12692	0.41%	0.037%
18	6.895	577	580	582	rBV4	5713	7185	0.23%	0.021%
19	7.418	662	669	679	rVB	501029	858267	27.52%	2.506%
20	7.559	691	693	695	rVB2	11800	8792	0.28%	0.026%
21	7.630	695	705	712	rBV	379329	656255	21.04%	1.916%
22	7.823	730	738	748	rBV	471605	809687	25.96%	2.364%
23	8.011	769	770	773	rBV2	6928	6581	0.21%	0.019%
24	8.311	814	821	829	rVB	308370	540262	17.32%	1.578%
25	8.417	835	839	841	rBV4	7507	9592	0.31%	0.028%
26	8.546	859	861	864	rVB3	7421	7869	0.25%	0.023%
27	8.587	864	868	870	rVB2	8678	10158	0.33%	0.030%
28	8.605	870	871	874	rBV3	9188	8863	0.28%	0.026%
29	8.646	876	878	880	rBV2	6990	6285	0.20%	0.018%
30	8.752	893	896	899	rVB3	6795	7806	0.25%	0.023%
31	8.799	902	904	907	rVB2	7050	7059	0.23%	0.021%
32	8.834	907	910	914	rBV3	8006	11117	0.36%	0.032%
33	8.905	919	922	924	rBV3	7416	8616	0.28%	0.025%
34	8.987	929	936	945	rBV	659632	1119573	35.90%	3.269%
35	9.093	951	954	957	rBV3	7258	8213	0.26%	0.024%
36	9.210	973	974	979	rVB3	8148	7478	0.24%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091223\
 Data File : BG059025.D
 Acq On : 13 Sep 2023 1:31
 Operator : MA/JU
 Sample : PB155220BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

37	9.310	988	991	994	rVB2	8418	9145	0.29%	0.027%
38	9.504	1016	1024	1035	rVB	469434	865286	27.75%	2.527%
39	9.692	1053	1056	1058	rBV3	5128	6907	0.22%	0.020%
40	10.127	1129	1130	1133	rBV3	8341	8093	0.26%	0.024%
41	10.226	1140	1147	1156	rVB	398854	725285	23.26%	2.118%
42	10.332	1161	1165	1166	rBV3	11352	8720	0.28%	0.025%
43	10.479	1189	1190	1192	rBV2	8035	7106	0.23%	0.021%
44	10.597	1208	1210	1213	rVB	7809	6904	0.22%	0.020%
45	10.749	1228	1236	1243	rBV	617617	1135774	36.42%	3.317%
46	11.155	1298	1305	1312	rVV	488050	868744	27.86%	2.537%
47	11.296	1320	1329	1337	rBV	646367	1206531	38.69%	3.523%
48	11.484	1358	1361	1363	rBV4	5271	6332	0.20%	0.018%
49	11.566	1372	1375	1377	rBV3	5199	8075	0.26%	0.024%
50	11.766	1407	1409	1412	rVB3	10883	8388	0.27%	0.024%
51	11.813	1415	1417	1420	rBV3	8257	9579	0.31%	0.028%
52	12.189	1478	1481	1482	rBV3	7930	7106	0.23%	0.021%
53	12.389	1513	1515	1518	rVB4	5733	6371	0.20%	0.019%
54	12.483	1528	1531	1533	rBV3	7069	9602	0.31%	0.028%
55	12.565	1544	1545	1548	rBV	5828	6873	0.22%	0.020%
56	12.782	1580	1582	1586	rBV3	10600	14094	0.45%	0.041%
57	12.959	1610	1612	1618	rVB2	4903	7546	0.24%	0.022%
58	13.199	1650	1653	1655	rVB2	6601	7223	0.23%	0.021%
59	13.270	1661	1665	1666	rBV3	6804	7664	0.25%	0.022%
60	13.399	1684	1687	1688	rBV3	6533	7624	0.24%	0.022%
61	13.446	1694	1695	1699	rVB4	7023	8017	0.26%	0.023%
62	13.476	1699	1700	1702	rBV	8663	6578	0.21%	0.019%
63	13.523	1707	1708	1712	rVB3	7468	7285	0.23%	0.021%
64	13.769	1745	1750	1754	rVV4	27895	47955	1.54%	0.140%
65	13.840	1760	1762	1765	rVB4	6279	6308	0.20%	0.018%
66	14.234	1827	1829	1830	rVB	10498	6487	0.21%	0.019%
67	14.245	1830	1831	1833	rBV2	10103	8334	0.27%	0.024%
68	14.333	1839	1846	1853	rBV	1355719	1976429	63.37%	5.771%
69	14.386	1853	1855	1860	rVB4	9680	10488	0.34%	0.031%
70	14.445	1863	1865	1866	rBV2	7632	6665	0.21%	0.019%
71	14.639	1890	1898	1906	rBV	1398623	2242217	71.90%	6.548%
72	14.792	1922	1924	1926	rBV2	5746	7272	0.23%	0.021%
73	14.868	1933	1937	1939	rBV4	7669	10061	0.32%	0.029%
74	14.939	1942	1949	1955	rVB	874536	1357555	43.53%	3.964%
75	15.103	1970	1977	1984	rBV	735502	1148537	36.83%	3.354%
76	15.373	2022	2023	2026	rVB3	11825	8225	0.26%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091223\
 Data File : BG059025.D
 Acq On : 13 Sep 2023 1:31
 Operator : MA/JU
 Sample : PB155220BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

77	15.526	2046	2049	2050	rBV2	7332	8300	0.27%	0.024%
78	15.561	2053	2055	2057	rVB2	7542	7360	0.24%	0.021%
79	15.591	2057	2060	2061	rBV	5811	6430	0.21%	0.019%
80	15.638	2065	2068	2071	rBV2	6664	6495	0.21%	0.019%
81	15.773	2088	2091	2093	rBV3	9725	10652	0.34%	0.031%
82	15.926	2109	2117	2123	rBV	1917959	2982077	95.62%	8.708%
83	16.026	2128	2134	2143	rVV	638773	945056	30.30%	2.760%
84	16.190	2159	2162	2165	rVB4	8969	8824	0.28%	0.026%
85	16.272	2174	2176	2178	rBV3	8673	7162	0.23%	0.021%
86	16.701	2248	2249	2252	rVB2	7334	6668	0.21%	0.019%
87	17.265	2341	2345	2349	rBV4	5156	8896	0.29%	0.026%
88	17.688	2410	2417	2424	rBV	877212	1414527	45.36%	4.131%
89	17.782	2427	2433	2442	rVV2	1623857	2582033	82.79%	7.540%
90	18.070	2478	2482	2484	rBV3	4616	6236	0.20%	0.018%
91	18.423	2538	2542	2544	rBV3	5429	9187	0.29%	0.027%
92	18.458	2547	2548	2554	rVB4	5505	6187	0.20%	0.018%
93	18.846	2610	2614	2615	rBV4	5960	6881	0.22%	0.020%
94	18.963	2633	2634	2639	rVB5	8464	6510	0.21%	0.019%
95	19.621	2742	2746	2749	rVB5	31789	36463	1.17%	0.106%
96	19.686	2753	2757	2763	rVV2	24007	38287	1.23%	0.112%
97	20.056	2814	2820	2828	rBV	2171012	3055946	97.99%	8.924%
98	22.007	3145	3152	3159	rVB	914701	1599742	51.30%	4.671%
99	25.309	3704	3714	3727	rVB2	1016010	3118626	100.00%	9.107%
100	25.556	3749	3756	3768	rVB2	541683	1646039	52.78%	4.807%




Sum of corrected areas: 34244983

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091223\
Data File : BG059025.D
Acq On : 13 Sep 2023 1:31
Operator : MA/JU
Sample : PB155220BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK220

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

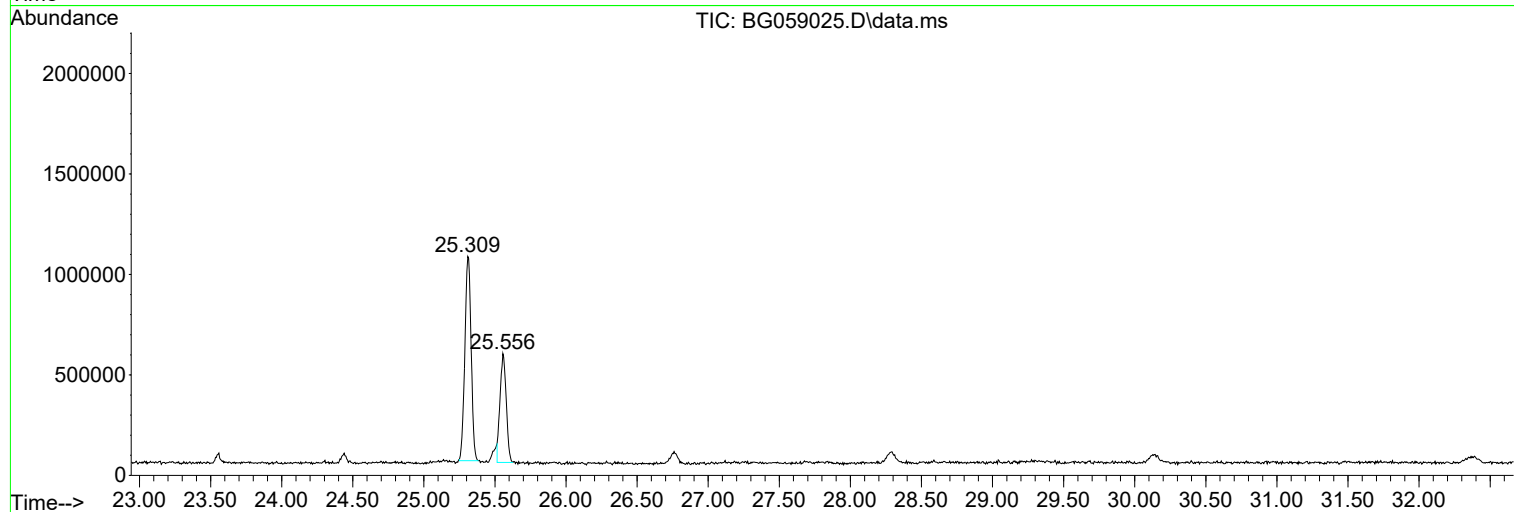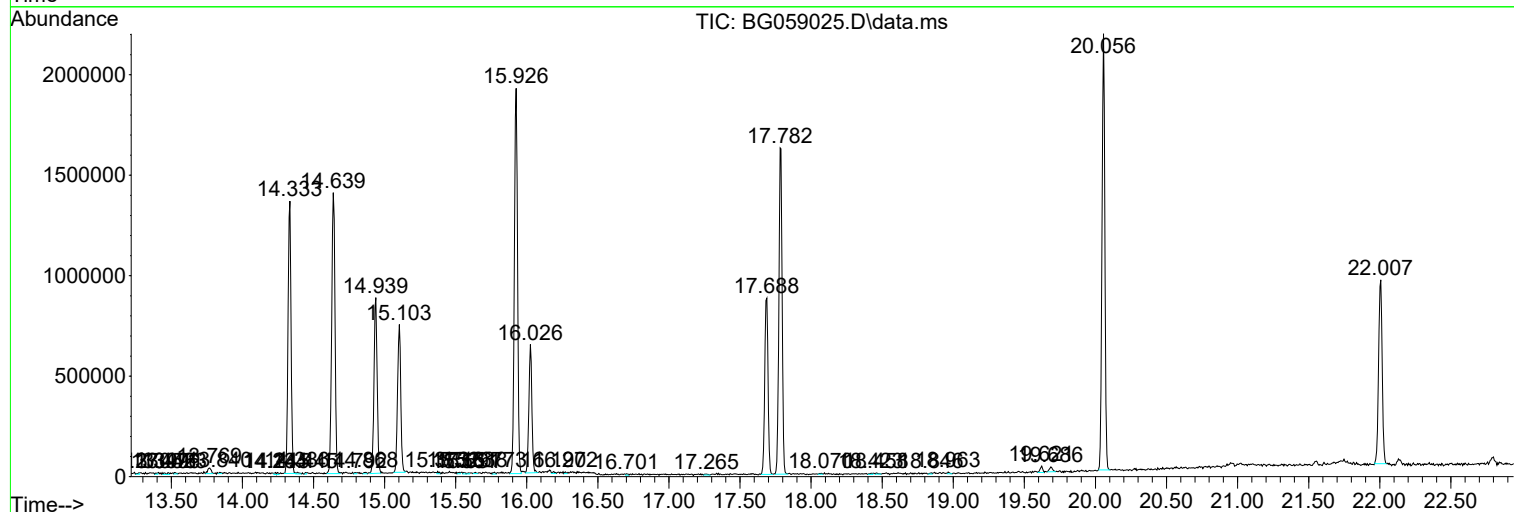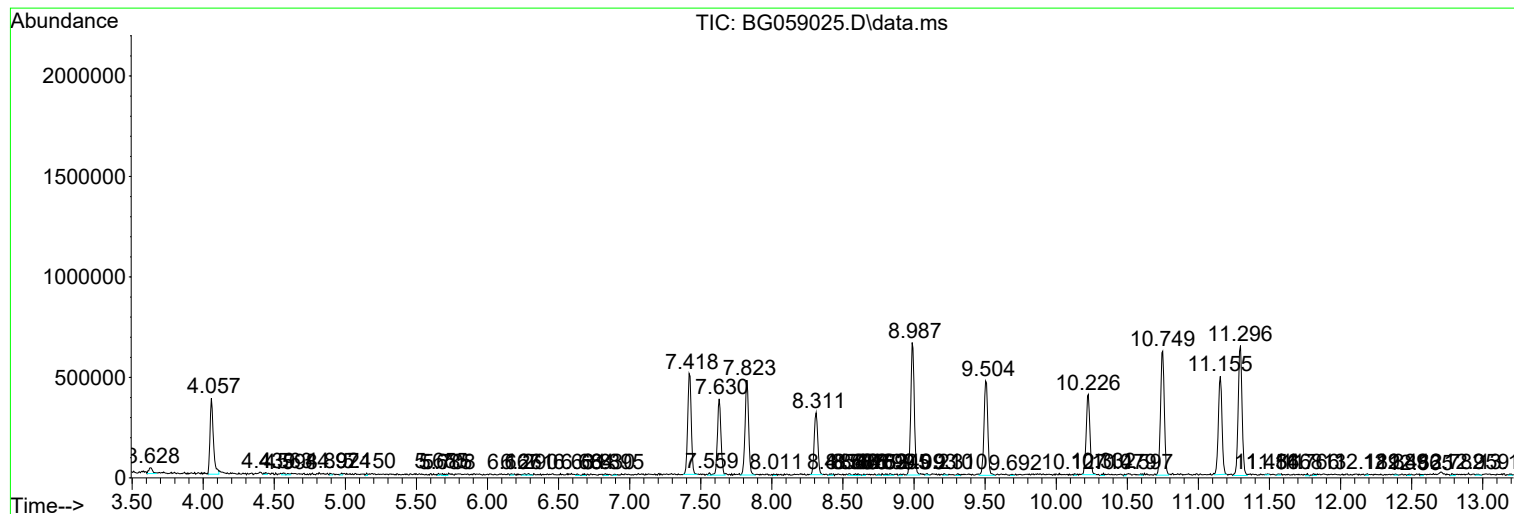

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091223\
Data File : BG059025.D
Acq On : 13 Sep 2023 1:31
Operator : MA/JU
Sample : PB155220BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK220

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091223\
Data File : BG059025.D
Acq On : 13 Sep 2023 1:31
Operator : MA/JU
Sample : PB155220BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK220

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------