
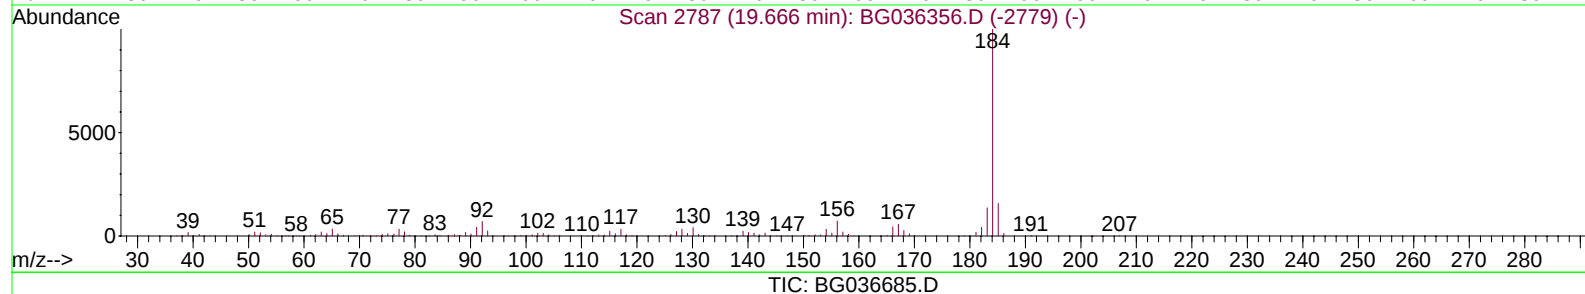
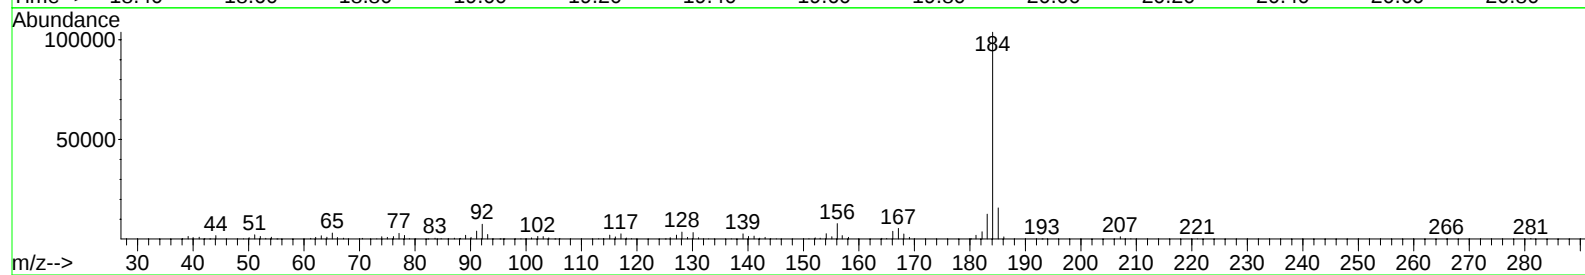


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091318\
Data File : BG036685.D
Acq On : 13 Sep 2018 16:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 19:19:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

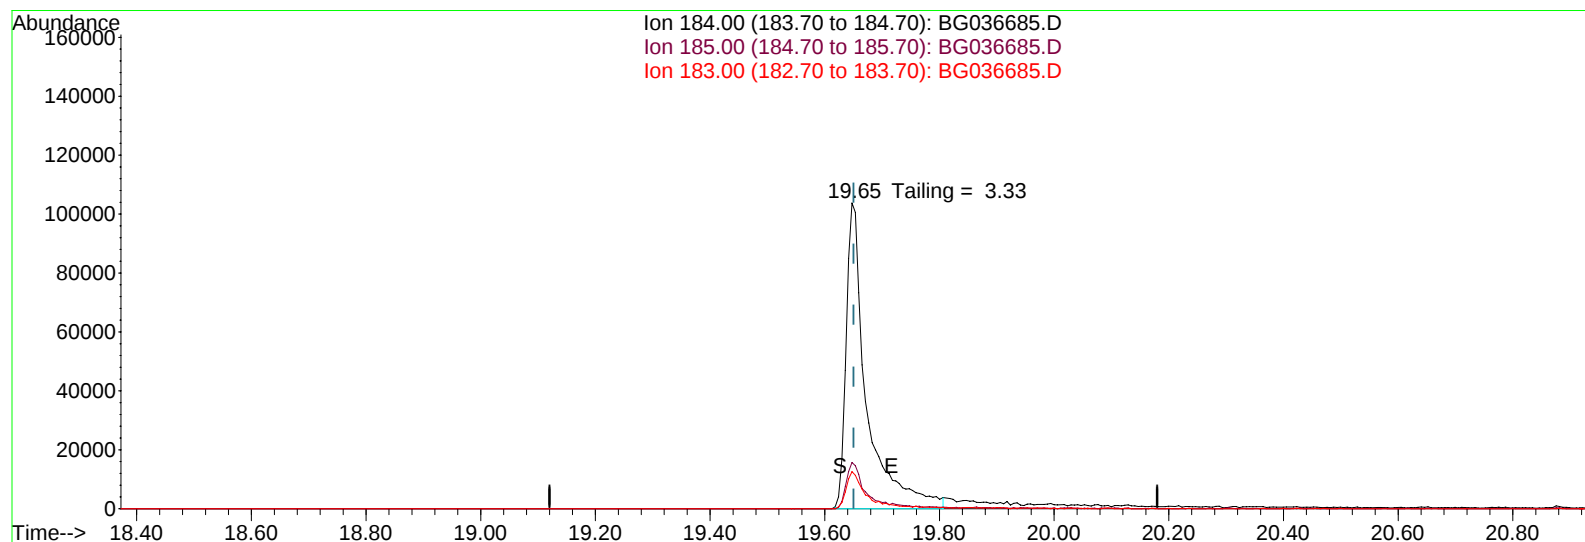

(76) Benzidine




19.647min (-0.003) 0.00ng

response 258855

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.13
183.00	13.60	12.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091318\
Data File : BG036685.D
Acq On : 13 Sep 2018 16:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 19:19:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

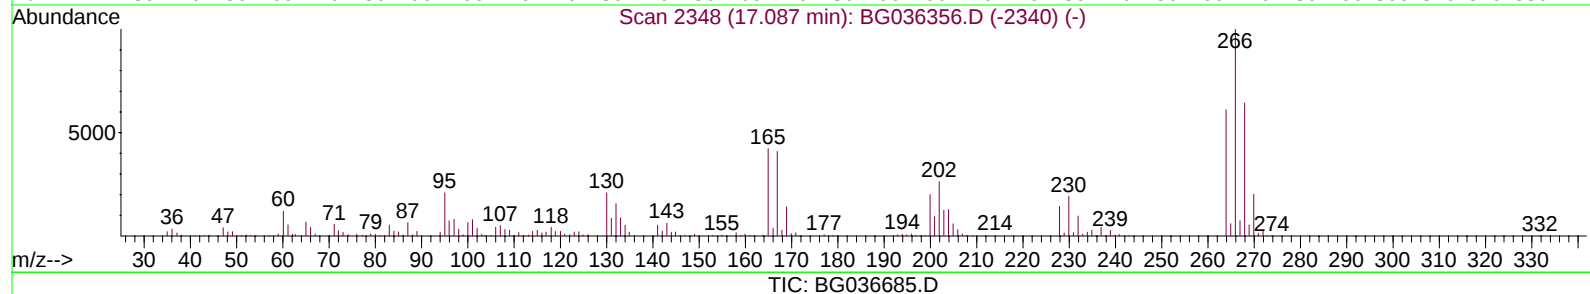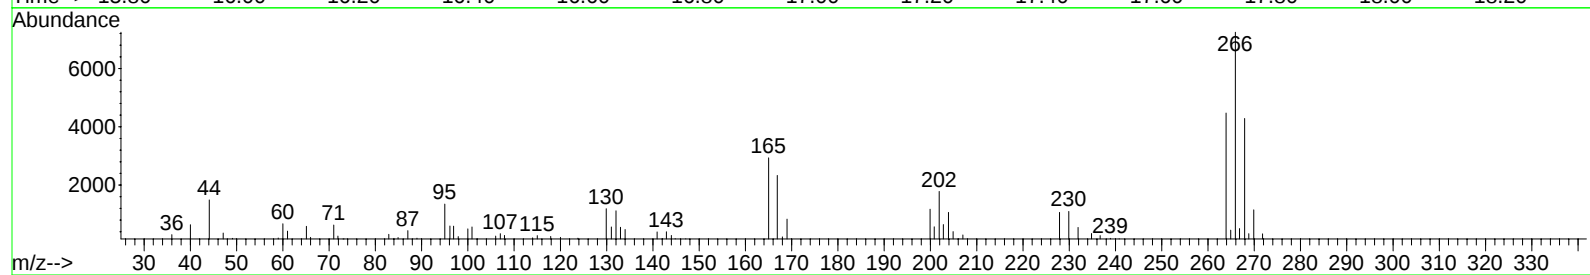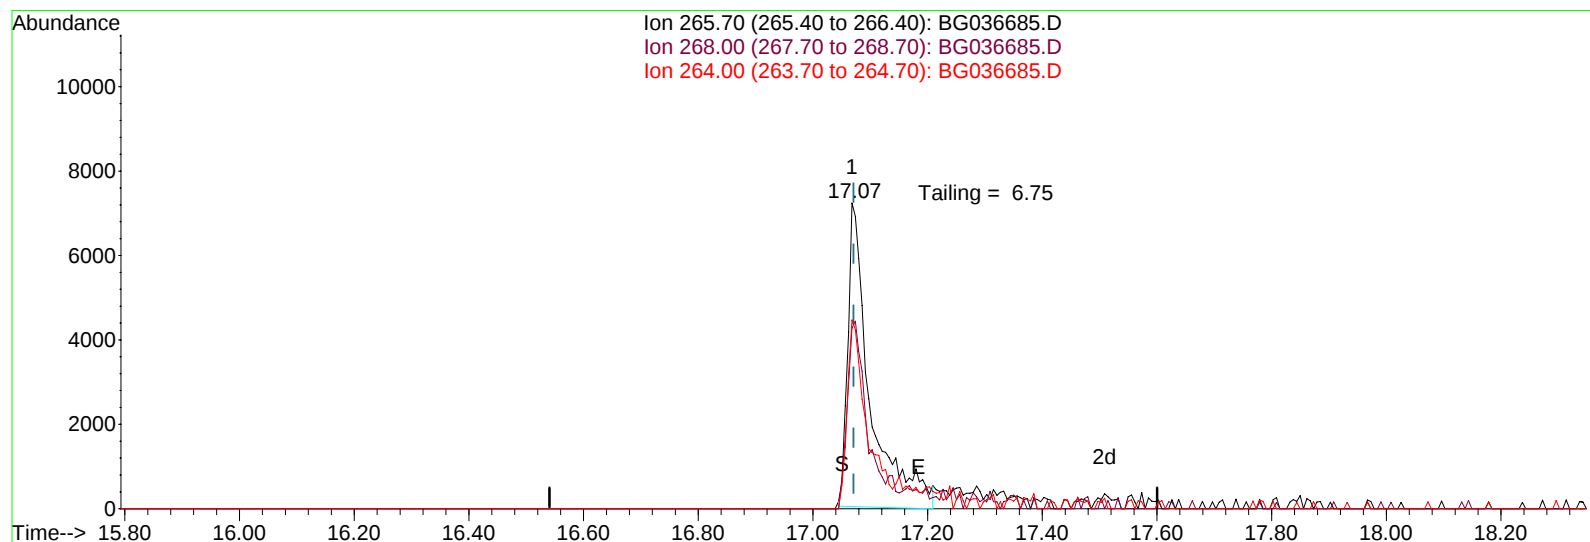

(69) Pentachlorophenol (C)

17.068min (-0.003) 6037.06ng

response 18764

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	59.15
264.00	61.10	61.73
0.00	0.00	0.00