


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091318\
 Data File : BG036685.D
 Acq On : 13 Sep 2018 16:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 31 13:03:20 2018

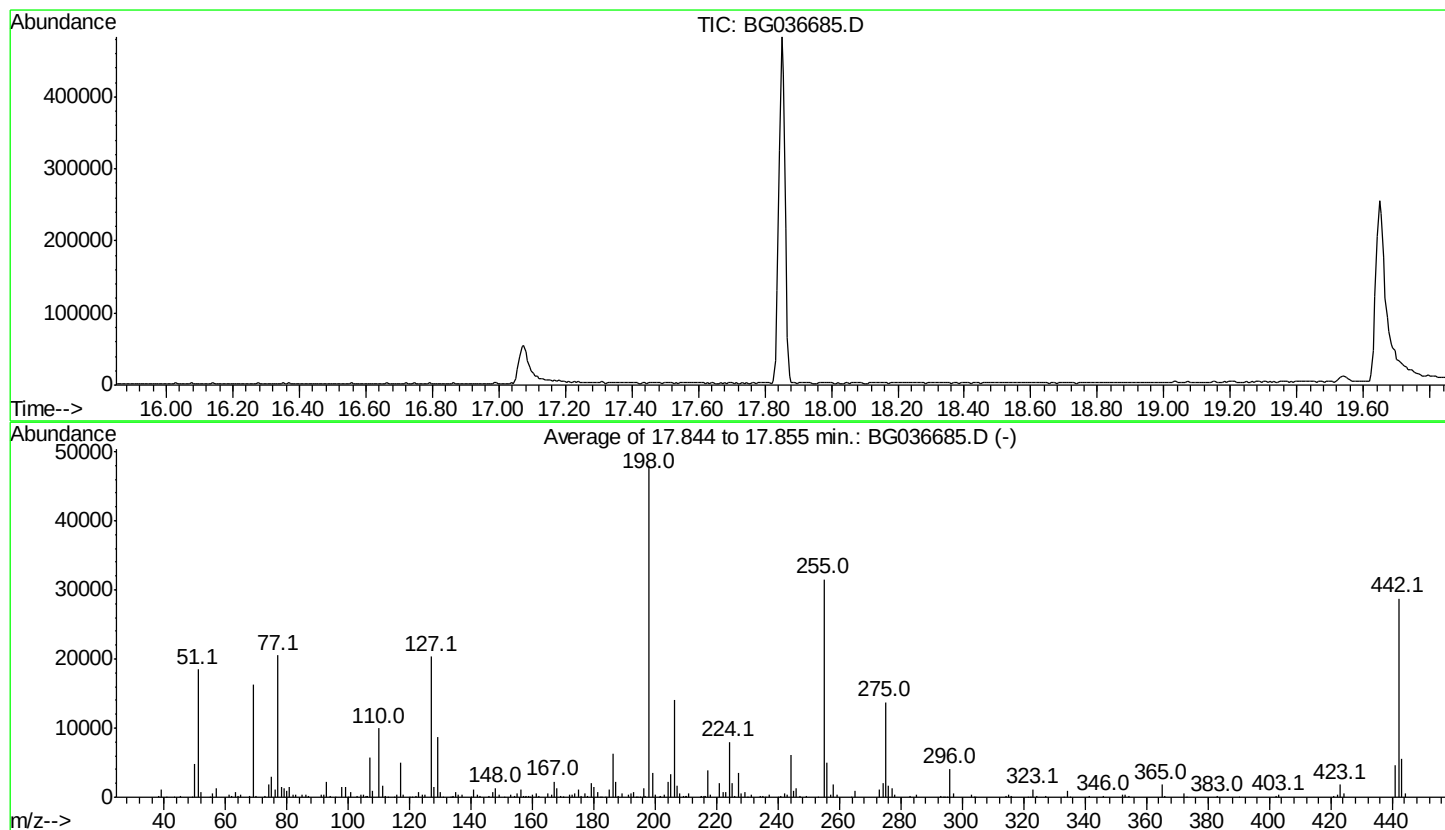

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	18490	PASS
68	69	0.00	2	0.7	118	PASS
69	198	0.00	100	34.2	16381	PASS
70	69	0.00	2	0.8	131	PASS
127	198	10	80	42.4	20314	PASS
197	198	0.00	2	0.2	105	PASS
198	198	100	100	100.0	47949	PASS
199	198	5	9	7.5	3574	PASS
275	198	10	60	28.7	13768	PASS
365	198	1	100	3.7	1794	PASS
441	198	0.01	100	9.8	4680	PASS
442	198	50	100	59.9	28712	PASS
443	442	15	24	19.5	5595	PASS