


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG091319\
 Data File : BG042816.D
 Acq On : 13 Sep 2019 14:44
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG091219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 12 14:06:09 2019

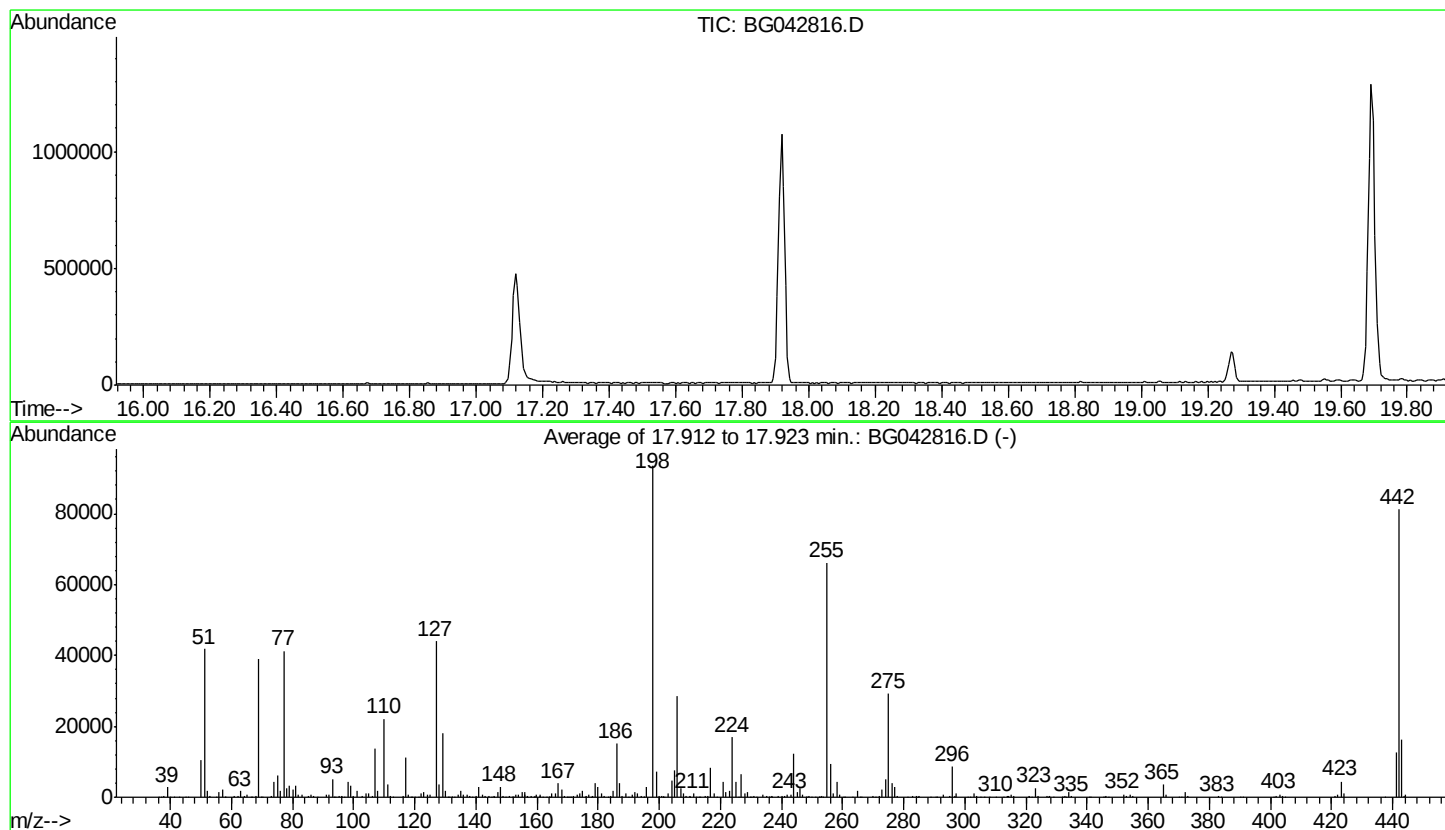

AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	41885	PASS
68	69	0.00	2	0.5	194	PASS
69	198	0.00	100	41.7	38970	PASS
70	69	0.00	2	0.4	166	PASS
127	198	10	80	47.0	43946	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	93560	PASS
199	198	5	9	7.6	7088	PASS
275	198	10	60	31.1	29109	PASS
365	198	1	100	3.9	3611	PASS
441	198	0.01	100	13.5	12612	PASS
442	198	50	100	86.8	81234	PASS
443	442	15	24	19.9	16199	PASS