


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG091319\
 Data File : BG042835.D
 Acq On : 14 Sep 2019 4:43
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG091219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 12 14:06:09 2019

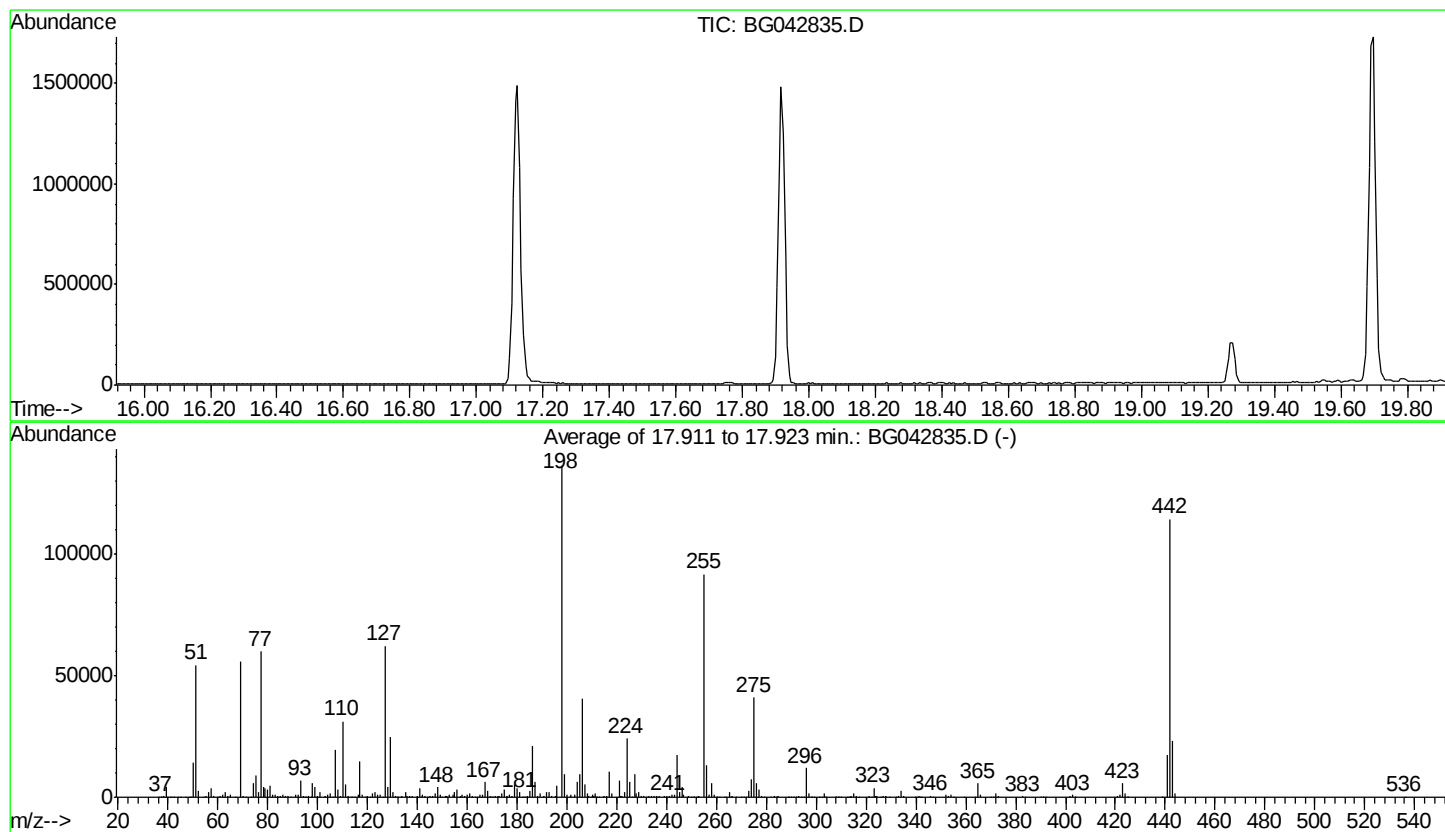

AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	54293	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.8	55600	PASS
70	69	0.00	2	0.6	344	PASS
127	198	10	80	45.7	62384	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	136437	PASS
199	198	5	9	6.8	9266	PASS
275	198	10	60	30.1	41080	PASS
365	198	1	100	4.1	5622	PASS
441	198	0.01	100	12.9	17641	PASS
442	198	50	100	83.8	114298	PASS
443	442	15	24	20.3	23173	PASS