

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
 Data File : BG059057.D
 Acq On : 14 Sep 2023 2:57
 Operator : MA/JU
 Sample : 04247-08DL 2X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBJ81DL

Quant Time: Sep 14 05:17:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 12 23:54:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.299	152	84018	20.000	ng/u1	-0.01
20) Naphthalene-d8	11.142	136	377528	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.926	164	306815	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.682	188	850658	20.000	ng/u1	0.00
79) Chrysene-d12	22.000	240	841768	20.000	ng/u1	-0.01
88) Perylene-d12	25.555	264	949620	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	4.045	84	39578	6.324	ng/u1	-0.01
7) Phenol-d5	7.412	99	36332	4.288	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.617	67	84373	16.983	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.811	132	87412	16.086	ng/u1	-0.01
15) 4-Methylphenol-d8	8.980	113	67777	10.354	ng/u1	-0.01
21) Nitrobenzene-d5	9.497	128	57046	20.832	ng/u1	-0.01
24) 2-Nitrophenol-d4	10.214	143	65206	21.701	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.737	165	118446	18.547	ng/u1	-0.01
31) 4-Chloroaniline-d4	11.283	131	105186	12.248	ng/u1	-0.01
46) Dimethylphthalate-d6	14.321	166	484504	20.358	ng/u1	-0.01
49) Acenaphthylene-d8	14.633	160	491552	18.548	ng/u1	0.00
54) 4-Nitrophenol-d4	15.091	143	19303	4.883	ng/u1	-0.02
60) Fluorene-d10	15.913	176	431218	20.417	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	16.019	200	90445	21.660	ng/u1	-0.01
73) Anthracene-d10	17.782	188	792097	20.976	ng/u1	0.00
81) Pyrene-d10	20.050	212	978508	21.944	ng/u1	-0.01
92) Benzo(a)pyrene-d12	25.308	264	941676	20.229	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.645	88	48530	19.054	ng/uL	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
Data File : BG059057.D
Acq On : 14 Sep 2023 2:57
Operator : MA/JU
Sample : 04247-08DL 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJ81DL

Quant Time: Sep 14 05:17:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 12 23:54:19 2023
Response via : Initial Calibration

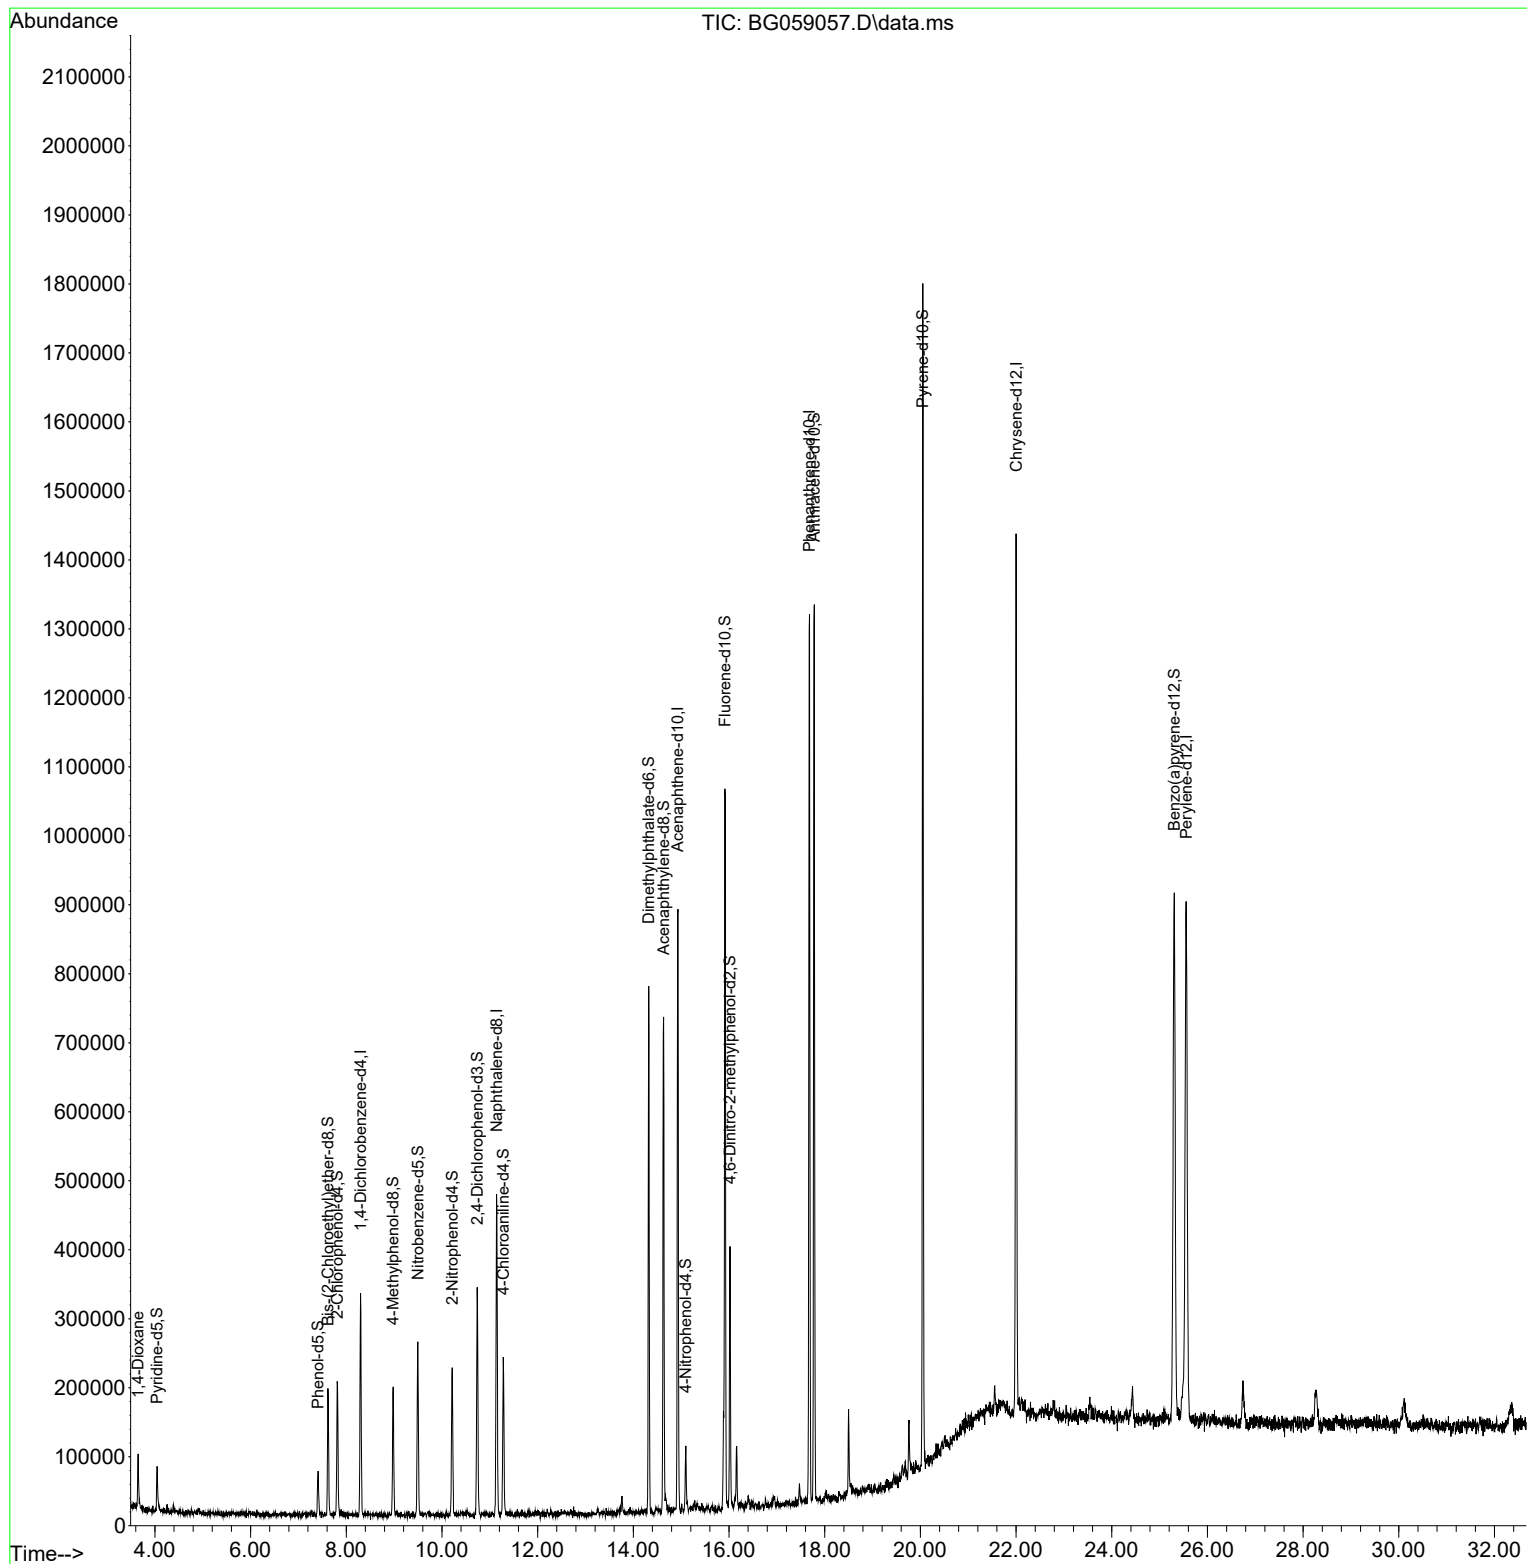

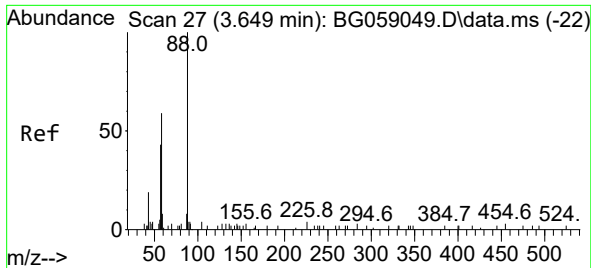

#2
 1,4-Dioxane
 Concen: 19.054 ng/uL
 RT: 3.645 min Scan# 21
 Delta R.T. -0.018 min
 Lab File: BG059057.D
 Acq: 14 Sep 2023 2:57

Instrument :
 BNA_G
 ClientSampleId :
 BBJ81DL

Tgt Ion	Ratio	Lower	Upper
88	100		
43	21.9	18.6	28.0
58	57.1	53.8	80.8

