

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
 Data File : BG059038.D
 Acq On : 13 Sep 2023 13:13
 Operator : MA/JU
 Sample : PB155387BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK387

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059038.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.611	18	21	25	rVB4	27129	35962	0.98%	0.112%
2	3.840	58	60	65	rBV4	7091	10562	0.29%	0.033%
3	3.952	77	79	83	rVV3	6424	8746	0.24%	0.027%
4	4.046	90	95	101	rBV	286991	487380	13.22%	1.517%
5	4.363	146	149	150	rBV3	7961	8760	0.24%	0.027%
6	4.381	150	152	155	rVB4	13728	16804	0.46%	0.052%
7	4.510	170	174	176	rBV3	6858	10005	0.27%	0.031%
8	4.546	178	180	183	rBV4	10423	11250	0.31%	0.035%
9	4.657	196	199	203	rBV5	8382	9676	0.26%	0.030%
10	4.810	224	225	228	rVB3	10283	7207	0.20%	0.022%
11	4.833	228	229	232	rBV3	8231	8617	0.23%	0.027%
12	4.886	236	238	241	rBV3	10216	12100	0.33%	0.038%
13	5.051	264	266	268	rBV3	8708	10765	0.29%	0.034%
14	5.251	298	300	302	rVB2	9750	6904	0.19%	0.021%
15	5.374	319	321	324	rBV4	7032	8402	0.23%	0.026%
16	5.503	340	343	344	rBV2	6264	6988	0.19%	0.022%
17	5.727	379	381	383	rBV2	8620	7015	0.19%	0.022%
18	5.897	407	410	413	rBV4	10209	14455	0.39%	0.045%
19	5.973	422	423	426	rVB3	9285	8373	0.23%	0.026%
20	6.044	432	435	436	rVB3	8638	8029	0.22%	0.025%
21	6.103	441	445	447	rBV5	5832	8123	0.22%	0.025%
22	6.461	501	506	508	rVB4	6855	9266	0.25%	0.029%
23	6.620	529	533	536	rBV5	5551	7204	0.20%	0.022%
24	6.672	539	542	546	rBV5	7731	9711	0.26%	0.030%
25	6.855	569	573	574	rVB4	9350	12142	0.33%	0.038%
26	6.960	586	591	594	rVB5	8566	15368	0.42%	0.048%
27	7.048	602	606	607	rBV4	5826	7968	0.22%	0.025%
28	7.060	607	608	613	rVB4	8406	8322	0.23%	0.026%
29	7.419	662	669	676	rBV	471697	822090	22.30%	2.559%
30	7.501	681	683	687	rVB4	10318	10209	0.28%	0.032%
31	7.624	697	704	711	rVB	366166	611557	16.59%	1.904%
32	7.718	719	720	724	rVB2	7457	7956	0.22%	0.025%
33	7.818	730	737	744	rBV	440634	780209	21.17%	2.429%
34	7.918	752	754	758	rVB4	7004	7499	0.20%	0.023%
35	8.177	795	798	802	rBV5	6609	7485	0.20%	0.023%
36	8.306	812	820	829	rVB	373956	663256	17.99%	2.065%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
 Data File : BG059038.D
 Acq On : 13 Sep 2023 13:13
 Operator : MA/JU
 Sample : PB155387BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK387

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

37	8.376	831	832	836	rVB4	9749	11775	0.32%	0.037%
38	8.406	836	837	840	rBV2	11121	11672	0.32%	0.036%
39	8.453	842	845	847	rBV4	9330	9243	0.25%	0.029%
40	8.987	929	936	945	rVB2	629252	1078461	29.26%	3.357%
41	9.275	983	985	988	rVB3	9160	9238	0.25%	0.029%
42	9.316	991	992	1000	rVV6	9329	13770	0.37%	0.043%
43	9.428	1008	1011	1014	rBV2	7621	7201	0.20%	0.022%
44	9.504	1016	1024	1030	rBV	487430	854818	23.19%	2.661%
45	9.687	1053	1055	1058	rBV	6008	8655	0.23%	0.027%
46	9.980	1103	1105	1108	rVB3	7175	6935	0.19%	0.022%
47	10.221	1138	1146	1153	rBV	400604	694081	18.83%	2.161%
48	10.497	1192	1193	1197	rVV4	7582	9748	0.26%	0.030%
49	10.533	1197	1199	1204	rVB5	8678	12952	0.35%	0.040%
50	10.627	1214	1215	1218	rVB3	8695	6940	0.19%	0.022%
51	10.744	1228	1235	1245	rBV	592584	1108553	30.07%	3.451%
52	10.926	1263	1266	1268	rBV2	5878	7283	0.20%	0.023%
53	10.973	1270	1274	1278	rVB6	5511	9117	0.25%	0.028%
54	11.150	1298	1304	1316	rVB	582096	1070513	29.04%	3.333%
55	11.296	1319	1329	1335	rBV2	279602	533915	14.48%	1.662%
56	11.514	1363	1366	1368	rBV3	7804	8078	0.22%	0.025%
57	11.543	1368	1371	1372	rVB2	8604	7606	0.21%	0.024%
58	11.813	1415	1417	1421	rBV4	6551	7633	0.21%	0.024%
59	12.013	1449	1451	1453	rBV3	6805	7583	0.21%	0.024%
60	12.160	1475	1476	1478	rBV	8148	6997	0.19%	0.022%
61	12.401	1513	1517	1520	rVB4	7892	11373	0.31%	0.035%
62	12.524	1537	1538	1540	rBV2	9713	7089	0.19%	0.022%
63	12.701	1563	1568	1575	rBV7	18278	47711	1.29%	0.149%
64	12.812	1584	1587	1589	rVB2	7429	7961	0.22%	0.025%
65	12.871	1593	1597	1599	rBV3	6740	7819	0.21%	0.024%
66	13.006	1618	1620	1623	rBV4	7099	9064	0.25%	0.028%
67	13.083	1630	1633	1635	rBV3	8053	7072	0.19%	0.022%
68	13.353	1677	1679	1682	rBV4	7485	7905	0.21%	0.025%
69	13.417	1687	1690	1693	rBV5	8982	11860	0.32%	0.037%
70	13.682	1733	1735	1737	rBV3	9258	7114	0.19%	0.022%
71	13.770	1744	1750	1753	rVB5	18325	34625	0.94%	0.108%
72	13.794	1753	1754	1757	rBV3	8101	7439	0.20%	0.023%
73	14.269	1833	1835	1839	rBV5	11197	14757	0.40%	0.046%
74	14.334	1839	1846	1852	rVV	1427636	2087348	56.63%	6.498%
75	14.405	1855	1858	1859	rVB3	8545	7241	0.20%	0.023%
76	14.422	1859	1861	1864	rBV3	10260	11358	0.31%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
 Data File : BG059038.D
 Acq On : 13 Sep 2023 13:13
 Operator : MA/JU
 Sample : PB155387BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK387

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

77	14.452	1864	1866	1868	rVB2	11750	9574	0.26%	0.030%
78	14.475	1868	1870	1872	rBV	10769	10488	0.28%	0.033%
79	14.499	1872	1874	1878	rBV3	7306	7348	0.20%	0.023%
80	14.575	1885	1887	1891	rBV5	4848	7518	0.20%	0.023%
81	14.640	1891	1898	1905	rVV2	1421869	2218938	60.20%	6.908%
82	14.698	1905	1908	1911	rVB5	8019	12017	0.33%	0.037%
83	14.734	1911	1914	1918	rBV4	10157	16842	0.46%	0.052%
84	14.886	1937	1940	1941	rBV3	7812	6897	0.19%	0.021%
85	14.939	1942	1949	1958	rVB	1046474	1663850	45.14%	5.180%
86	15.039	1964	1966	1970	rBV5	7995	7768	0.21%	0.024%
87	15.110	1970	1978	1987	rBV	662109	1095780	29.73%	3.411%
88	15.333	2014	2016	2021	rVB6	10636	16868	0.46%	0.053%
89	15.591	2058	2060	2062	rBV3	10999	9799	0.27%	0.031%
90	15.650	2068	2070	2073	rBV3	11832	12235	0.33%	0.038%
91	15.826	2098	2100	2106	rBV5	7353	8156	0.22%	0.025%
92	15.926	2110	2117	2125	rBV	1912503	2893687	78.50%	9.008%
93	16.032	2129	2135	2143	rBV	612035	928456	25.19%	2.890%
94	16.150	2153	2155	2156	rBV2	11498	7959	0.22%	0.025%
95	17.025	2302	2304	2305	rBV2	14426	9408	0.26%	0.029%
96	17.043	2305	2307	2310	rVB4	14424	11765	0.32%	0.037%
97	17.689	2411	2417	2424	rBV	1550632	2377730	64.50%	7.402%
98	17.789	2428	2434	2445	rVV2	2260699	3481161	94.44%	10.837%
99	20.063	2816	2821	2827	rBV	2706351	3686147	100.00%	11.475%
100	22.013	3149	3153	3160	rVB2	1225212	2145305	58.20%	6.678%




Sum of corrected areas: 32122564

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
Data File : BG059038.D
Acq On : 13 Sep 2023 13:13
Operator : MA/JU
Sample : PB155387BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK387

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

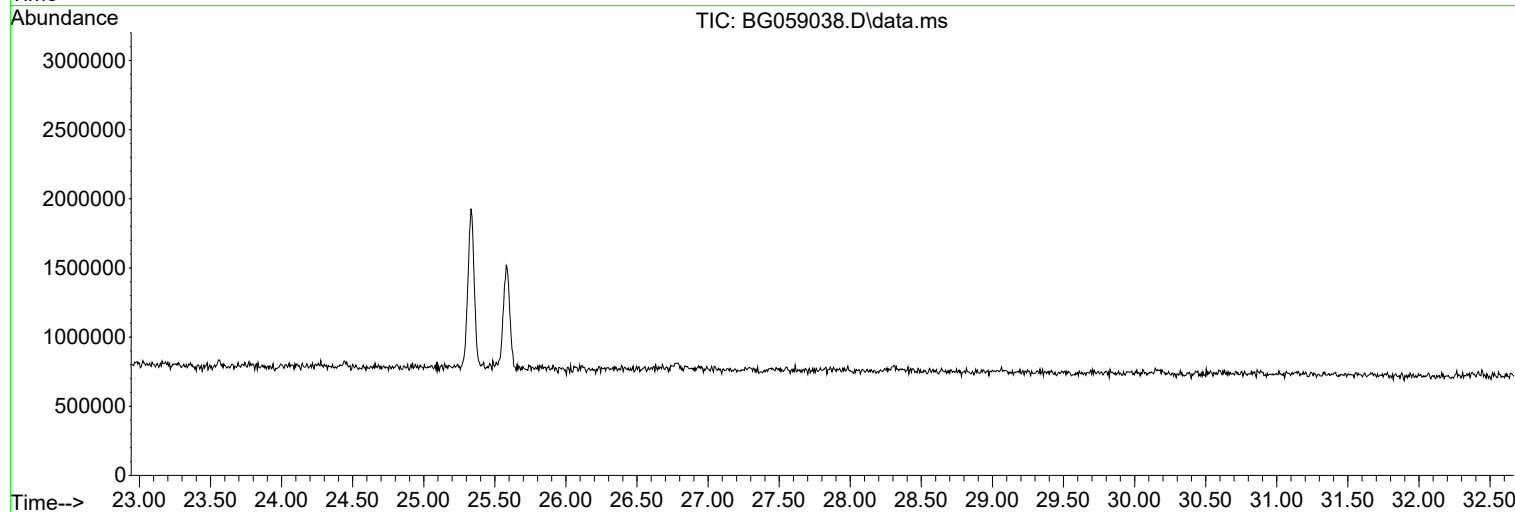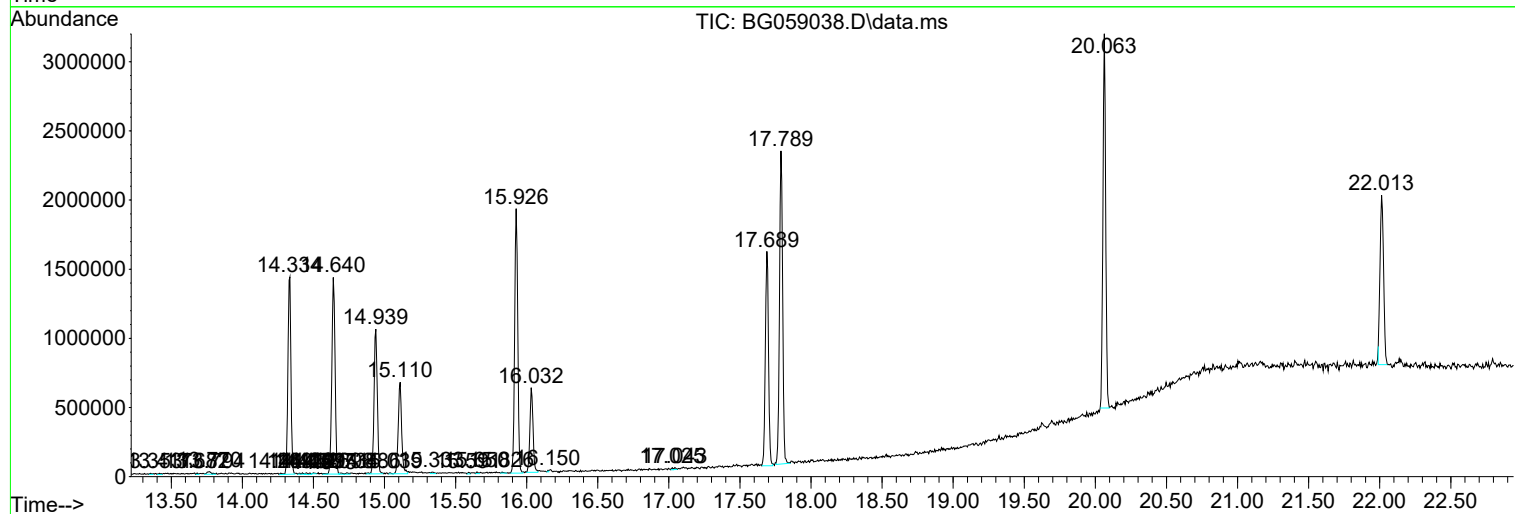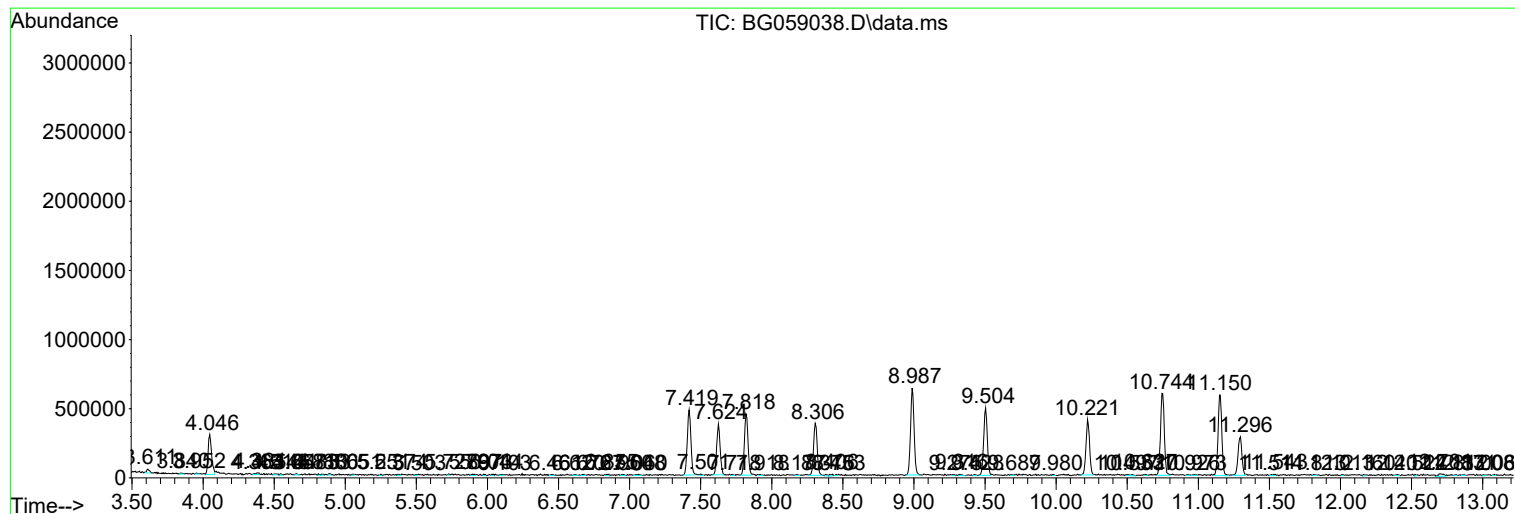

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
Data File : BG059038.D
Acq On : 13 Sep 2023 13:13
Operator : MA/JU
Sample : PB155387BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK387

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
Data File : BG059038.D
Acq On : 13 Sep 2023 13:13
Operator : MA/JU
Sample : PB155387BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK387

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc