

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
 Data File : BG059050.D
 Acq On : 13 Sep 2023 22:10
 Operator : MA/JU
 Sample : PB155407BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK407

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059050.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.608	17	20	24	rBV2	21895	30911	0.80%	0.084%
2	3.666	27	30	33	rVB5	8472	8627	0.22%	0.024%
3	3.813	53	55	59	rVB4	7016	7425	0.19%	0.020%
4	3.860	59	63	64	rBV4	7518	7697	0.20%	0.021%
5	3.925	72	74	77	rVB2	6209	6970	0.18%	0.019%
6	4.042	89	94	105	rBV	233094	419229	10.84%	1.144%
7	4.272	131	133	137	rVB5	8448	11585	0.30%	0.032%
8	4.389	149	153	156	rVB6	8414	11879	0.31%	0.032%
9	4.489	167	170	172	rVB3	10331	10427	0.27%	0.028%
10	4.512	172	174	178	rBV2	8258	9552	0.25%	0.026%
11	4.559	181	182	188	rVV5	7803	11302	0.29%	0.031%
12	4.612	188	191	195	rVV5	5478	9202	0.24%	0.025%
13	4.659	197	199	202	rVB4	7564	6928	0.18%	0.019%
14	4.683	202	203	206	rBV3	4705	6331	0.16%	0.017%
15	4.806	220	224	225	rBV3	6719	7321	0.19%	0.020%
16	4.900	238	240	244	rBV4	6119	7049	0.18%	0.019%
17	5.088	268	272	275	rBV3	4629	7536	0.19%	0.021%
18	5.112	275	276	281	rVB4	5227	6446	0.17%	0.018%
19	5.541	345	349	352	rVB4	6460	7907	0.20%	0.022%
20	5.688	373	374	378	rBV3	8530	8095	0.21%	0.022%
21	5.834	396	399	400	rBV3	5931	6426	0.17%	0.018%
22	6.158	451	454	458	rBV4	5203	6524	0.17%	0.018%
23	6.469	504	507	509	rBV	6817	7405	0.19%	0.020%
24	6.810	564	565	568	rVB2	7355	6827	0.18%	0.019%
25	6.839	568	570	571	rBV	8693	6211	0.16%	0.017%
26	6.880	574	577	581	rVV2	5455	9207	0.24%	0.025%
27	6.921	581	584	586	rVB4	5689	6342	0.16%	0.017%
28	7.133	618	620	624	rVB4	6825	8026	0.21%	0.022%
29	7.250	637	640	642	rBV3	5271	7258	0.19%	0.020%
30	7.309	648	650	654	rVB5	4933	6256	0.16%	0.017%
31	7.356	657	658	661	rBV2	7168	6819	0.18%	0.019%
32	7.415	661	668	675	rBV	441617	770970	19.94%	2.103%
33	7.621	694	703	710	rVB	322355	547023	14.15%	1.492%
34	7.814	729	736	745	rVB	409251	702457	18.17%	1.916%
35	7.950	755	759	760	rVB2	8901	7929	0.21%	0.022%
36	8.138	789	791	793	rBV2	7959	6803	0.18%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
 Data File : BG059050.D
 Acq On : 13 Sep 2023 22:10
 Operator : MA/JU
 Sample : PB155407BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK407

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

37	8.302	812	819	827	rBV	339207	562884	14.56%	1.535%
38	8.378	829	832	835	rVB4	5660	7330	0.19%	0.020%
39	8.561	860	863	864	rVB3	7785	6555	0.17%	0.018%
40	8.719	886	890	892	rBV3	4727	6344	0.16%	0.017%

41	8.931	923	926	928	rBV3	7241	6880	0.18%	0.019%
42	8.984	928	935	942	rVV	580733	1021646	26.43%	2.787%
43	9.495	1016	1022	1029	rVB2	436351	788277	20.39%	2.150%
44	9.648	1044	1048	1049	rBV2	6412	8794	0.23%	0.024%
45	9.700	1053	1057	1059	rVB3	6896	6840	0.18%	0.019%

46	9.730	1059	1062	1064	rBV2	8276	8721	0.23%	0.024%
47	10.218	1136	1145	1155	rVB2	392883	719305	18.61%	1.962%
48	10.488	1190	1191	1195	rVB3	5445	7047	0.18%	0.019%
49	10.570	1203	1205	1208	rVB	7171	6852	0.18%	0.019%
50	10.740	1226	1234	1244	rVB	606656	1091833	28.24%	2.978%

51	11.146	1295	1303	1310	rBV	508922	933389	24.14%	2.546%
52	11.199	1310	1312	1314	rVB2	9516	8105	0.21%	0.022%
53	11.287	1320	1327	1335	rBV2	371382	692988	17.93%	1.890%
54	11.363	1338	1340	1344	rVB3	6951	8010	0.21%	0.022%
55	11.404	1344	1347	1349	rBV3	5280	6418	0.17%	0.018%

56	11.769	1406	1409	1410	rBV3	7762	9349	0.24%	0.026%
57	11.845	1420	1422	1427	rVB5	6438	8985	0.23%	0.025%
58	12.609	1549	1552	1555	rVB2	6647	7164	0.19%	0.020%
59	12.703	1564	1568	1572	rBV3	14108	21278	0.55%	0.058%
60	12.903	1598	1602	1604	rVB3	6010	8675	0.22%	0.024%

61	12.955	1609	1611	1615	rVB4	8036	11164	0.29%	0.030%
62	13.008	1619	1620	1623	rBV2	8738	9314	0.24%	0.025%
63	13.185	1646	1650	1652	rBV2	5604	7987	0.21%	0.022%
64	13.279	1665	1666	1669	rVB	7146	6473	0.17%	0.018%
65	13.314	1669	1672	1675	rBV4	8698	12992	0.34%	0.035%

66	13.760	1746	1748	1751	rVB3	10709	8496	0.22%	0.023%
67	13.854	1762	1764	1766	rBV2	8855	7806	0.20%	0.021%
68	13.890	1766	1770	1774	rVB4	5740	10582	0.27%	0.029%
69	14.095	1802	1805	1807	rBV2	6562	7505	0.19%	0.020%
70	14.230	1826	1828	1831	rBV3	9889	10484	0.27%	0.029%

71	14.324	1837	1844	1850	rBV	1330140	1890869	48.91%	5.158%
72	14.383	1852	1854	1857	rVB4	7565	8489	0.22%	0.023%
73	14.413	1857	1859	1862	rBV2	7062	6649	0.17%	0.018%
74	14.636	1890	1897	1905	rVB	1310721	2134727	55.22%	5.823%
75	14.930	1940	1947	1954	rVB	965308	1505005	38.93%	4.105%

76	15.100	1970	1976	1984	rBV	693074	1093902	28.30%	2.984%
----	--------	------	------	------	-----	--------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
 Data File : BG059050.D
 Acq On : 13 Sep 2023 22:10
 Operator : MA/JU
 Sample : PB155407BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK407

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

77	15.235	1997	1999	2002	rVB4	9346	8107	0.21%	0.022%
78	15.282	2002	2007	2008	rBV6	8621	11966	0.31%	0.033%
79	15.470	2037	2039	2043	rBV4	6987	7410	0.19%	0.020%
80	15.623	2063	2065	2066	rBV2	9364	7454	0.19%	0.020%
81	15.852	2100	2104	2105	rBV2	6778	7730	0.20%	0.021%
82	15.917	2108	2115	2122	rVV	1863233	2815584	72.83%	7.680%
83	15.975	2122	2125	2126	rVV3	6561	6978	0.18%	0.019%
84	16.022	2127	2133	2142	rVB	698942	1059220	27.40%	2.889%
85	16.210	2163	2165	2167	rVB2	8500	7044	0.18%	0.019%
86	16.493	2210	2213	2215	rBV4	7359	8269	0.21%	0.023%
87	16.722	2250	2252	2254	rVB2	7621	6793	0.18%	0.019%
88	17.039	2304	2306	2308	rVB2	10095	7949	0.21%	0.022%
89	17.162	2326	2327	2330	rBV3	6970	6901	0.18%	0.019%
90	17.327	2353	2355	2359	rBV3	4901	6208	0.16%	0.017%
91	17.679	2409	2415	2422	rVB	1385761	2145477	55.50%	5.852%
92	17.779	2425	2432	2440	rBV2	2194437	3404970	88.08%	9.288%
93	18.061	2475	2480	2481	rBV5	14057	19625	0.51%	0.054%
94	18.132	2490	2492	2495	rBV4	8123	9270	0.24%	0.025%
95	18.461	2547	2548	2550	rBV2	12832	7283	0.19%	0.020%
96	18.543	2560	2562	2565	rVB4	11702	11259	0.29%	0.031%
97	20.053	2813	2819	2825	rBV	2674518	3865975	100.00%	10.545%
98	22.004	3145	3151	3159	rVB2	1294075	2219504	57.41%	6.054%
99	25.312	3707	3714	3724	rVB2	1186454	3473978	89.86%	9.476%
100	25.558	3751	3756	3768	rVB2	732500	2134833	55.22%	5.823%




Sum of corrected areas: 36660802

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
Data File : BG059050.D
Acq On : 13 Sep 2023 22:10
Operator : MA/JU
Sample : PB155407BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK407

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

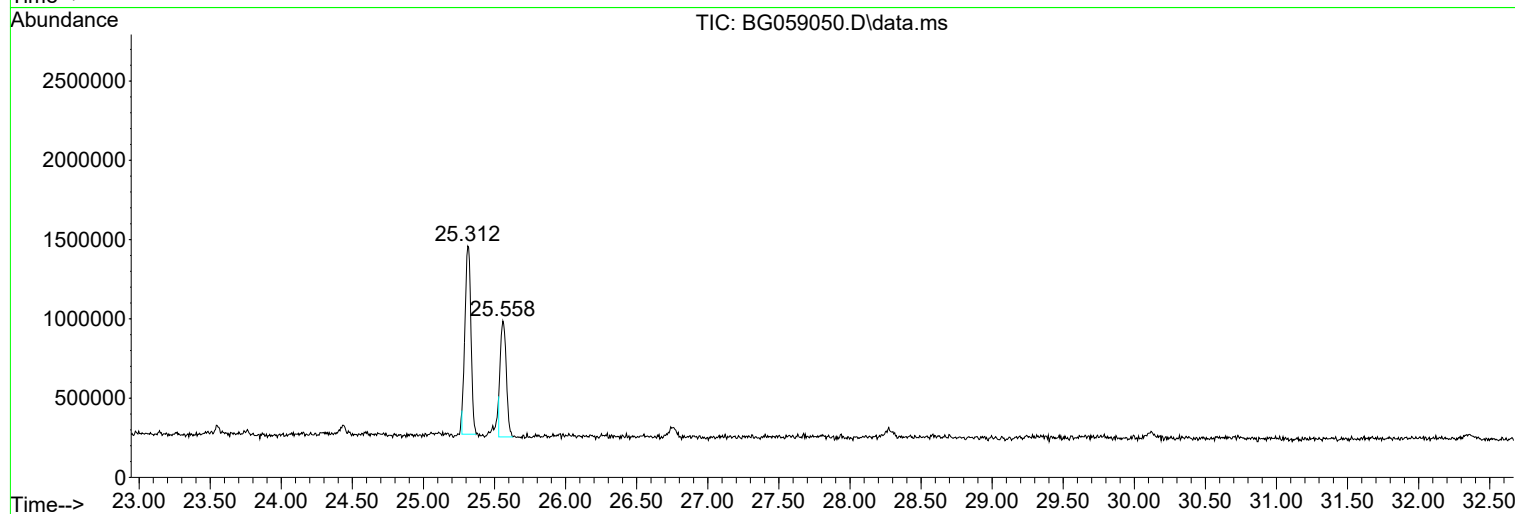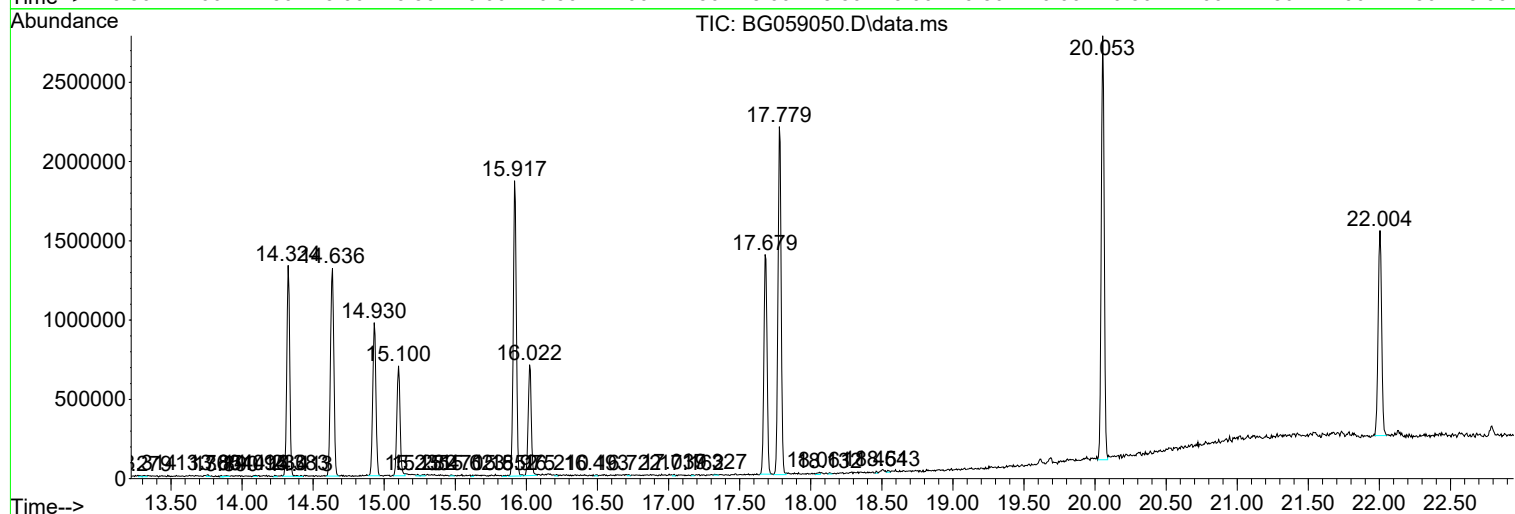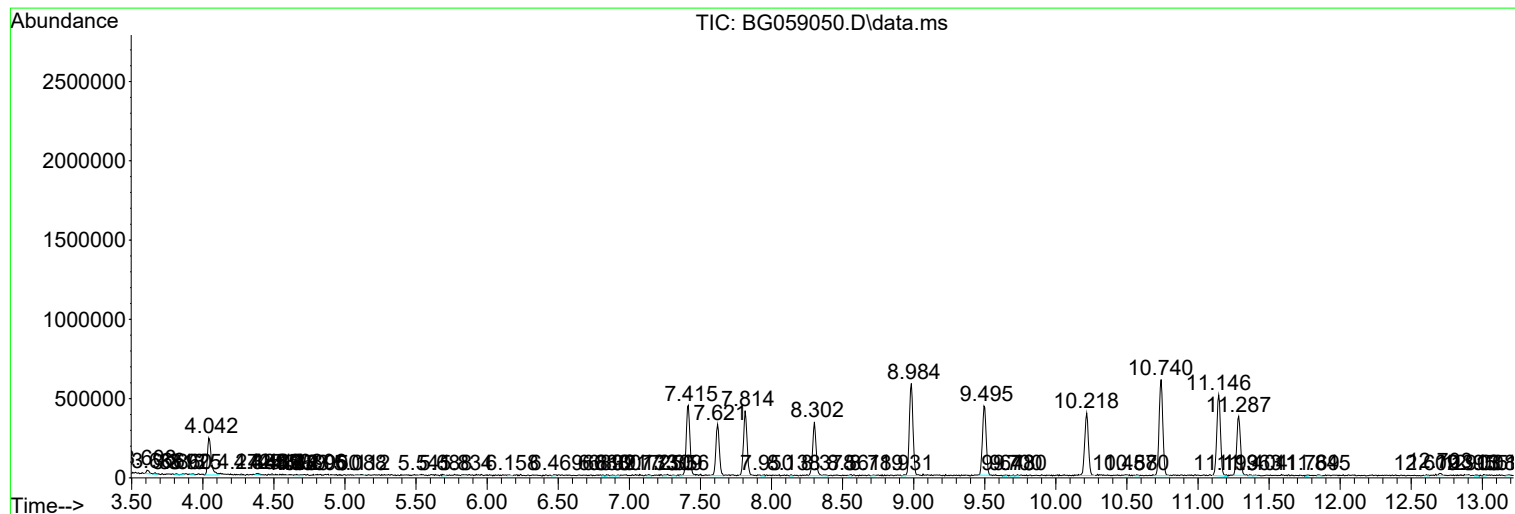

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
Data File : BG059050.D
Acq On : 13 Sep 2023 22:10
Operator : MA/JU
Sample : PB155407BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK407

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
Data File : BG059050.D
Acq On : 13 Sep 2023 22:10
Operator : MA/JU
Sample : PB155407BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK407

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------