

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
 Data File : BG059051.D
 Acq On : 13 Sep 2023 22:51
 Operator : MA/JU
 Sample : PB155393TB 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLEB393

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059051.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.613	16	21	23	rBV3	26859	38774	1.03%	0.110%
2	4.042	89	94	102	rBV2	234028	378163	10.04%	1.073%
3	4.301	136	138	142	rBV3	5723	6874	0.18%	0.020%
4	4.418	157	158	161	rVB3	9056	6965	0.19%	0.020%
5	4.542	175	179	180	rBV3	5126	6708	0.18%	0.019%
6	4.612	188	191	194	rBV3	10274	15016	0.40%	0.043%
7	4.788	219	221	223	rBV2	7649	6841	0.18%	0.019%
8	4.941	245	247	249	rBV2	9094	8768	0.23%	0.025%
9	5.018	256	260	261	rBV3	5342	6229	0.17%	0.018%
10	5.059	266	267	271	rVB2	9620	10002	0.27%	0.028%
11	5.112	271	276	277	rBV3	7989	13303	0.35%	0.038%
12	5.200	287	291	292	rVB3	5349	6459	0.17%	0.018%
13	5.212	292	293	295	rBV2	10801	6313	0.17%	0.018%
14	5.353	315	317	319	rVV3	11628	6905	0.18%	0.020%
15	5.940	412	417	420	rVB4	8216	11576	0.31%	0.033%
16	6.016	427	430	432	rBV3	5917	6306	0.17%	0.018%
17	6.199	457	461	463	rVB4	7040	8232	0.22%	0.023%
18	6.345	483	486	491	rBV5	6281	9643	0.26%	0.027%
19	6.428	496	500	502	rBV3	5945	8507	0.23%	0.024%
20	6.680	541	543	547	rVB3	6241	6643	0.18%	0.019%
21	6.763	554	557	558	rVB	8488	8065	0.21%	0.023%
22	6.786	558	561	565	rBV3	8330	12294	0.33%	0.035%
23	6.898	579	580	584	rVB2	7560	9402	0.25%	0.027%
24	6.933	584	586	589	rBV2	9649	11492	0.31%	0.033%
25	6.968	589	592	595	rVB3	6795	7787	0.21%	0.022%
26	6.992	595	596	598	rBV	8273	6363	0.17%	0.018%
27	7.015	598	600	603	rVB3	5803	6831	0.18%	0.019%
28	7.109	613	616	617	rBV2	5831	6217	0.17%	0.018%
29	7.350	656	657	660	rBV2	6030	6584	0.17%	0.019%
30	7.415	661	668	678	rVB	439600	759855	20.18%	2.157%
31	7.620	697	703	710	rVB	321267	520911	13.84%	1.479%
32	7.814	728	736	746	rVB	395313	710260	18.87%	2.016%
33	7.891	746	749	752	rVB4	10899	12652	0.34%	0.036%
34	7.932	755	756	760	rVB3	6273	6308	0.17%	0.018%
35	8.302	810	819	828	rVB	290304	535866	14.23%	1.521%
36	8.384	828	833	836	rBV6	6812	11425	0.30%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
 Data File : BG059051.D
 Acq On : 13 Sep 2023 22:51
 Operator : MA/JU
 Sample : PB155393TB 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLEB393

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

37	8.625	872	874	879	rVB3	6775	10147	0.27%	0.029%
38	8.984	926	935	946	rBV	575894	1000952	26.59%	2.841%
39	9.407	1005	1007	1010	rVB2	7656	6305	0.17%	0.018%
40	9.501	1013	1023	1031	rVB	419944	785216	20.86%	2.229%
41	9.577	1034	1036	1040	rVB2	4854	6434	0.17%	0.018%
42	9.724	1058	1061	1063	rVB3	7629	8071	0.21%	0.023%
43	9.830	1076	1079	1082	rVB3	5828	8386	0.22%	0.024%
44	9.971	1100	1103	1105	rVB	5176	6336	0.17%	0.018%
45	9.994	1105	1107	1110	rBV2	8075	8250	0.22%	0.023%
46	10.217	1137	1145	1154	rBV2	374985	695318	18.47%	1.974%
47	10.382	1171	1173	1176	rVB3	6126	7307	0.19%	0.021%
48	10.564	1202	1204	1207	rBV3	8981	8573	0.23%	0.024%
49	10.740	1226	1234	1243	rBV	595498	1057185	28.08%	3.001%
50	10.905	1259	1262	1264	rVV	8200	7101	0.19%	0.020%
51	10.946	1266	1269	1272	rBV3	4879	7141	0.19%	0.020%
52	10.999	1274	1278	1279	rBV3	8241	7590	0.20%	0.022%
53	11.146	1296	1303	1311	rBV	429348	824115	21.89%	2.339%
54	11.287	1320	1327	1335	rBV2	369923	682090	18.12%	1.936%
55	11.393	1342	1345	1348	rBV3	7430	9196	0.24%	0.026%
56	11.745	1401	1405	1406	rBV3	9618	11798	0.31%	0.033%
57	11.921	1433	1435	1440	rBV3	7490	9144	0.24%	0.026%
58	12.333	1503	1505	1508	rVB2	6553	7570	0.20%	0.021%
59	12.427	1518	1521	1524	rBV3	7244	10817	0.29%	0.031%
60	12.462	1524	1527	1530	rBV3	6333	8763	0.23%	0.025%
61	12.703	1564	1568	1572	rBV6	11173	17666	0.47%	0.050%
62	12.838	1588	1591	1594	rBV3	10116	12153	0.32%	0.034%
63	12.873	1594	1597	1599	rVB4	5335	6296	0.17%	0.018%
64	13.214	1652	1655	1656	rBV3	9898	8151	0.22%	0.023%
65	13.355	1675	1679	1682	rVB5	9385	15751	0.42%	0.045%
66	13.390	1682	1685	1686	rBV2	6287	7314	0.19%	0.021%
67	13.590	1717	1719	1721	rVV2	9004	6983	0.19%	0.020%
68	13.613	1721	1723	1726	rVB4	8279	7545	0.20%	0.021%
69	13.643	1726	1728	1731	rBV2	8056	8465	0.22%	0.024%
70	13.760	1744	1748	1753	rVB3	21850	31181	0.83%	0.089%
71	13.884	1764	1769	1770	rBV2	4681	6954	0.18%	0.020%
72	13.913	1772	1774	1777	rVB3	6572	7738	0.21%	0.022%
73	14.042	1793	1796	1799	rBV3	7625	11513	0.31%	0.033%
74	14.066	1799	1800	1803	rVB	9851	6982	0.19%	0.020%
75	14.324	1838	1844	1851	rBV	1298137	1867685	49.61%	5.301%
76	14.636	1888	1897	1903	rBV2	1278345	2079200	55.23%	5.901%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
 Data File : BG059051.D
 Acq On : 13 Sep 2023 22:51
 Operator : MA/JU
 Sample : PB155393TB 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLEB393

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

77	14.883	1936	1939	1940	rBV2	6409	6732	0.18%	0.019%
78	14.930	1940	1947	1955	rVB2	898446	1416842	37.63%	4.021%
79	15.029	1960	1964	1967	rVB5	5655	7906	0.21%	0.022%
80	15.100	1968	1976	1985	rBV	669422	1091294	28.99%	3.097%
81	15.917	2109	2115	2122	rVB	1818196	2755028	73.18%	7.820%
82	16.022	2126	2133	2139	rBV	699532	1031356	27.40%	2.927%
83	16.158	2152	2156	2161	rVB4	16297	25202	0.67%	0.072%
84	16.522	2217	2218	2221	rVB3	9062	8079	0.21%	0.023%
85	17.280	2346	2347	2351	rVB4	10175	10119	0.27%	0.029%
86	17.309	2351	2352	2355	rBV3	8686	10074	0.27%	0.029%
87	17.591	2398	2400	2402	rBV3	9841	8043	0.21%	0.023%
88	17.679	2407	2415	2422	rBV	1350182	2025676	53.81%	5.750%
89	17.779	2426	2432	2439	rBV2	2078235	3315780	88.07%	9.411%
90	17.979	2464	2466	2468	rBV3	10133	10375	0.28%	0.029%
91	18.014	2471	2472	2474	rBV2	10591	8790	0.23%	0.025%
92	18.055	2478	2479	2482	rVV3	7593	7303	0.19%	0.021%
93	18.196	2501	2503	2508	rVB5	8775	10241	0.27%	0.029%
94	18.402	2536	2538	2540	rBV3	11741	9279	0.25%	0.026%
95	18.502	2552	2555	2558	rBV5	12288	17602	0.47%	0.050%
96	19.060	2648	2650	2651	rBV2	11868	9635	0.26%	0.027%
97	20.053	2813	2819	2826	rVB2	2588178	3764753	100.00%	10.686%
98	22.004	3145	3151	3159	rVB2	1181259	2028720	53.89%	5.758%
99	25.311	3705	3714	3722	rVB2	1117377	3267472	86.79%	9.274%
100	25.558	3751	3756	3769	rVB3	674548	1889665	50.19%	5.364%




Sum of corrected areas: 35231887

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
Data File : BG059051.D
Acq On : 13 Sep 2023 22:51
Operator : MA/JU
Sample : PB155393TB 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLEB393

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

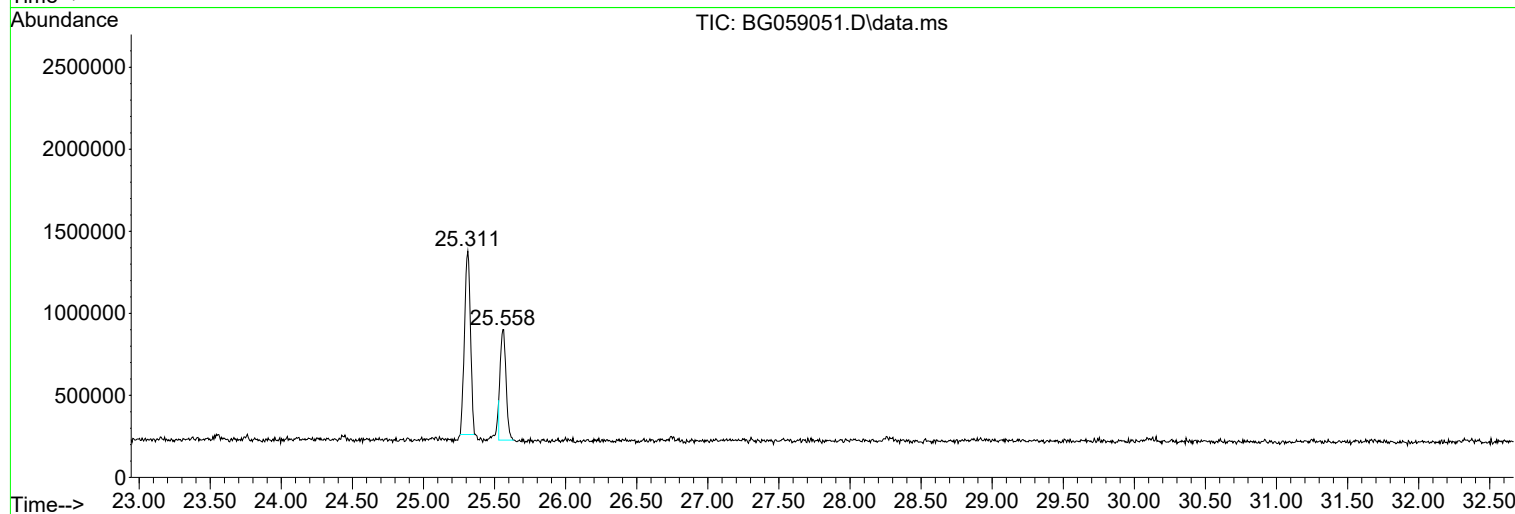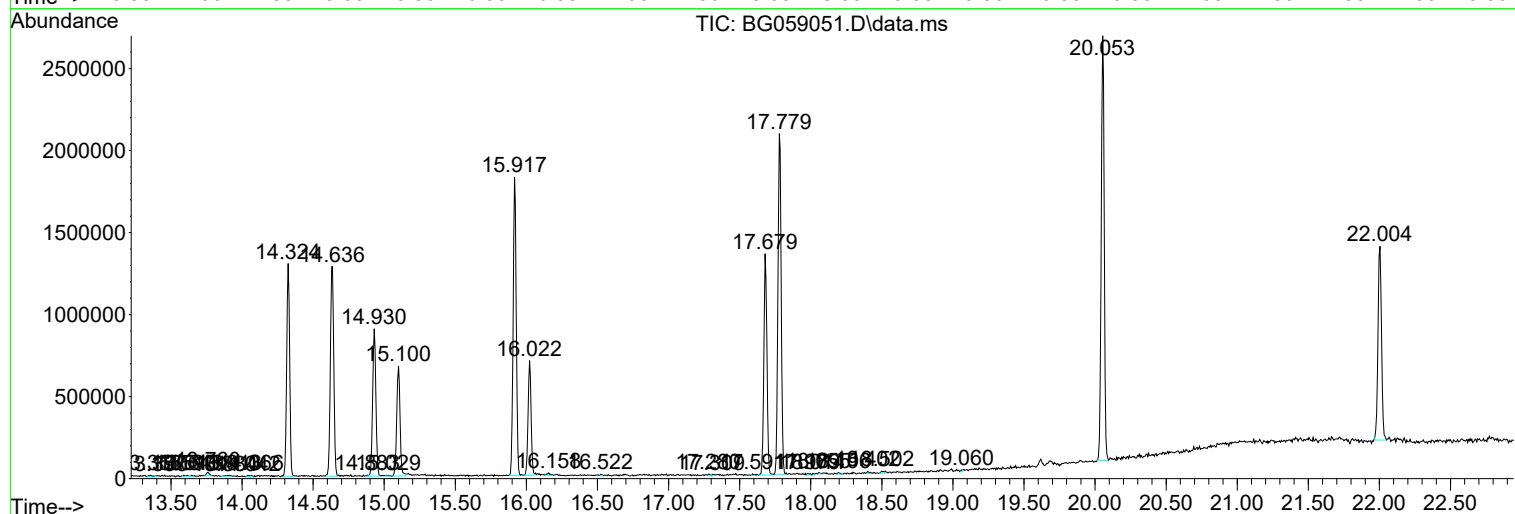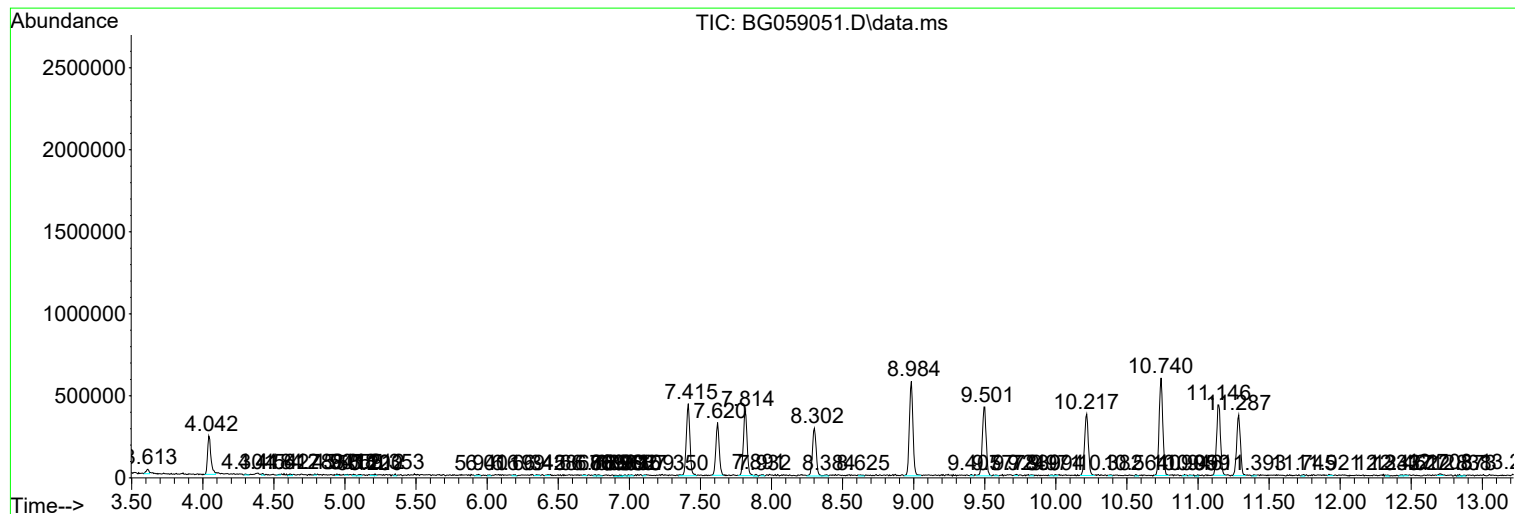

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
Data File : BG059051.D
Acq On : 13 Sep 2023 22:51
Operator : MA/JU
Sample : PB155393TB 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLEB393

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
Data File : BG059051.D
Acq On : 13 Sep 2023 22:51
Operator : MA/JU
Sample : PB155393TB 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLEB393

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------