

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
 Data File : BG059057.D
 Acq On : 14 Sep 2023 2:57
 Operator : MA/JU
 Sample : 04247-08DL 2X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBJ81DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.651	23	28	32	rBV2	76282	105669	4.35%	0.418%
2	3.745	43	44	49	rVB3	8783	11272	0.46%	0.045%
3	3.833	57	59	62	rBV3	7713	6613	0.27%	0.026%
4	4.045	91	95	103	rBV2	64513	106623	4.39%	0.422%
5	4.256	129	131	134	rBV4	13702	14669	0.60%	0.058%
6	4.386	150	153	156	rVB3	12089	10491	0.43%	0.041%
7	4.768	215	218	220	rBV2	7963	8079	0.33%	0.032%
8	5.432	330	331	335	rBV3	6284	7561	0.31%	0.030%
9	5.549	345	351	353	rBV5	6574	10752	0.44%	0.043%
10	5.907	409	412	413	rVB3	10139	7008	0.29%	0.028%
11	6.131	447	450	451	rBV2	11417	9527	0.39%	0.038%
12	6.172	455	457	461	rVV3	6293	7824	0.32%	0.031%
13	7.024	599	602	606	rVB3	9474	10121	0.42%	0.040%
14	7.412	661	668	673	rBV2	66200	119832	4.93%	0.474%
15	7.459	673	676	679	rVB4	8063	10938	0.45%	0.043%
16	7.494	679	682	686	rBV2	8147	12419	0.51%	0.049%
17	7.617	697	703	712	rBV2	183497	309166	12.73%	1.223%
18	7.811	728	736	745	rVB2	194955	360573	14.84%	1.426%
19	8.017	766	771	773	rBV2	7296	10648	0.44%	0.042%
20	8.058	775	778	780	rBV3	8258	10538	0.43%	0.042%
21	8.299	811	819	829	rBV2	323972	572619	23.57%	2.265%
22	8.516	854	856	857	rBV2	7339	6668	0.27%	0.026%
23	8.604	868	871	876	rBV3	4298	6728	0.28%	0.027%
24	8.698	884	887	889	rBV2	7795	6994	0.29%	0.028%
25	8.781	899	901	904	rBV4	6319	7961	0.33%	0.031%
26	8.904	918	922	924	rBV2	6720	8323	0.34%	0.033%
27	8.980	929	935	942	rVB2	185915	325539	13.40%	1.288%
28	9.262	977	983	985	rVB4	8929	12292	0.51%	0.049%
29	9.292	985	988	990	rBV3	8839	10356	0.43%	0.041%
30	9.392	1004	1005	1009	rVB4	8318	8108	0.33%	0.032%
31	9.497	1015	1023	1031	rBV	252331	465455	19.16%	1.841%
32	9.709	1053	1059	1061	rBV5	7436	14870	0.61%	0.059%
33	9.897	1089	1091	1094	rVB2	6595	6572	0.27%	0.026%
34	10.097	1120	1125	1126	rBV2	8806	12236	0.50%	0.048%
35	10.214	1137	1145	1151	rVV2	215184	410264	16.89%	1.623%
36	10.390	1173	1175	1180	rVV5	7323	12227	0.50%	0.048%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
 Data File : BG059057.D
 Acq On : 14 Sep 2023 2:57
 Operator : MA/JU
 Sample : 04247-08DL 2X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBJ81DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

37	10.502	1191	1194	1196	rBV2	7500	7090	0.29%	0.028%
38	10.696	1224	1227	1228	rBV2	10442	10859	0.45%	0.043%
39	10.737	1228	1234	1246	rVB2	334347	626523	25.79%	2.478%
40	10.825	1246	1249	1250	rBV2	7106	7201	0.30%	0.028%

41	10.990	1276	1277	1281	rBV2	8677	7205	0.30%	0.028%
42	11.037	1283	1285	1287	rBV	6558	7803	0.32%	0.031%
43	11.142	1294	1303	1314	rVB	466479	881827	36.30%	3.488%
44	11.283	1316	1327	1336	rBV2	230745	432610	17.81%	1.711%
45	11.795	1412	1414	1416	rVV2	7979	7842	0.32%	0.031%

46	11.836	1418	1421	1424	rBV4	9019	9242	0.38%	0.037%
47	11.947	1438	1440	1443	rBV3	8660	7811	0.32%	0.031%
48	12.030	1452	1454	1458	rVB4	10038	13645	0.56%	0.054%
49	12.065	1458	1460	1462	rBV2	8426	10006	0.41%	0.040%
50	12.106	1465	1467	1470	rBV4	8576	9551	0.39%	0.038%

51	12.200	1479	1483	1485	rBV4	11063	12589	0.52%	0.050%
52	12.276	1495	1496	1503	rVB5	11751	17570	0.72%	0.069%
53	12.335	1503	1506	1507	rBV	6526	6686	0.28%	0.026%
54	12.388	1513	1515	1518	rBV3	6385	6897	0.28%	0.027%
55	12.423	1520	1521	1524	rBV3	8961	6805	0.28%	0.027%

56	12.564	1543	1545	1551	rVB3	6270	10067	0.41%	0.040%
57	12.688	1565	1566	1570	rVV4	6860	6594	0.27%	0.026%
58	12.752	1575	1577	1579	rVV3	12736	6942	0.29%	0.027%
59	13.346	1675	1678	1681	rVV3	6583	8131	0.33%	0.032%
60	13.387	1683	1685	1690	rVB2	9019	13365	0.55%	0.053%

61	13.434	1690	1693	1696	rBV4	13052	15690	0.65%	0.062%
62	13.734	1741	1744	1745	rBV2	12016	10248	0.42%	0.041%
63	13.763	1745	1749	1754	rVB5	24307	37800	1.56%	0.150%
64	13.933	1776	1778	1780	rBV2	10524	7200	0.30%	0.028%
65	14.057	1796	1799	1802	rBV3	8089	9833	0.40%	0.039%

66	14.268	1833	1835	1837	rVB3	7435	6474	0.27%	0.026%
67	14.321	1837	1844	1851	rVB	765243	1108363	45.62%	4.384%
68	14.368	1851	1852	1856	rBV4	7333	8205	0.34%	0.032%
69	14.468	1866	1869	1870	rBV3	7557	7433	0.31%	0.029%
70	14.633	1888	1897	1902	rBV2	720084	1194388	49.16%	4.724%

71	14.674	1902	1904	1909	rVV2	24199	40934	1.68%	0.162%
72	14.721	1910	1912	1913	rVB2	11269	7173	0.30%	0.028%
73	14.844	1931	1933	1936	rBV4	6081	8034	0.33%	0.032%
74	14.932	1941	1948	1957	rVB	876376	1409283	58.01%	5.574%
75	15.009	1959	1961	1964	rBV4	11056	12000	0.49%	0.047%

76	15.097	1970	1976	1980	rBV2	92810	144783	5.96%	0.573%
----	--------	------	------	------	------	-------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
 Data File : BG059057.D
 Acq On : 14 Sep 2023 2:57
 Operator : MA/JU
 Sample : 04247-08DL 2X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBJ81DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
 Title : SVOA CALIBRATION

77	15.267	2002	2005	2007	rBV3	10472	12436	0.51%	0.049%
78	15.332	2012	2016	2017	rBV3	10004	11120	0.46%	0.044%
79	15.913	2105	2115	2122	rBV2	1045522	1780216	73.28%	7.041%
80	16.019	2127	2133	2141	rBV	379402	575424	23.69%	2.276%
81	16.119	2147	2150	2151	rBV3	13552	12573	0.52%	0.050%
82	16.160	2152	2157	2162	rVV	87422	132926	5.47%	0.526%
83	16.348	2185	2189	2192	rBV6	12668	18529	0.76%	0.073%
84	16.401	2195	2198	2200	rVV4	11625	13293	0.55%	0.053%
85	16.466	2207	2209	2211	rBV3	9248	8164	0.34%	0.032%
86	16.630	2235	2237	2238	rBV2	11619	7214	0.30%	0.029%
87	16.736	2253	2255	2256	rBV2	7487	6902	0.28%	0.027%
88	16.759	2257	2259	2261	rVV3	11303	9980	0.41%	0.039%
89	16.924	2285	2287	2288	rBV2	11178	7590	0.31%	0.030%
90	17.423	2370	2372	2373	rBV	11098	7089	0.29%	0.028%
91	17.470	2375	2380	2384	rVV5	30513	50135	2.06%	0.198%
92	17.682	2407	2416	2423	rBV	1289595	2063348	84.93%	8.161%
93	17.782	2426	2433	2441	rVB	1299973	2006387	82.59%	7.936%
94	18.405	2537	2539	2544	rBV6	11365	20163	0.83%	0.080%
95	18.499	2551	2555	2560	rBV3	120026	158071	6.51%	0.625%
96	19.762	2767	2770	2774	rBV4	72782	97286	4.00%	0.385%
97	20.050	2813	2819	2825	rBV	1714758	2429461	100.00%	9.609%
98	22.000	3145	3151	3158	rVB	1261996	2184186	89.90%	8.639%
99	25.308	3706	3714	3724	rVB2	757881	2243980	92.37%	8.876%
100	25.555	3749	3756	3767	rVB	747054	2225685	91.61%	8.803%




Sum of corrected areas: 25282395

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
Data File : BG059057.D
Acq On : 14 Sep 2023 2:57
Operator : MA/JU
Sample : 04247-08DL 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJ81DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

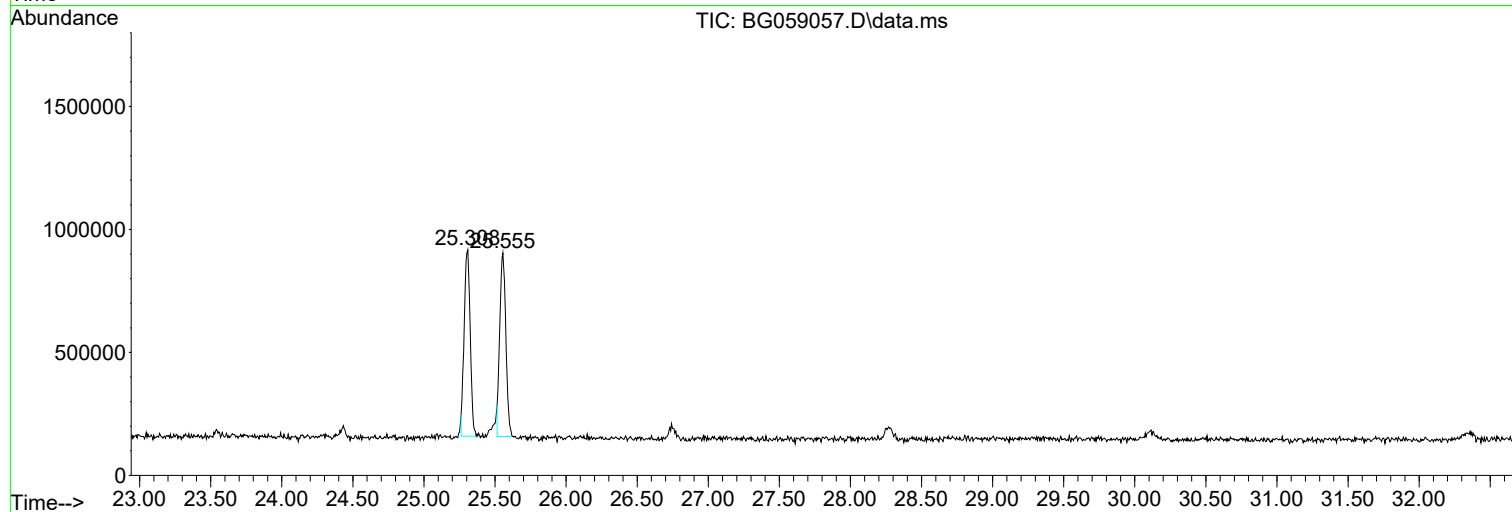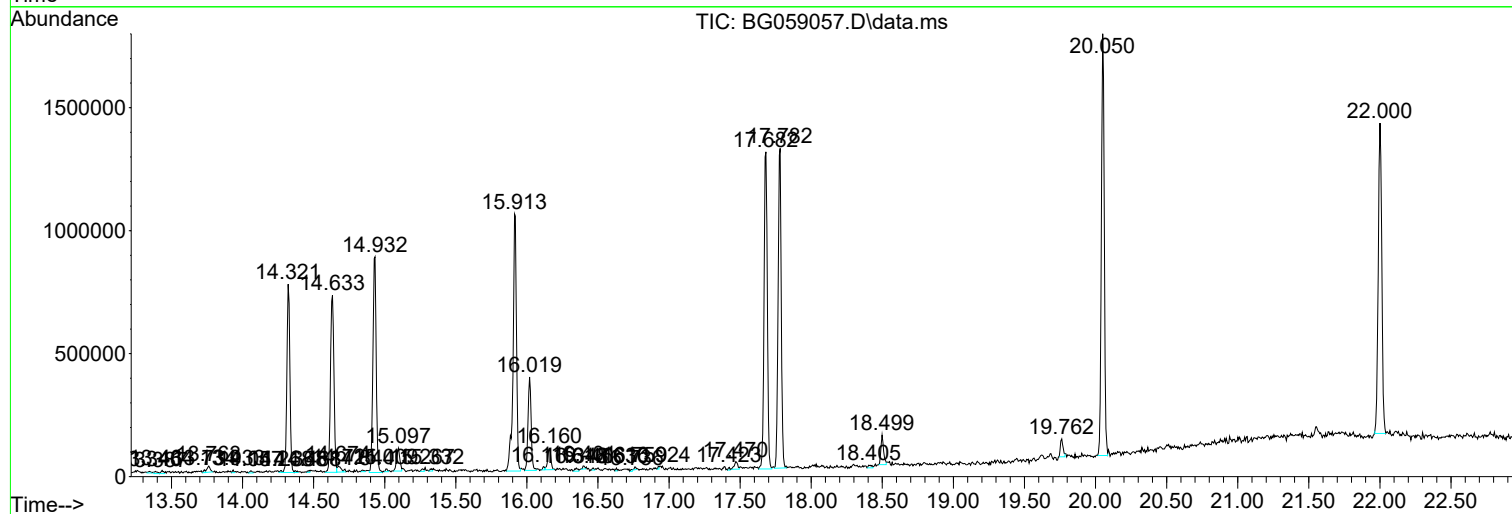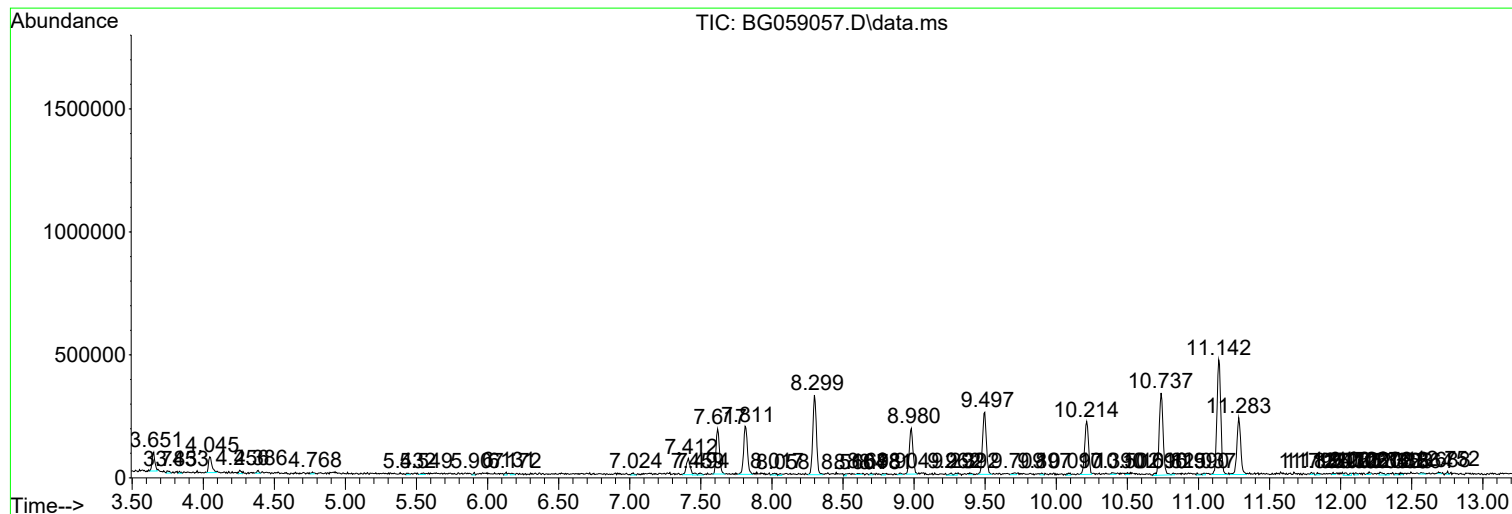

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
Data File : BG059057.D
Acq On : 14 Sep 2023 2:57
Operator : MA/JU
Sample : 04247-08DL 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJ81DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091323\
Data File : BG059057.D
Acq On : 14 Sep 2023 2:57
Operator : MA/JU
Sample : 04247-08DL 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJ81DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc