
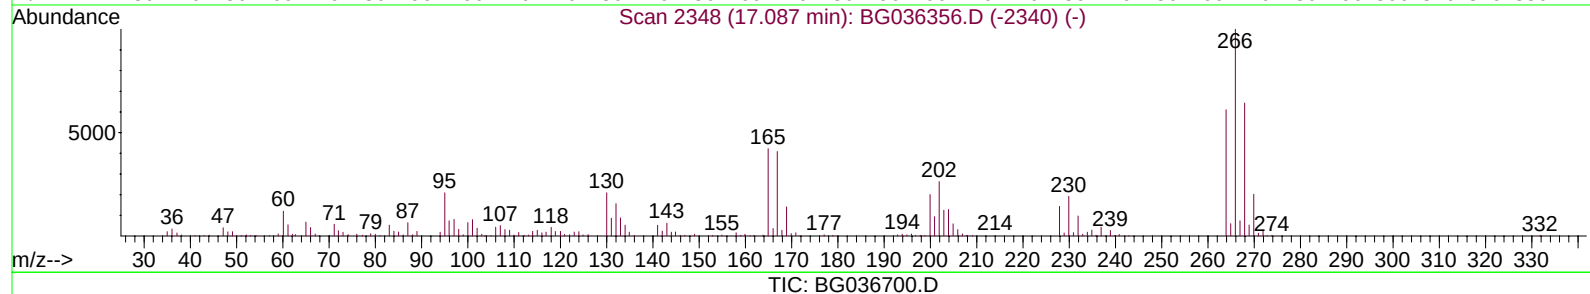
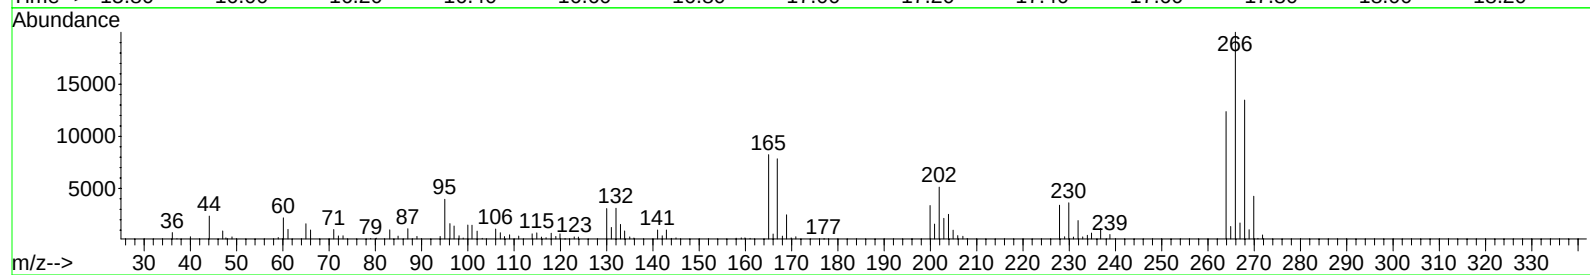


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091418\
Data File : BG036700.D
Acq On : 14 Sep 2018 9:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 13:41:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

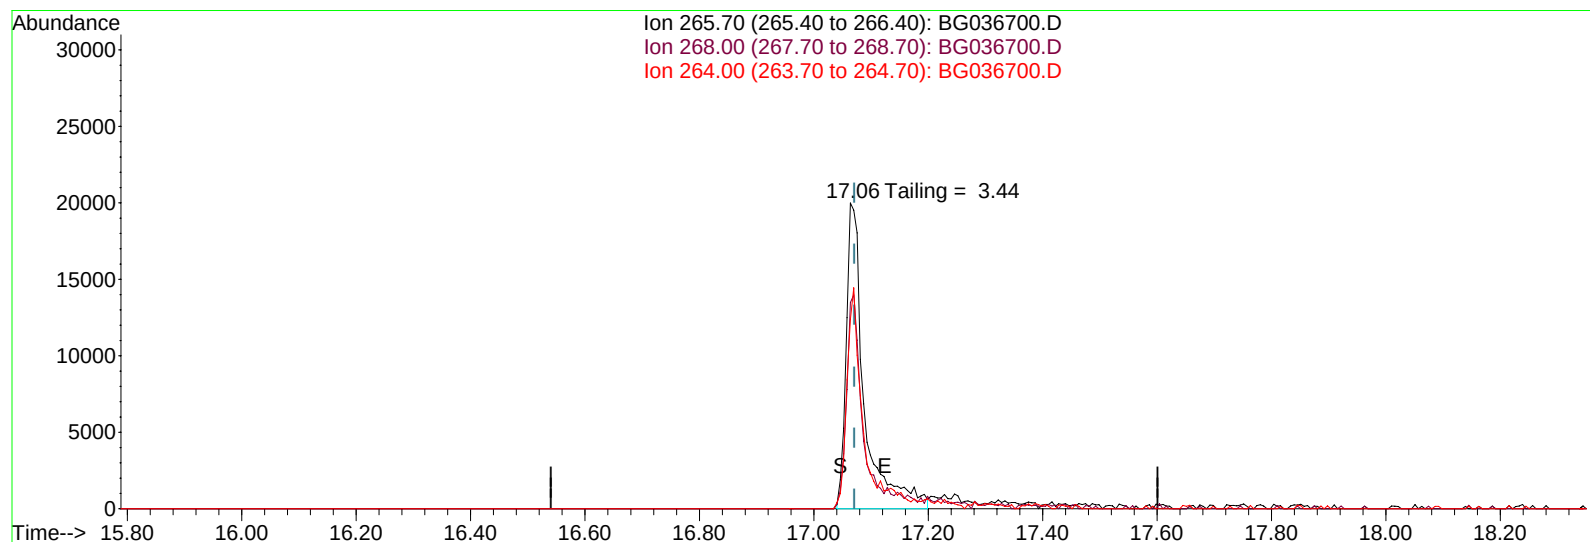

(69) Pentachlorophenol (C)




17.064min (-0.007) 25030.56ng

response 44398

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	67.46
264.00	61.10	61.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091418\
 Data File : BG036700.D
 Acq On : 14 Sep 2018 9:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 13:41:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 31 13:03:20 2018
 Response via : Initial Calibration

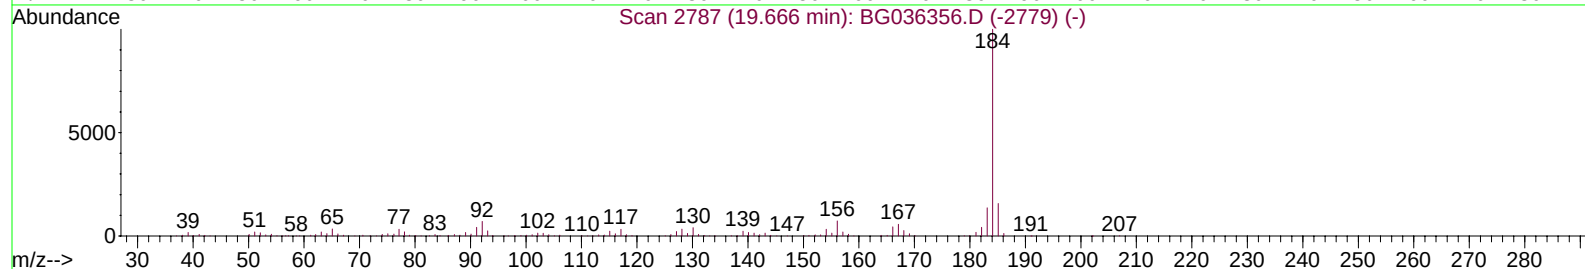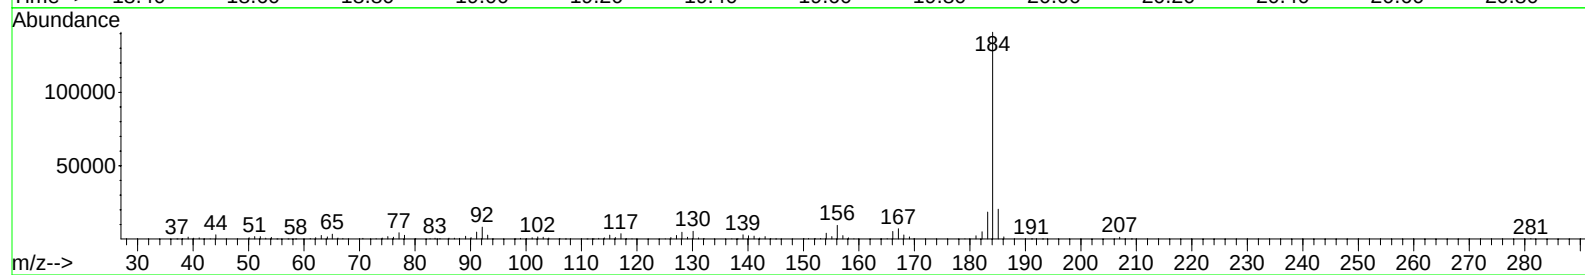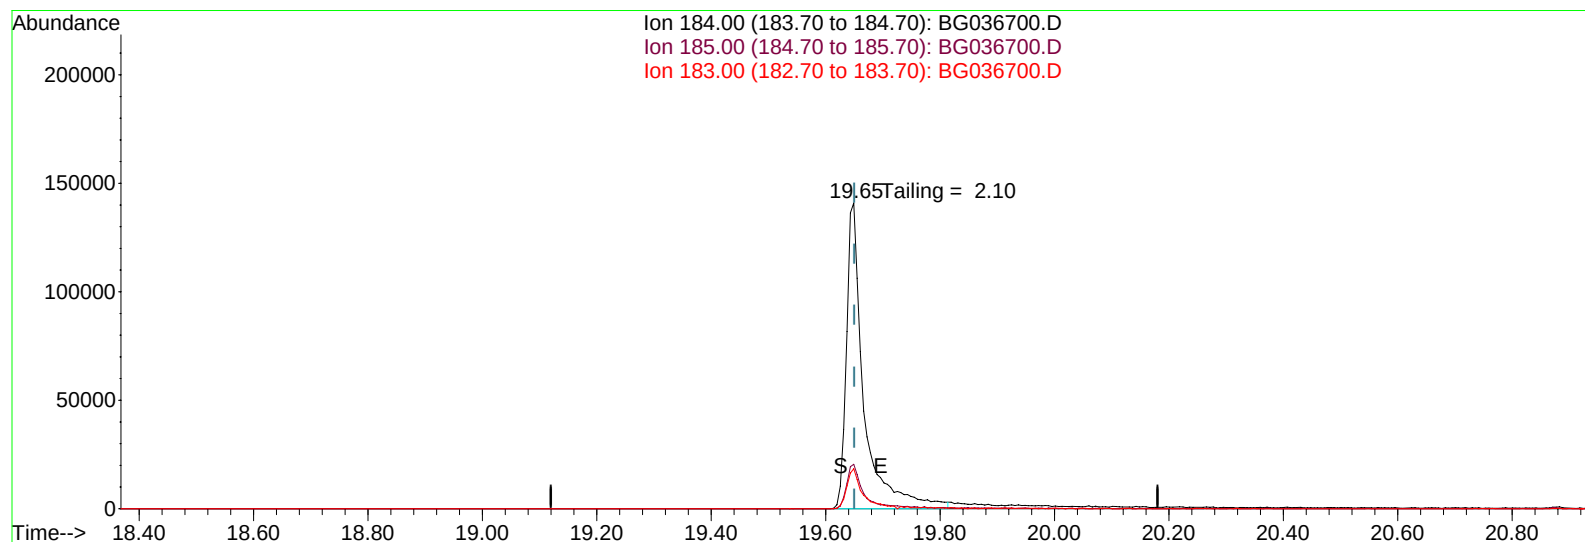

TIC: BG036700.D

(76) Benzidine

19.649min (-0.001) 37557.65ng

response 307952

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.53
183.00	13.60	13.09
0.00	0.00	0.00