
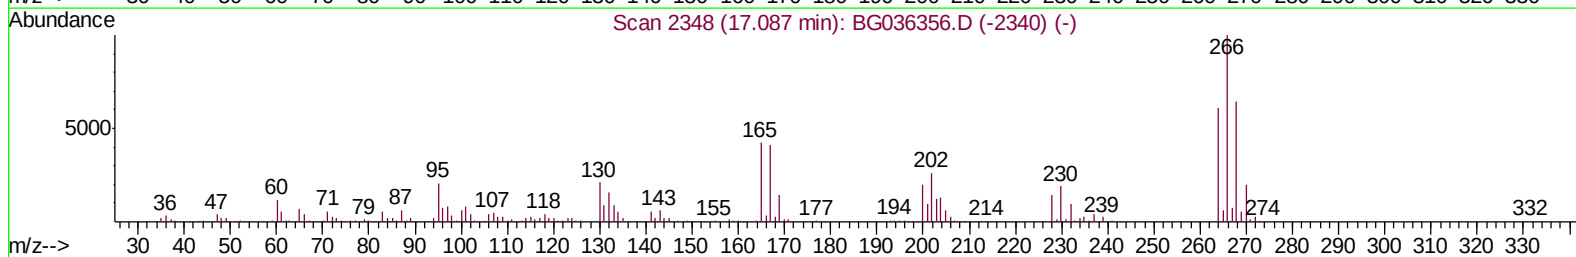
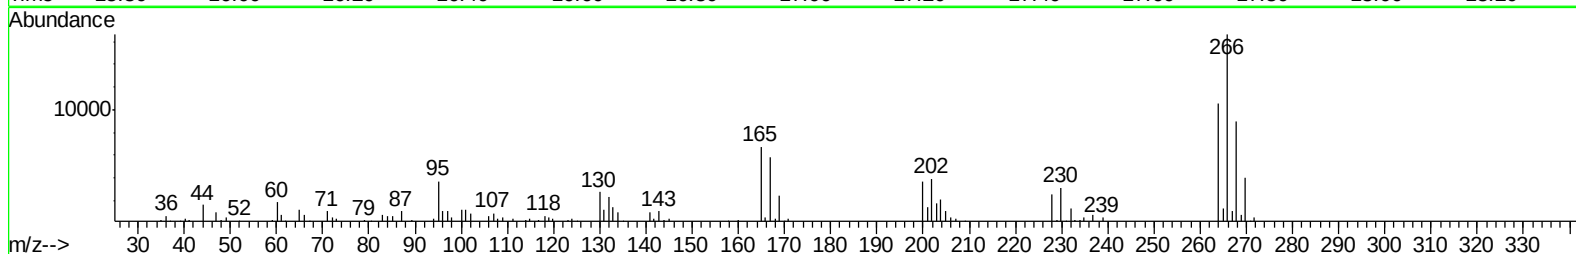


Data File : BG036709.D
Acq On : 14 Sep 2018 17:24
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 05:39:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

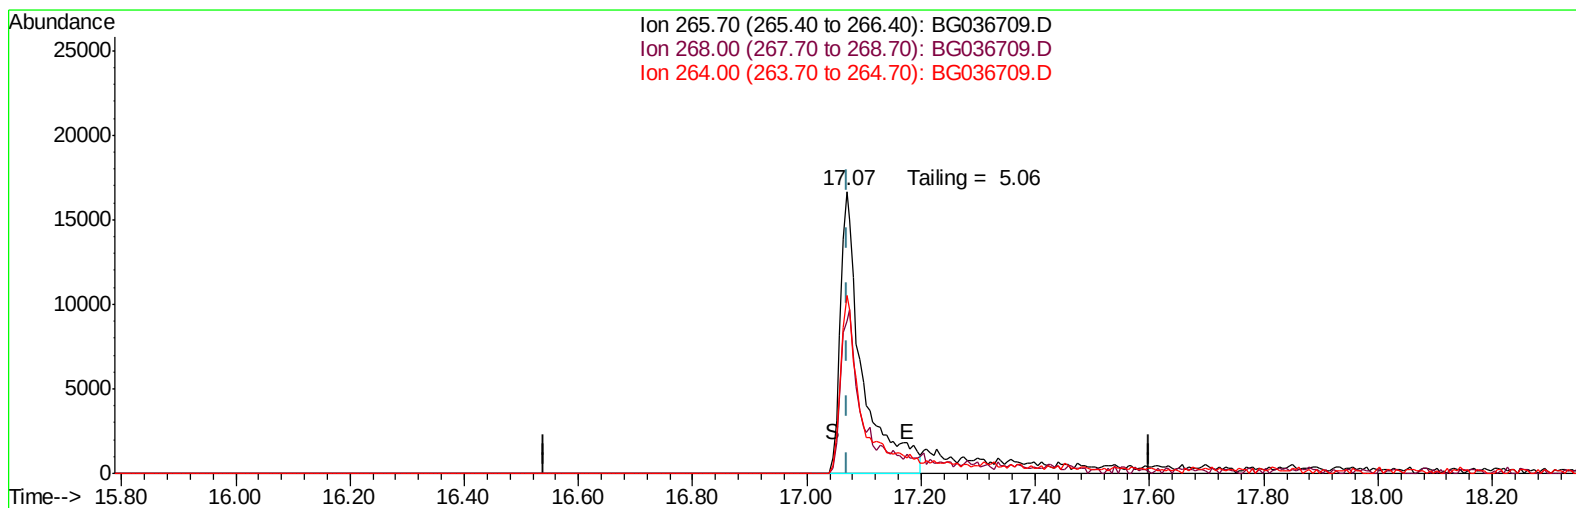

TIC: BG036709.D

(69) Pentachlorophenol (C)




17.069min (-0.002) 4116.50ng

response 40561

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	54.10
264.00	61.10	63.16
0.00	0.00	0.00

Data File : BG036709.D
Acq On : 14 Sep 2018 17:24
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 05:39:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

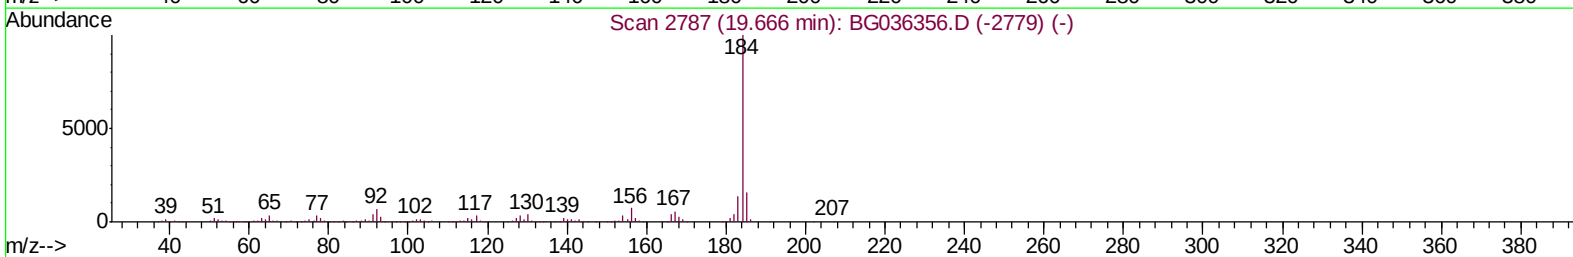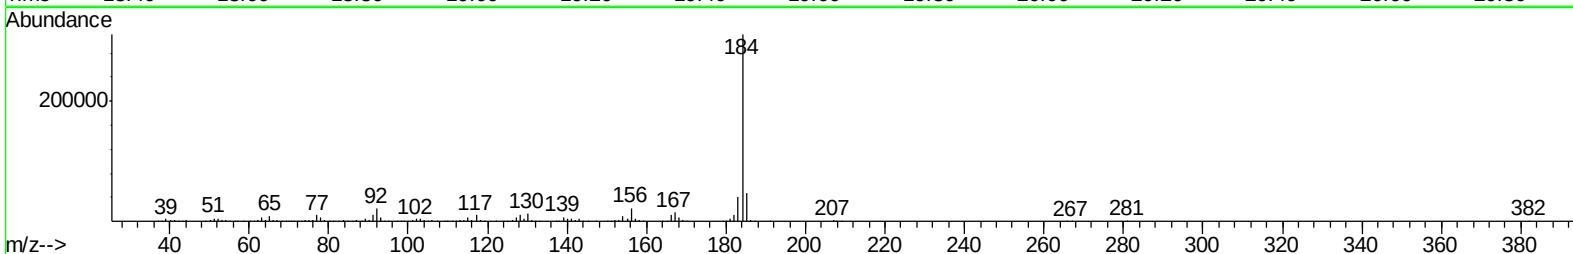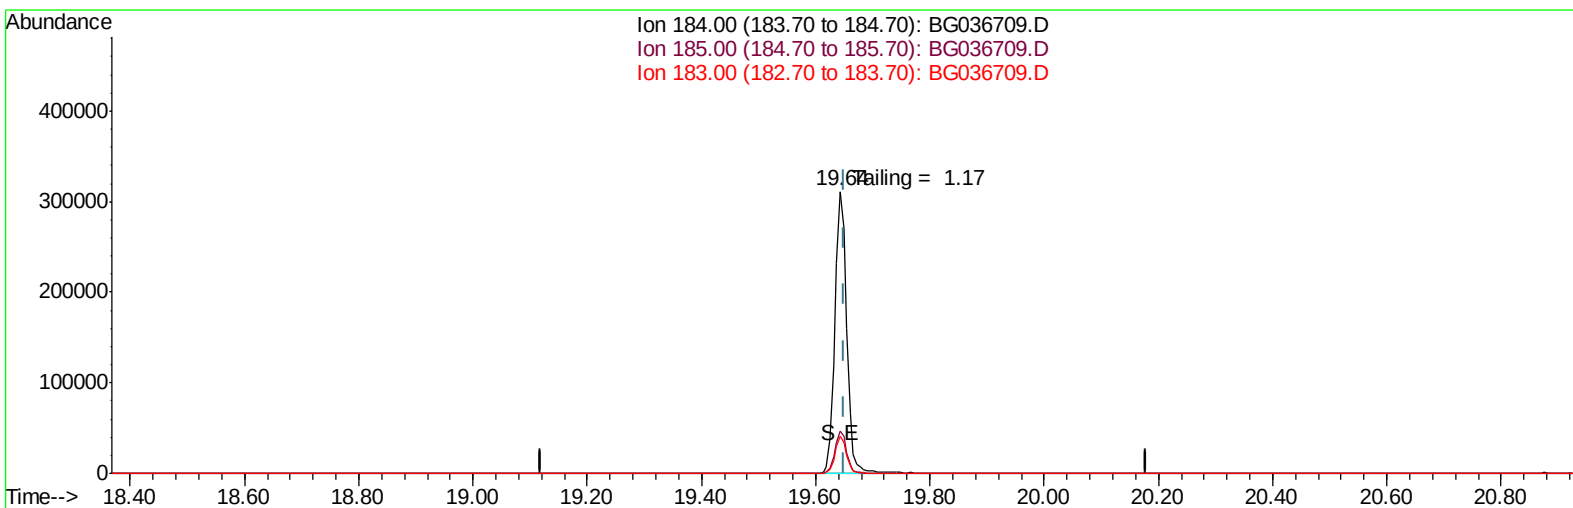

TIC: BG036709.D

(76) Benzidine

19.642min (-0.008) 10441.28ng

response 447718

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.04
183.00	13.60	13.14
0.00	0.00	0.00