

Data File : BG036728.D

Acq On : 15 Sep 2018 6:28

Operator : JU/SJ

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1




Quant Time: Sep 17 05:40:46 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Aug 31 13:03:20 2018

Response via : Initial Calibration

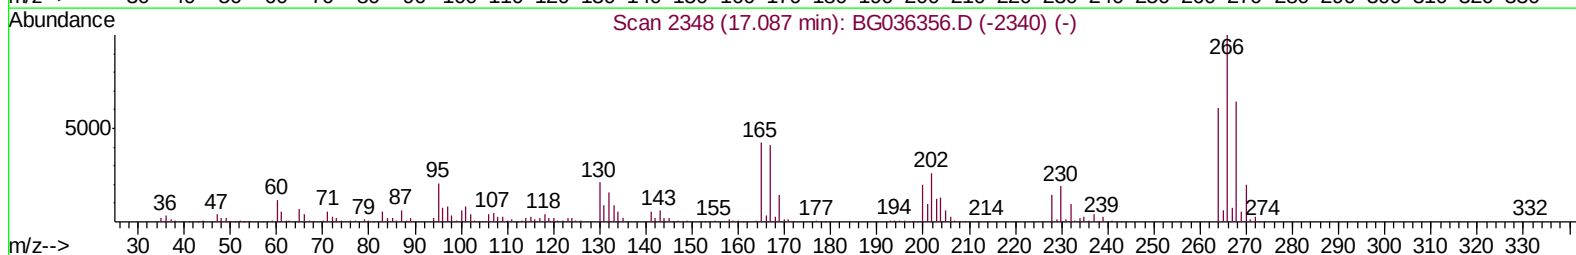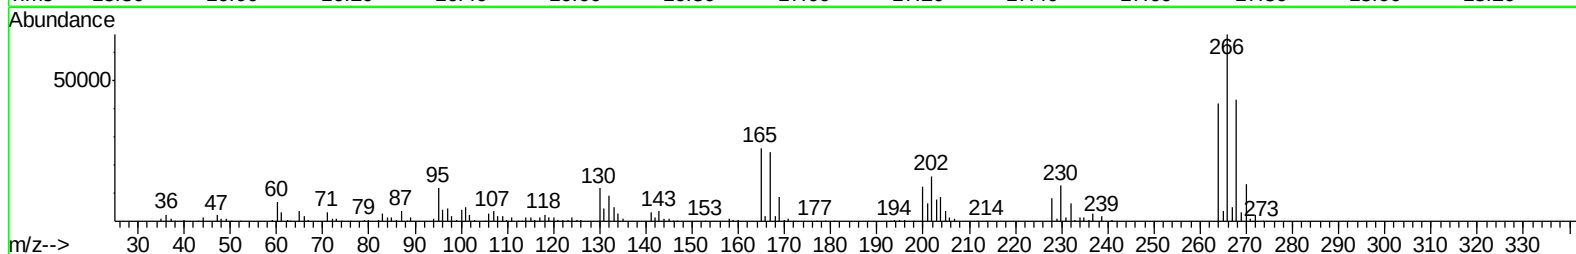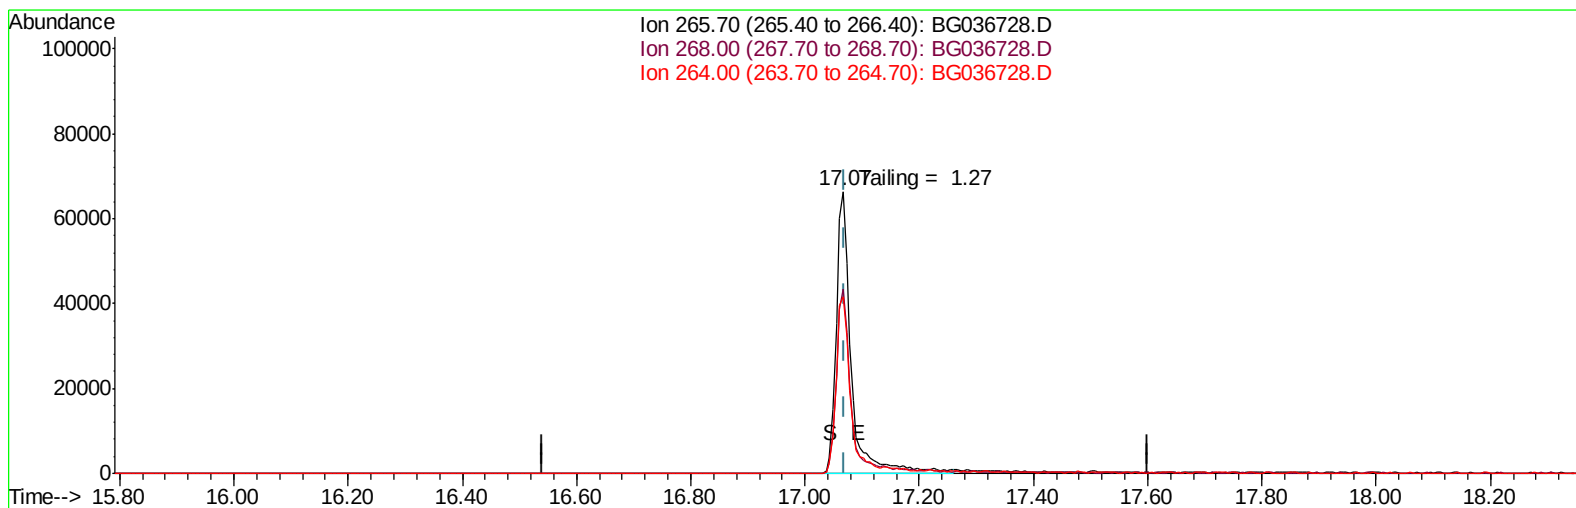

TIC: BG036728.D

(69) Pentachlorophenol (C)




17.067min (-0.004) 11585.36ng

response 117830

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	65.25
264.00	61.10	62.88
0.00	0.00	0.00

Data File : BG036728.D
Acq On : 15 Sep 2018 6:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 05:40:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

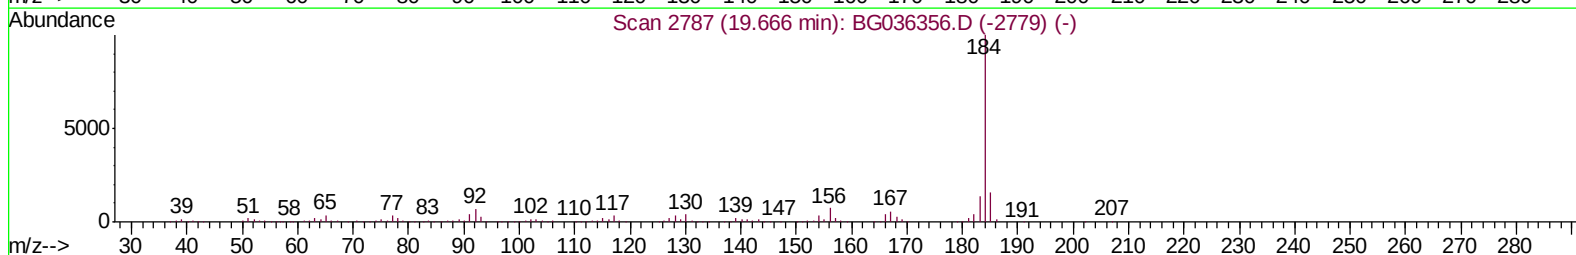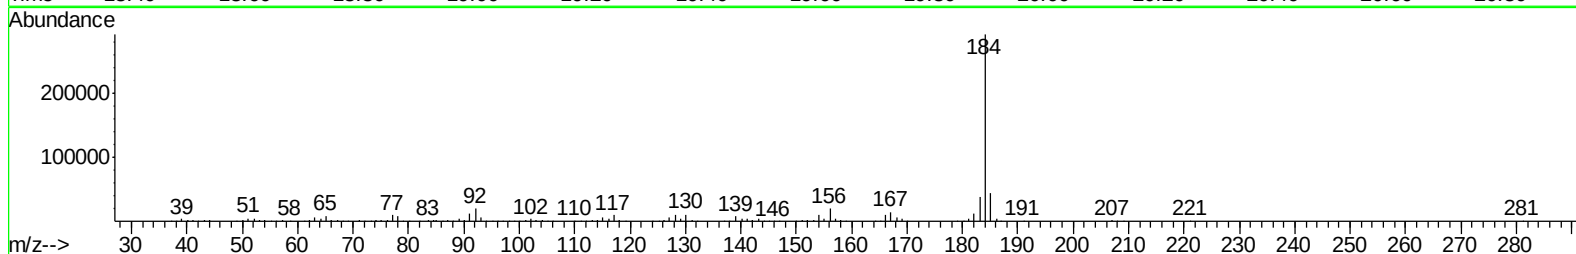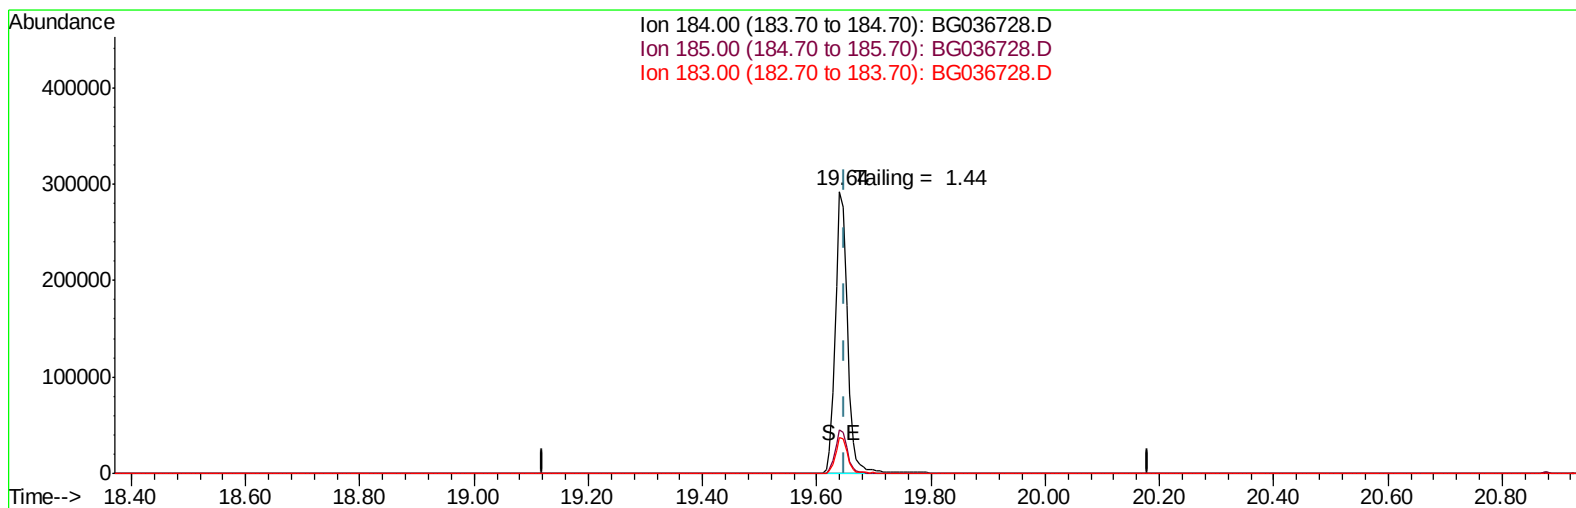

TIC: BG036728.D

(76) Benzidine

19.640min (-0.010) 8774.87ng

response 429175

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.43
183.00	13.60	12.78
0.00	0.00	0.00