

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091418\
 Data File : BG036717.D
 Acq On : 14 Sep 2018 22:37
 Operator : JU/SJ
 Sample : J4892-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C-MW-07-091118

Quant Time: Sep 15 02:47:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 31 13:03:20 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	52251	20.00	ng	-0.01
21) Naphthalene-d8	10.85	136	224784	20.00	ng	-0.01
38) Acenaphthene-d10	14.67	164	158149	20.00	ng	-0.01
63) Phenanthrene-d10	17.42	188	410477	20.00	ng	-0.01
75) Chrysene-d12	21.68	240	399453	20.00	ng	-0.02
86) Perylene-d12	24.89	264	408096	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	156475	47.50	ng	0.00
7) Phenol-d6	7.21	99	137327	29.12	ng	-0.01
23) Nitrobenzene-d5	9.21	82	349557	84.37	ng	-0.01
41) 2,4,6-Tribromophenol	16.16	330	273024	144.68	ng	-0.01
44) 2-Fluorobiphenyl	13.30	172	849270	76.67	ng	-0.01
78) Terphenyl-d14	20.03	244	1483427	86.80	ng	0.00
Target Compounds						
49) Dimethylphthalate	14.12	163	144526	11.192	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091418\
Data File : BG036717.D
Acq On : 14 Sep 2018 22:37
Operator : JU/SJ
Sample : J4892-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C-MW-07-091118

Quant Time: Sep 15 02:47:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

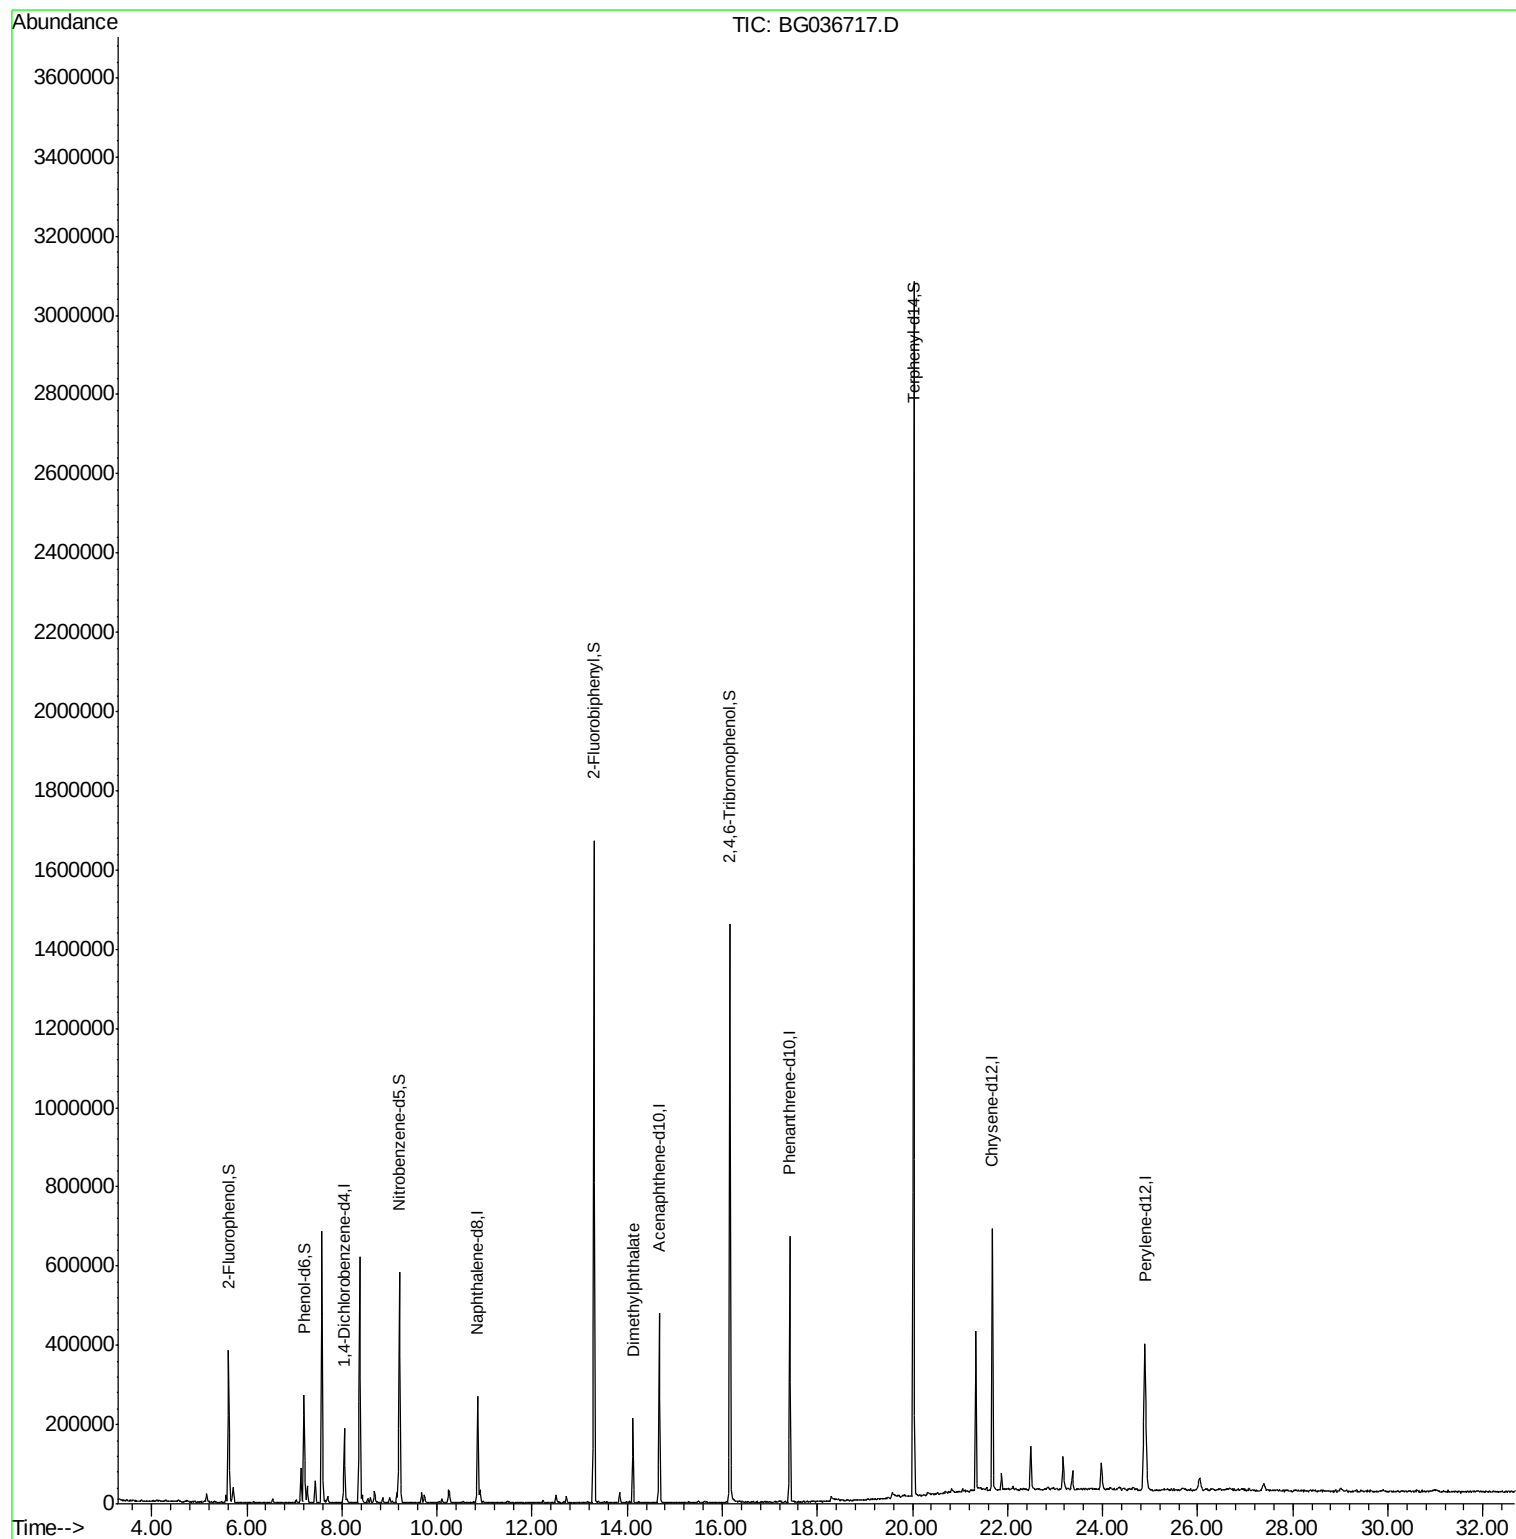

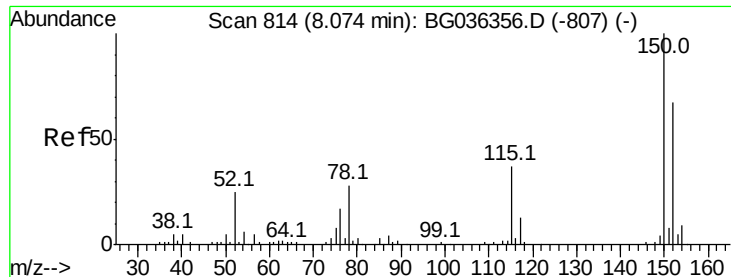


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.05 min Scan# 811
 Delta R.T. -0.01 min
 Lab File: BG036717.D
 Acq: 14 Sep 2018 22:37

Instrument :
 BNA_G
 ClientSampleId :
 C-MW-07-091118

Tot Ion	Ratio	Lower	Upper
152	100		
150	152.1	119.5	179.3
115	59.1	44.5	66.7



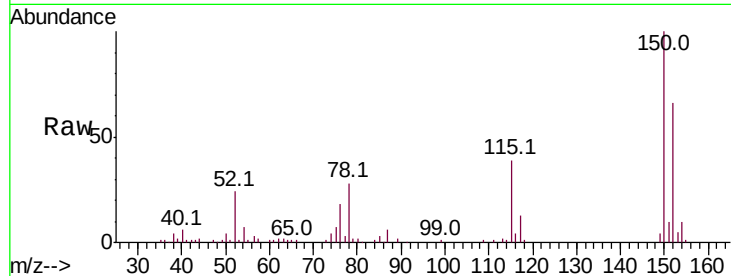


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

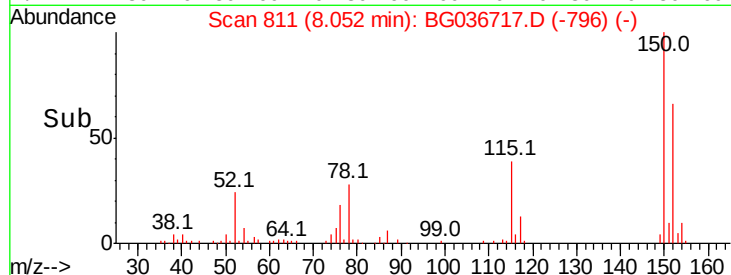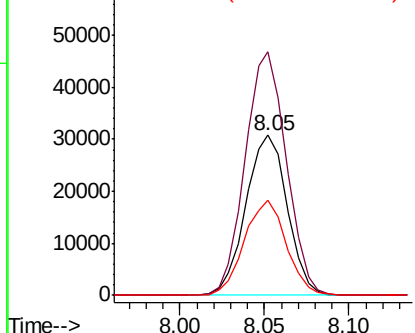

#5

2-Fluorophenol
 Concen: 47.504 ng
 RT: 5.62 min Scan# 397
 Delta R.T. -0.01 min
 Lab File: BG036717.D
 Acq: 14 Sep 2018 22:37

Tgt Ion	Ratio	Lower	Upper
112	100		
64	66.1	57.2	85.8
63	35.6	30.8	46.2






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

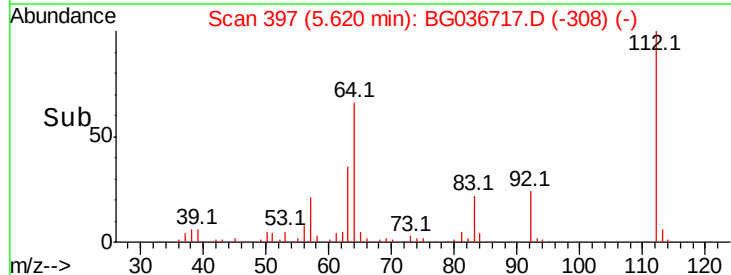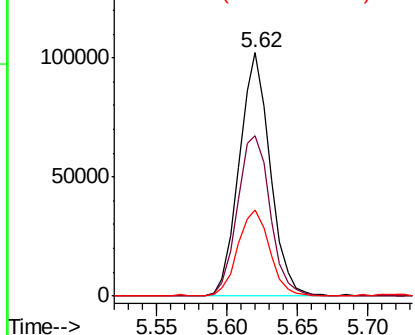

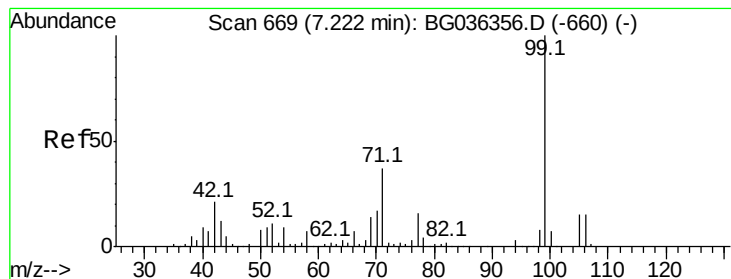

#7

Phenol-d6

Concen: 29.119 ng

RT: 7.21 min Scan# 667

Delta R.T. -0.01 min

Lab File: BG036717.D

Acq: 14 Sep 2018 22:37

Instrument :

BNA_G

ClientSampleId :

C-MW-07-091118


Tot Ion: 99 Resp: 137327

Ion Ratio Lower Upper




99 100

42 19.5 16.5 24.7

71 34.2 29.4 44.2



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

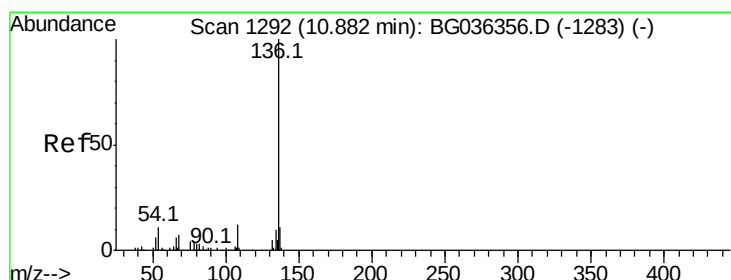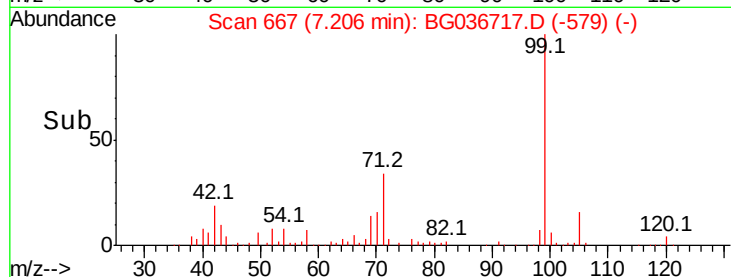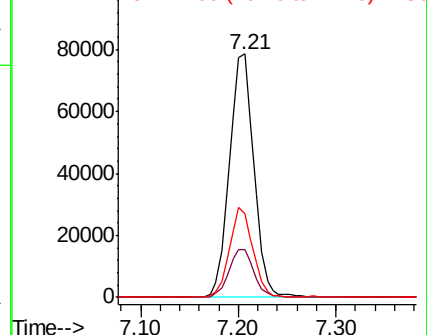

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.85 min Scan# 1288

Delta R.T. -0.01 min

Lab File: BG036717.D

Acq: 14 Sep 2018 22:37

Tgt Ion: 136 Resp: 224784


Ion Ratio Lower Upper

136 100



137 10.8 8.8 13.2


54 10.2 9.2 13.8

68 6.8 5.8 8.6



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

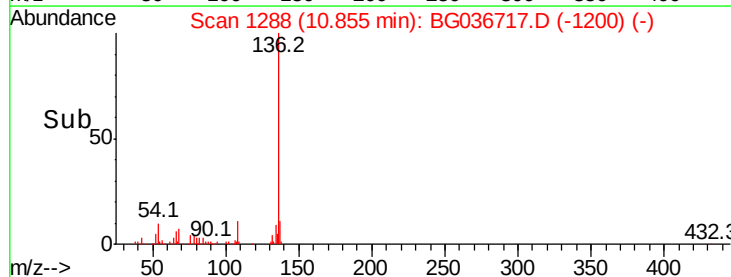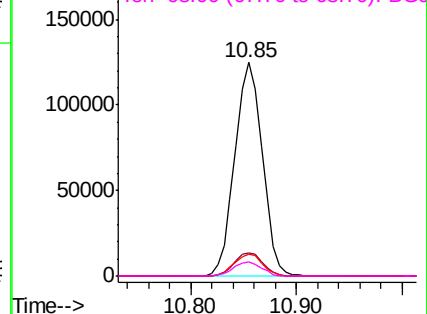

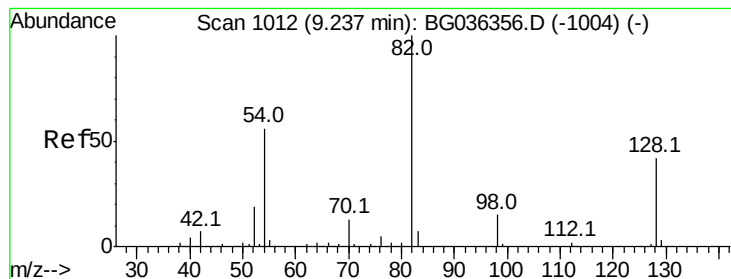

#23

Nitrobenzene-d5

Concen: 84.373 ng

RT: 9.21 min Scan# 1008

Delta R.T. -0.01 min

Lab File: BG036717.D

Acq: 14 Sep 2018 22:37

Instrument :

BNA_G

ClientSampleId :

C-MW-07-091118


Tot Ion: 82 Resp: 349557

Ion Ratio Lower Upper




82 100

128 40.8 33.3 49.9

54 55.5 45.1 67.7



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

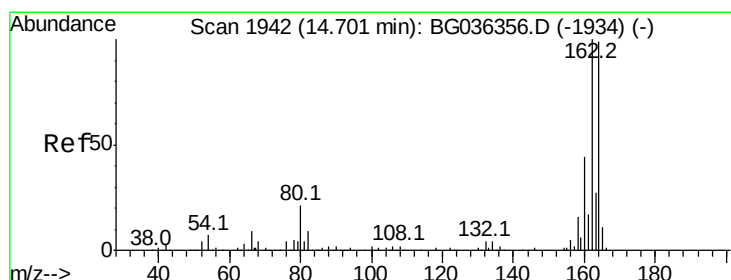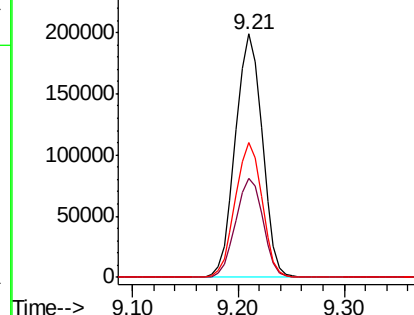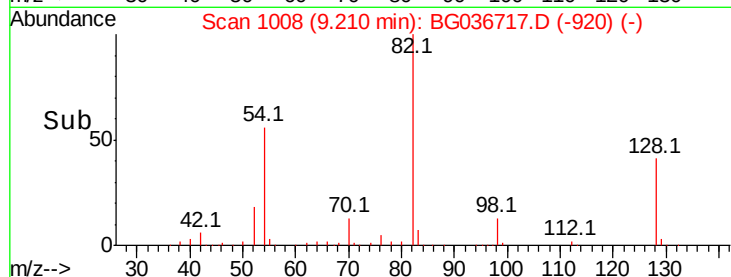

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.67 min Scan# 1938

Delta R.T. -0.01 min

Lab File: BG036717.D

Acq: 14 Sep 2018 22:37


Tgt Ion:164 Resp: 158149

Ion Ratio Lower Upper



164 100


162 103.8 80.7 121.1

160 45.1 35.3 52.9



Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

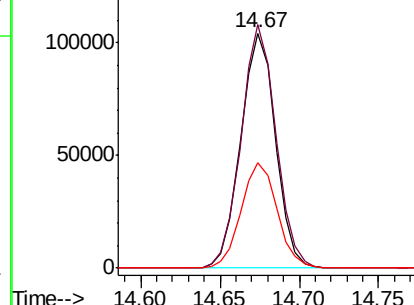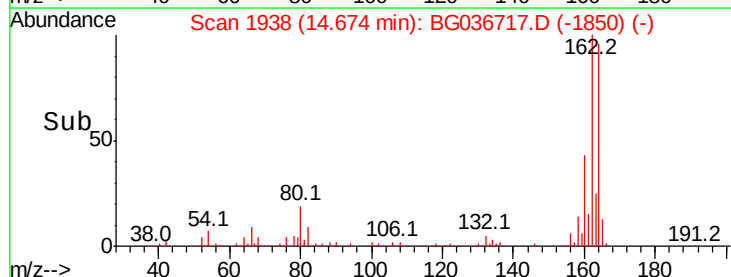


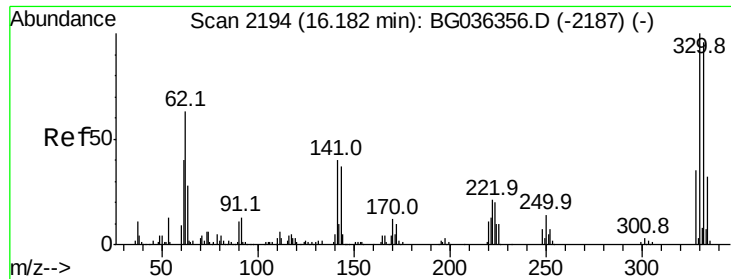




#41
 2,4,6-Tribromophenol
 Concen: 144.681 ng
 RT: 16.16 min Scan# 2191
 Delta R.T. -0.01 min
 Lab File: BG036717.D
 Acq: 14 Sep 2018 22:37

Instrument :
 BNA_G
 ClientSampleId :
 C-MW-07-091118

Tot Ion:330 Resp: 273024
 Ion Ratio Lower Upper
 330 100
 332 97.4 75.4 113.2
 141 36.6 30.7 46.1




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

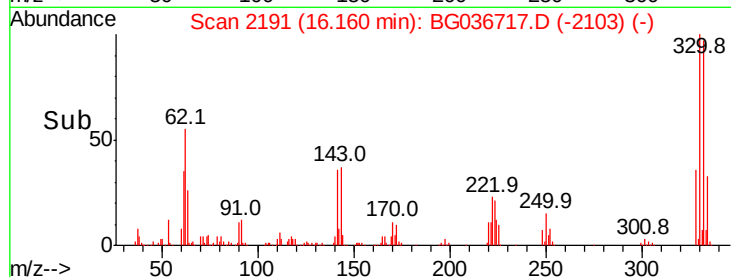
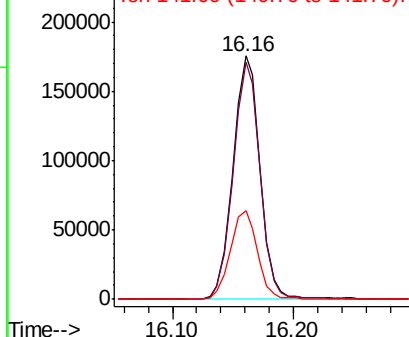



#44
 2-Fluorobiphenyl
 Concen: 76.675 ng
 RT: 13.30 min Scan# 1704
 Delta R.T. -0.01 min
 Lab File: BG036717.D
 Acq: 14 Sep 2018 22:37

Tgt Ion:172 Resp: 849270
 Ion Ratio Lower Upper
 172 100
 171 38.3 31.3 46.9
 170 25.5 21.0 31.6



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



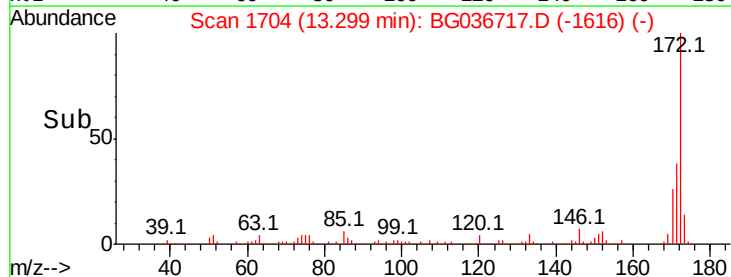
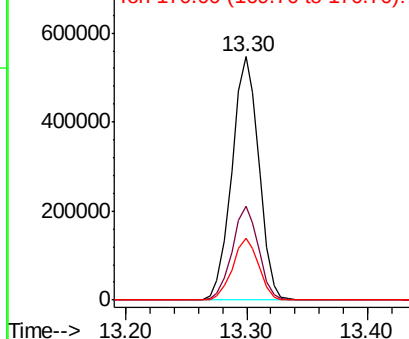


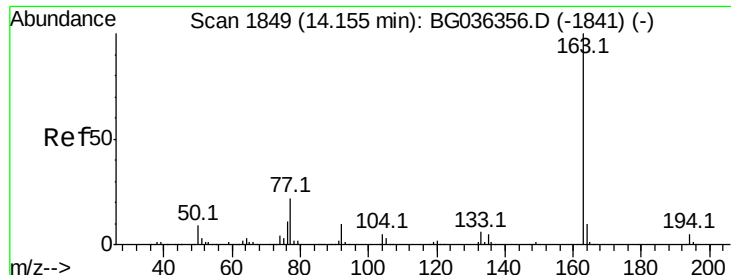

#49
Dimethylphthalate
Concen: 11.192 ng
RT: 14.12 min Scan# 1844
Delta R.T. -0.02 min
Lab File: BG036717.D
Acq: 14 Sep 2018 22:37




Instrument :
BNA_G
ClientSampleId :
C-MW-07-091118


Tot Ion:163 Resp: 144526
Ion Ratio Lower Upper
163 100
194 5.3 4.0 6.0
164 10.7 8.1 12.1

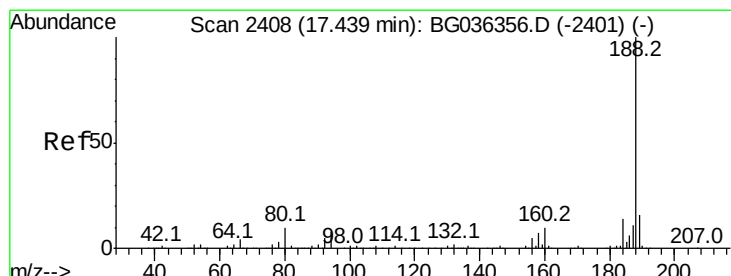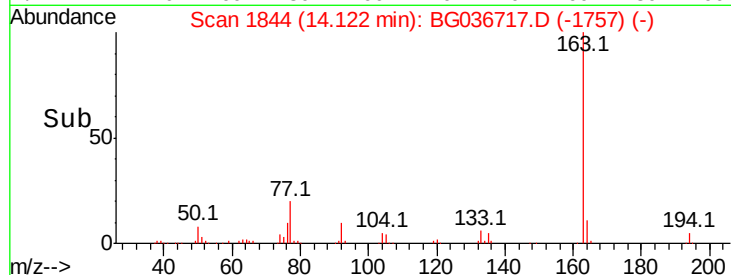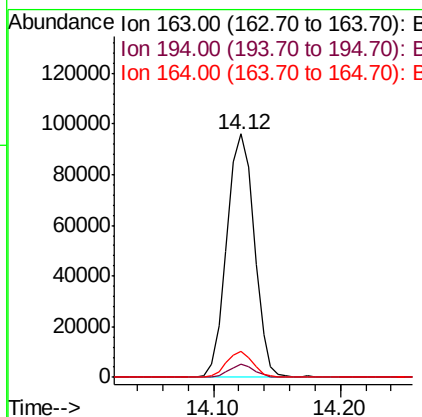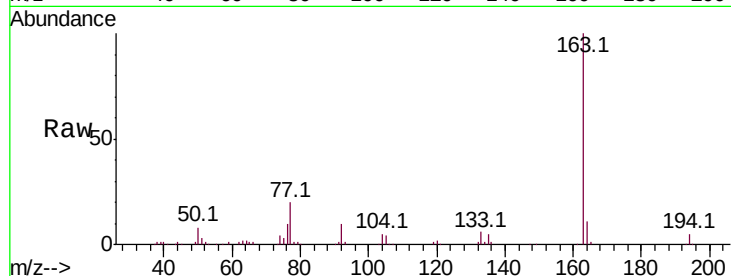

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.42 min Scan# 2405
Delta R.T. -0.01 min
Lab File: BG036717.D
Acq: 14 Sep 2018 22:37

Tgt Ion:188 Resp: 410477
Ion Ratio Lower Upper
188 100
94 7.4 6.7 10.1
80 9.2 8.1 12.1

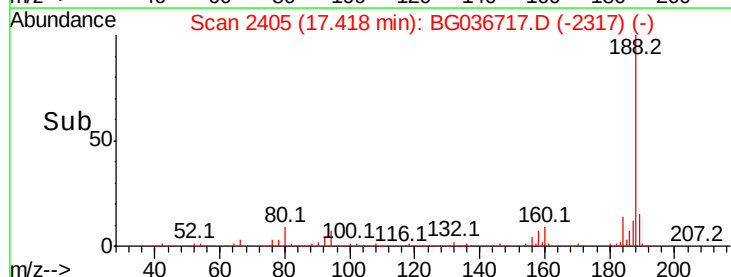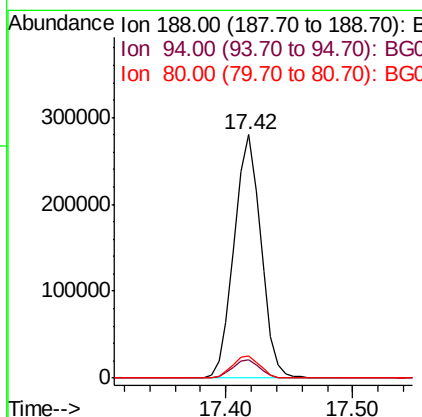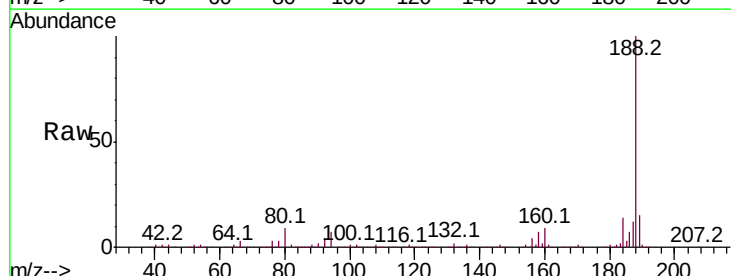

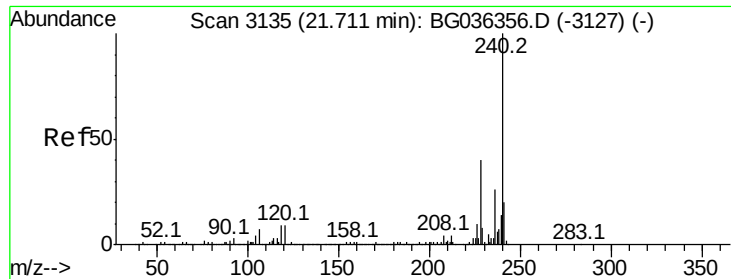

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.68 min Scan# 3130

Delta R.T. -0.02 min

Lab File: BG036717.D

Acq: 14 Sep 2018 22:37

Instrument :

BNA_G

ClientSampleId :

C-MW-07-091118


Tot Ion:240 Resp: 399453

Ion Ratio Lower Upper

240 100

120 7.7 6.9 10.3




236 25.6 21.2 31.8

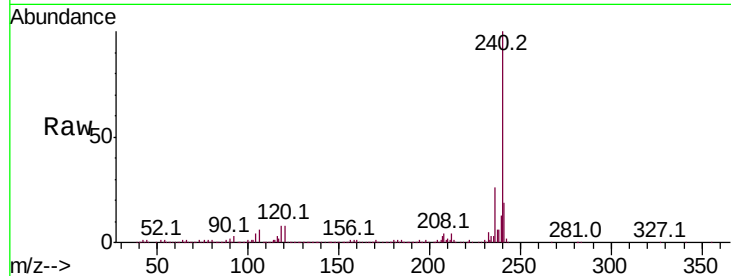

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

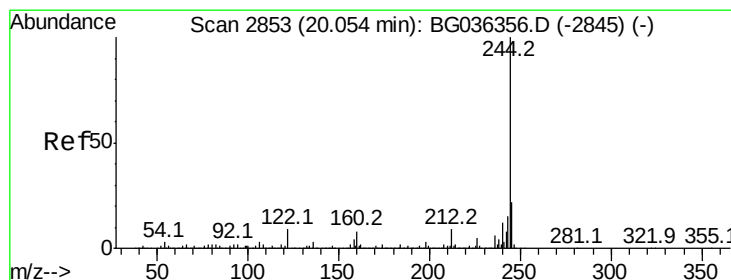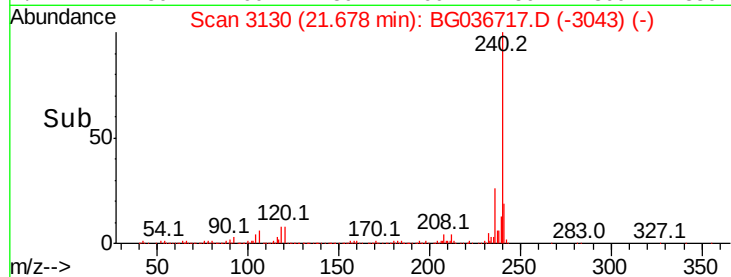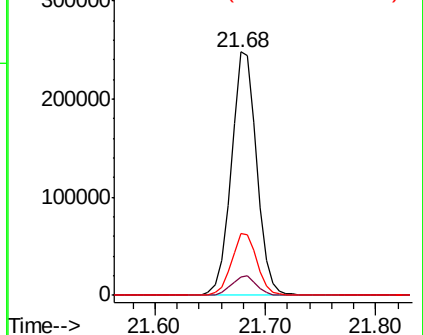

#78

Terphenyl-d14

Concen: 86.801 ng

RT: 20.03 min Scan# 2849

Delta R.T. -0.01 min

Lab File: BG036717.D

Acq: 14 Sep 2018 22:37


Tgt Ion:244 Resp: 1483427

Ion Ratio Lower Upper

244 100

212 8.8 7.0 10.6



122 8.7 7.1 10.7




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

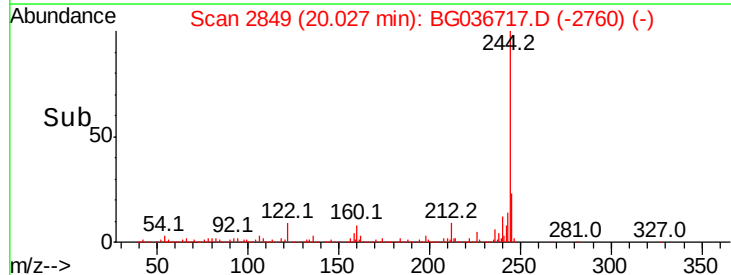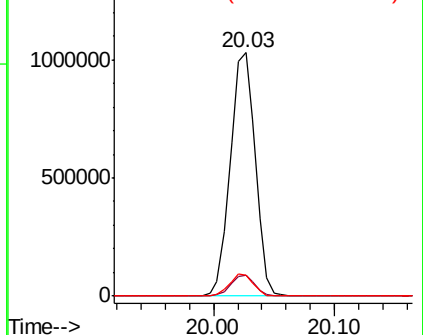

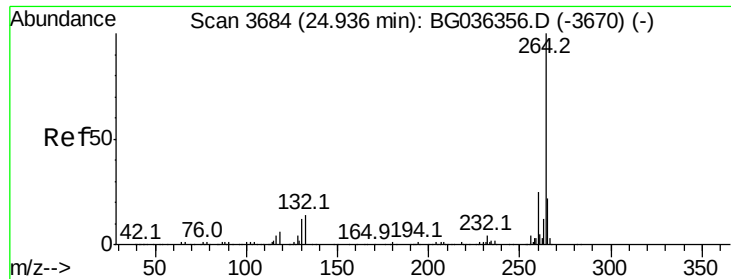

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.89 min Scan# 3676
Delta R.T. -0.02 min
Lab File: BG036717.D
Acq: 14 Sep 2018 22:37

Instrument :
BNA_G
ClientSampleId :
C-MW-07-091118

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.6	19.6	29.4
265	21.3	17.4	26.0

