

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091418\
 Data File : BG036733.D
 Acq On : 15 Sep 2018 9:45
 Operator : JU/SJ
 Sample : J4873-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 NF-CON-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.157	310	318	327	rBV2	162510	259285	6.09%	1.229%
2	5.621	387	397	408	rBV	887222	1397213	32.80%	6.620%
3	7.207	659	667	677	rBV	805534	1383942	32.49%	6.558%
4	7.583	723	731	739	rBV	906117	1568687	36.83%	7.433%
5	8.053	803	811	818	rBV	210288	360732	8.47%	1.709%
6	8.371	858	865	874	rVB	647074	1120922	26.32%	5.311%
7	9.211	1000	1008	1021	rVB	593141	1054448	24.76%	4.996%
8	10.856	1280	1288	1296	rVB	286852	513981	12.07%	2.435%
9	13.294	1695	1703	1712	rBV	1533195	2429711	57.05%	11.513%
10	14.675	1931	1938	1947	rBV2	481044	773747	18.17%	3.666%
11	16.162	2184	2191	2208	rBV	1338443	2129456	50.00%	10.090%
12	17.419	2398	2405	2417	rBV2	693970	1052745	24.72%	4.988%
13	20.022	2842	2848	2856	rBV	3299214	4259273	100.00%	20.182%
14	21.679	3123	3130	3138	rBV2	743868	1204421	28.28%	5.707%
15	22.478	3261	3266	3271	rBV2	33946	52623	1.24%	0.249%
16	23.171	3378	3384	3392	rVB2	51538	94943	2.23%	0.450%
17	23.970	3513	3520	3528	rVB3	51643	117096	2.75%	0.555%
18	24.887	3665	3676	3690	rVB2	407436	1223459	28.72%	5.797%
19	26.038	3865	3872	3877	rVB5	22404	52104	1.22%	0.247%
20	27.378	4094	4100	4111	rVB5	17229	55715	1.31%	0.264%


Sum of corrected areas: 21104503

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091418\
Data File : BG036733.D
Acq On : 15 Sep 2018 9:45
Operator : JU/SJ
Sample : J4873-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
NF-CON-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

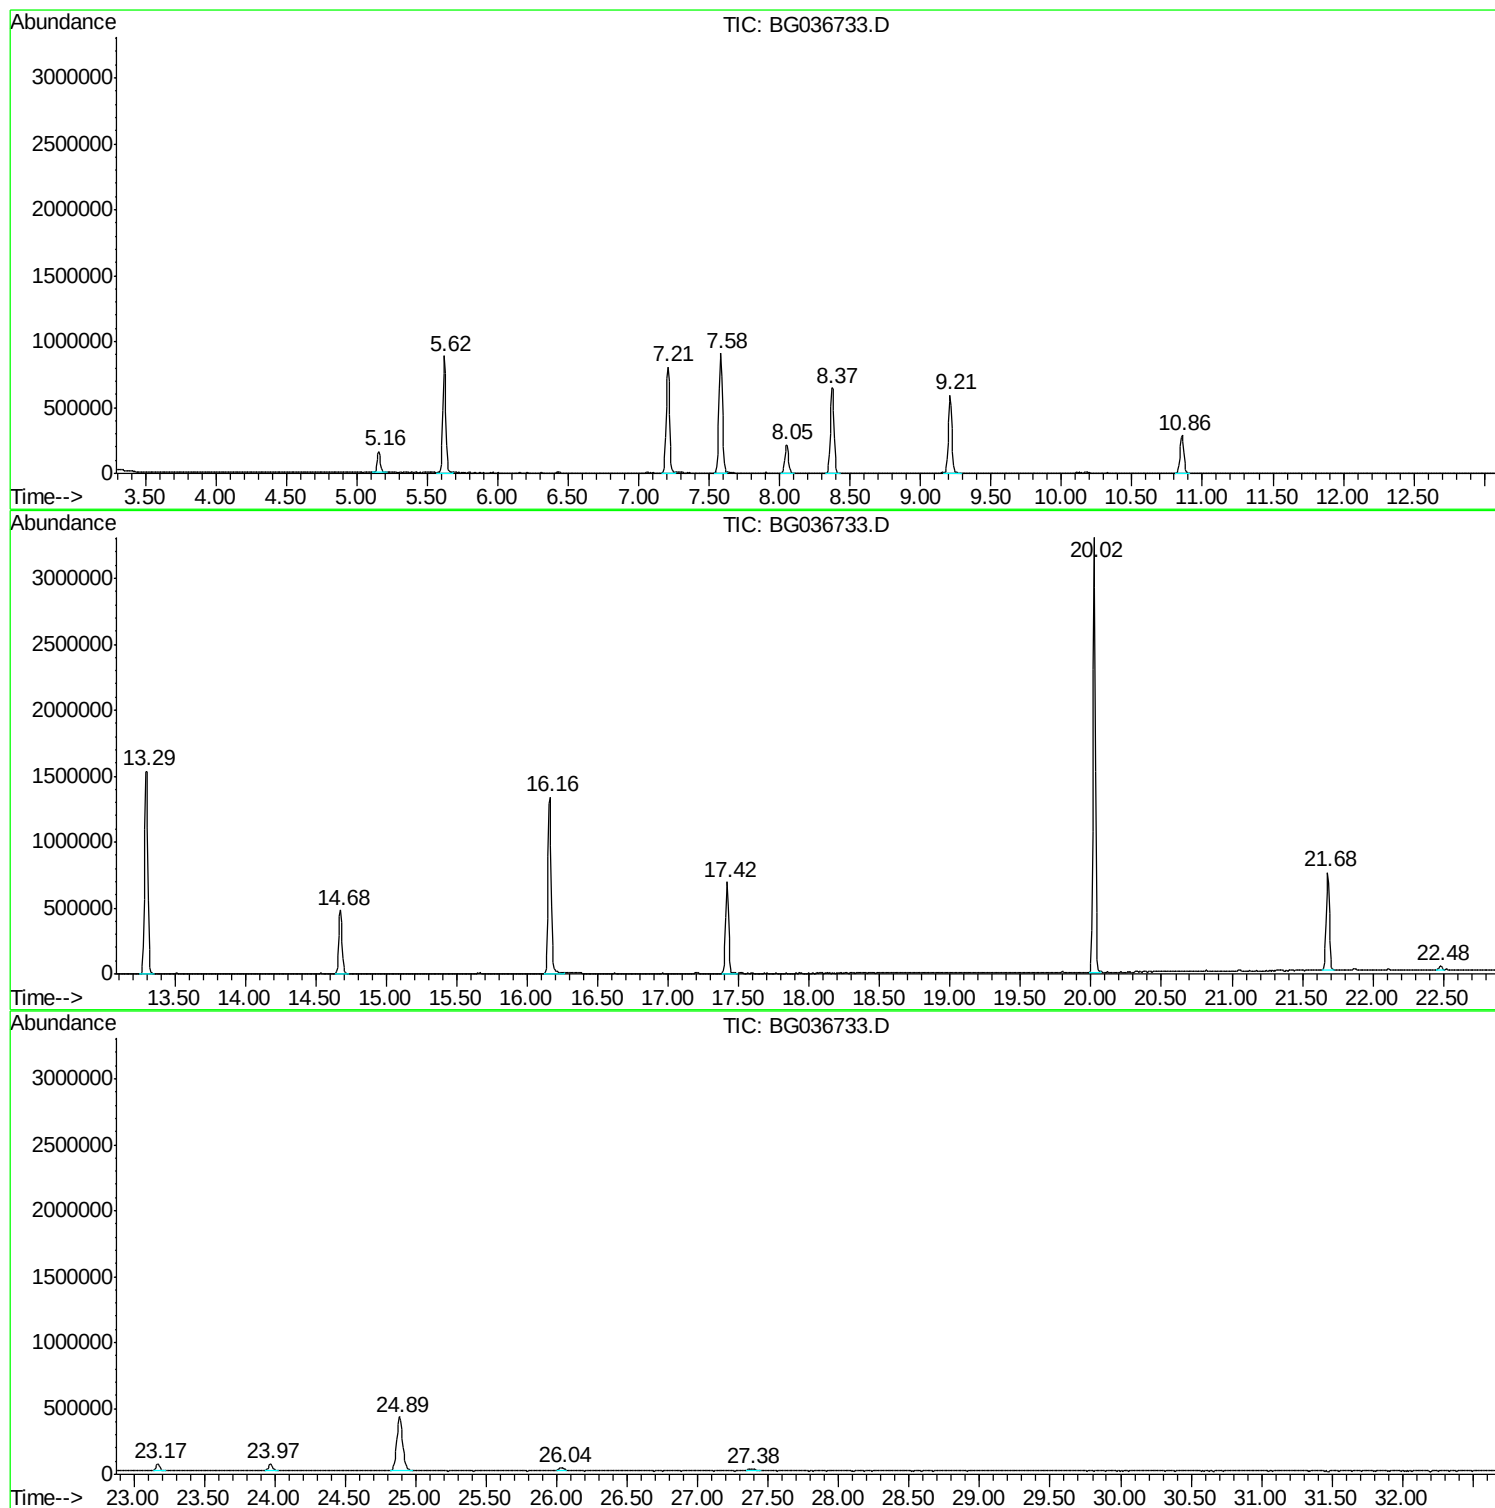

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091418\
Data File : BG036733.D
Acq On : 15 Sep 2018 9:45
Operator : JU/SJ
Sample : J4873-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
NF-CON-1










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.16	14.38 ng	259285	1,4-Dichlorobenzene-d4	8.05

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	40
2		3-Hexanol	102	C6H14O	000623-37-0	38
3		2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	38
4		Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	33
5		3-Pentanol, 2-methyl-	102	C6H14O	000565-67-3	33

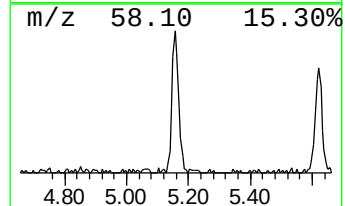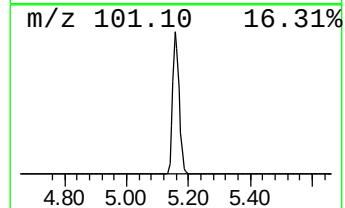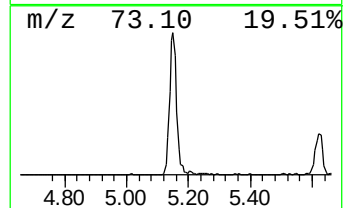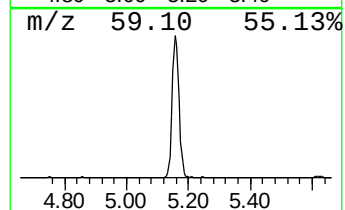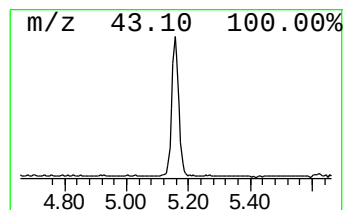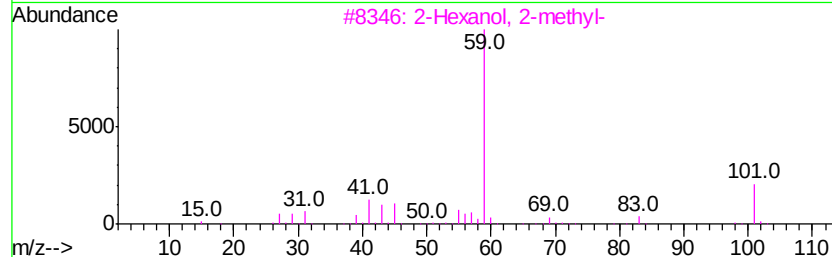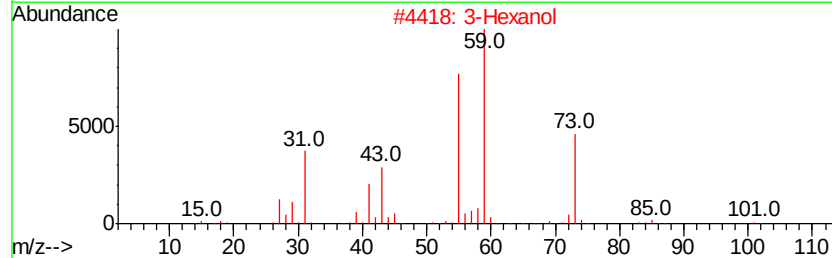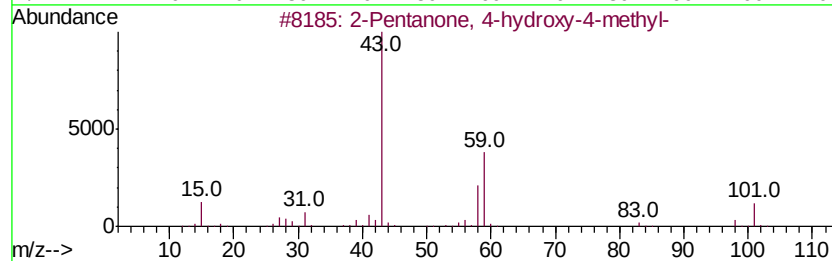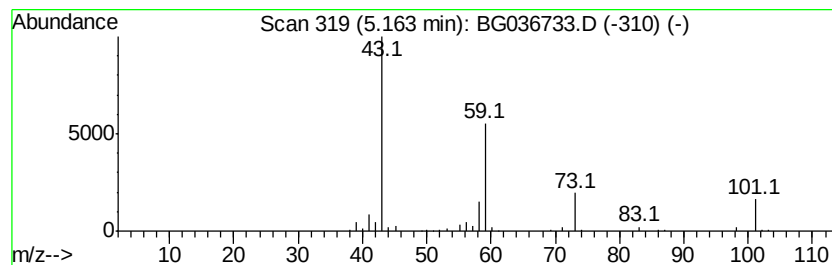

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091418\
Data File : BG036733.D
Acq On : 15 Sep 2018 9:45
Operator : JU/SJ
Sample : J4873-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
NF-CON-1










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.58 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.58	86.97 ng	1568690	1,4-Dichlorobenzene-d4	8.05

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	3	Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2	1H	Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
3	5	Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
4	Tranvl	cypromine-propionyl	189	C12H15NO	1000123-86-3	10
5	(5-Methyl-2-pyridyl)	acetonitrile	132	C8H8N2	1000241-93-9	10

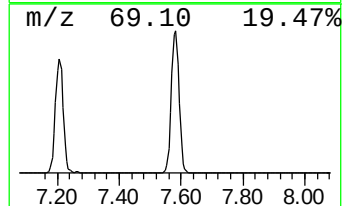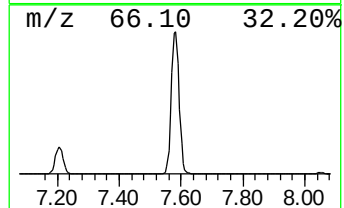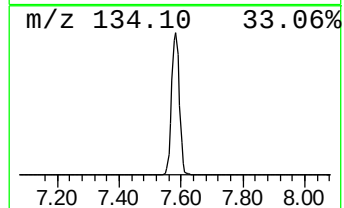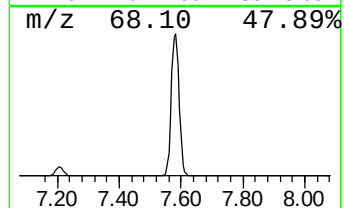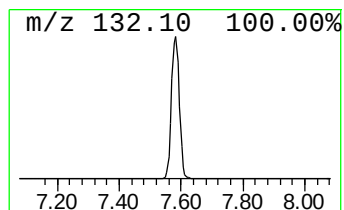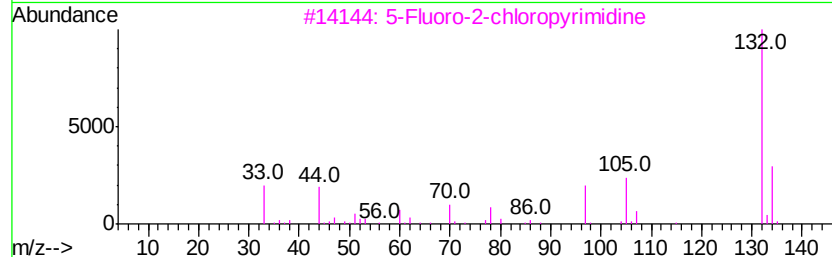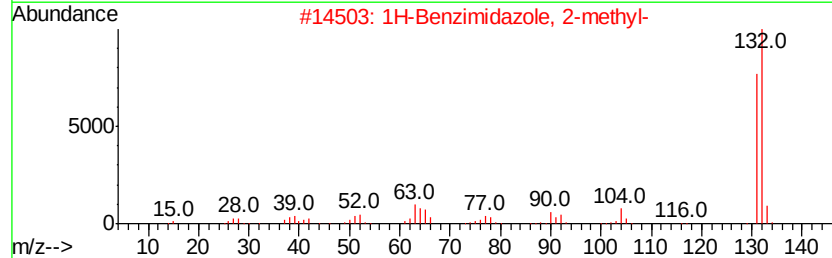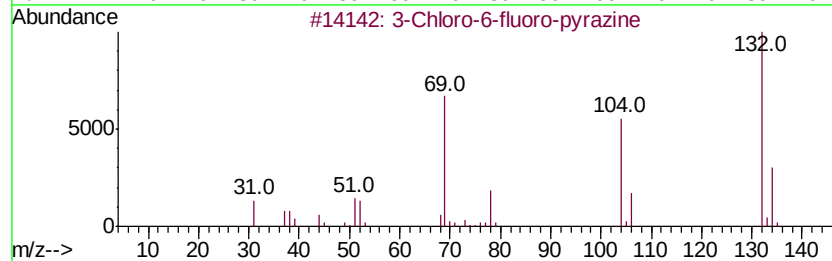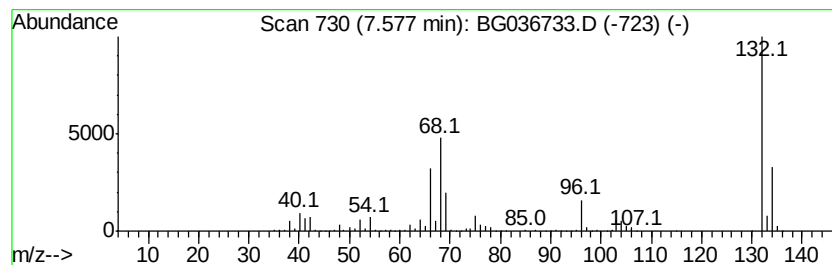

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG091418\
Data File : BG036733.D
Acq On : 15 Sep 2018 9:45
Operator : JU/SJ
Sample : J4873-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
NF-CON-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.16	14.4	ng	259285	1	8.05	360732	20.0
unknown7.58	7.58	87.0	ng	1568690	1	8.05	360732	20.0