


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091418\
 Data File : BG036700.D
 Acq On : 14 Sep 2018 9:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 31 13:03:20 2018

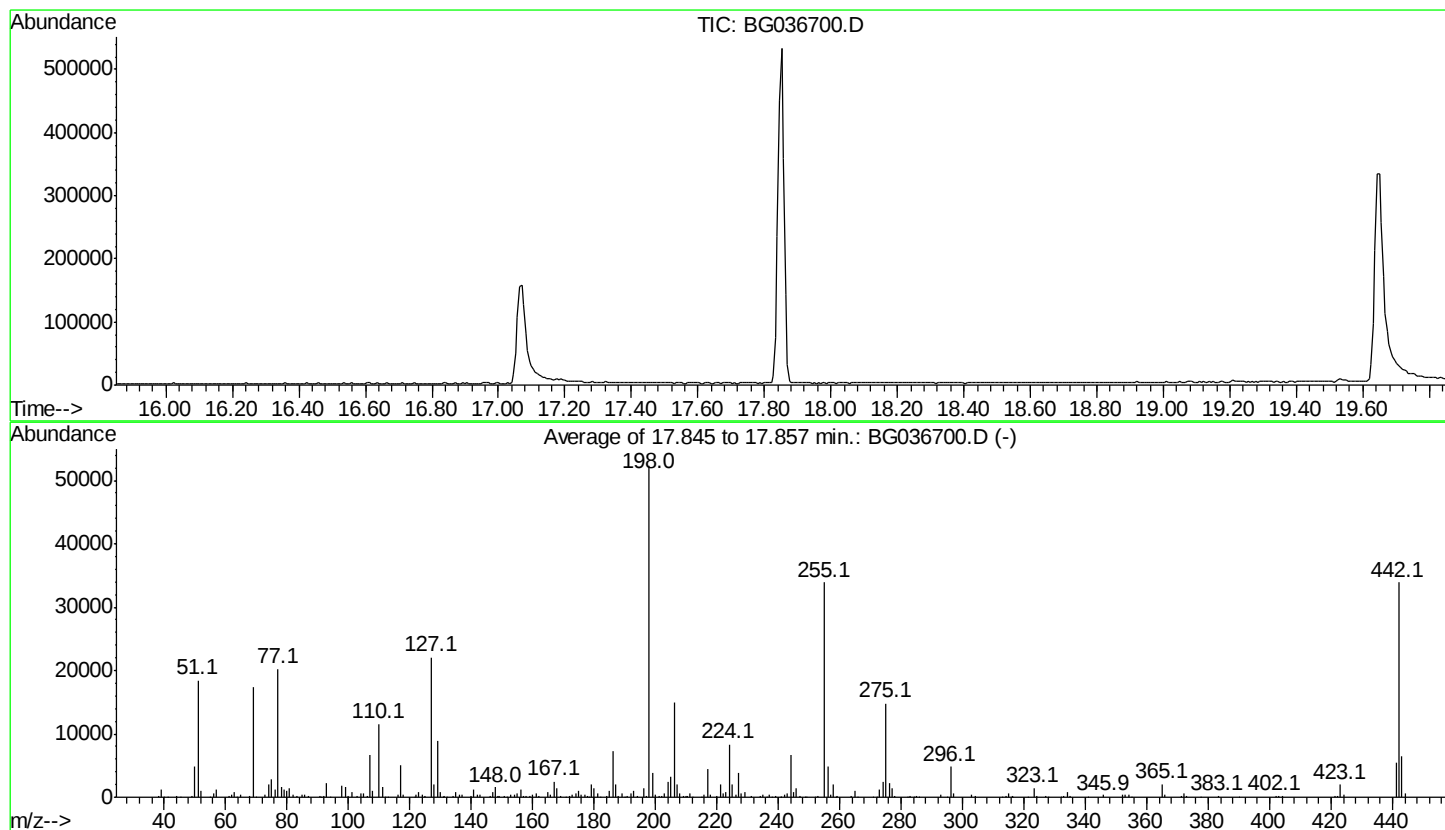

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	18409	PASS
68	69	0.00	2	0.7	122	PASS
69	198	0.00	100	33.4	17479	PASS
70	69	0.00	2	0.4	62	PASS
127	198	10	80	42.3	22115	PASS
197	198	0.00	2	0.4	189	PASS
198	198	100	100	100.0	52330	PASS
199	198	5	9	7.3	3809	PASS
275	198	10	60	28.2	14752	PASS
365	198	1	100	4.1	2126	PASS
441	198	0.01	100	10.3	5395	PASS
442	198	50	100	64.7	33853	PASS
443	442	15	24	18.9	6403	PASS