


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091418\
 Data File : BG036709.D
 Acq On : 14 Sep 2018 17:24
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 31 13:03:20 2018

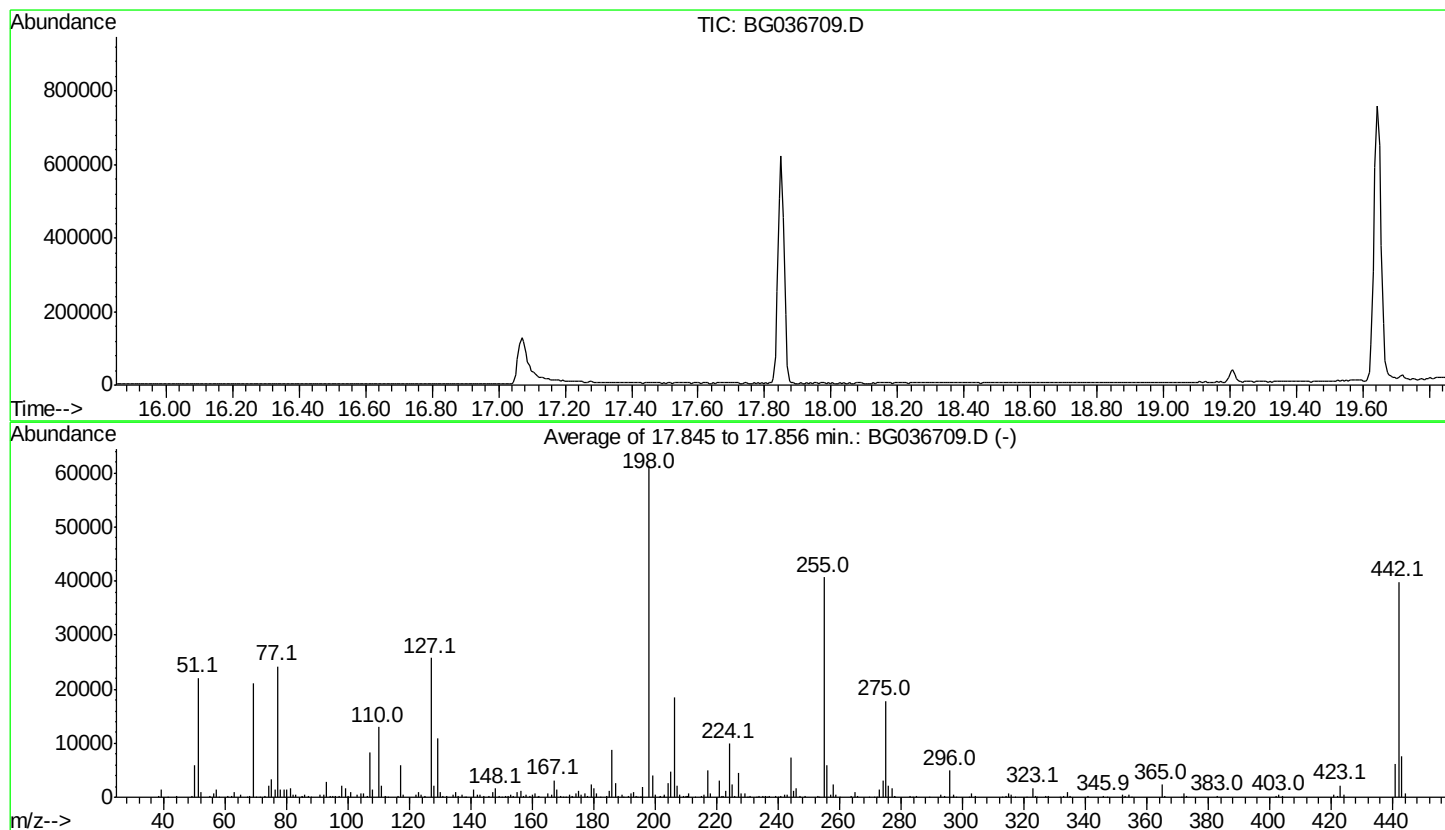

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	22064	PASS
68	69	0.00	2	1.2	257	PASS
69	198	0.00	100	34.2	20992	PASS
70	69	0.00	2	0.3	56	PASS
127	198	10	80	41.9	25733	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61392	PASS
199	198	5	9	6.8	4146	PASS
275	198	10	60	29.1	17858	PASS
365	198	1	100	3.7	2263	PASS
441	198	0.01	100	10.2	6279	PASS
442	198	50	100	64.9	39848	PASS
443	442	15	24	18.9	7520	PASS