

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091422\
 Data File : BG054941.D
 Acq On : 14 Sep 2022 13:16
 Operator : CG/JU
 Sample : N4579-15
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CHERRY-HILL-COMP-14

Quant Time: Sep 15 03:19:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 15 03:14:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.130	152	33245	20.000	ng	0.00
21) Naphthalene-d8	10.962	136	140459	20.000	ng	# 0.00
39) Acenaphthene-d10	14.775	164	109827	20.000	ng	0.00
64) Phenanthrene-d10	17.519	188	264294	20.000	ng	0.00
76) Chrysene-d12	21.814	240	261131	20.000	ng	0.00
86) Perylene-d12	25.187	264	274296	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.674	112	240470	125.957	ng	0.00
7) Phenol-d6	7.290	99	332567	127.376	ng	0.00
23) Nitrobenzene-d5	9.305	82	185524	69.339	ng	0.00
42) 2,4,6-Tribromophenol	16.262	330	185976	135.515	ng	0.00
45) 2-Fluorobiphenyl	13.395	172	508596	69.603	ng	0.00
79) Terphenyl-d14	20.116	244	862018	65.408	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propyla...	9.311	70	23716	13.209	ng	# 74
51) 2,6-Dinitrotoluene	14.775	165	14648	8.464	ng	# 25
57) 2,4-Dinitrotoluene	14.775	165	14648	6.119	ng	# 22
67) 4-Bromophenyl-phenylether	16.262	248	11596	3.996	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091422\
Data File : BG054941.D
Acq On : 14 Sep 2022 13:16
Operator : CG/JU
Sample : N4579-15
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CHERRY-HILL-COMP-14

Quant Time: Sep 15 03:19:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 03:14:10 2022
Response via : Initial Calibration



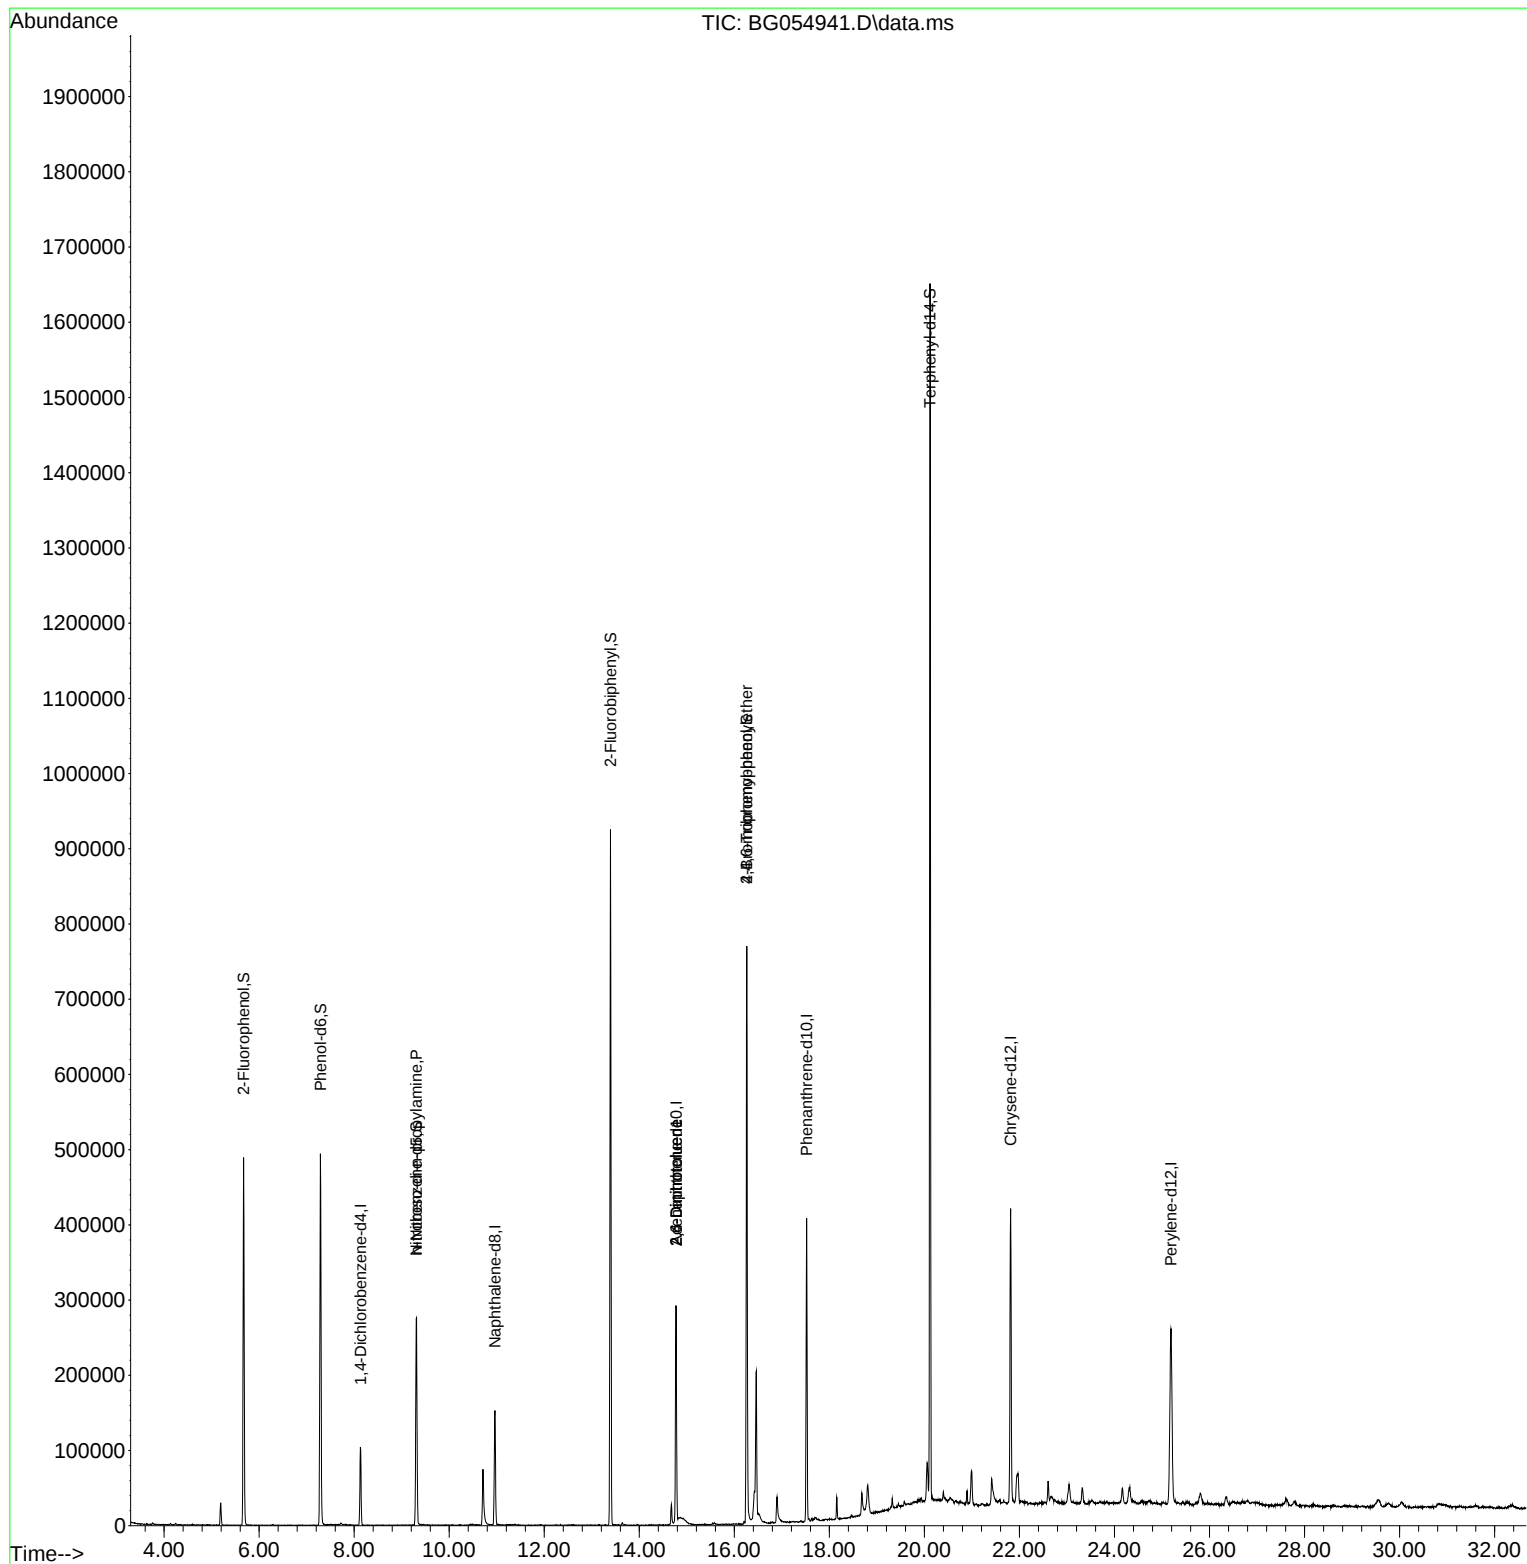




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.130 min Scan# 81
Delta R.T. -0.005 min
Lab File: BG054941.D
Acq: 14 Sep 2022 13:16




Instrument :
BNA_G
ClientSampleId :
CHERRY-HILL-COMP-14

Tgt Ion:152 Resp: 33245
Ion Ratio Lower Upper
152 100
150 153.5 125.2 187.8
115 57.6 47.9 71.9

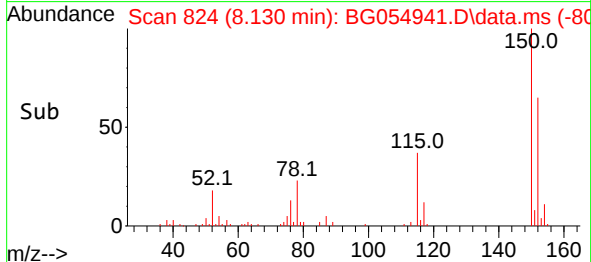

#5
2-Fluorophenol
Concen: 125.957 ng
RT: 5.674 min Scan# 406
Delta R.T. 0.001 min
Lab File: BG054941.D
Acq: 14 Sep 2022 13:16

Tgt Ion:112 Resp: 240470
Ion Ratio Lower Upper
112 100
64 55.2 49.3 73.9
63 28.6 26.3 39.5


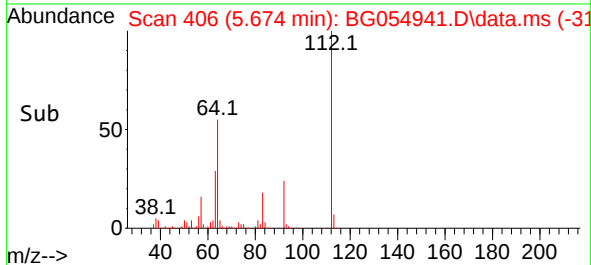

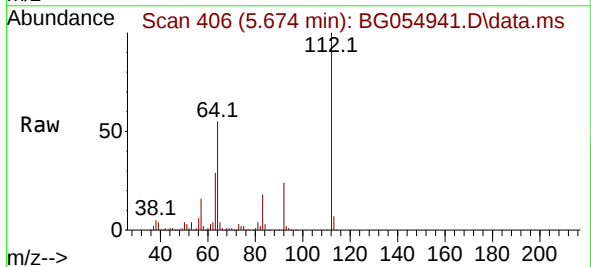




#7
Phenol-d6
Concen: 127.376 ng
RT: 7.290 min Scan# 61
Delta R.T. 0.001 min
Lab File: BG054941.D
Acq: 14 Sep 2022 13:16




Instrument :
BNA_G
ClientSampleId :
CHERRY-HILL-COMP-14

Tgt Ion: 99 Resp: 332567
Ion Ratio Lower Upper
99 100
42 14.6 14.6 22.0#
71 30.0 24.6 37.0

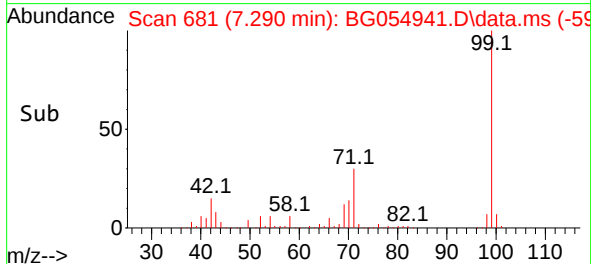

#19
n-Nitroso-di-n-propylamine
Concen: 13.209 ng
RT: 9.311 min Scan# 1025
Delta R.T. 0.371 min
Lab File: BG054941.D
Acq: 14 Sep 2022 13:16

Tgt Ion: 70 Resp: 23716
Ion Ratio Lower Upper
70 100
42 40.3 46.6 69.8#
101 0.0 7.7 11.5#
130 2.7 13.9 20.9#


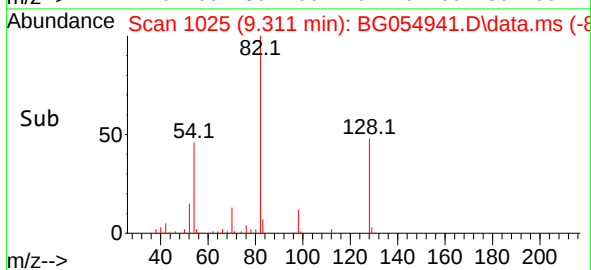

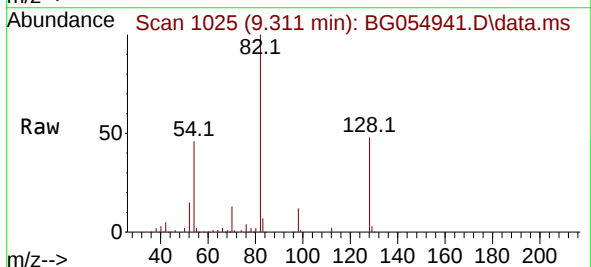




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.962 min Scan# 11
Delta R.T. 0.001 min
Lab File: BG054941.D
Acq: 14 Sep 2022 13:16




Instrument :
BNA_G
ClientSampleId :
CHERRY-HILL-COMP-14

Tgt Ion:	136	Resp:	140459
Ion Ratio	Lower	Upper	
136	100		
137	11.4	9.2	13.8
54	7.3	7.7	11.5#
68	5.8	5.6	8.4

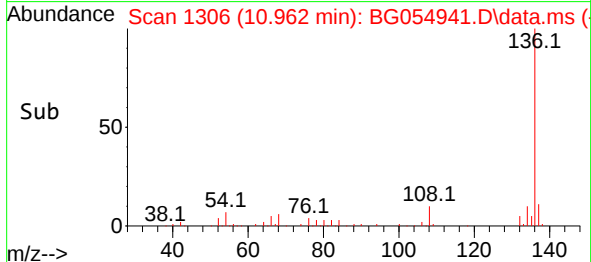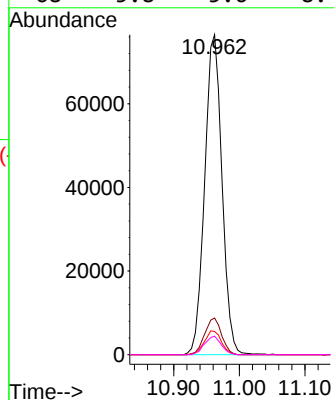

#23
Nitrobenzene-d5
Concen: 69.339 ng
RT: 9.305 min Scan# 1024
Delta R.T. -0.005 min
Lab File: BG054941.D
Acq: 14 Sep 2022 13:16

Tgt Ion:	82	Resp:	185524
Ion Ratio	Lower	Upper	
82	100		
128	45.8	32.2	48.2
54	45.4	41.4	62.0


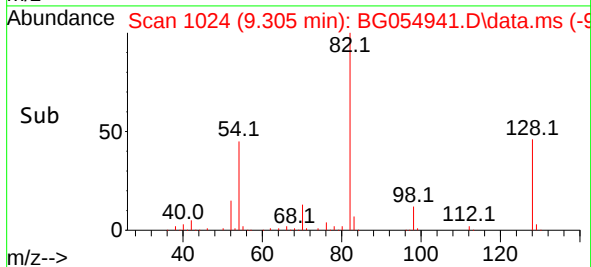
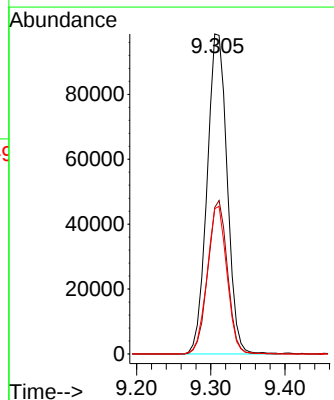
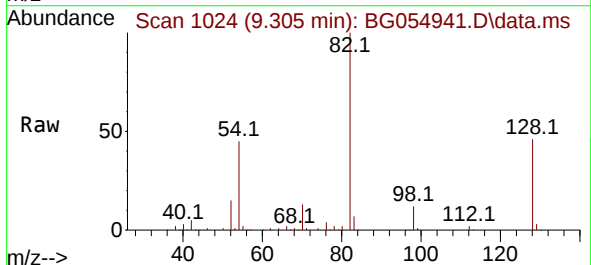




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.775 min Scan# 1955
Delta R.T. 0.001 min
Lab File: BG054941.D
Acq: 14 Sep 2022 13:16




Instrument :
BNA_G
ClientSampleId :
CHERRY-HILL-COMP-14


Tgt Ion:164 Resp: 109827
Ion Ratio Lower Upper
164 100
162 100.5 83.0 124.4
160 44.4 38.0 57.0

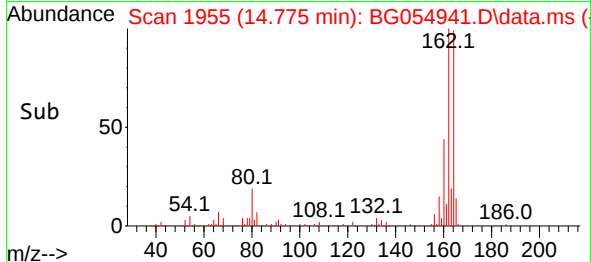

#42
2,4,6-Tribromophenol
Concen: 135.515 ng
RT: 16.262 min Scan# 2208
Delta R.T. 0.001 min
Lab File: BG054941.D
Acq: 14 Sep 2022 13:16

Tgt Ion:330 Resp: 185976
Ion Ratio Lower Upper
330 100
332 96.1 79.8 119.6
141 27.4 26.8 40.2

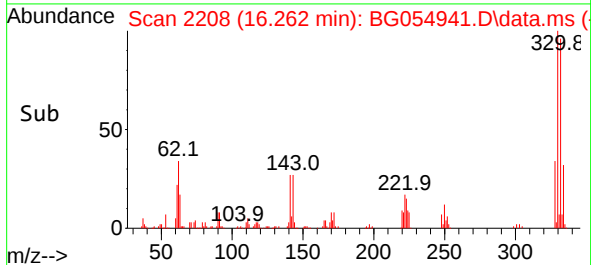

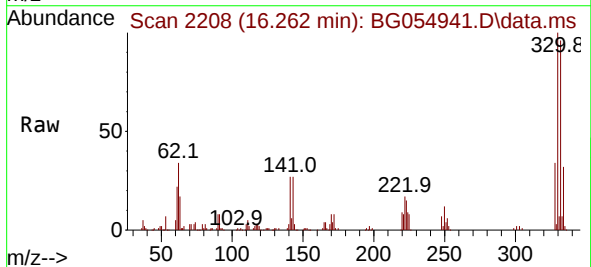


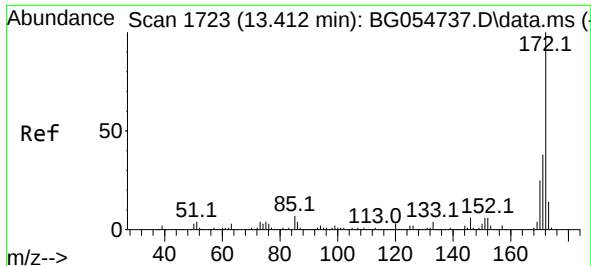

#45
2-Fluorobiphenyl
Concen: 69.603 ng
RT: 13.395 min Scan# 1
Delta R.T. 0.001 min
Lab File: BG054941.D
Acq: 14 Sep 2022 13:16




Instrument :
BNA_G
ClientSampleId :
CHERRY-HILL-COMP-14


Tgt Ion:172 Resp: 508596
Ion Ratio Lower Upper
172 100
171 37.1 31.2 46.8
170 24.8 20.6 30.8

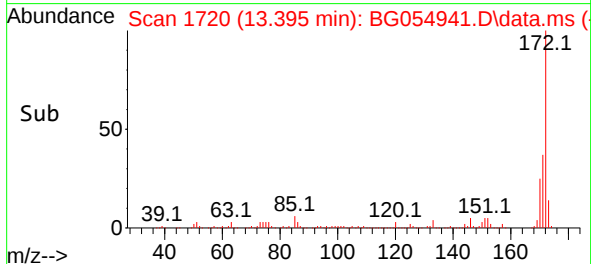

#51
2,6-Dinitrotoluene
Concen: 8.464 ng
RT: 14.775 min Scan# 1955
Delta R.T. 0.430 min
Lab File: BG054941.D
Acq: 14 Sep 2022 13:16

Tgt Ion:165 Resp: 14648
Ion Ratio Lower Upper
165 100
63 3.7 46.0 69.0#
89 3.1 50.3 75.5#


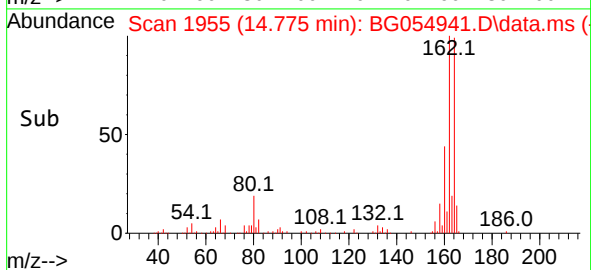

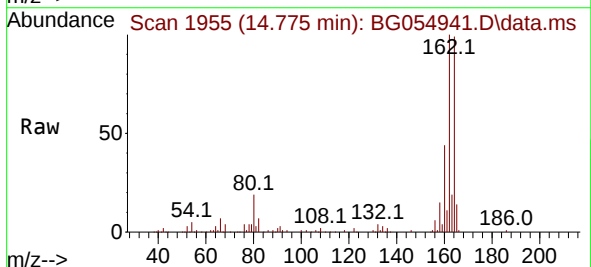




#57
2,4-Dinitrotoluene
Concen: 6.119 ng
RT: 14.775 min Scan# 1955
Delta R.T. -0.363 min
Lab File: BG054941.D
Acq: 14 Sep 2022 13:16




Instrument :
BNA_G
ClientSampleId :
CHERRY-HILL-COMP-14


Tgt Ion:165 Resp: 14648
Ion Ratio Lower Upper
165 100
63 3.7 36.8 55.2#
89 3.1 64.3 96.5#
182 0.0 1.8 2.6#

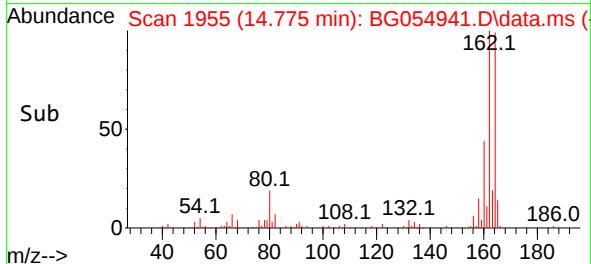

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.519 min Scan# 2422
Delta R.T. -0.005 min
Lab File: BG054941.D
Acq: 14 Sep 2022 13:16

Tgt Ion:188 Resp: 264294
Ion Ratio Lower Upper
188 100
94 8.2 7.0 10.4
80 8.4 7.9 11.9


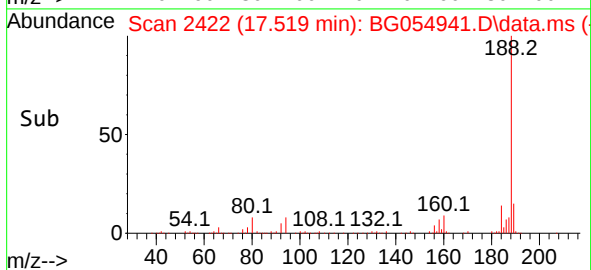

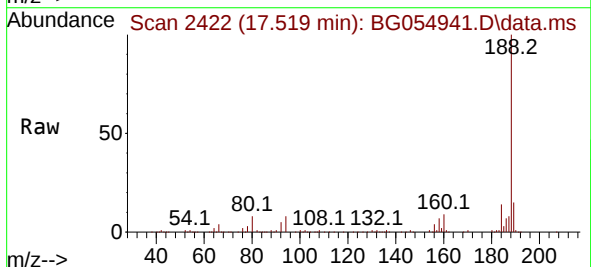


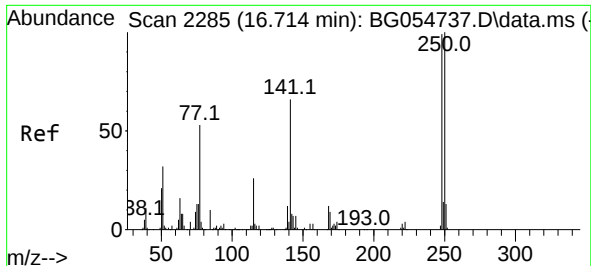

#67
4-Bromophenyl-phenylether
Concen: 3.996 ng
RT: 16.262 min Scan# 211
Delta R.T. -0.439 min
Lab File: BG054941.D
Acq: 14 Sep 2022 13:16




Instrument :
BNA_G
ClientSampleId :
CHERRY-HILL-COMP-14


Tgt Ion:248 Resp: 11596
Ion Ratio Lower Upper
248 100
250 190.1 78.8 118.2#
141 417.6 51.9 77.9#

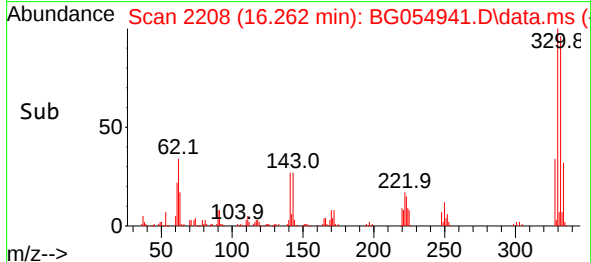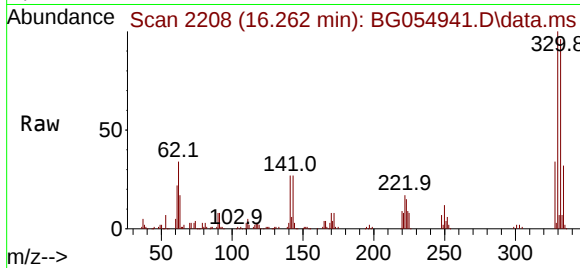

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.814 min Scan# 3153
Delta R.T. -0.005 min
Lab File: BG054941.D
Acq: 14 Sep 2022 13:16

Tgt Ion:240 Resp: 261131
Ion Ratio Lower Upper
240 100
120 9.1 8.2 12.4
236 25.7 21.2 31.8

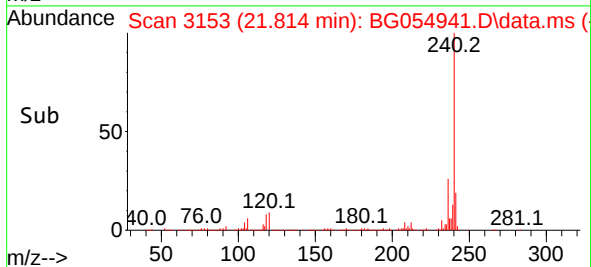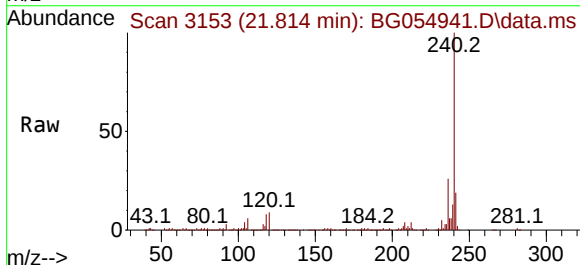



#79

Terphenyl-d14

Concen: 65.408 ng

RT: 20.116 min Scan# 21

Delta R.T. -0.005 min

Lab File: BG054941.D


Acq: 14 Sep 2022 13:16

Instrument :

BNA_G

ClientSampleId :

CHERRY-HILL-COMP-14

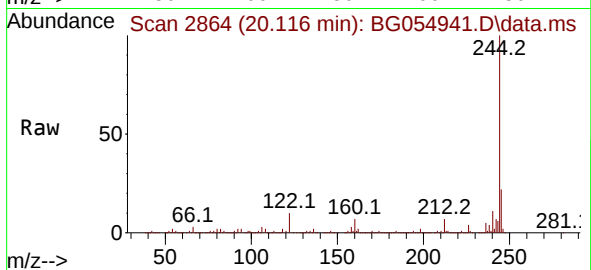




Tgt Ion:244 Resp: 862018

Ion Ratio Lower Upper

244 100

212 7.3 6.2 9.2

122 9.6 9.0 13.6

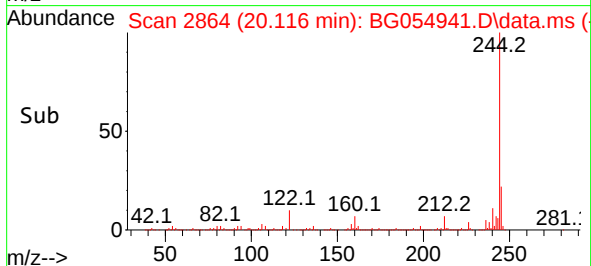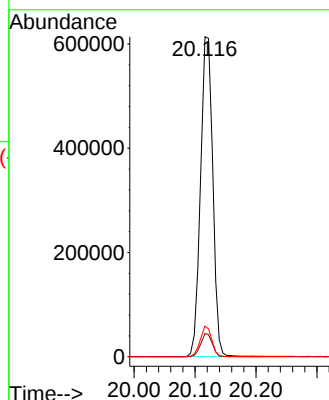

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.187 min Scan# 3727

Delta R.T. 0.001 min

Lab File: BG054941.D

Acq: 14 Sep 2022 13:16

Tgt Ion:264 Resp: 274296

Ion Ratio Lower Upper

264 100

260 23.9 19.9 29.9

265 22.1 16.9 25.3

