
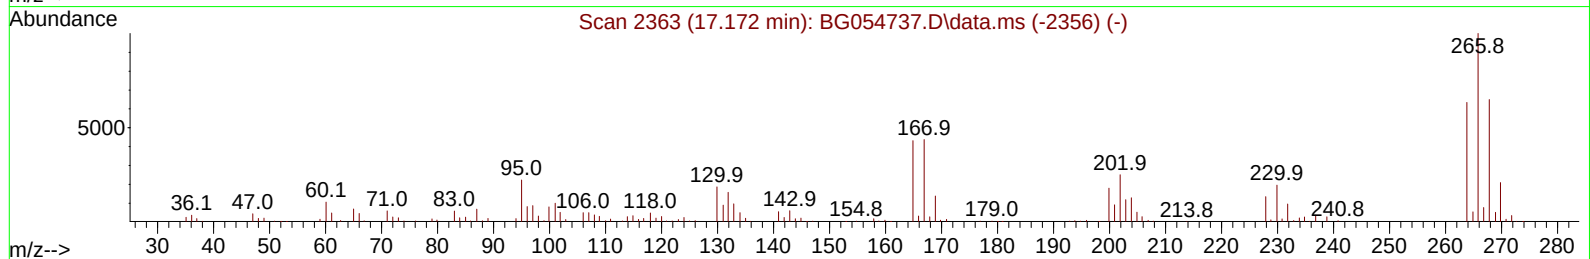
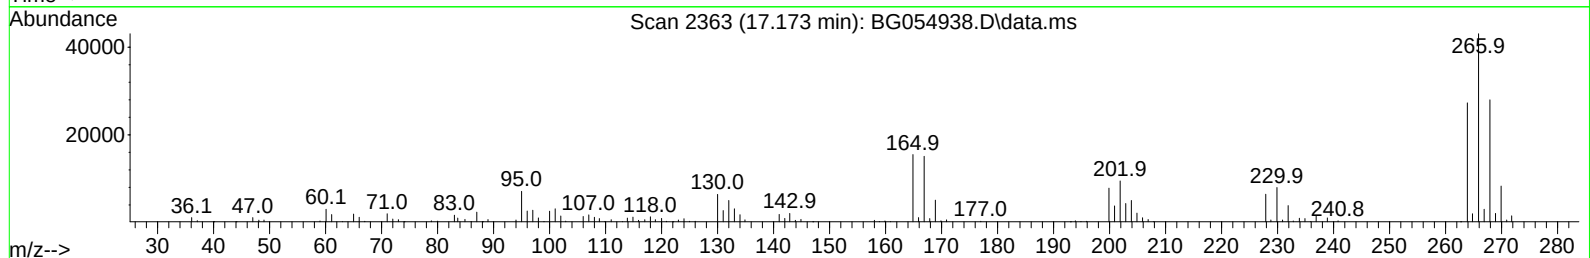


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091422\
Data File : BG054938.D
Acq On : 14 Sep 2022 9:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 06:04:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 03:14:10 2022
Response via : Initial Calibration

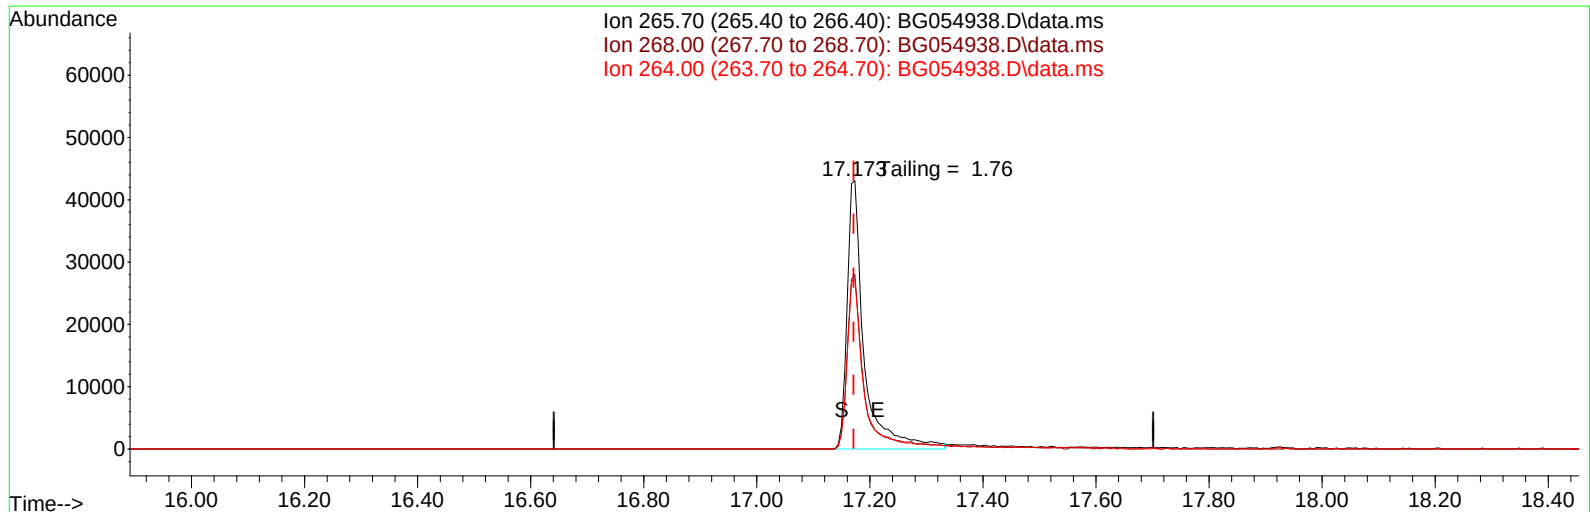

TIC: BG054938.D\data.ms

(70) Pentachlorophenol (C)




17.173min (+ 0.002) 34557.53 ng

response 88295

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	65.00
264.00	61.70	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091422\
Data File : BG054938.D
Acq On : 14 Sep 2022 9:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 06:04:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 03:14:10 2022
Response via : Initial Calibration

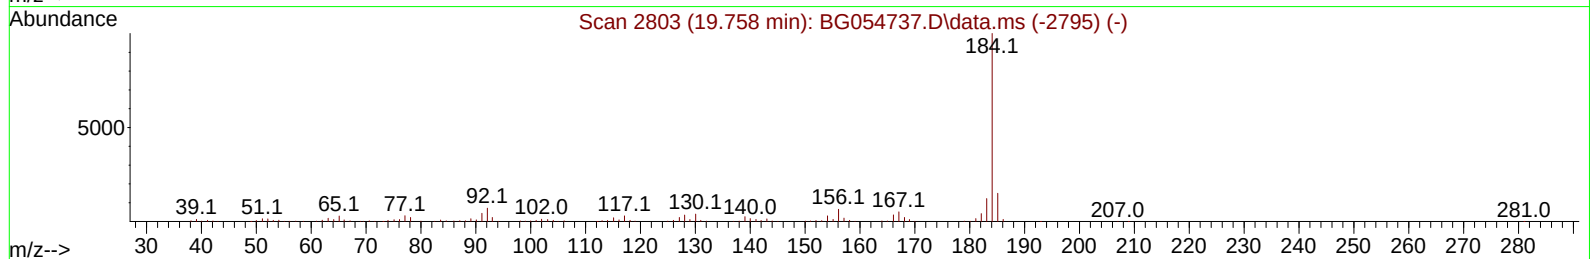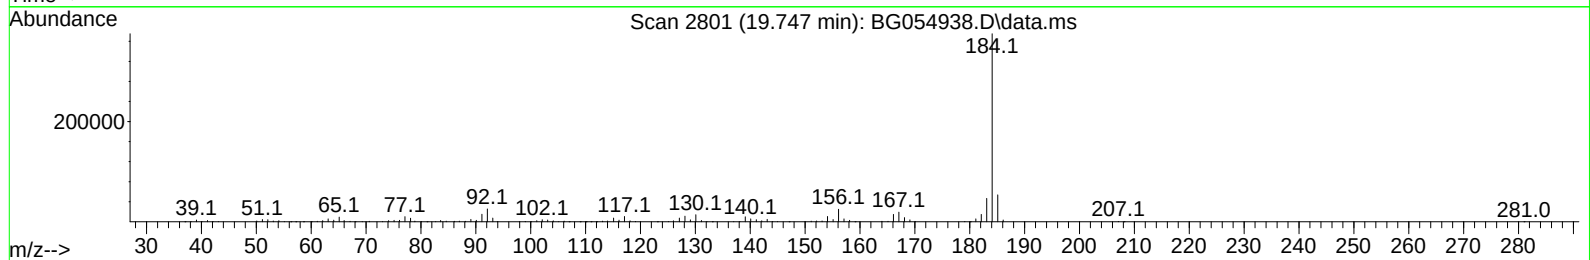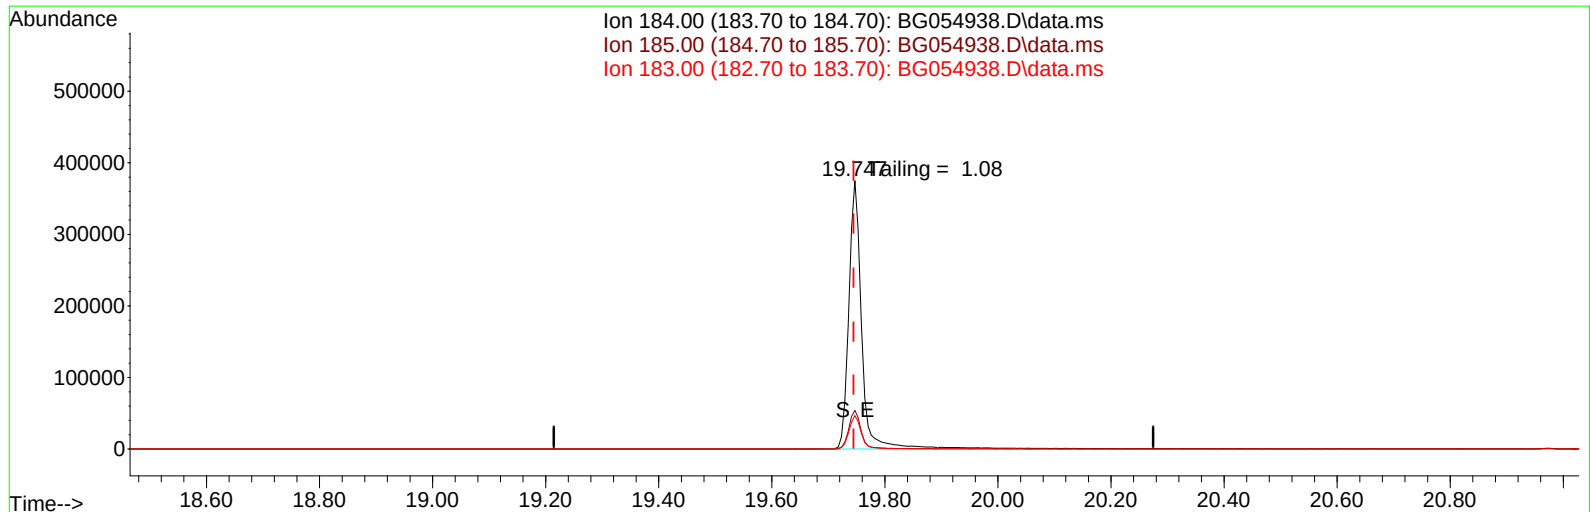

TIC: BG054938.D\data.ms

(77) Benzidine

19.747min (+ 0.002) 0.00 ng

response 583914

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.37
183.00	12.30	12.48
0.00	0.00	0.00