
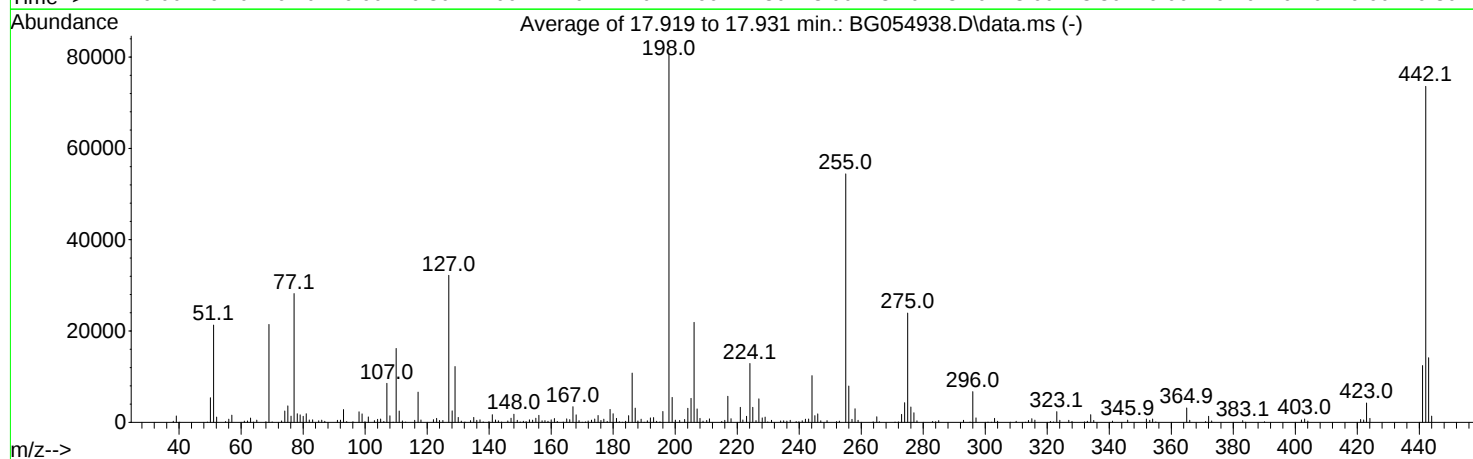


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091422\
 Data File : BG054938.D
 Acq On : 14 Sep 2022 9:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 15 03:14:10 2022

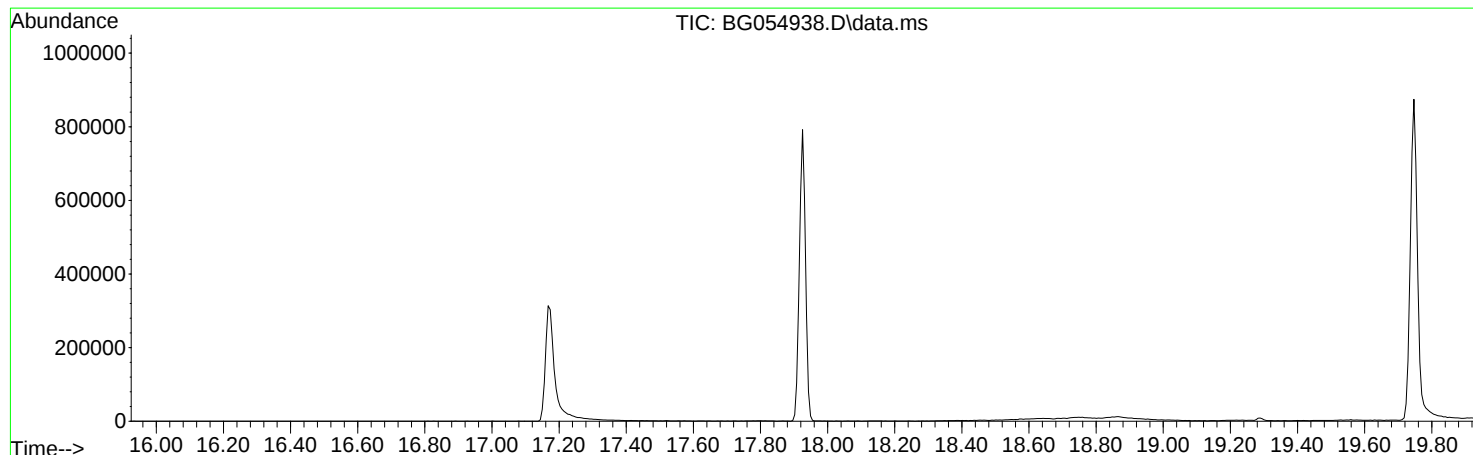




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	21298	PASS
68	69	0.00	2	0.6	133	PASS
69	198	0.00	100	26.6	21435	PASS
70	69	0.00	2	0.6	120	PASS
127	198	10	80	40.0	32195	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80552	PASS
199	198	5	9	6.8	5482	PASS
275	198	10	60	29.7	23923	PASS
365	198	1	100	3.9	3143	PASS
441	198	0.01	100	15.4	12425	PASS
442	442	50	100	100.0	73584	PASS
443	442	15	24	19.2	14158	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091422\
Data File : BG054938.D
Acq On : 14 Sep 2022 9:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 15 06:04:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 03:14:10 2022
Response via : Initial Calibration

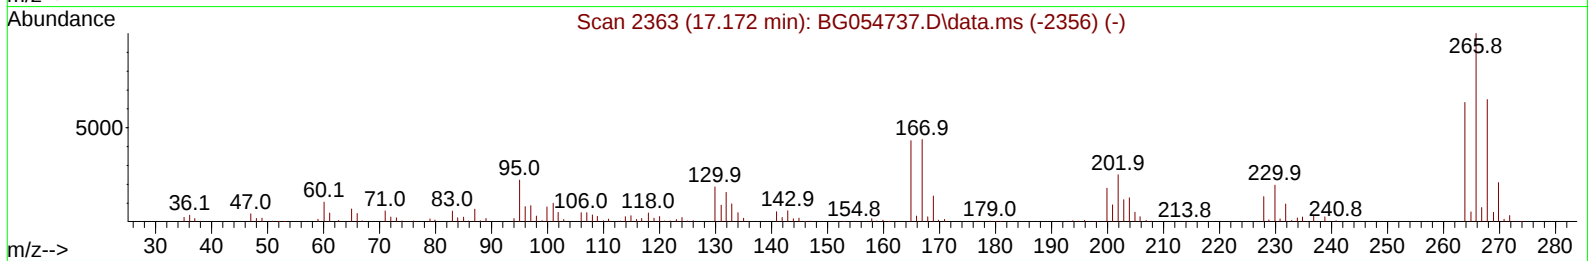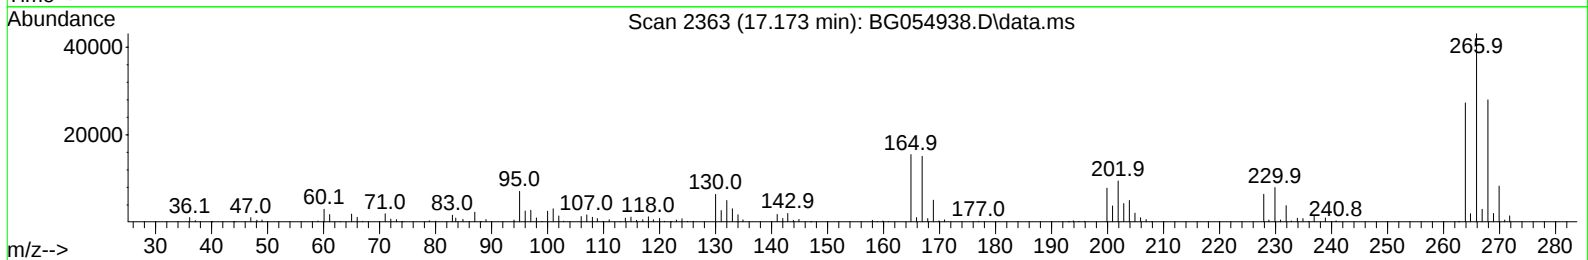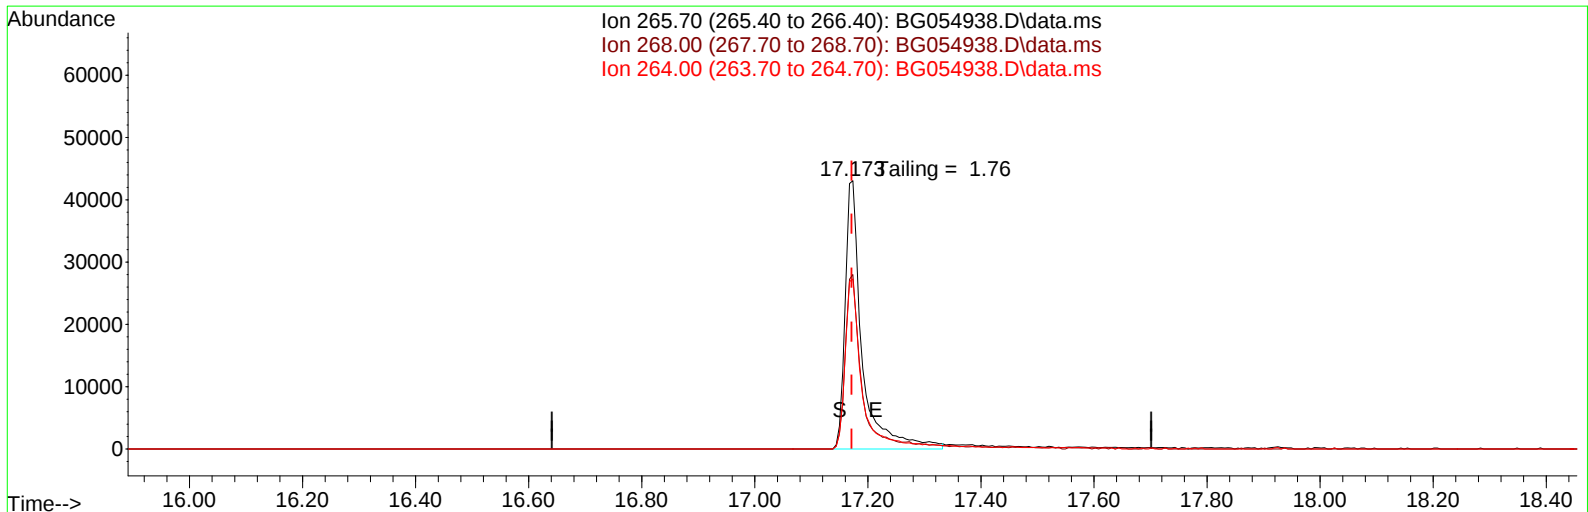

TIC: BG054938.D\data.ms

(70) Pentachlorophenol (C)

17.173min (+ 0.002) 34557.53 ng




response 88295

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	65.00
264.00	61.70	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091422\
Data File : BG054938.D
Acq On : 14 Sep 2022 9:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 15 06:04:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 03:14:10 2022
Response via : Initial Calibration

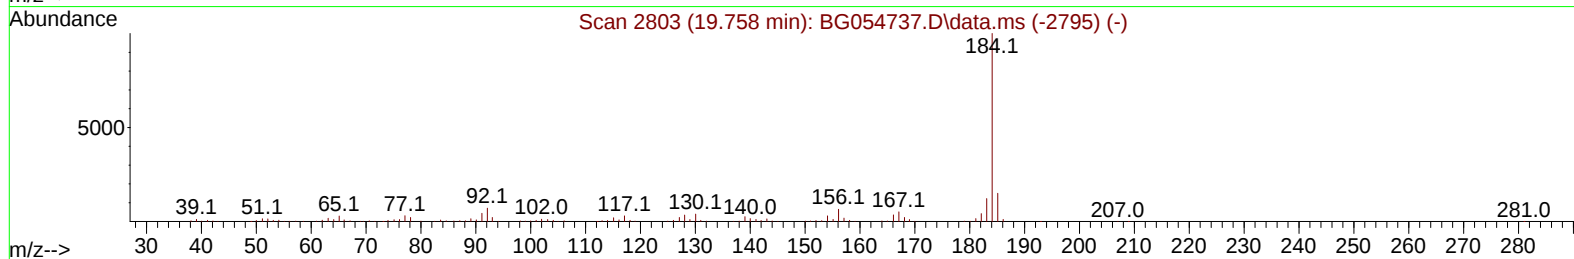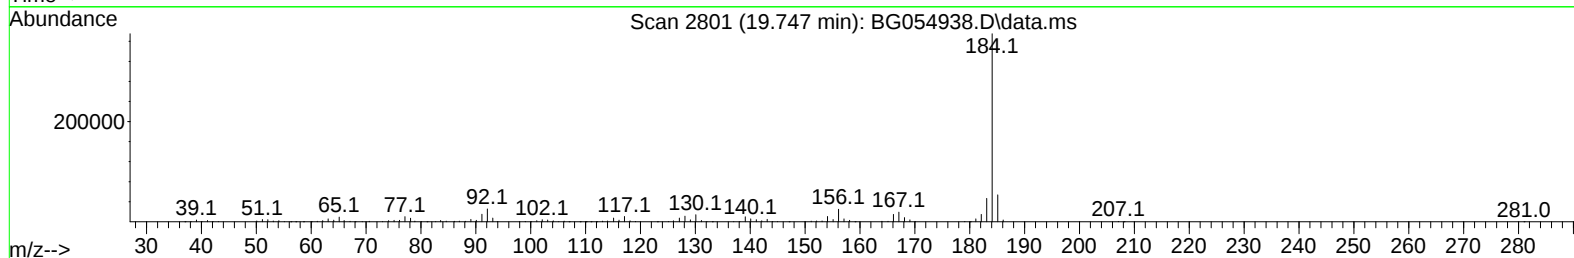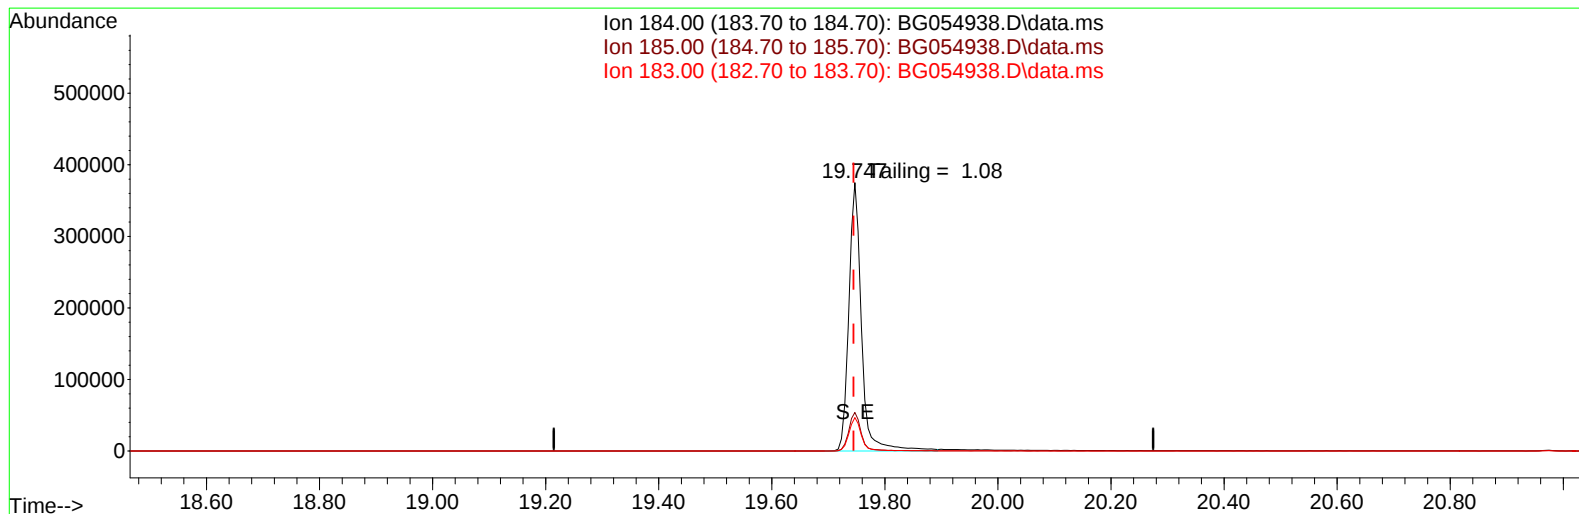

TIC: BG054938.D\data.ms

(77) Benzidine

19.747min (+ 0.002) 0.00 ng

response 583914

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.37
183.00	12.30	12.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/14/2022	BNA_G	<u>BG054938.D</u>
Compound Name	Response	Retention Time
DDT	296175	20.975
DDD	8256	20.528
DDE	599	20.017
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8855	305030	2.90

Instrument :
BNA_G
ClientSampleId :
DFTPP