




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
 Data File : BG059060.D
 Acq On : 14 Sep 2023 11:46
 Operator : MA/JU
 Sample : SST00513
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:39:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 14 15:36:44 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
 Supervised By :mohammad ahmed 09/15/2023

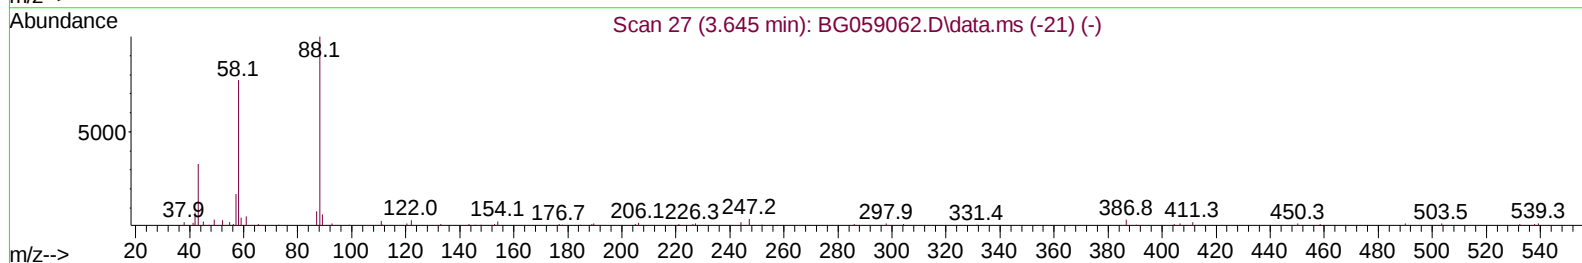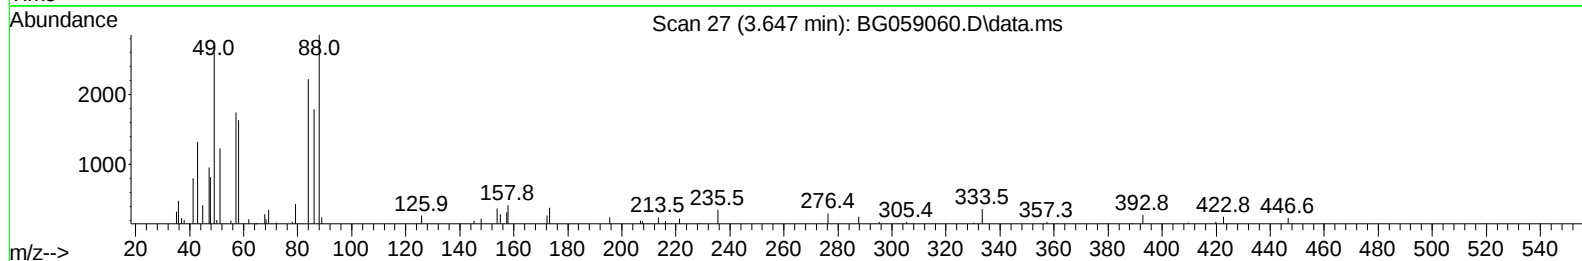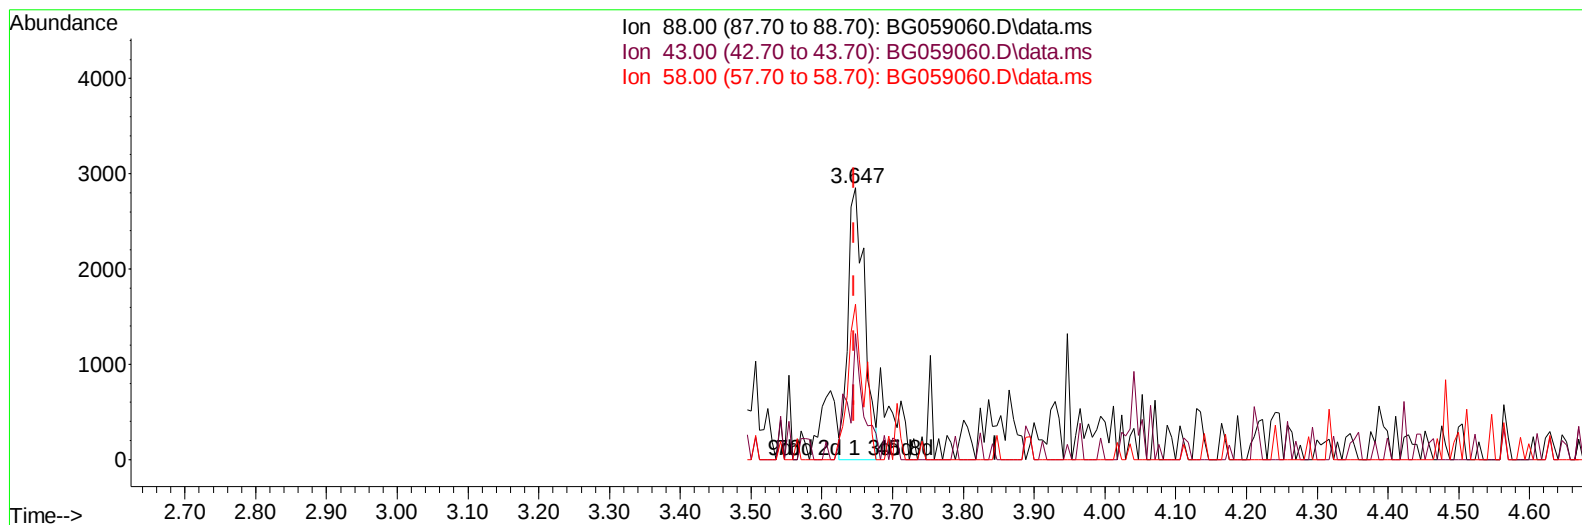

TIC: BG059060.D\data.ms

(2) 1,4-Dioxane

3.647min (+ 0.002) 2.14 ng/uL

response 4651

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	33.30	46.26#
58.00	77.00	57.28#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
Data File : BG059060.D
Acq On : 14 Sep 2023 11:46
Operator : MA/JU
Sample : SST00513
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:39:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 14 15:36:44 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
Supervised By :mohammad ahmed 09/15/2023

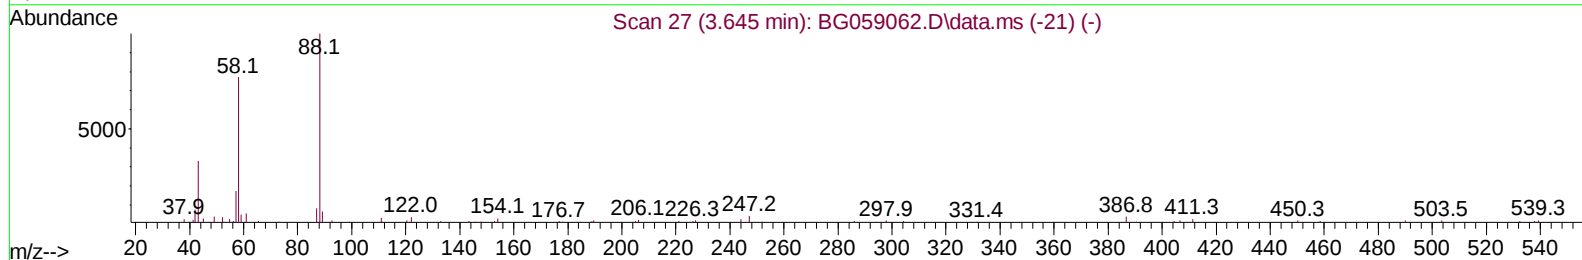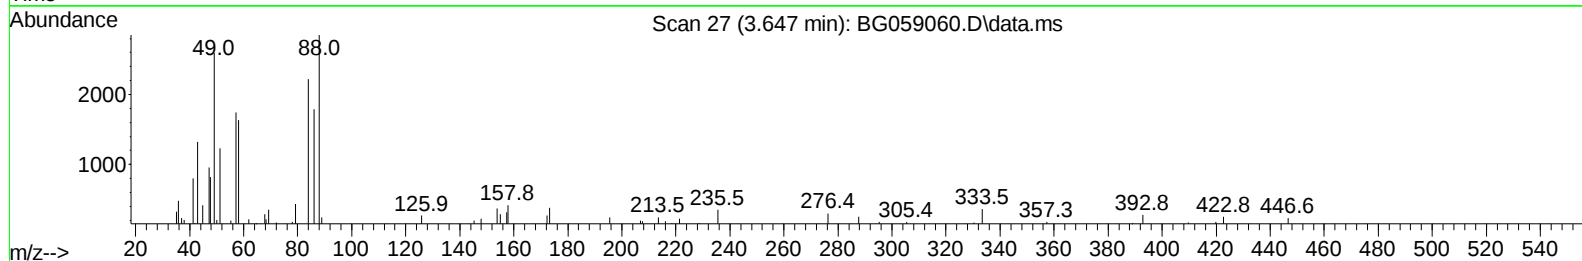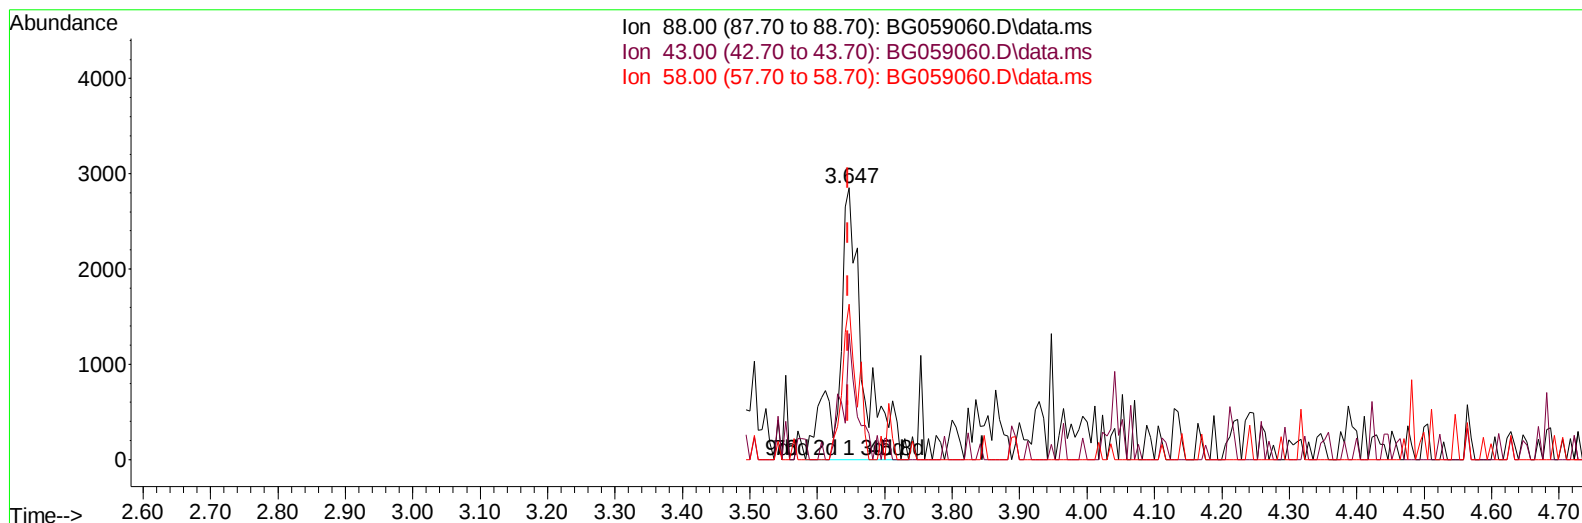

TIC: BG059060.D\data.ms

(2) 1,4-Dioxane

3.647min (+ 0.002) 3.32 ng/uL m

response 7213

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	33.30	46.26#
58.00	77.00	57.28#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
Data File : BG059060.D
Acq On : 14 Sep 2023 11:46
Operator : MA/JU
Sample : SST00513
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:39:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 14 15:36:44 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
Supervised By :mohammad ahmed 09/15/2023

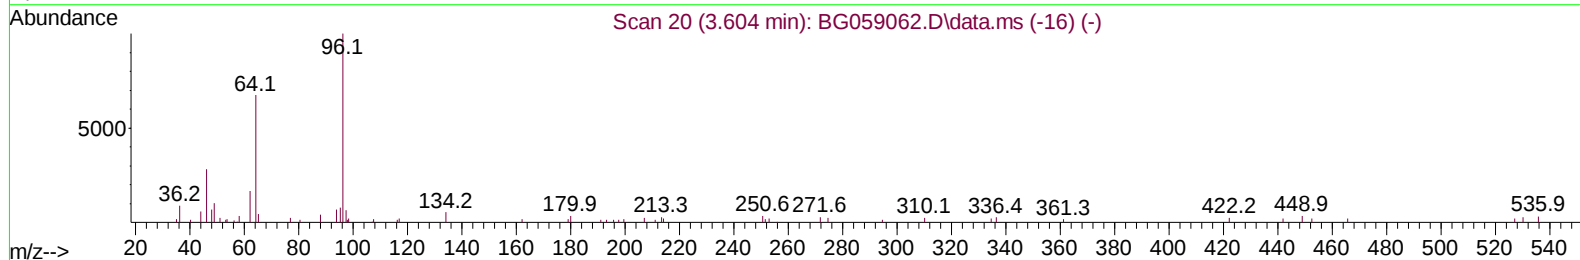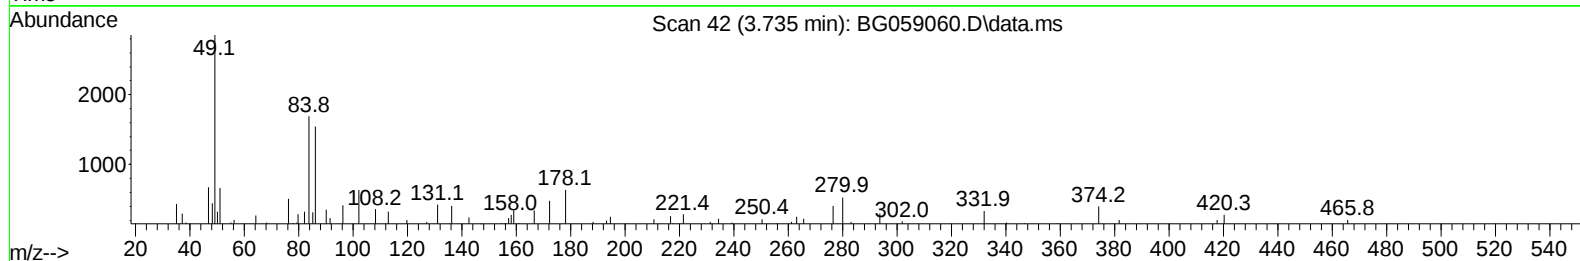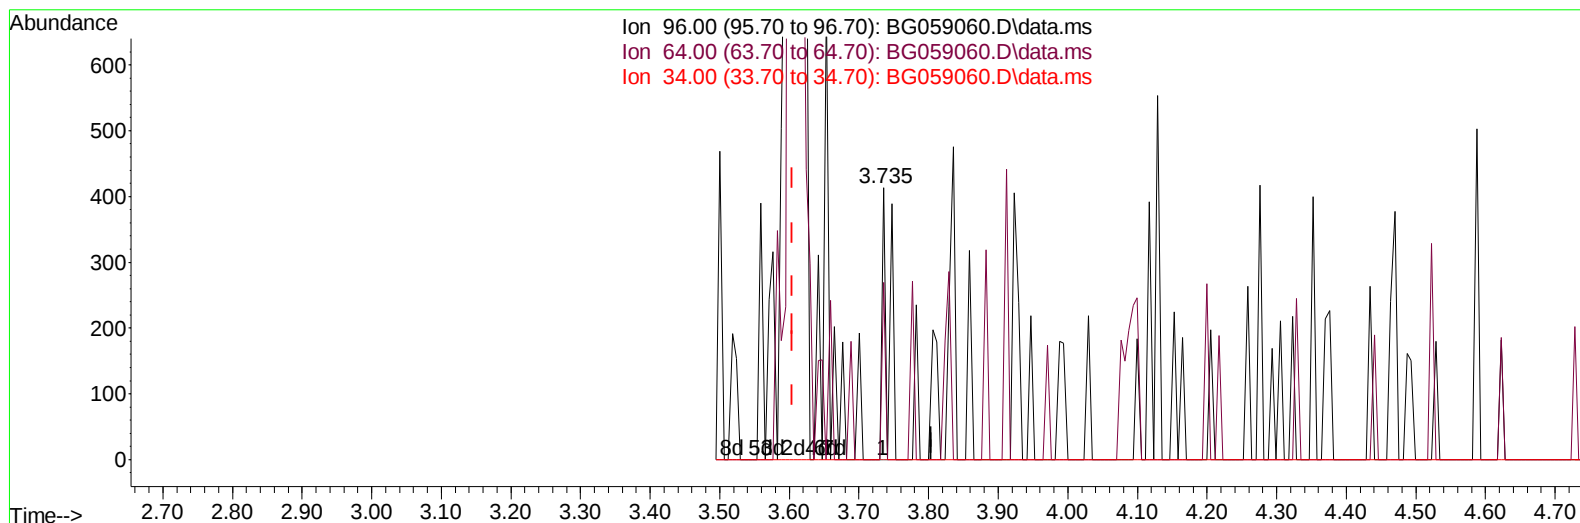

TIC: BG059060.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.735min (+ 0.131) 0.08 ng/uL

response 146

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	67.40	65.13
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
Data File : BG059060.D
Acq On : 14 Sep 2023 11:46
Operator : MA/JU
Sample : SST00513
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:39:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 14 15:36:44 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
Supervised By :mohammad ahmed 09/15/2023

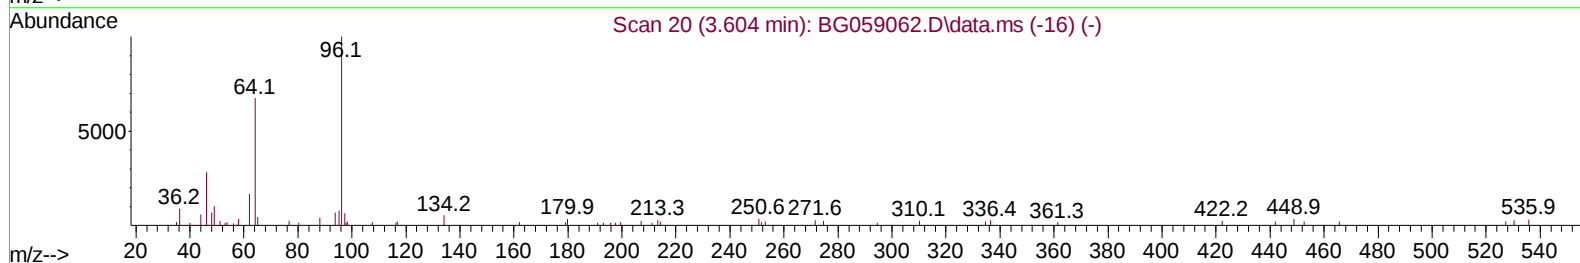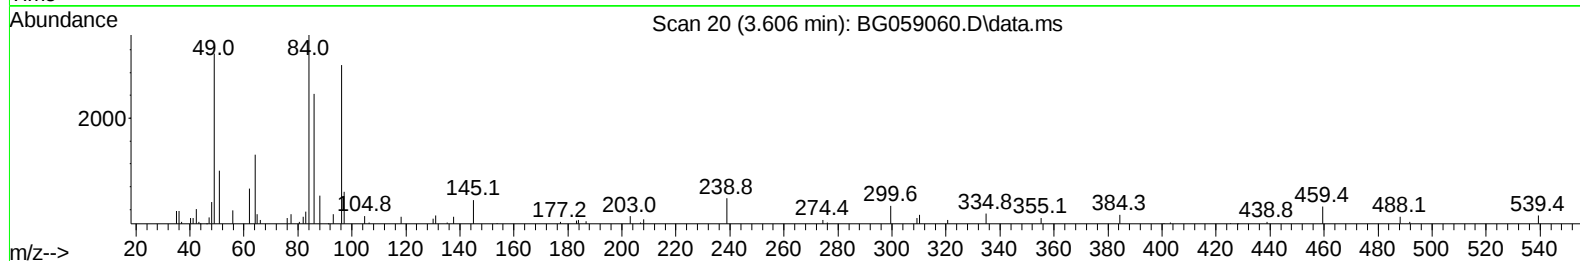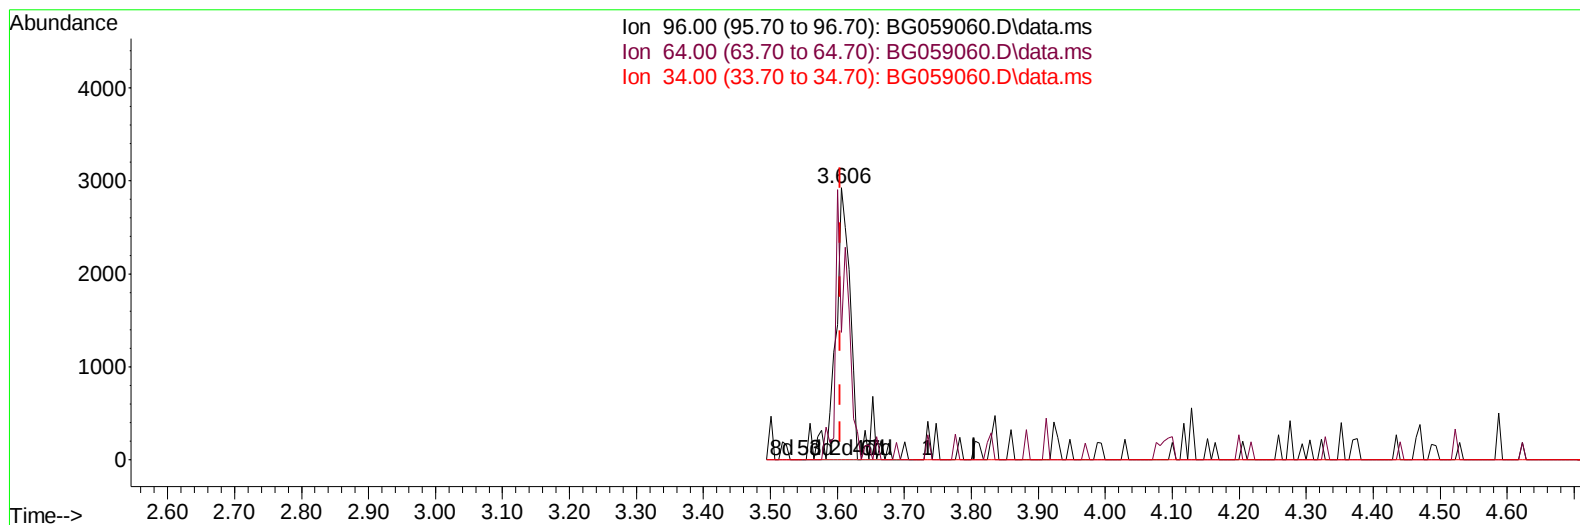

TIC: BG059060.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.606min (+ 0.002) 2.80 ng/uL m

response 4955

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	67.40	46.70#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
 Data File : BG059060.D
 Acq On : 14 Sep 2023 11:46
 Operator : MA/JU
 Sample : SST00513
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:39:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 14 15:36:44 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
 Supervised By :mohammad ahmed 09/15/2023

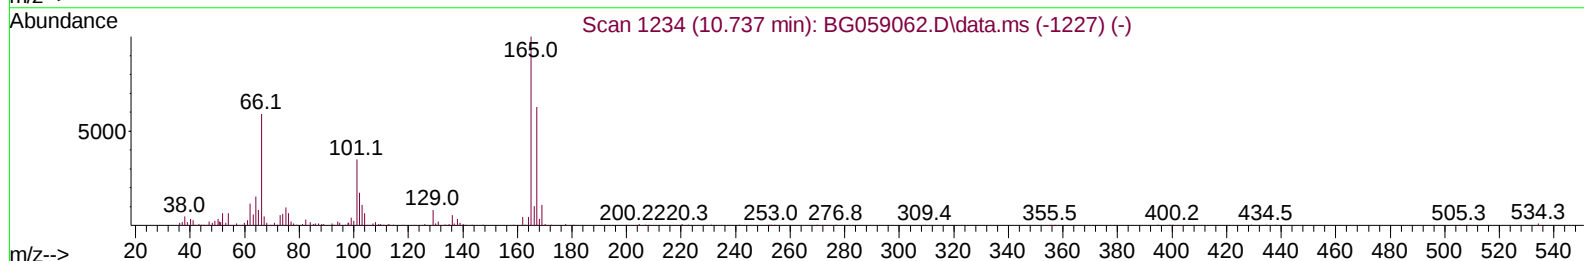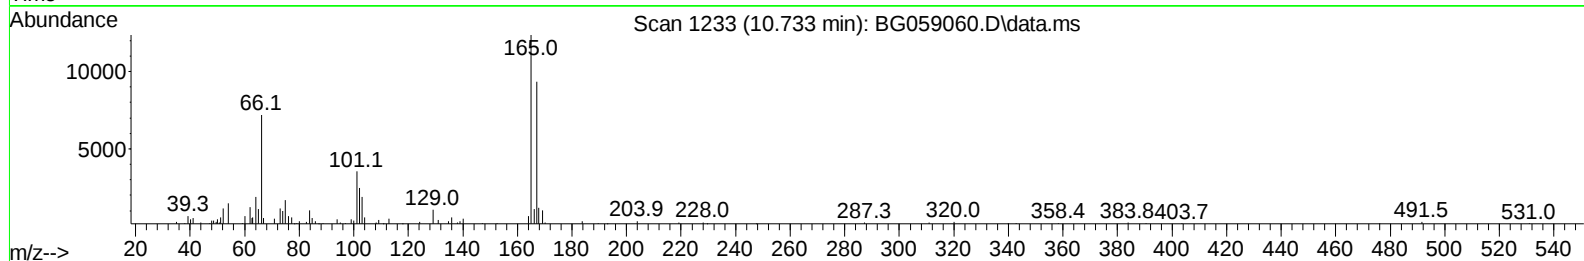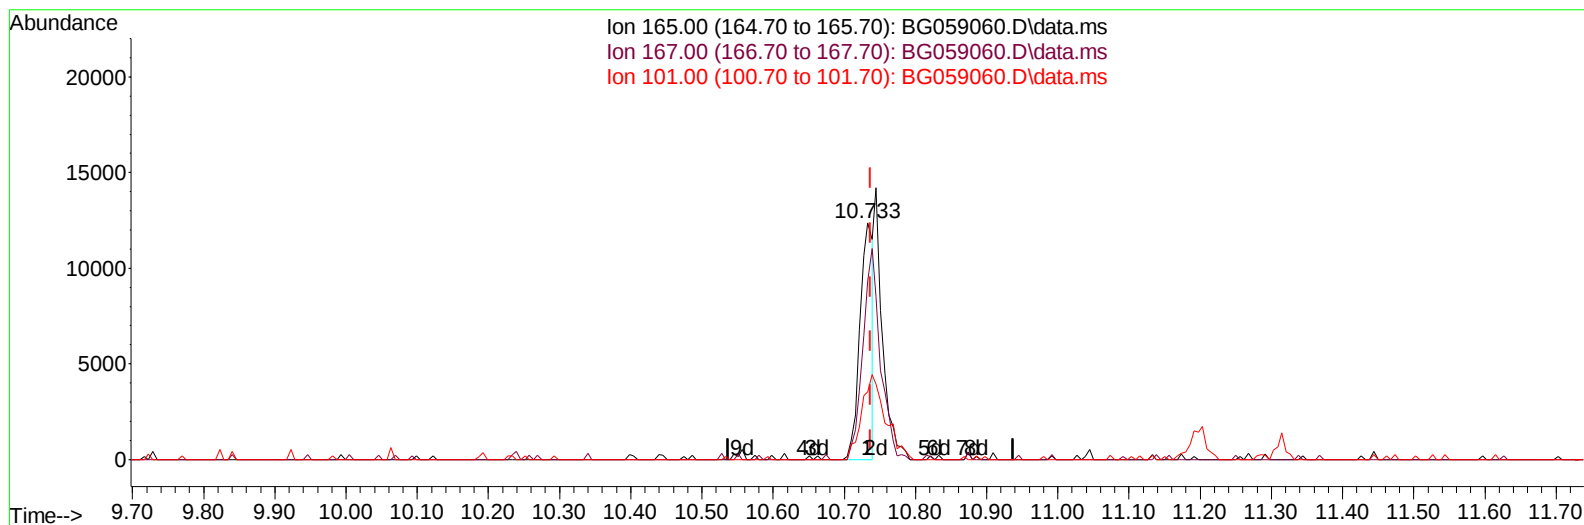

TIC: BG059060.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.733min (-0.004) 2.47 ng/ul

response 15757

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.60	75.47#
101.00	34.90	28.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
 Data File : BG059060.D
 Acq On : 14 Sep 2023 11:46
 Operator : MA/JU
 Sample : SST00513
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:39:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 14 15:36:44 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
 Supervised By :mohammad ahmed 09/15/2023

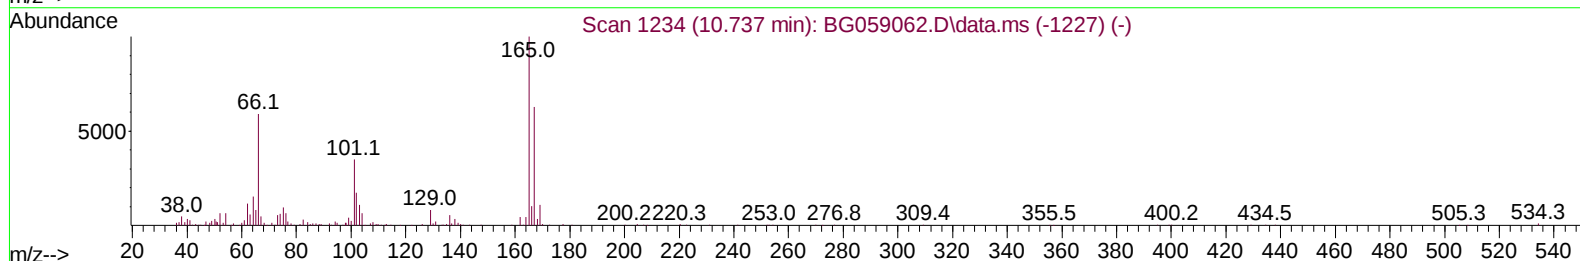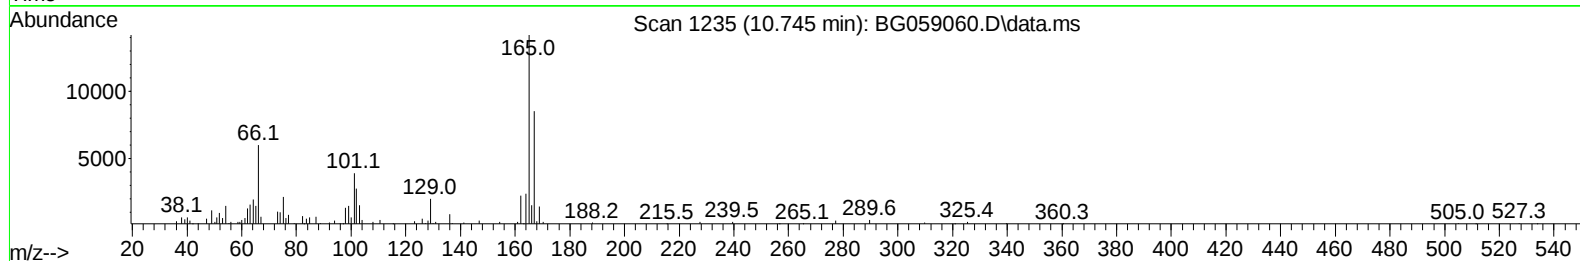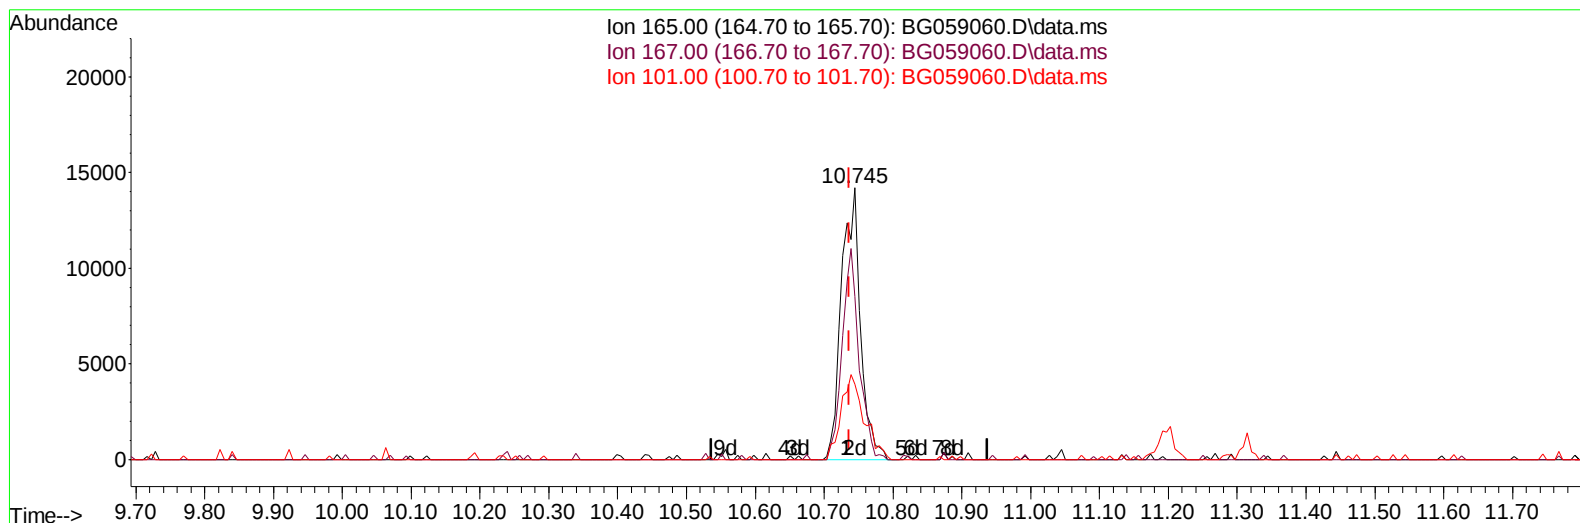

TIC: BG059060.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.745min (+ 0.008) 4.26 ng/ul m

response 27181

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.60	60.04
101.00	34.90	27.67#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
Data File : BG059060.D
Acq On : 14 Sep 2023 11:46
Operator : MA/JU
Sample : SST00513
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD005414

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/15/2023
Supervised By :mohammad ahmed 09/15/2023

Quant Time: Sep 14 15:39:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 14 15:36:44 2023
Response via : Initial Calibration

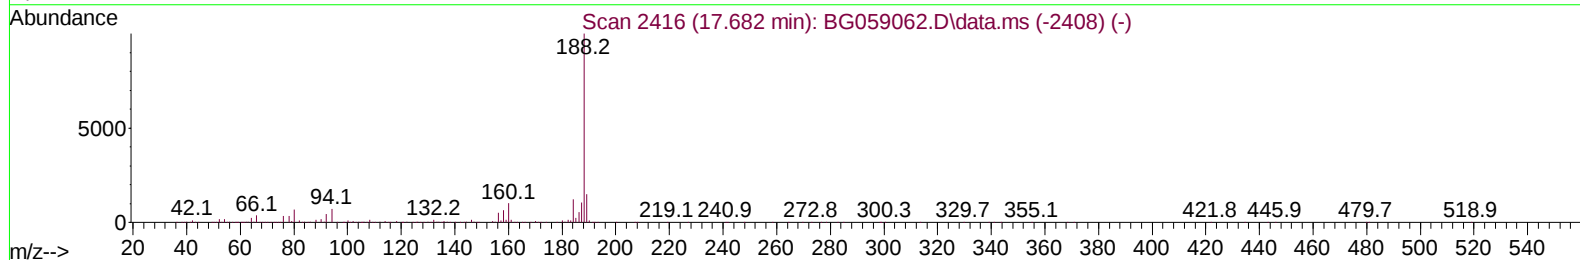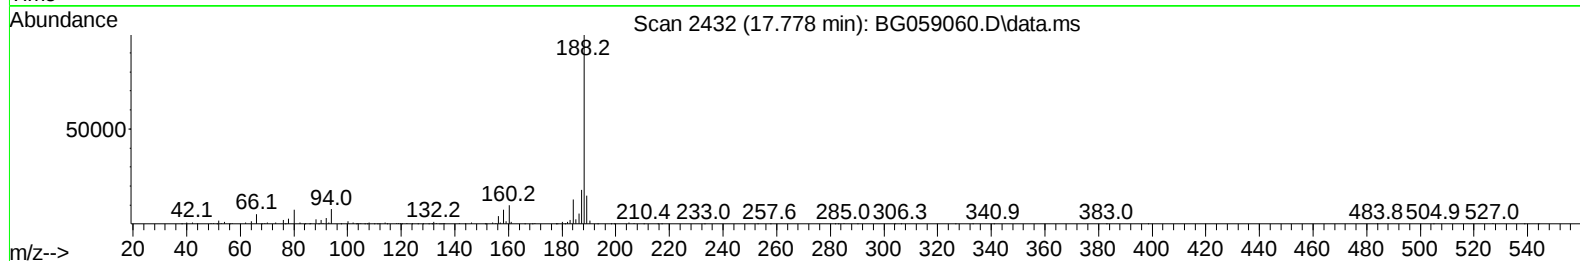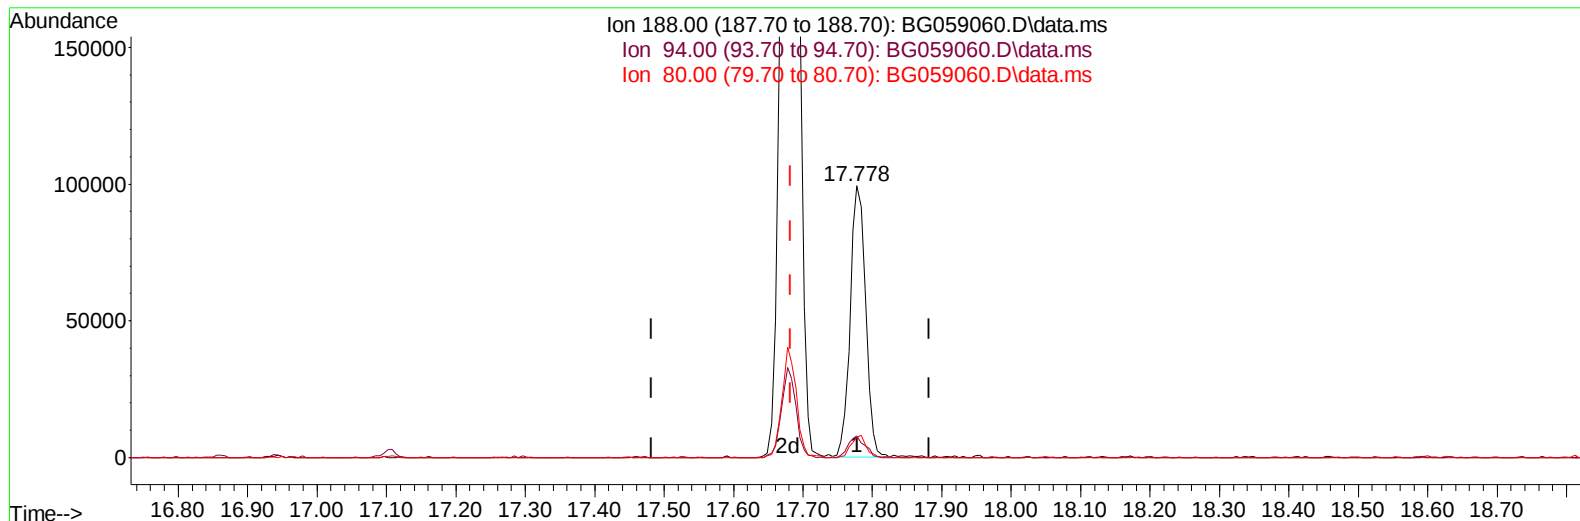

TIC: BG059060.D\data.ms

(64) Phenanthrene-d10 (I)

17.778min (+ 0.096) 20.00 ng/u1

response 152610

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.20	7.81
80.00	6.80	7.56
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
 Data File : BG059060.D
 Acq On : 14 Sep 2023 11:46
 Operator : MA/JU
 Sample : SST00513
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:39:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 14 15:36:44 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
 Supervised By :mohammad ahmed 09/15/2023

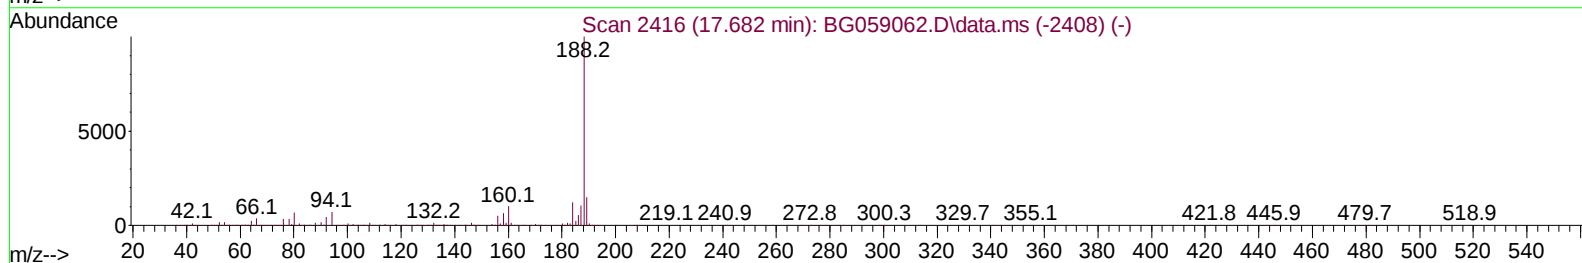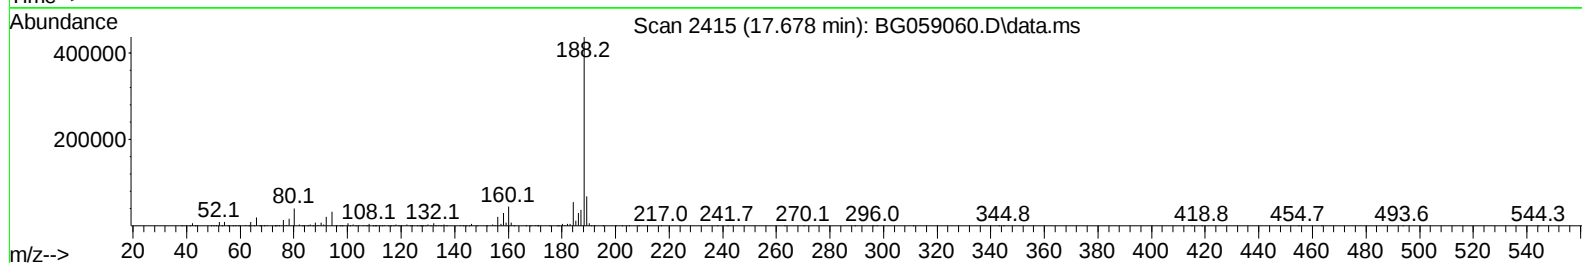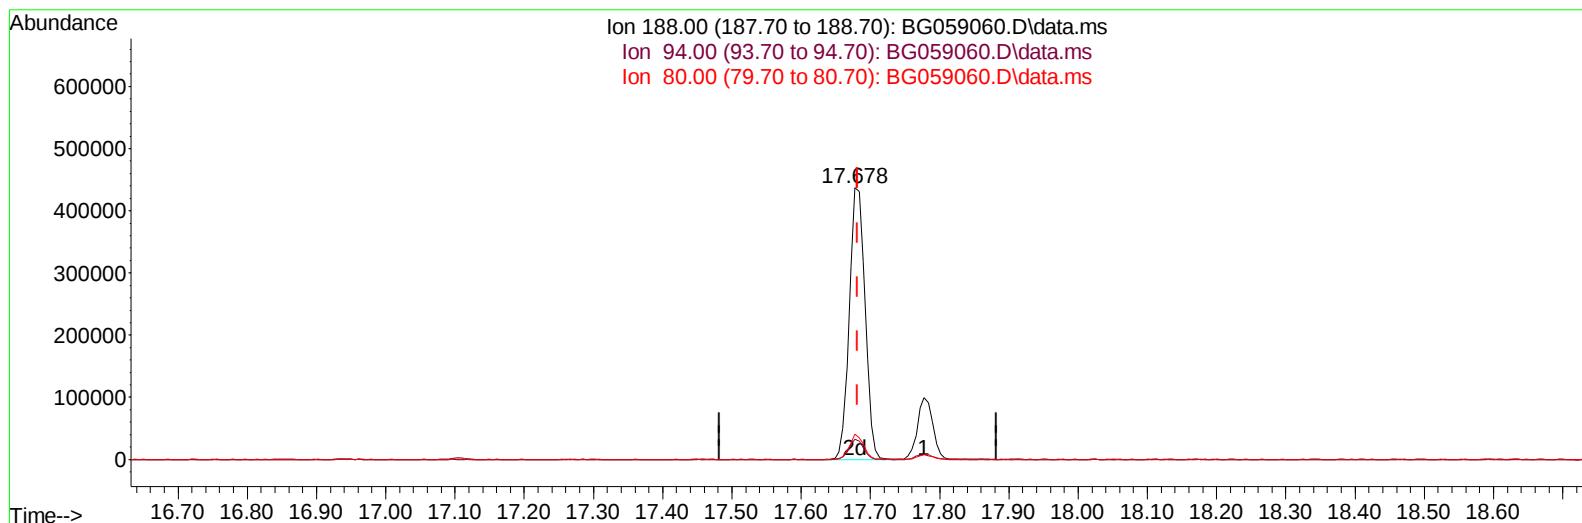

TIC: BG059060.D\data.ms

(64) Phenanthrene-d10 (I)

17.678min (-0.004) 20.00 ng/ul m

response 686115

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.20	7.51
80.00	6.80	9.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
 Data File : BG059060.D
 Acq On : 14 Sep 2023 11:46
 Operator : MA/JU
 Sample : SST00513
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:42:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 14 15:36:44 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
 Supervised By :mohammad ahmed 09/15/2023

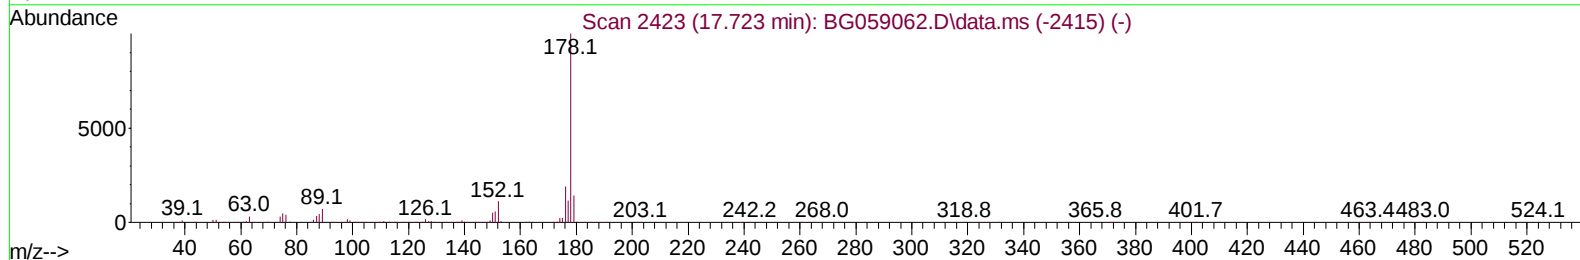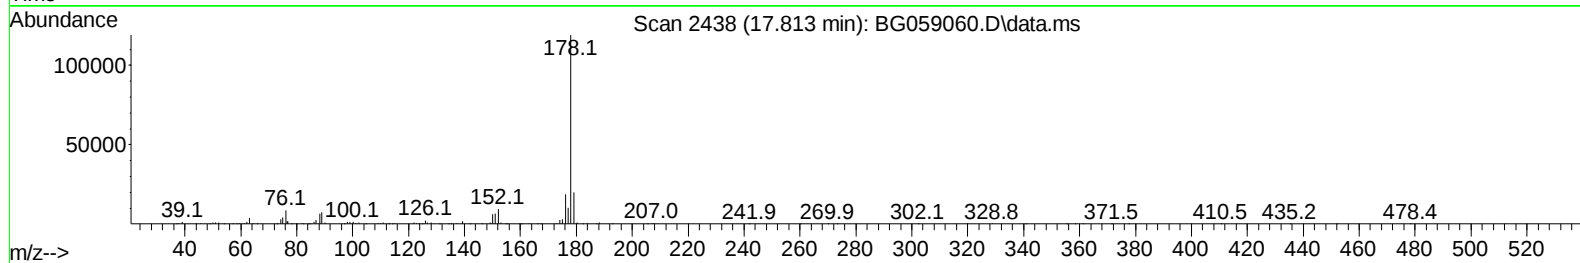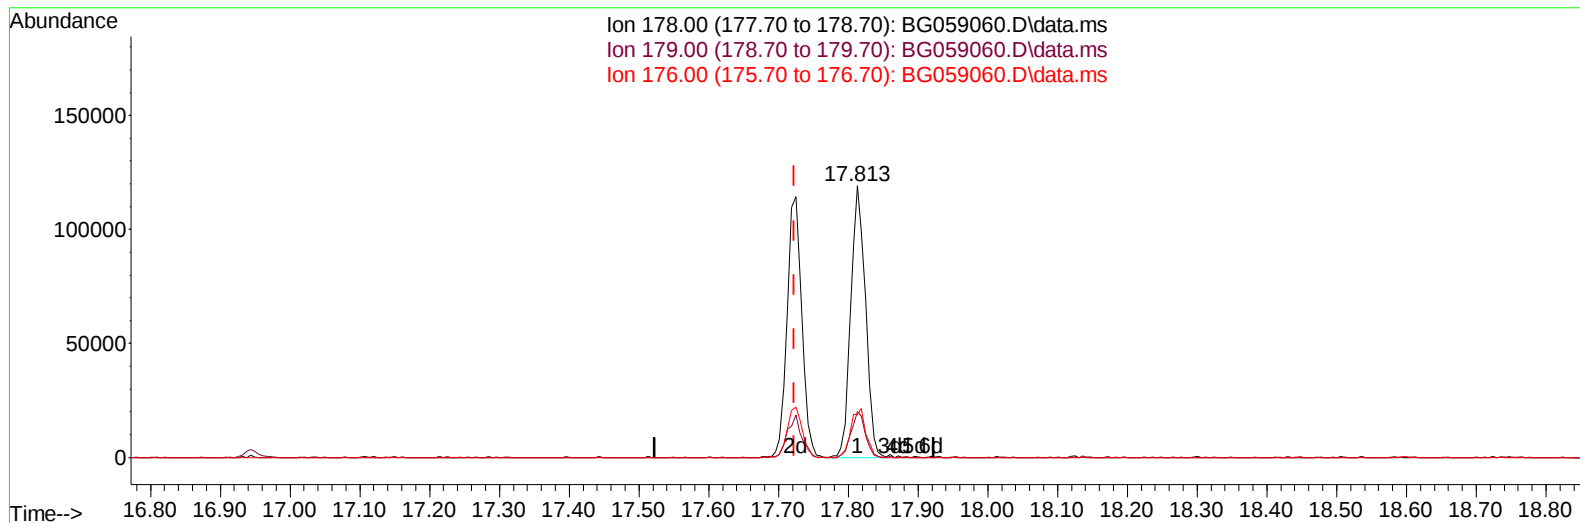

TIC: BG059060.D\data.ms

(72) Phenanthrene

17.813min (+ 0.090) 4.68 ng/u1

response 175152

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	14.20	16.80
176.00	18.80	15.67
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
 Data File : BG059060.D
 Acq On : 14 Sep 2023 11:46
 Operator : MA/JU
 Sample : SST00513
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:42:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 14 15:36:44 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
 Supervised By :mohammad ahmed 09/15/2023

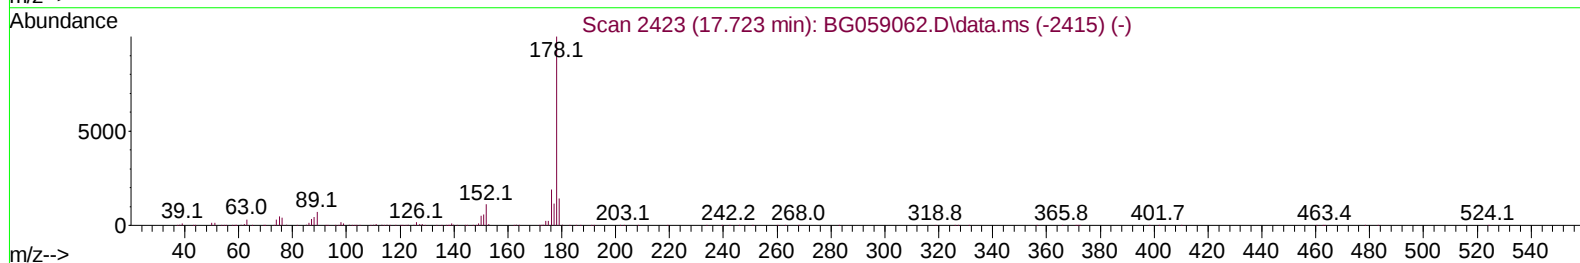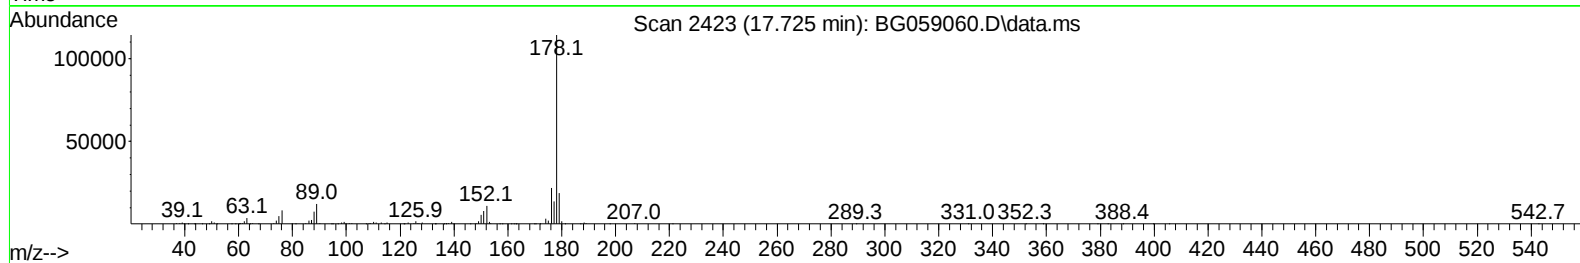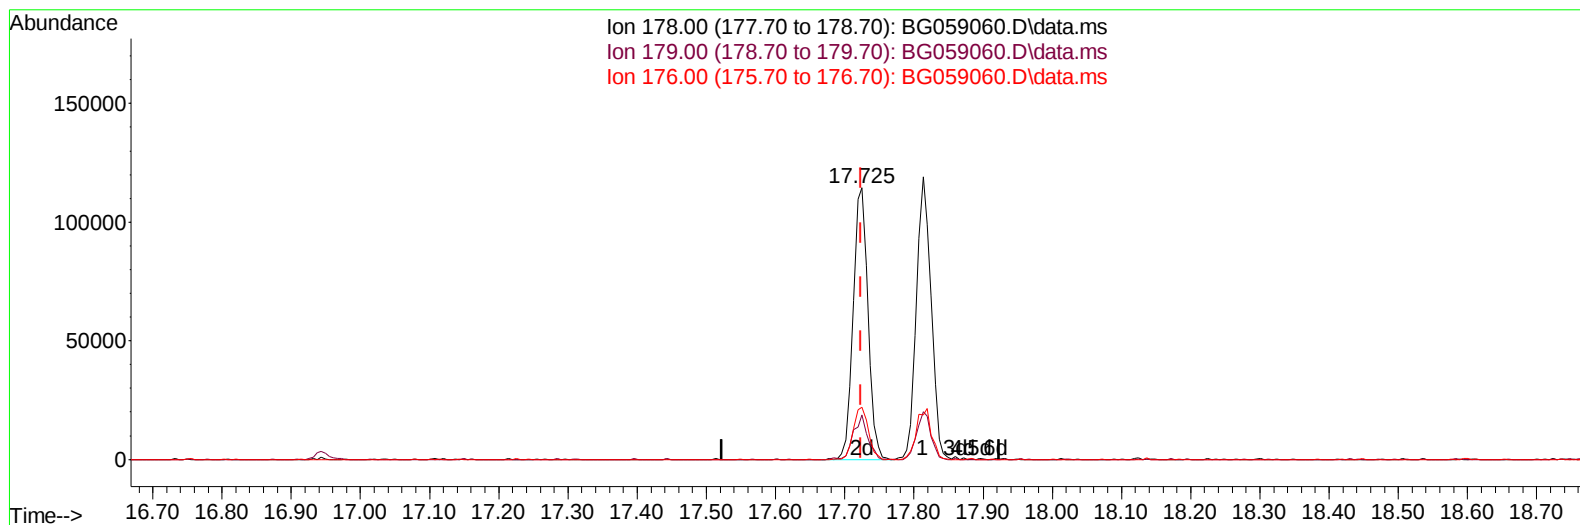

TIC: BG059060.D\data.ms

(72) Phenanthrene

17.725min (+ 0.002) 4.48 ng/ul m

response 167731

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	14.20	16.34
176.00	18.80	19.20
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
 Data File : BG059060.D
 Acq On : 14 Sep 2023 11:46
 Operator : MA/JU
 Sample : SST00513
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:42:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 14 15:36:44 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
 Supervised By :mohammad ahmed 09/15/2023

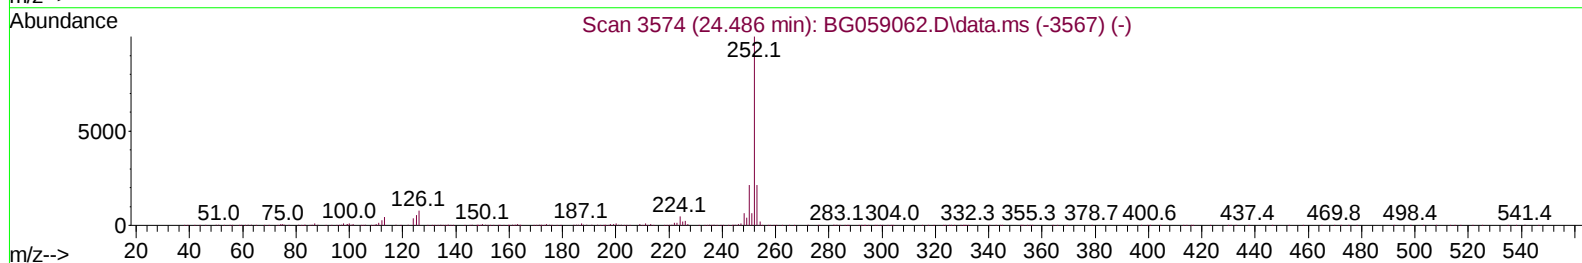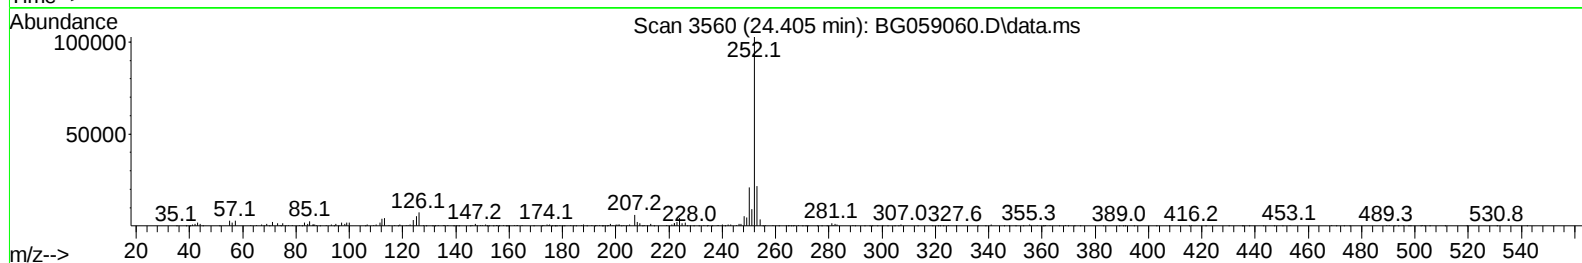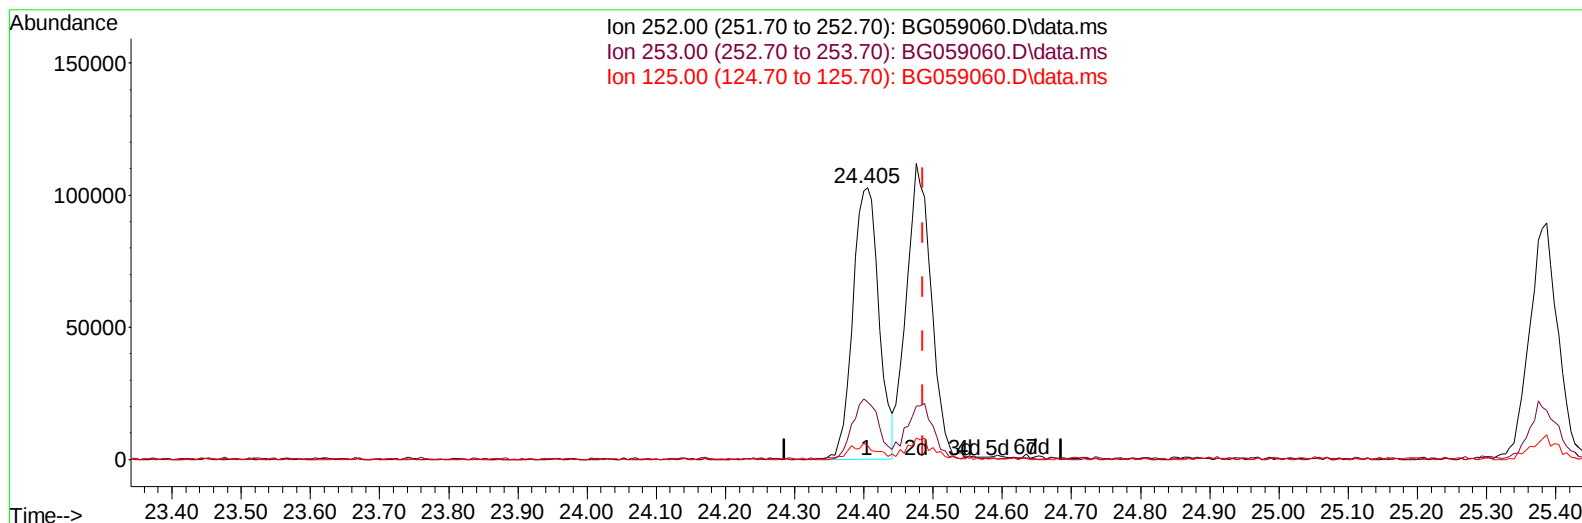

TIC: BG059060.D\data.ms

(91) Benzo(k)fluoranthene

24.405min (-0.080) 4.26 ng/u1

response 269836

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.80	21.01
125.00	5.60	5.17
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
 Data File : BG059060.D
 Acq On : 14 Sep 2023 11:46
 Operator : MA/JU
 Sample : SST00513
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:42:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 14 15:36:44 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
 Supervised By :mohammad ahmed 09/15/2023

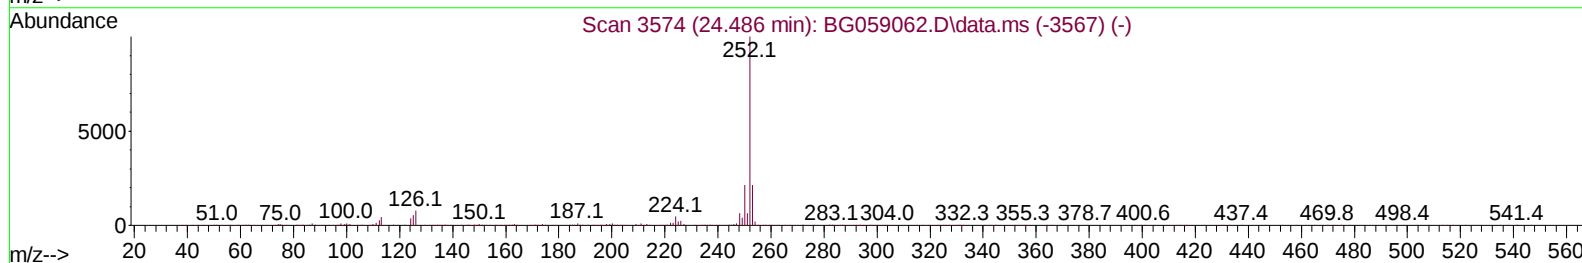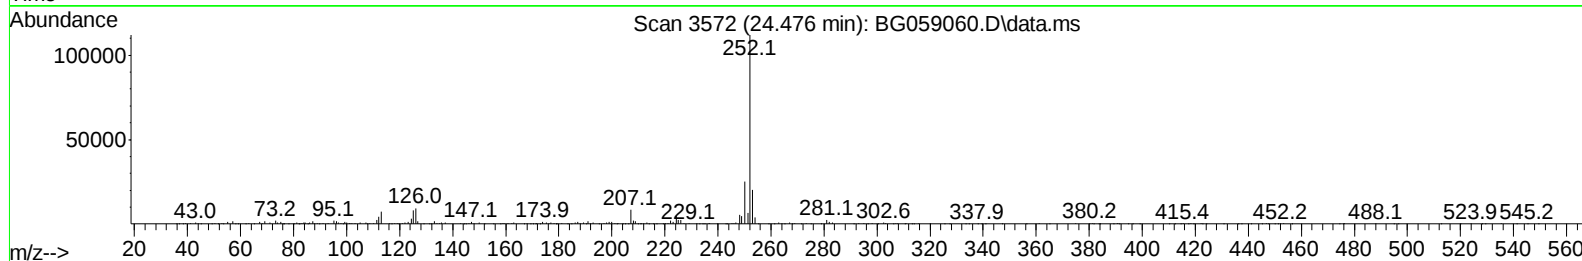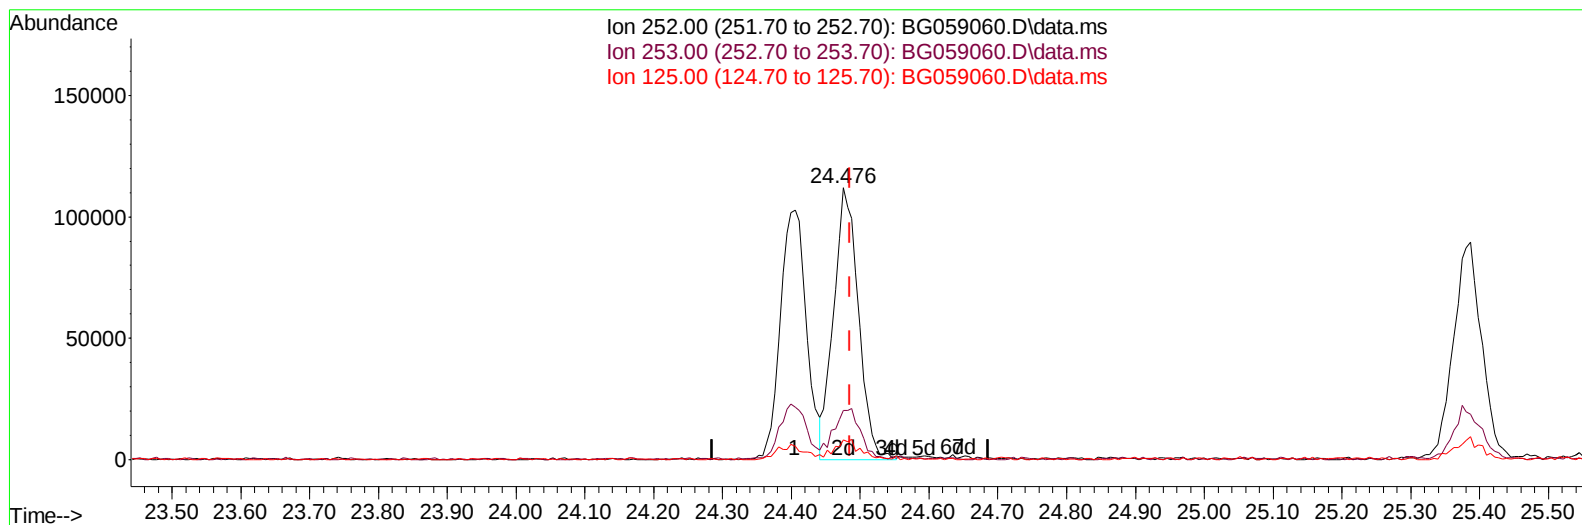

TIC: BG059060.D\data.ms

(91) Benzo(k)fluoranthene

24.476min (-0.010) 4.42 ng/ul m

response 279656

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.80	18.07
125.00	5.60	7.25#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
Data File : BG059060.D
Acq On : 14 Sep 2023 11:46
Operator : MA/JU
Sample : SST00513
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:42:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 14 15:36:44 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
Supervised By :mohammad ahmed 09/15/2023

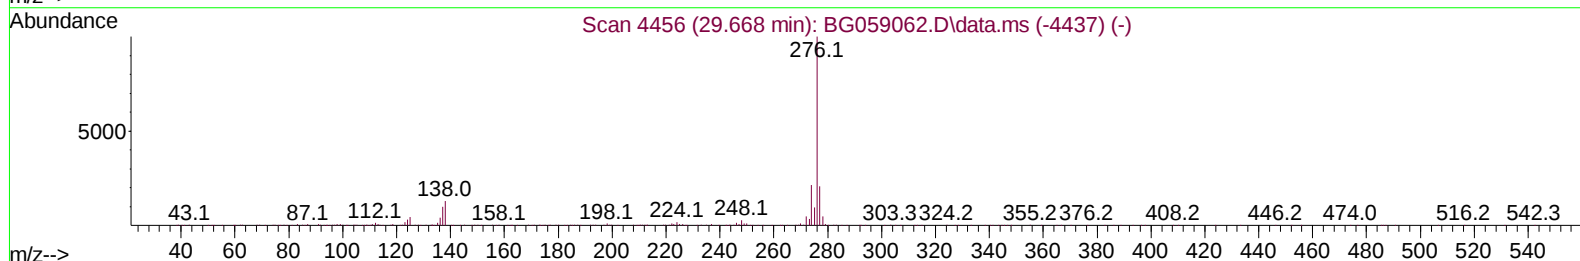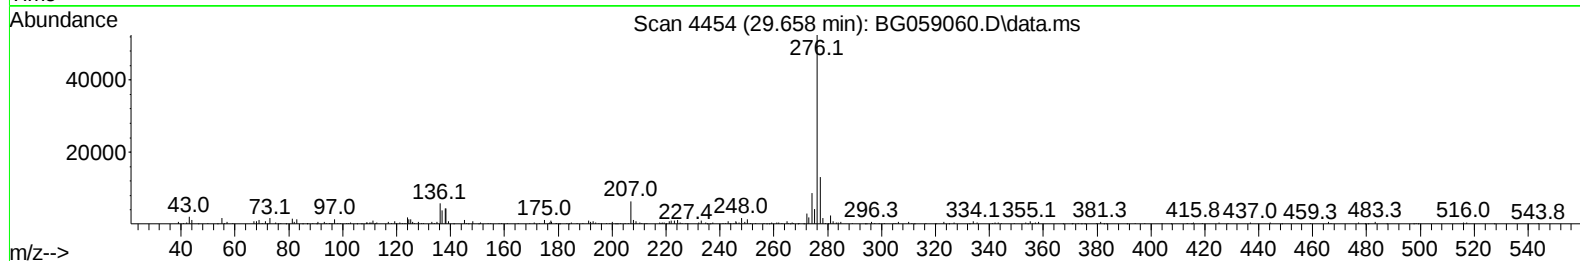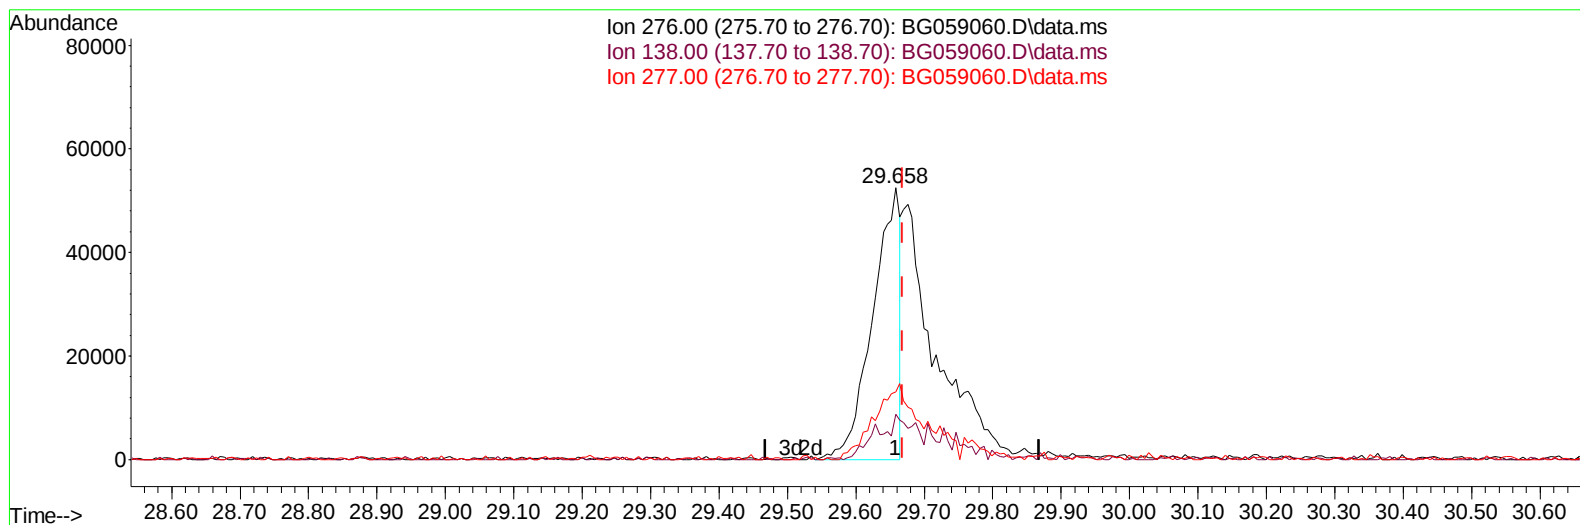

TIC: BG059060.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

29.658min (-0.010) 1.98 ng/u1

response 144795

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	12.90	16.67#
277.00	20.90	24.97
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
 Data File : BG059060.D
 Acq On : 14 Sep 2023 11:46
 Operator : MA/JU
 Sample : SST00513
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:42:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 14 15:36:44 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
 Supervised By :mohammad ahmed 09/15/2023

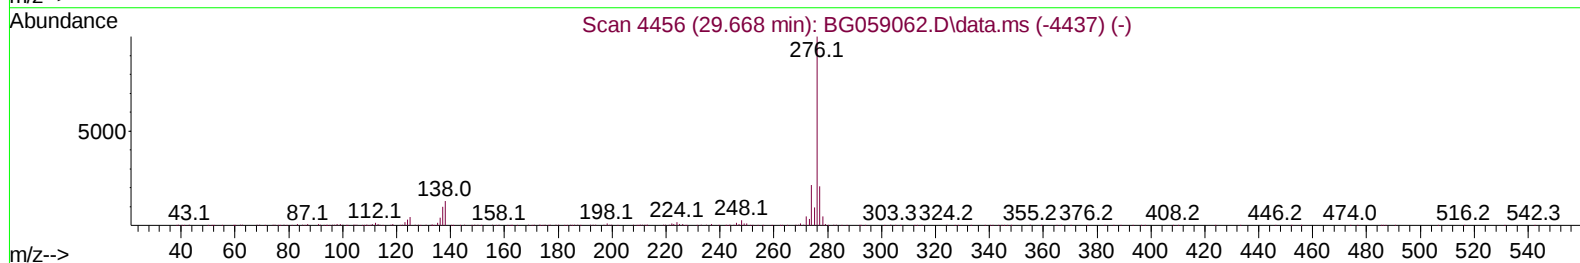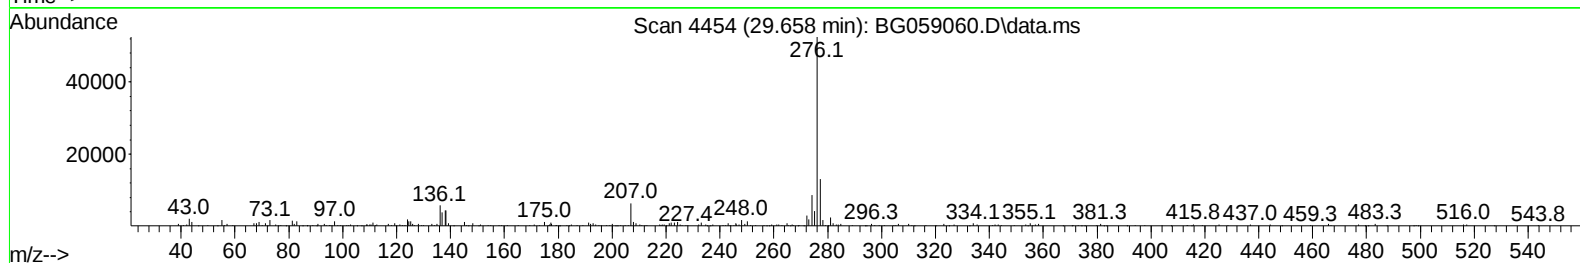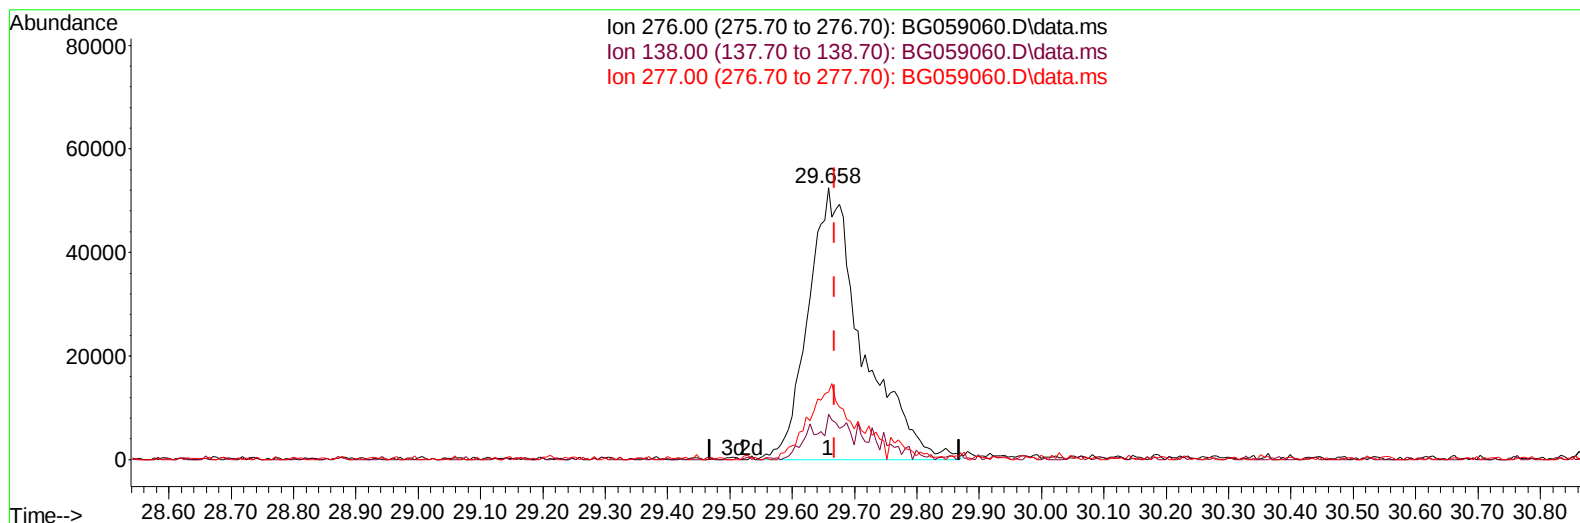

TIC: BG059060.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

29.658min (-0.010) 4.32 ng/ul m

response 316700

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	12.90	8.42#
277.00	20.90	24.97
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
 Data File : BG059060.D
 Acq On : 14 Sep 2023 11:46
 Operator : MA/JU
 Sample : SSTD00513
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:42:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 14 15:36:44 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
 Supervised By :mohammad ahmed 09/15/2023

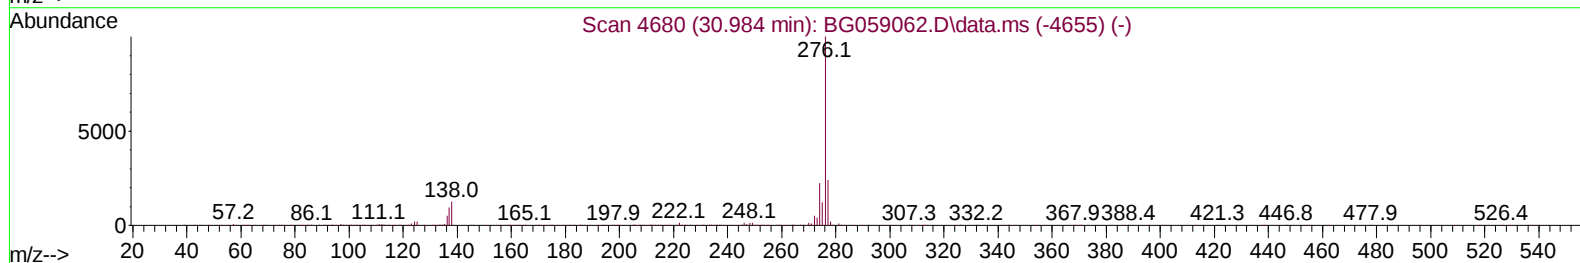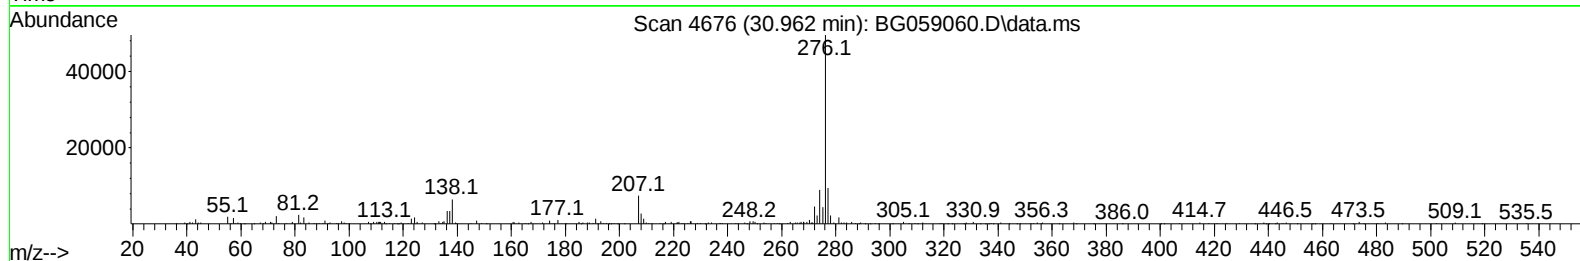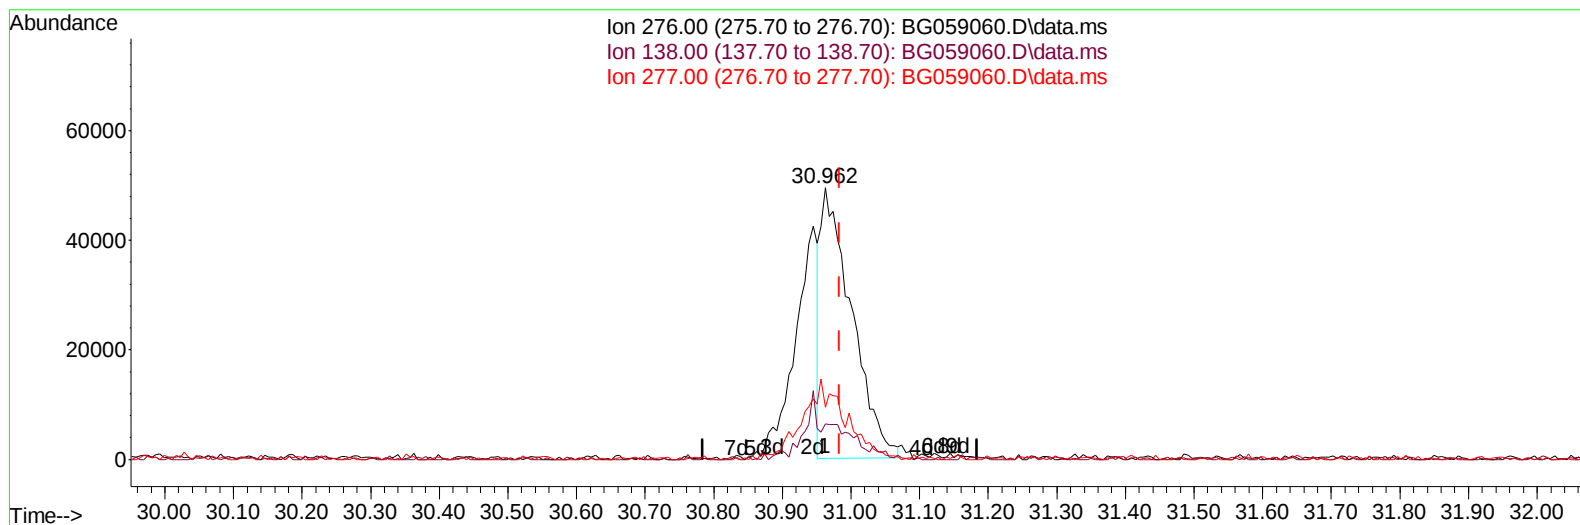

TIC: BG059060.D\data.ms

(96) Benzo(g,h,i)perylene

30.962min (-0.022) 2.60 ng/u1

response 153620

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	12.40	13.16
277.00	24.10	19.18#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
 Data File : BG059060.D
 Acq On : 14 Sep 2023 11:46
 Operator : MA/JU
 Sample : SST00513
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:42:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 14 15:36:44 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
 Supervised By :mohammad ahmed 09/15/2023

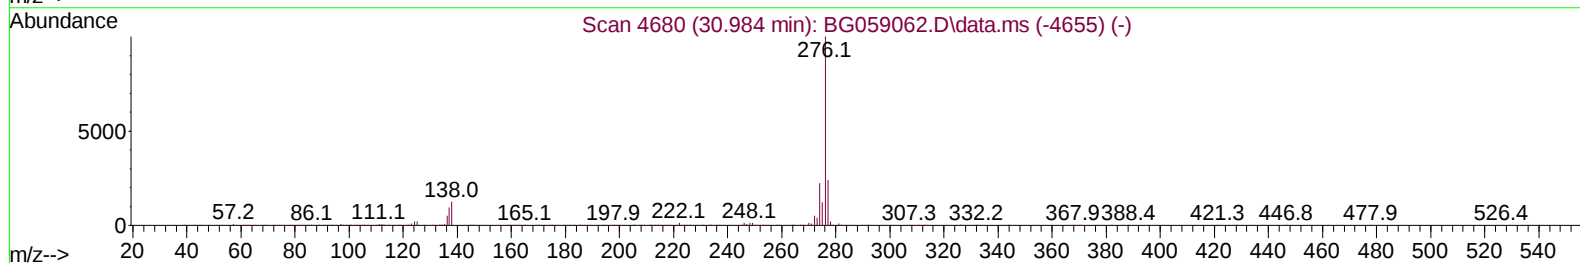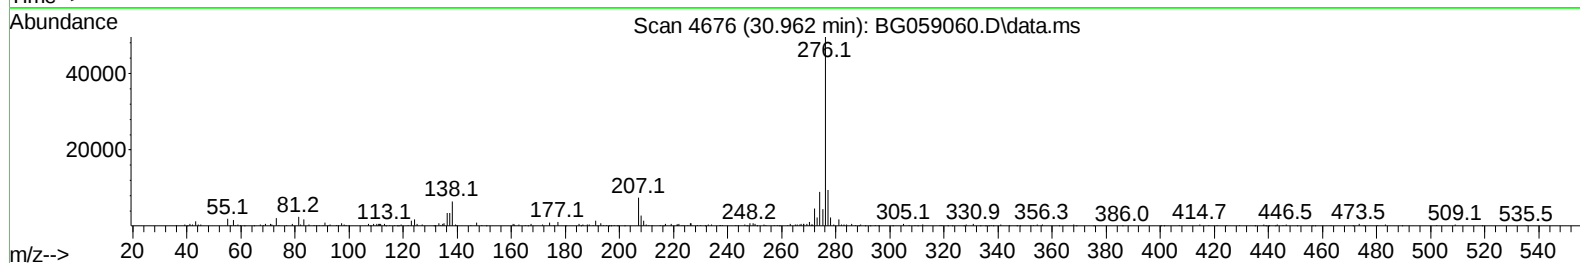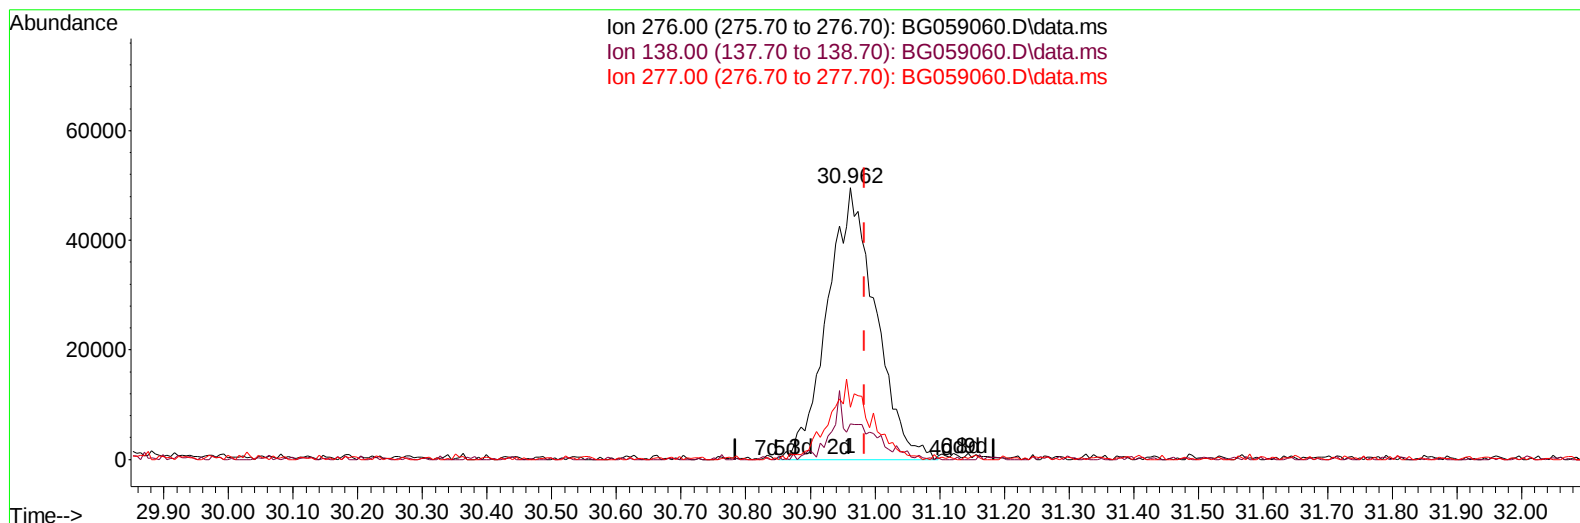

TIC: BG059060.D\data.ms

(96) Benzo(g,h,i)perylene

30.962min (-0.022) 4.34 ng/ul m

response 256391

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	12.40	13.16
277.00	24.10	19.18#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
 Data File : BG059060.D
 Acq On : 14 Sep 2023 11:46
 Operator : MA/JU
 Sample : SST00513
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST005414

Manual IntegrationsAPPROVED

Quant Time: Sep 14 15:43:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 14 15:36:44 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/15/2023
 Supervised By :mohammad ahmed 09/15/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.301	152	74040	20.000	ng/ul	0.00
20) Naphthalene-d8	11.144	136	332927	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.928	164	243295	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.678	188	686115m	20.000	ng/ul	0.00
79) Chrysene-d12	22.002	240	648219	20.000	ng/ul	0.00
88) Perylene-d12	25.557	264	987570	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.606	96	4955m	2.803	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	0.000	99	0d	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	0.000	67	0d	0.000	ng/ul	
11) 2-Chlorophenol-d4	7.819	132	21794	4.012	ng/ul	0.00
15) 4-Methylphenol-d8	0.000	113	0d	0.000	ng/ul	
21) Nitrobenzene-d5	9.488	128	12385	4.663	ng/ul	0.00
24) 2-Nitrophenol-d4	10.210	143	14565	4.236	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.745	165	27181m	4.258	ng/ul	0.00
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/ul	
46) Dimethylphthalate-d6	14.323	166	95493	4.412	ng/ul	0.00
49) Acenaphthylene-d8	14.634	160	99536	4.218	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.915	176	88917	4.461	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.778	188	152610	4.553	ng/ul	0.00
81) Pyrene-d10	20.052	212	171191	4.397	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.304	264	225767	4.271	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.647	88	7213m	3.323	ng/uL	
12) 2-Chlorophenol	7.842	128	24094	4.696	ng/ul	97
17) N-Nitroso-di-n-propyla...	9.100	70	26855	4.462	ng/ul#	86
19) Hexachloroethane	9.388	117	11029	4.984	ng/ul	94
22) Nitrobenzene	9.540	77	36423	4.580	ng/ul#	81
23) Isophorone	10.046	82	84303	4.890	ng/ul	98
25) 2-Nitrophenol	10.251	139	14541	4.516	ng/ul	91
26) 2,4-Dimethylphenol	10.269	107	34195	4.444	ng/ul	97
27) Bis(2-Chloroethoxy)met...	10.527	93	39020	4.542	ng/ul#	85
29) 2,4-Dichlorophenol	10.768	162	23768	3.865	ng/ul#	81
30) Naphthalene	11.197	128	73679	3.835	ng/ul#	95
33) Hexachlorobutadiene	11.432	225	18184	3.868	ng/ul#	87
35) 4-Chloro-3-methylphenol	12.378	107	32856	4.092	ng/ul#	84
36) 2-Methylnaphthalene	12.784	142	54697	3.704	ng/ul	93
37) 1-Methylnaphthalene	12.995	142	58519	3.917	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	13.119	216	35369	4.192	ng/ul#	91
41) 2,4,6-Trichlorophenol	13.359	196	25253	4.556	ng/ul#	91
42) 2,4,5-Trichlorophenol	13.424	196	25414	4.134	ng/ul	93
43) 1,1'-Biphenyl	13.765	154	85925	4.339	ng/ul	98
44) 2-Chloronaphthalene	13.818	162	67034	4.484	ng/ul	94
45) 2-Nitroaniline	14.035	65	20807	3.981	ng/ul	92
47) Dimethylphthalate	14.370	163	92660	4.440	ng/ul	99
48) 2,6-Dinitrotoluene	14.511	165	17885	4.296	ng/ul#	77

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
 Data File : BG059060.D
 Acq On : 14 Sep 2023 11:46
 Operator : MA/JU
 Sample : SSTD00513
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD005414

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/15/2023
 Supervised By :mohammad ahmed 09/15/2023

Quant Time: Sep 14 15:43:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 14 15:36:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
50) Acenaphthylene	14.658	152	114763	4.513	ng/ul#	96
52) Acenaphthene	14.993	153	75694	4.480	ng/ul	94
56) Dibenzofuran	15.328	168	112522	4.480	ng/ul	95
57) 2,4-Dinitrotoluene	15.287	165	24661	3.886	ng/ul#	98
58) 2,3,4,6-Tetrachlorophenol	15.533	232	25875	3.846	ng/ul#	96
59) Diethylphthalate	15.716	149	94960	4.457	ng/ul	99
61) Fluorene	15.974	166	96042	4.534	ng/ul#	98
62) 4-Chlorophenyl-phenyle...	15.956	204	52940	4.598	ng/ul	95
67) N-Nitrosodiphenylamine	16.174	169	83166	4.450	ng/ul	95
68) 4-Bromophenyl-phenylether	16.855	248	39147	4.616	ng/ul	84
69) Hexachlorobenzene	16.949	284	41039	4.402	ng/ul	94
72) Phenanthrene	17.725	178	167731m	4.479	ng/ul	
74) Anthracene	17.813	178	175152	4.508	ng/ul	95
75) 1,2,3,4-Tetrachloroben...	13.724	216	40207	4.128	ng/uL	96
76) Pentachlorobenzene	15.222	250	43845	4.341	ng/uL	94
78) Di-n-butylphthalate	18.600	149	172919	4.601	ng/ul#	96
80) Fluoranthene	19.717	202	205576	4.533	ng/ul#	95
82) Pyrene	20.081	202	213328	4.578	ng/ul	97
83) Butylbenzylphthalate	20.945	149	73076	4.506	ng/ul	95
85) Benzo(a)anthracene	21.985	228	215074	4.557	ng/ul	95
86) Bis(2-ethylhexyl)phtha...	21.820	149	104510	4.412	ng/ul#	96
87) Chrysene	22.049	228	198902	4.479	ng/ul	99
90) Benzo(b)fluoranthene	24.405	252	269284	4.298	ng/ul	96
91) Benzo(k)fluoranthene	24.476	252	279656m	4.420	ng/ul	
93) Benzo(a)pyrene	25.387	252	253393	4.325	ng/ul#	96
94) Indeno(1,2,3-cd)pyrene	29.658	276	316700m	4.324	ng/ul	
95) Dibenzo(a,h)anthracene	29.740	278	241701	4.163	ng/ul#	90
96) Benzo(g,h,i)perylene	30.962	276	256391m	4.335	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091423\
 Data File : BG059060.D
 Acq On : 14 Sep 2023 11:46
 Operator : MA/JU
 Sample : SSTD00513
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD005414

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/15/2023
 Supervised By :mohammad ahmed 09/15/2023

Quant Time: Sep 14 15:43:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 14 15:36:44 2023
 Response via : Initial Calibration

