

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091523\
 Data File : BG059075.D
 Acq On : 15 Sep 2023 20:20
 Operator : MA/JU
 Sample : PB155284BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK284

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.607	34	37	43	rVB3	8582	12988	1.03%	0.104%
2	4.036	106	110	123	rBV	128671	217793	17.25%	1.751%
3	4.383	165	169	173	rVB4	2915	4334	0.34%	0.035%
4	4.506	187	190	193	rBV4	1248	2018	0.16%	0.016%
5	4.653	212	215	220	rBV4	1481	1984	0.16%	0.016%
6	6.016	445	447	450	rVB2	1741	1673	0.13%	0.013%
7	7.409	677	684	696	rVB	159889	271526	21.50%	2.182%
8	7.614	711	719	728	rBV	122520	214263	16.97%	1.722%
9	7.808	745	752	763	rBV	149174	265532	21.03%	2.134%
10	8.067	791	796	798	rBV2	1050	1674	0.13%	0.013%
11	8.296	829	835	842	rBV	114508	193475	15.32%	1.555%
12	8.977	943	951	961	rBV2	203779	352832	27.94%	2.836%
13	9.494	1031	1039	1048	rVB	161482	287861	22.79%	2.314%
14	10.211	1155	1161	1168	rBV	130949	227581	18.02%	1.829%
15	10.734	1243	1250	1259	rBV	195132	346282	27.42%	2.783%
16	11.140	1312	1319	1327	rVB	180991	330531	26.17%	2.657%
17	11.281	1334	1343	1351	rBV	217762	396559	31.40%	3.187%
18	12.697	1580	1584	1590	rVB2	3258	6084	0.48%	0.049%
19	13.754	1758	1764	1770	rVB	4986	8740	0.69%	0.070%
20	14.318	1855	1860	1866	rVB	424133	614923	48.69%	4.943%
21	14.630	1905	1913	1920	rBV	450811	705837	55.89%	5.673%
22	14.929	1957	1964	1972	rBV	316970	505221	40.01%	4.061%
23	15.094	1986	1992	2000	rBV	223466	354653	28.08%	2.851%
24	15.916	2125	2132	2139	rVB	617994	915413	72.49%	7.358%
25	16.016	2142	2149	2161	rBV	222665	328627	26.02%	2.641%
26	16.145	2169	2171	2177	rVB2	2385	3797	0.30%	0.031%
27	17.156	2339	2343	2347	rVB	1166	1843	0.15%	0.015%
28	17.203	2347	2351	2353	rBV	1283	1693	0.13%	0.014%
29	17.456	2393	2394	2402	rVB2	2163	2439	0.19%	0.020%
30	17.679	2424	2432	2438	rBV	416289	637916	50.51%	5.127%
31	17.773	2442	2448	2456	rBV	676756	1051014	83.22%	8.448%
32	18.596	2583	2588	2591	rVB2	1174	2170	0.17%	0.017%
33	18.784	2618	2620	2624	rBV3	1280	1781	0.14%	0.014%
34	19.612	2757	2761	2766	rVB3	9688	13548	1.07%	0.109%
35	19.677	2766	2772	2778	rBV	8788	15216	1.20%	0.122%
36	19.841	2795	2800	2803	rBV2	882	1907	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091523\
 Data File : BG059075.D
 Acq On : 15 Sep 2023 20:20
 Operator : MA/JU
 Sample : PB155284BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK284

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091523.MA.M
 Title : SVOA CALIBRATION

37	19.906	2808	2811	2815	rVV2	1571	1888	0.15%	0.015%
38	19.982	2821	2824	2827	rBV2	1911	2146	0.17%	0.017%
39	20.012	2827	2829	2830	rBV	2077	1826	0.14%	0.015%
40	20.053	2830	2836	2844	rVV	829693	1211148	95.91%	9.735%
41	20.499	2910	2912	2915	rBV	2677	1977	0.16%	0.016%
42	20.728	2947	2951	2953	rBV2	2761	3777	0.30%	0.030%
43	20.746	2953	2954	2956	rBV2	2498	2159	0.17%	0.017%
44	20.793	2958	2962	2963	rVV3	2744	2835	0.22%	0.023%
45	21.028	3001	3002	3004	rVB	3727	1906	0.15%	0.015%
46	21.710	3116	3118	3122	rBV5	2806	2795	0.22%	0.022%
47	21.774	3125	3129	3131	rBV4	3615	5441	0.43%	0.044%
48	21.880	3144	3147	3149	rBV3	2945	3433	0.27%	0.028%
49	21.997	3160	3167	3176	rBV2	371238	646013	51.15%	5.192%
50	22.415	3236	3238	3241	rVB4	2566	2435	0.19%	0.020%
51	23.314	3389	3391	3394	rVB3	3000	2544	0.20%	0.020%
52	23.872	3485	3486	3490	rBV4	3192	3469	0.27%	0.028%
53	23.936	3495	3497	3499	rVB2	3193	1693	0.13%	0.014%
54	23.954	3499	3500	3502	rBV2	2881	1941	0.15%	0.016%
55	23.995	3505	3507	3510	rBV3	3002	2885	0.23%	0.023%
56	24.124	3527	3529	3532	rBV4	2742	3864	0.31%	0.031%
57	24.218	3543	3545	3546	rBV2	2582	1770	0.14%	0.014%
58	24.424	3575	3580	3586	rVB5	11299	24293	1.92%	0.195%
59	24.888	3657	3659	3662	rBV4	2847	2949	0.23%	0.024%
60	25.305	3717	3730	3745	rBV2	411234	1262861	100.00%	10.150%
61	25.435	3750	3752	3753	rVV	4593	3543	0.28%	0.028%
62	25.476	3753	3759	3760	rVV2	18512	32811	2.60%	0.264%
63	25.546	3762	3771	3784	rVB2	229510	729606	57.77%	5.864%
64	25.828	3817	3819	3820	rBV2	3119	2658	0.21%	0.021%
65	26.110	3863	3867	3868	rBV3	8098	9526	0.75%	0.077%
66	26.727	3968	3972	3984	rVB5	20249	65312	5.17%	0.525%
67	28.249	4222	4231	4238	rBV8	19746	69932	5.54%	0.562%
68	28.695	4305	4307	4310	rVB4	5105	3034	0.24%	0.024%
69	28.725	4310	4312	4315	rBV4	4726	5773	0.46%	0.046%
70	29.683	4474	4475	4476	rBV	6052	2703	0.21%	0.022%
71	30.047	4535	4537	4538	rBV2	5730	3393	0.27%	0.027%
72	31.128	4719	4721	4722	rBV2	4154	2540	0.20%	0.020%
73	31.163	4725	4727	4729	rBV3	3661	2880	0.23%	0.023%
74	31.692	4815	4817	4818	rBV2	4562	3596	0.28%	0.029%
75	32.086	4883	4884	4886	rBV	4357	4321	0.34%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091523\
Data File : BG059075.D
Acq On : 15 Sep 2023 20:20
Operator : MA/JU
Sample : PB155284BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK284

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091523.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 12441404

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091523\
Data File : BG059075.D
Acq On : 15 Sep 2023 20:20
Operator : MA/JU
Sample : PB155284BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK284

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

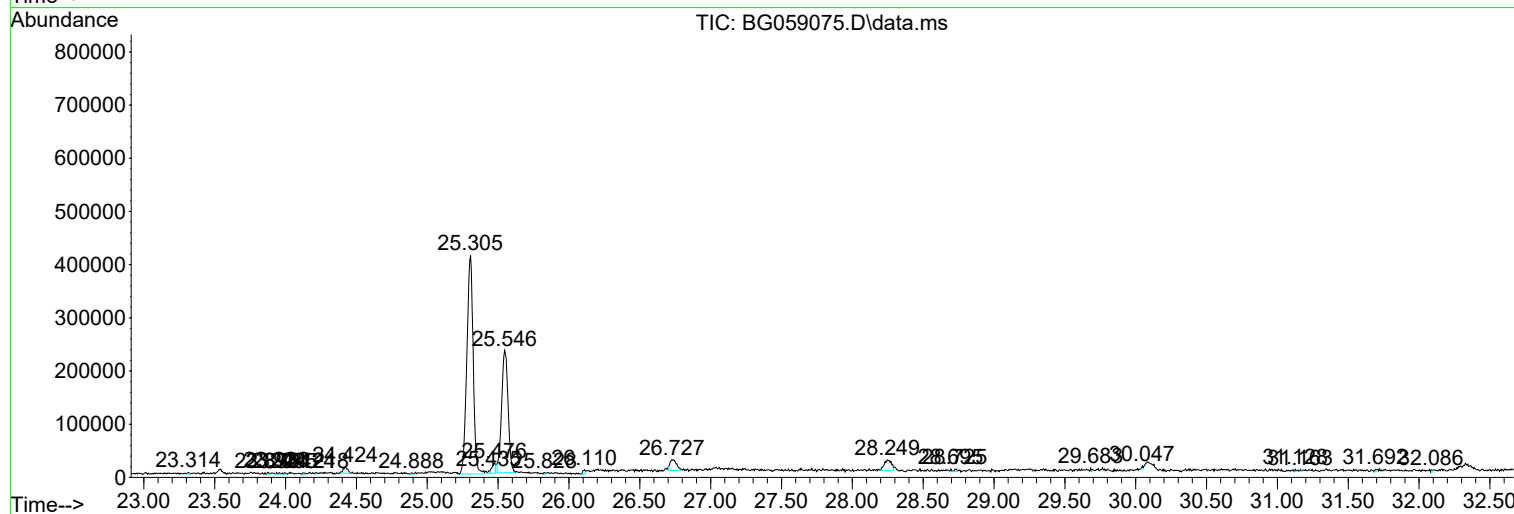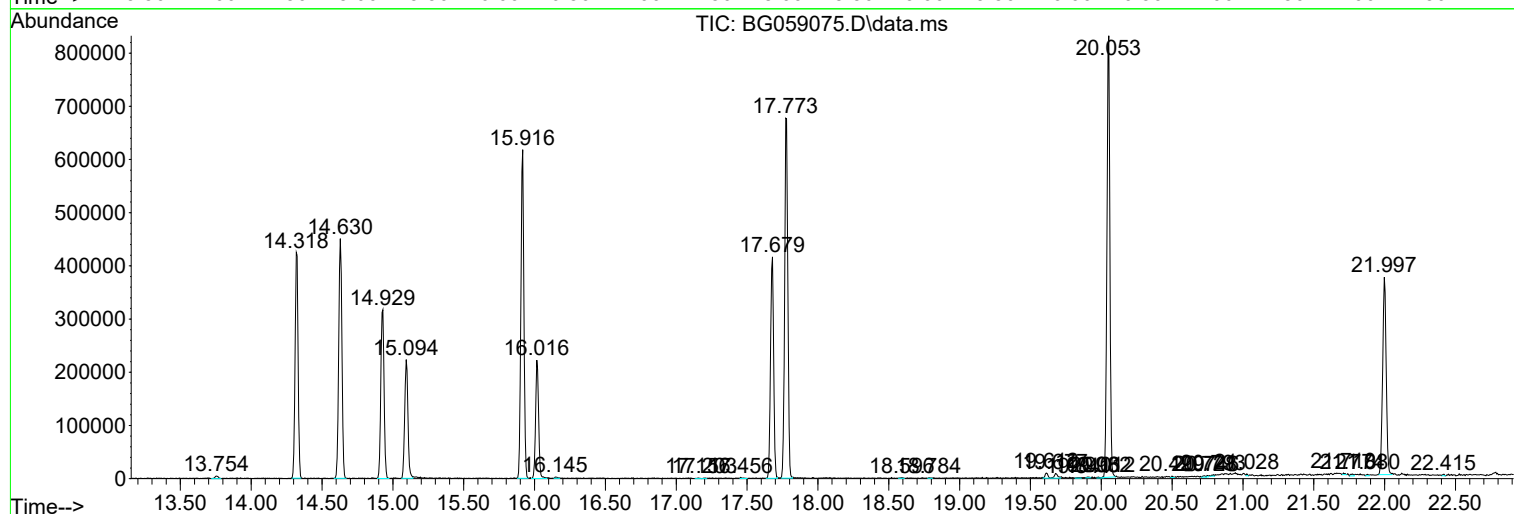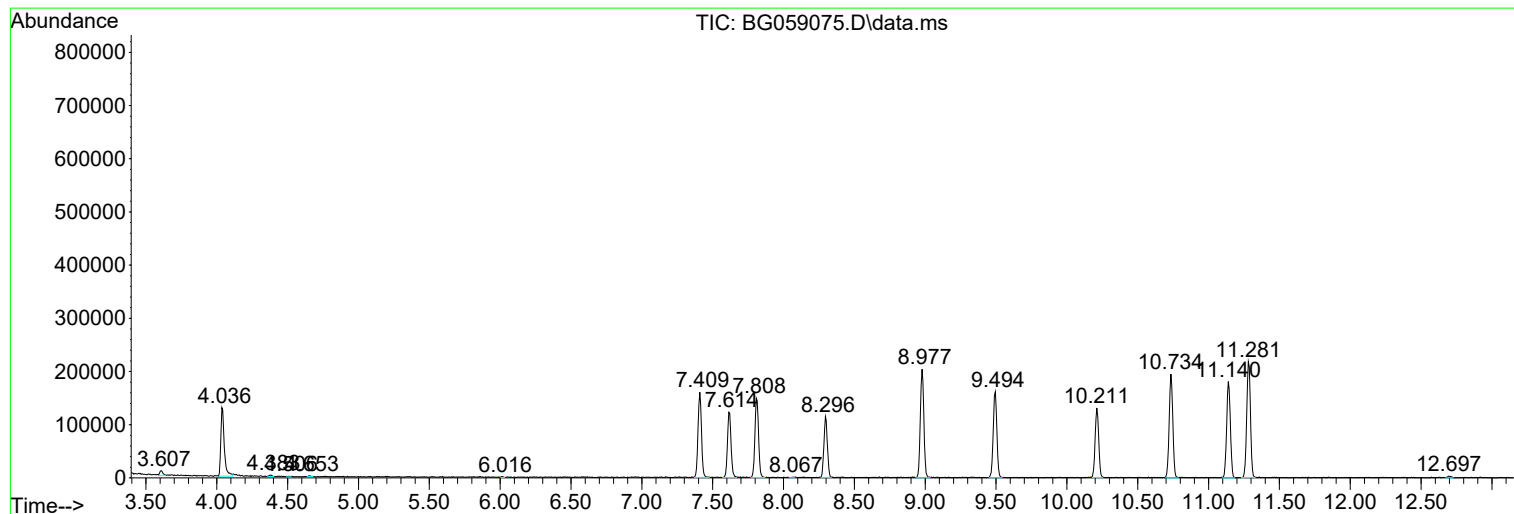

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091523\
Data File : BG059075.D
Acq On : 15 Sep 2023 20:20
Operator : MA/JU
Sample : PB155284BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK284

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091523\
Data File : BG059075.D
Acq On : 15 Sep 2023 20:20
Operator : MA/JU
Sample : PB155284BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK284

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc