

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091523\
 Data File : BG059076.D
 Acq On : 15 Sep 2023 21:02
 Operator : MA/JU
 Sample : PB155287BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK287

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.608	34	37	40	rVB3	6643	8296	0.51%	0.056%
2	4.037	106	110	120	rBV	120448	202613	12.49%	1.374%
3	4.225	139	142	143	rBV2	1668	2164	0.13%	0.015%
4	4.378	164	168	172	rBV4	4222	6939	0.43%	0.047%
5	5.253	315	317	320	rVB4	2420	2494	0.15%	0.017%
6	5.300	320	325	326	rBV4	1848	2438	0.15%	0.017%
7	5.917	426	430	433	rBV4	2000	2921	0.18%	0.020%
8	7.409	677	684	693	rBV	193503	342346	21.11%	2.321%
9	7.615	713	719	728	rBV	158546	266853	16.45%	1.809%
10	7.809	745	752	761	rBV	180554	326768	20.15%	2.215%
11	7.885	763	765	768	rBV2	1435	2239	0.14%	0.015%
12	8.226	821	823	826	rVB	2340	2293	0.14%	0.016%
13	8.297	829	835	843	rVV	111210	198442	12.24%	1.345%
14	8.978	944	951	960	rVB	252356	435063	26.83%	2.950%
15	9.495	1030	1039	1048	rBV	198980	353095	21.77%	2.394%
16	10.212	1154	1161	1170	rVB	163455	282574	17.42%	1.916%
17	10.735	1241	1250	1261	rBV	243764	434524	26.79%	2.946%
18	11.140	1312	1319	1328	rVB	188285	325062	20.04%	2.204%
19	11.281	1336	1343	1353	rVB	274614	500716	30.87%	3.395%
20	11.534	1382	1386	1389	rBV	1711	2666	0.16%	0.018%
21	11.963	1456	1459	1461	rBV	1390	2262	0.14%	0.015%
22	12.697	1581	1584	1590	rVB2	4814	6625	0.41%	0.045%
23	12.880	1610	1615	1618	rBV	1791	2537	0.16%	0.017%
24	13.467	1712	1715	1719	rBV2	1545	2225	0.14%	0.015%
25	13.749	1760	1763	1773	rVB3	6866	12046	0.74%	0.082%
26	14.319	1853	1860	1868	rBV	539177	768316	47.37%	5.209%
27	14.448	1880	1882	1887	rVB2	1390	2214	0.14%	0.015%
28	14.630	1905	1913	1920	rBV	555948	871422	53.73%	5.908%
29	14.713	1923	1927	1930	rBV	1686	2301	0.14%	0.016%
30	14.924	1956	1963	1973	rBV	315715	492344	30.36%	3.338%
31	15.018	1973	1979	1981	rBV2	2029	2979	0.18%	0.020%
32	15.095	1986	1992	2002	rBV	287891	471216	29.05%	3.195%
33	15.341	2031	2034	2036	rVB2	2934	3048	0.19%	0.021%
34	15.841	2114	2119	2124	rVB	1456	2714	0.17%	0.018%
35	15.917	2124	2132	2141	rBV	712227	1148185	70.79%	7.784%
36	16.017	2143	2149	2158	rBV	281557	419146	25.84%	2.842%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091523\
 Data File : BG059076.D
 Acq On : 15 Sep 2023 21:02
 Operator : MA/JU
 Sample : PB155287BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK287

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091523.MA.M
 Title : SVOA CALIBRATION

37	16.146	2168	2171	2176	rVB3	3899	5242	0.32%	0.036%
38	16.528	2233	2236	2240	rBV	2095	2721	0.17%	0.018%
39	16.693	2259	2264	2269	rVB2	1766	3462	0.21%	0.023%
40	16.775	2274	2278	2281	rBV2	1912	2219	0.14%	0.015%

41	17.468	2395	2396	2403	rVB3	2589	2422	0.15%	0.016%
42	17.615	2417	2421	2424	rVB2	1789	2274	0.14%	0.015%
43	17.680	2424	2432	2438	rBV	414887	639458	39.43%	4.335%
44	17.774	2442	2448	2461	rVB2	846124	1346829	83.04%	9.131%
45	18.708	2603	2607	2608	rBV	1887	2444	0.15%	0.017%

46	19.037	2659	2663	2665	rVB	1791	2152	0.13%	0.015%
47	19.437	2730	2731	2734	rBV	2107	2268	0.14%	0.015%
48	19.613	2757	2761	2765	rBV2	12714	19309	1.19%	0.131%
49	19.683	2768	2773	2778	rVV2	9559	14992	0.92%	0.102%
50	20.048	2829	2835	2843	rBV	1100226	1592683	98.20%	10.798%

51	20.283	2871	2875	2876	rBV3	2782	3056	0.19%	0.021%
52	20.335	2881	2884	2886	rBV2	1889	2817	0.17%	0.019%
53	20.541	2917	2919	2923	rBV4	2785	2825	0.17%	0.019%
54	20.576	2923	2925	2928	rVB4	2589	2121	0.13%	0.014%
55	20.612	2928	2931	2933	rBV3	2994	3441	0.21%	0.023%

56	20.788	2957	2961	2963	rBV5	2820	3222	0.20%	0.022%
57	21.041	3003	3004	3008	rBV3	3992	3514	0.22%	0.024%
58	21.845	3139	3141	3143	rBV3	3664	3640	0.22%	0.025%
59	21.998	3159	3167	3175	rBV2	381603	675388	41.64%	4.579%
60	22.081	3179	3181	3184	rVB4	5152	4124	0.25%	0.028%

61	22.345	3224	3226	3228	rVB2	3994	2681	0.17%	0.018%
62	22.539	3257	3259	3260	rBV2	3845	2538	0.16%	0.017%
63	23.250	3377	3380	3381	rBV2	4198	5575	0.34%	0.038%
64	24.019	3509	3511	3512	rBV2	3739	2527	0.16%	0.017%
65	24.272	3552	3554	3556	rBV3	3964	4067	0.25%	0.028%

66	24.413	3573	3578	3579	rBV6	11708	14695	0.91%	0.100%
67	24.977	3673	3674	3676	rBV2	4966	2554	0.16%	0.017%
68	25.306	3718	3730	3740	rBV2	534744	1621851	100.00%	10.996%
69	25.447	3752	3754	3755	rBV2	7546	5547	0.34%	0.038%
70	25.465	3755	3757	3758	rBV2	14358	13137	0.81%	0.089%

71	25.547	3763	3771	3786	rVB	239587	732835	45.19%	4.968%
72	27.627	4123	4125	4127	rBV3	4085	4843	0.30%	0.033%
73	27.768	4147	4149	4151	rBV3	4435	3179	0.20%	0.022%
74	28.097	4203	4205	4207	rBV2	3921	3472	0.21%	0.024%
75	28.256	4224	4232	4243	rVB4	20387	69184	4.27%	0.469%

76	28.638	4295	4297	4300	rBV4	4469	3358	0.21%	0.023%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091523\
Data File : BG059076.D
Acq On : 15 Sep 2023 21:02
Operator : MA/JU
Sample : PB155287BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK287

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091523.MA.M
Title : SVOA CALIBRATION

77	29.824	4497	4499	4501	rBV3	3783	2128	0.13%	0.014%
78	31.223	4735	4737	4738	rBV2	4726	2763	0.17%	0.019%




Sum of corrected areas: 14749643

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091523\
Data File : BG059076.D
Acq On : 15 Sep 2023 21:02
Operator : MA/JU
Sample : PB155287BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK287

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

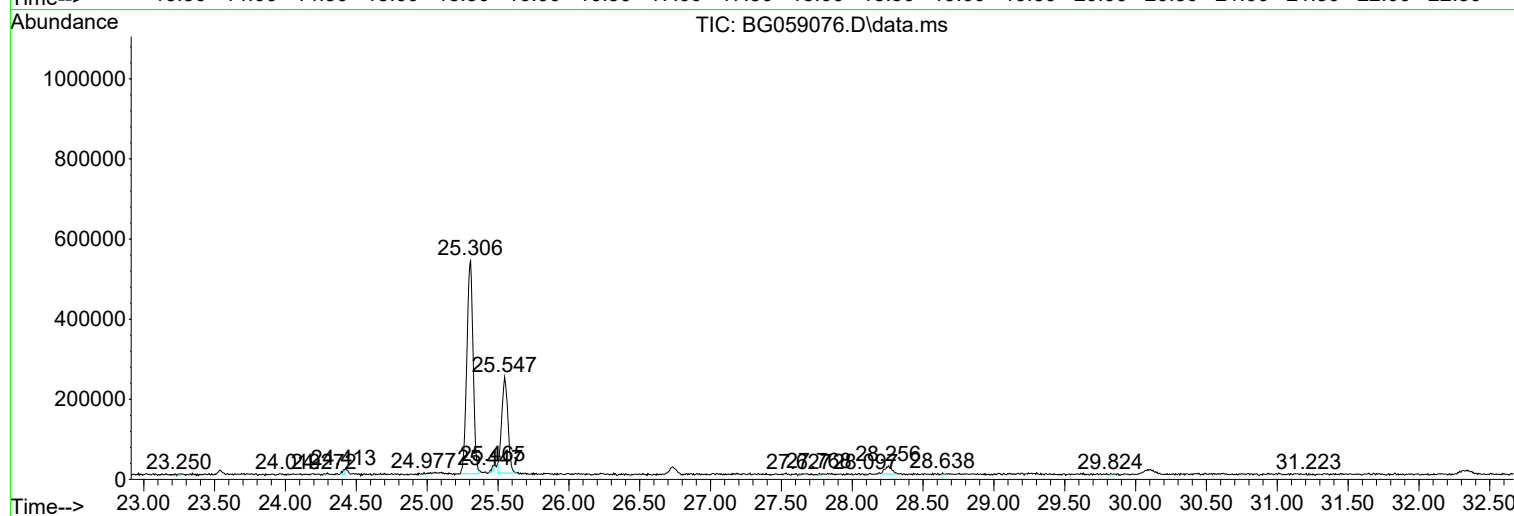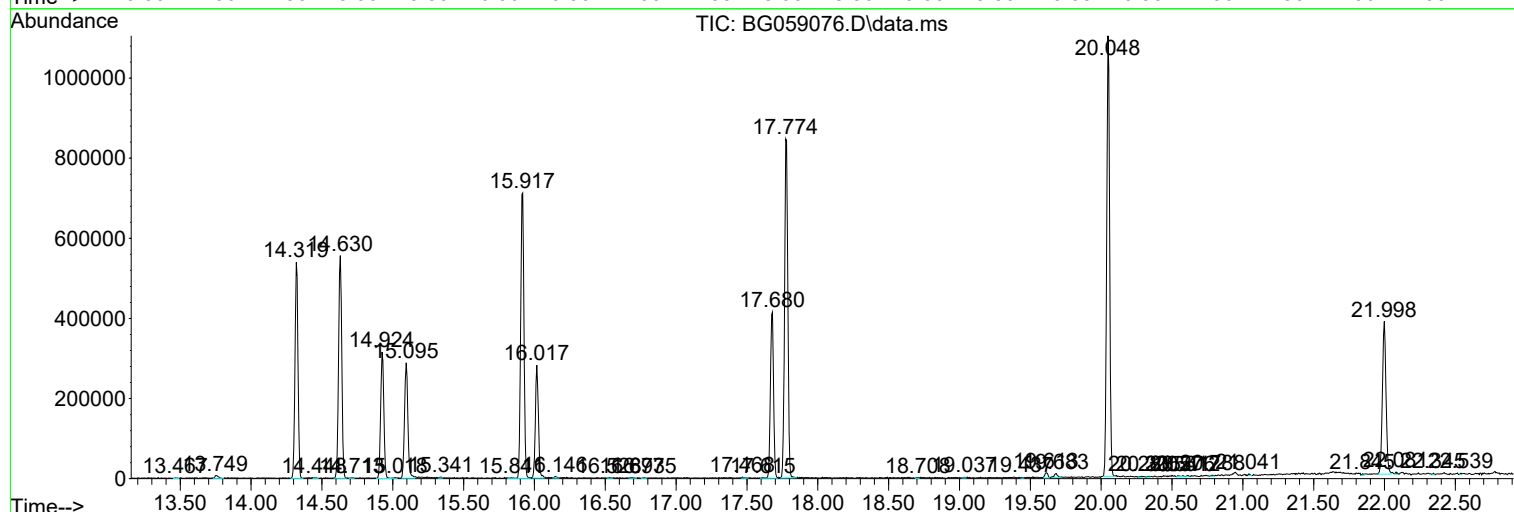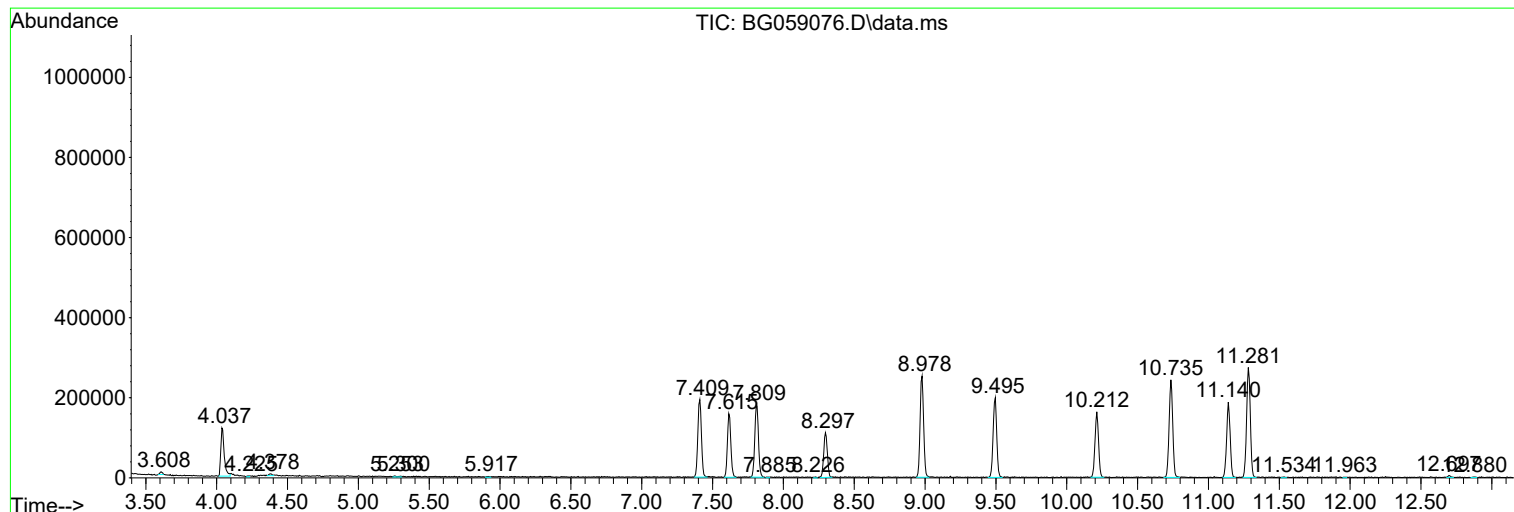

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091523\
Data File : BG059076.D
Acq On : 15 Sep 2023 21:02
Operator : MA/JU
Sample : PB155287BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK287

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091523\
Data File : BG059076.D
Acq On : 15 Sep 2023 21:02
Operator : MA/JU
Sample : PB155287BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK287

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc