

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091619\
 Data File : BG042847.D
 Acq On : 16 Sep 2019 13:24
 Operator : HP/JU
 Sample : PB123110BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB123110BL

Quant Time: Sep 17 02:19:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG091219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 12 14:06:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	81889	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	327666	20.00	ng	0.00
39) Acenaphthene-d10	14.74	164	240919	20.00	ng	0.00
64) Phenanthrene-d10	17.47	188	629790	20.00	ng	-0.01
76) Chrysene-d12	21.76	240	660178	20.00	ng	0.00
87) Perylene-d12	25.03	264	709064	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	534299	113.43	ng	0.00
7) Phenol-d6	7.27	99	809204	119.69	ng	0.00
23) Nitrobenzene-d5	9.27	82	486101	77.24	ng	-0.01
42) 2,4,6-Tribromophenol	16.22	330	385747	120.35	ng	0.00
45) 2-Fluorobiphenyl	13.36	172	1165714	76.59	ng	-0.01
79) Terphenyl-d14	20.08	244	2265374	76.05	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091619\
Data File : BG042847.D
Acq On : 16 Sep 2019 13:24
Operator : HP/JU
Sample : PB123110BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB123110BL

Quant Time: Sep 17 02:19:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG091219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 12 14:06:09 2019
Response via : Initial Calibration

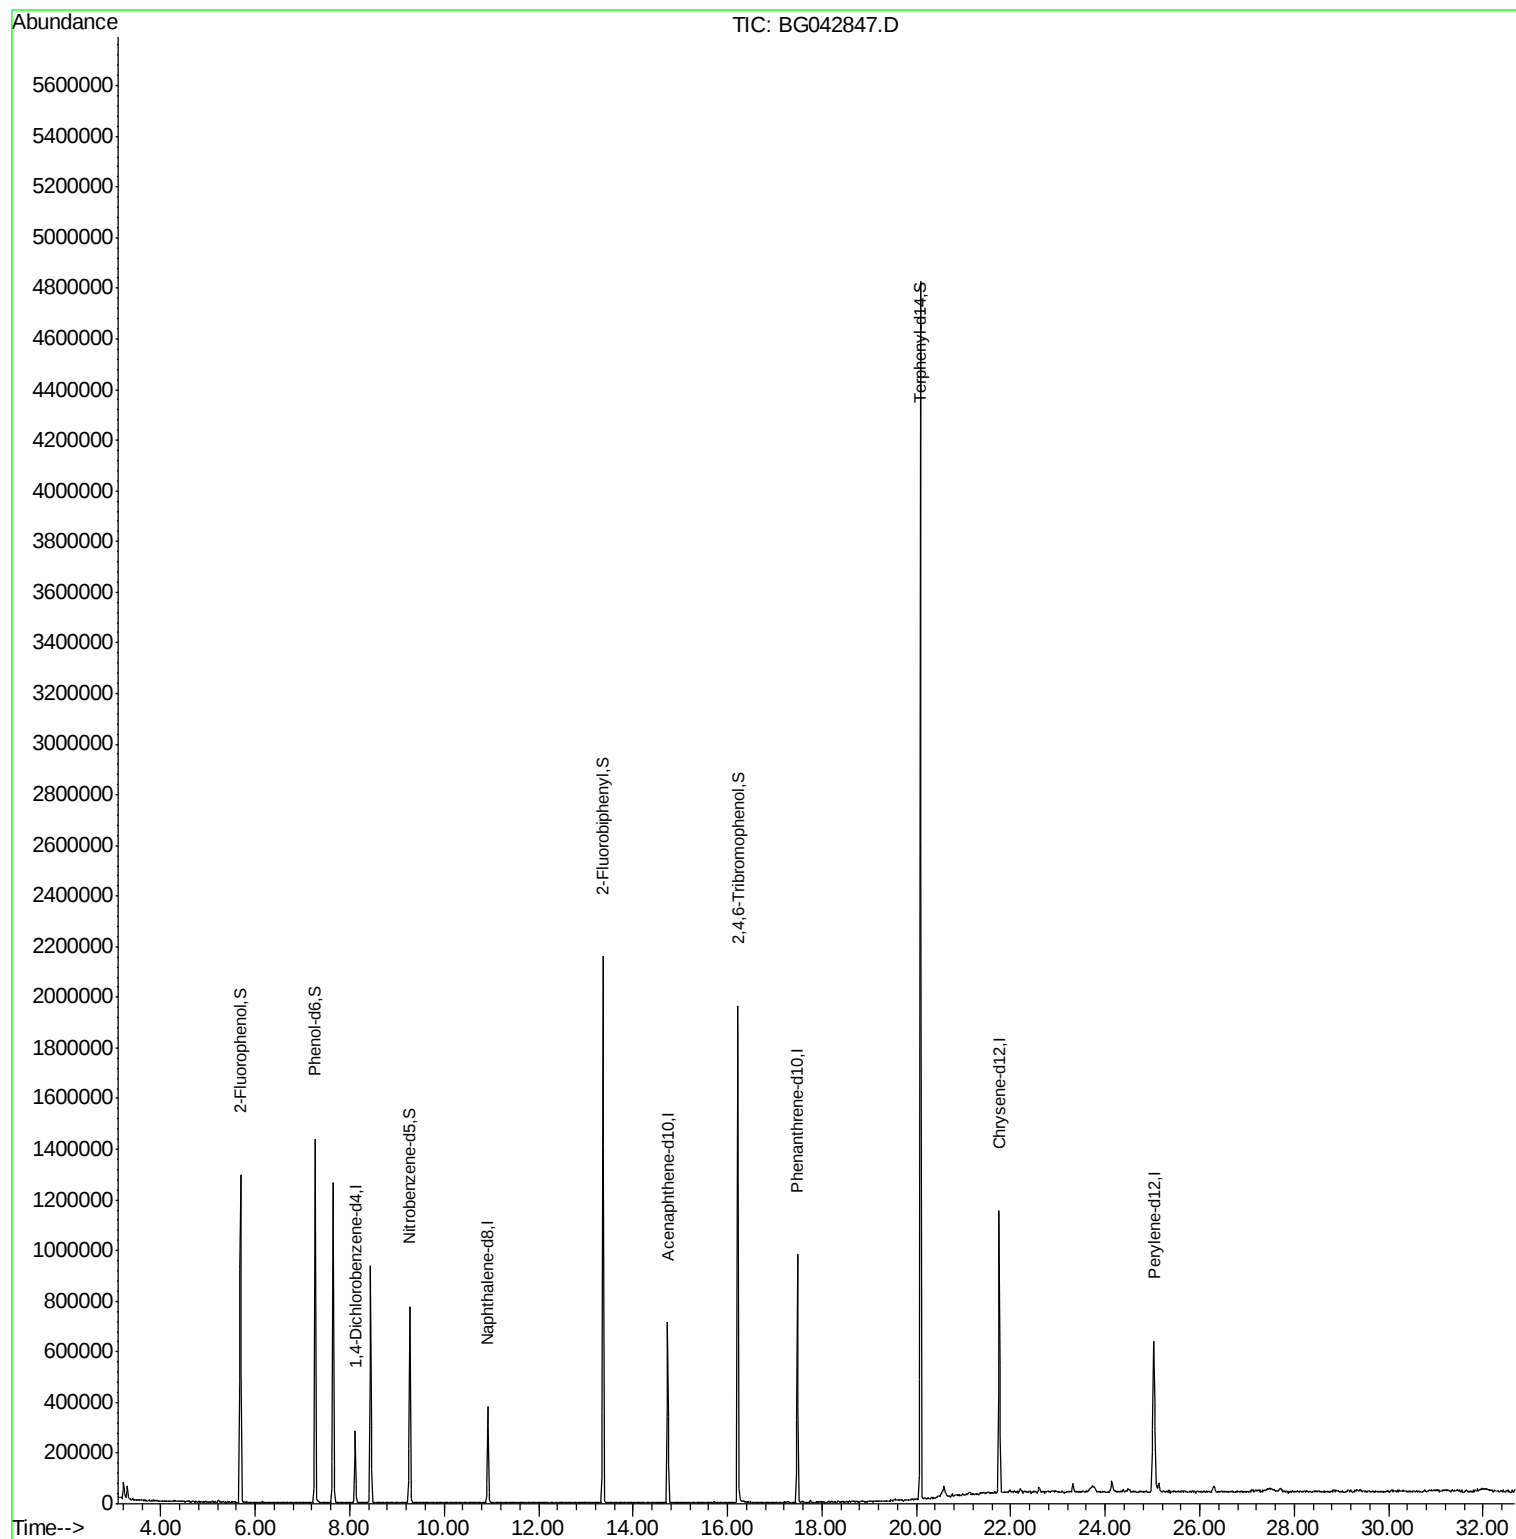




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.12 min Scan# 856
Delta R.T. -0.01 min
Lab File: BG042847.D
Acq: 16 Sep 2019 13:24

Instrument :
BNA_G
ClientSampleId :
PB123110BL

Tot Ion	Ratio	Lower	Upper
152	100		
150	158.6	118.9	178.3
115	63.2	47.4	71.2

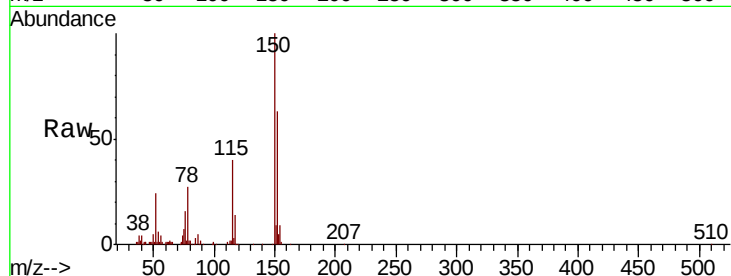


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

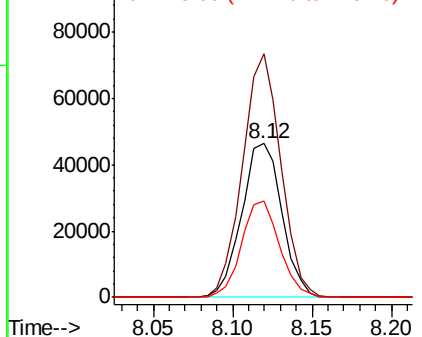



#5


2-Fluorophenol
Concen: 113.435 ng
RT: 5.69 min Scan# 442
Delta R.T. -0.00 min
Lab File: BG042847.D
Acq: 16 Sep 2019 13:24

Tgt Ion	Ratio	Lower	Upper
112	100		
64	72.7	60.2	90.2
63	37.7	31.2	46.8



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

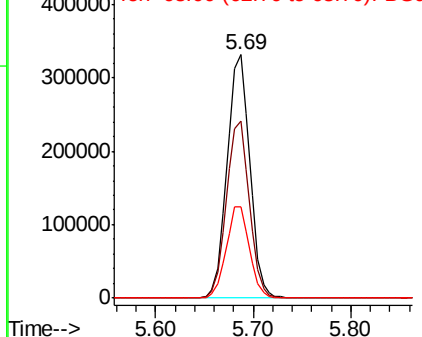

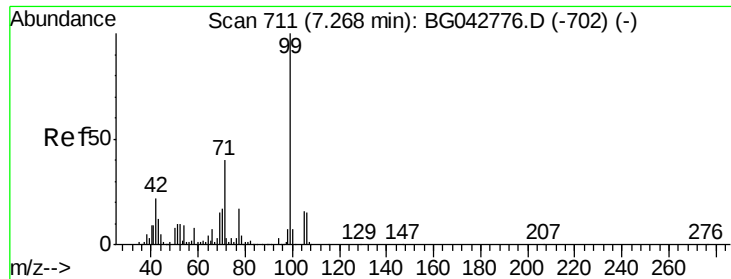

#7

Phenol-d6

Concen: 119.692 ng

RT: 7.27 min Scan# 711

Delta R.T. -0.00 min

Lab File: BG042847.D

Acq: 16 Sep 2019 13:24

Instrument :

BNA_G

ClientSampleId :

PB123110BL


Tot Ion: 99 Resp: 809204

Ion Ratio Lower Upper




99 100

42 19.5 17.5 26.3

71 38.6 32.0 48.0

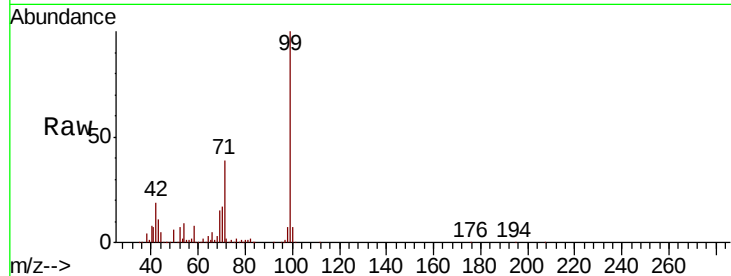

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

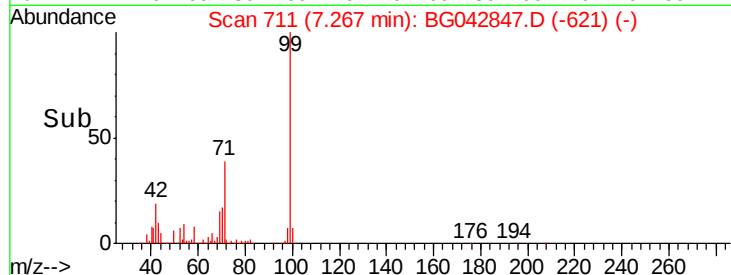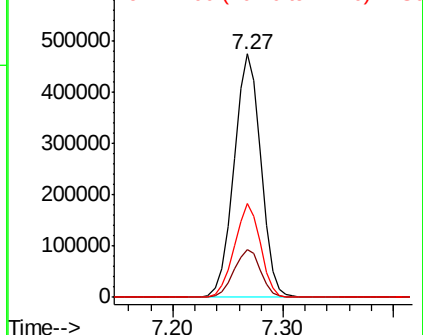

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.93 min Scan# 1334

Delta R.T. -0.01 min

Lab File: BG042847.D

Acq: 16 Sep 2019 13:24

Tgt Ion: 136 Resp: 327666


Ion Ratio Lower Upper

136 100



137 11.3 9.0 13.6


54 11.7 9.4 14.0

68 6.0 5.4 8.2



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

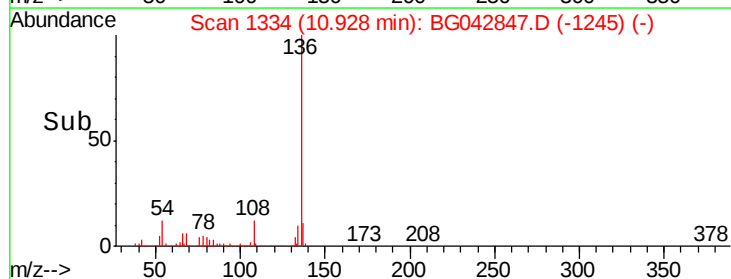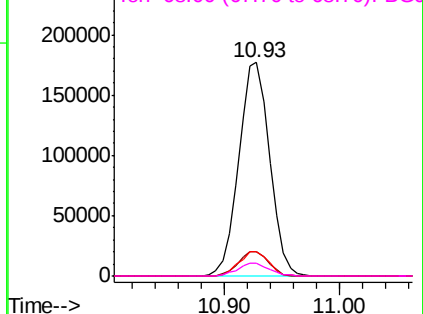







#23
 Nitrobenzene-d5
 Concen: 77.236 ng
 RT: 9.27 min Scan# 1052
 Delta R.T. -0.01 min
 Lab File: BG042847.D
 Acq: 16 Sep 2019 13:24

Instrument :
 BNA_G
 ClientSampleId :
 PB123110BL

Tot Ion	82	Resp	486101
Ion Ratio	Lower	Upper	
82	100		
128	37.6	29.8	44.8
54	52.4	46.1	69.1

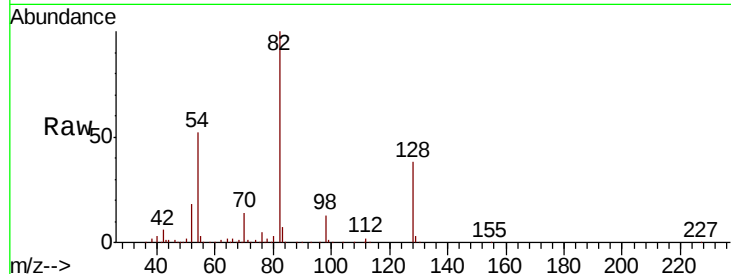


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

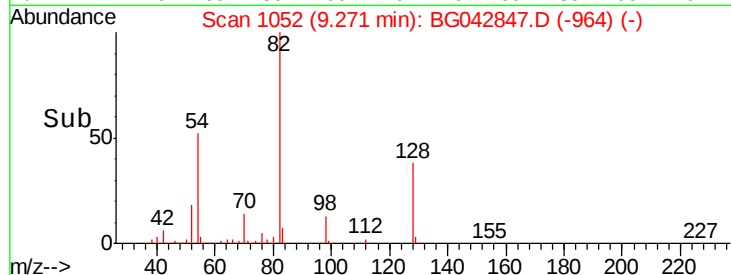
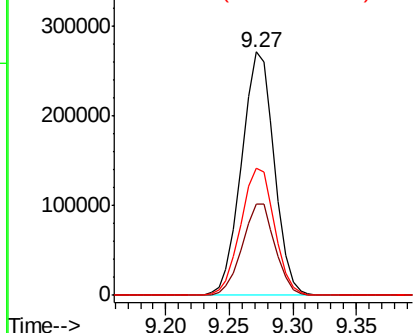



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.74 min Scan# 1982
 Delta R.T. -0.01 min
 Lab File: BG042847.D
 Acq: 16 Sep 2019 13:24

Tgt Ion	164	Resp	240919
Ion Ratio	Lower	Upper	
164	100		
162	101.9	84.6	126.8
160	45.9	34.2	51.2

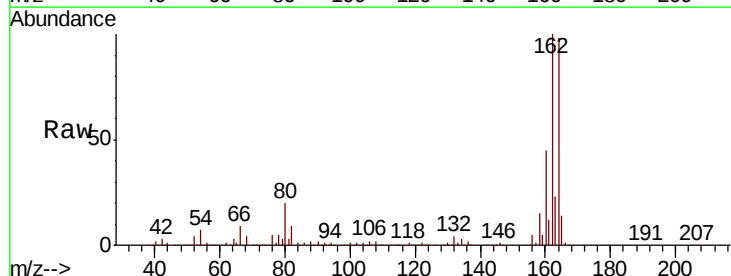

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

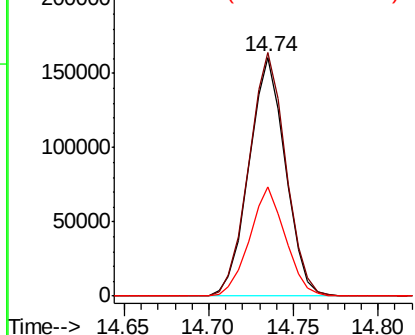


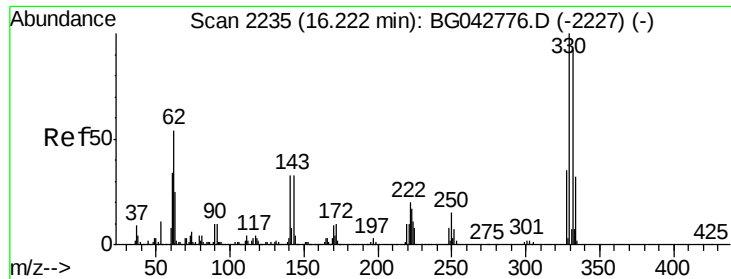

#42
 2,4,6-Tribromophenol
 Concen: 120.349 ng
 RT: 16.22 min Scan# 2234
 Delta R.T. -0.01 min
 Lab File: BG042847.D
 Acq: 16 Sep 2019 13:24

Instrument :
 BNA_G
 ClientSampleId :
 PB123110BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.3	76.7	115.1
141	34.6	27.0	40.6



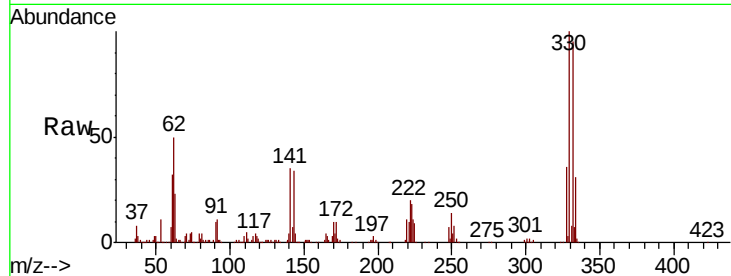


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

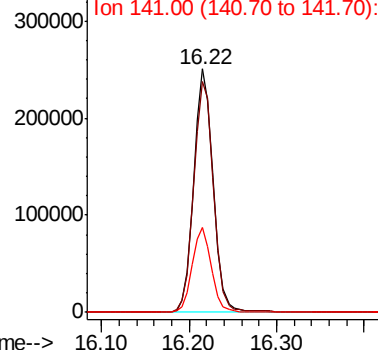

#45
 2-Fluorobiphenyl
 Concen: 76.592 ng
 RT: 13.36 min Scan# 1748
 Delta R.T. -0.01 min
 Lab File: BG042847.D
 Acq: 16 Sep 2019 13:24

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.9	28.9	43.3
170	24.4	19.1	28.7






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

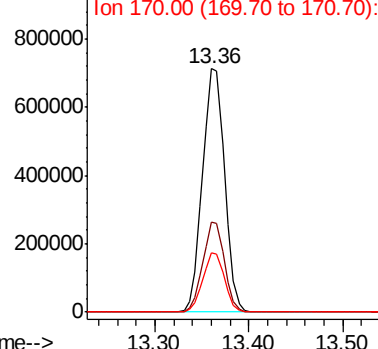



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.47 min Scan# 2448

Delta R.T. -0.01 min

Lab File: BG042847.D

Acq: 16 Sep 2019 13:24

Instrument :

BNA_G

ClientSampleId :

PB123110BL


Tot Ion:188 Resp: 629790

Ion Ratio Lower Upper

188 100

94 6.9 4.8 7.2




80 8.8 6.6 9.8

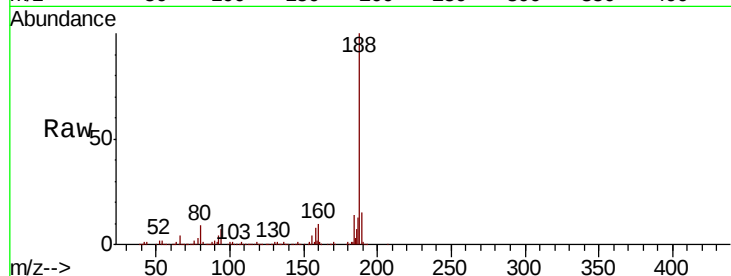

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG042847.D (-3088) (-)

Ion 80.00 (79.70 to 80.70): BG042847.D (-3088) (-)

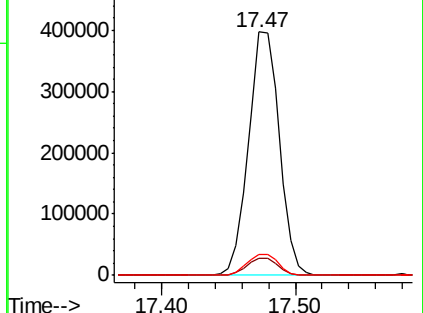

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.76 min Scan# 3177

Delta R.T. -0.01 min

Lab File: BG042847.D

Acq: 16 Sep 2019 13:24


Tgt Ion:240 Resp: 660178

Ion Ratio Lower Upper

240 100

120 6.7 5.4 8.2



236 27.3 21.7 32.5




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

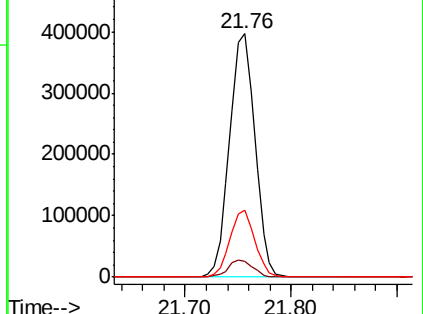

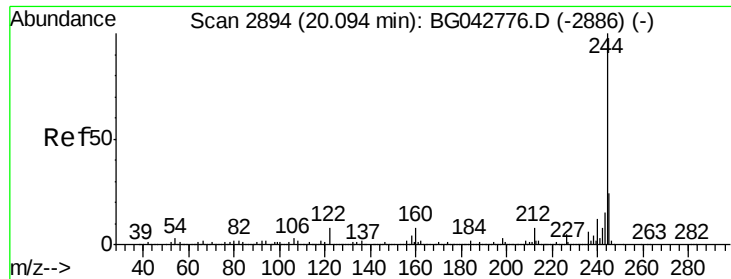

#79

Terphenyl-d14

Concen: 76.051 ng

RT: 20.08 min Scan# 2892

Delta R.T. -0.01 min

Lab File: BG042847.D

Acq: 16 Sep 2019 13:24

Instrument :

BNA_G

ClientSampleId :

PB123110BL


Tot Ion:244 Resp: 2265374

Ion Ratio Lower Upper

244 100

212 8.5 6.6 10.0




122 9.6 6.2 9.4#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

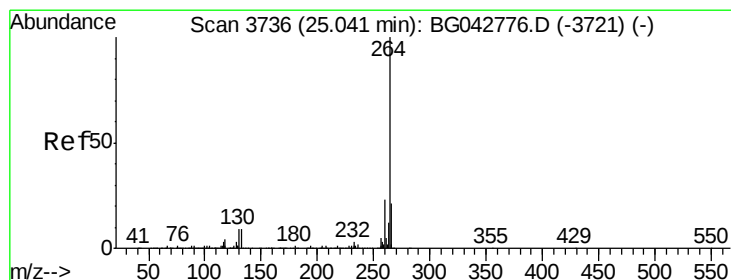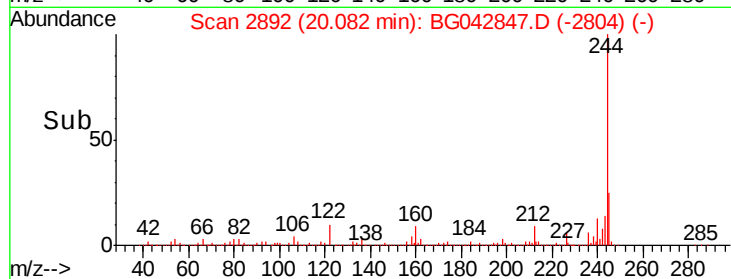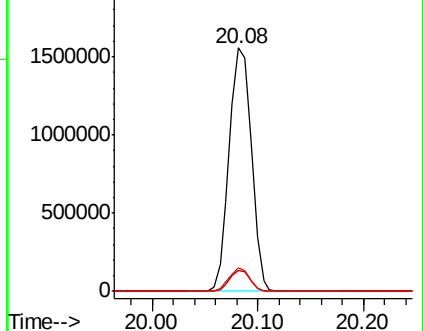

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.03 min Scan# 3734

Delta R.T. -0.01 min

Lab File: BG042847.D

Acq: 16 Sep 2019 13:24


Tgt Ion:264 Resp: 709064

Ion Ratio Lower Upper

264 100

260 23.2 18.2 27.2

265 21.1 16.9 25.3

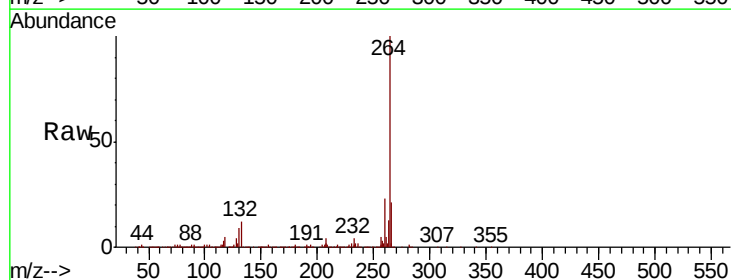

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

