
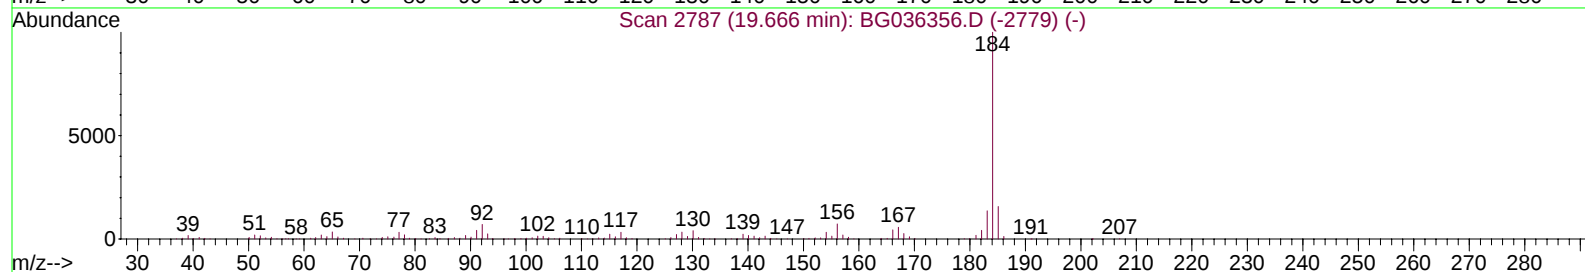
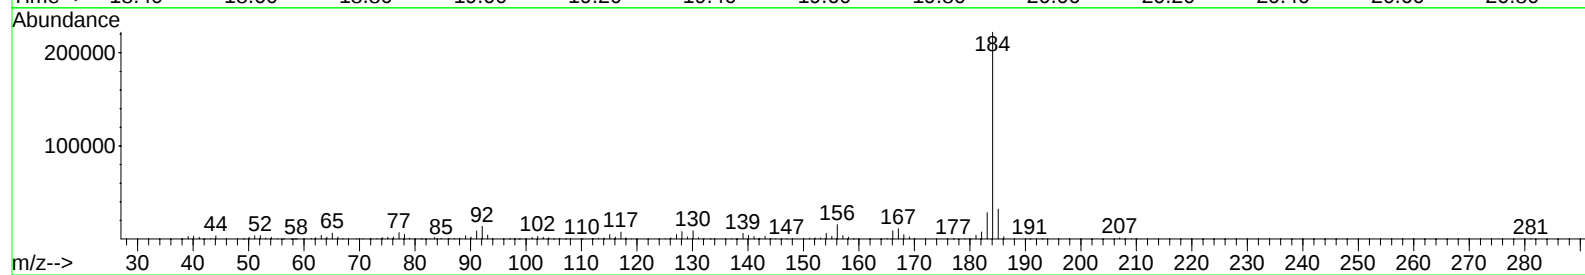


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091718\  
Data File : BG036747.D  
Acq On : 17 Sep 2018 10:12  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 13:30:53 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 31 13:03:20 2018  
Response via : Initial Calibration

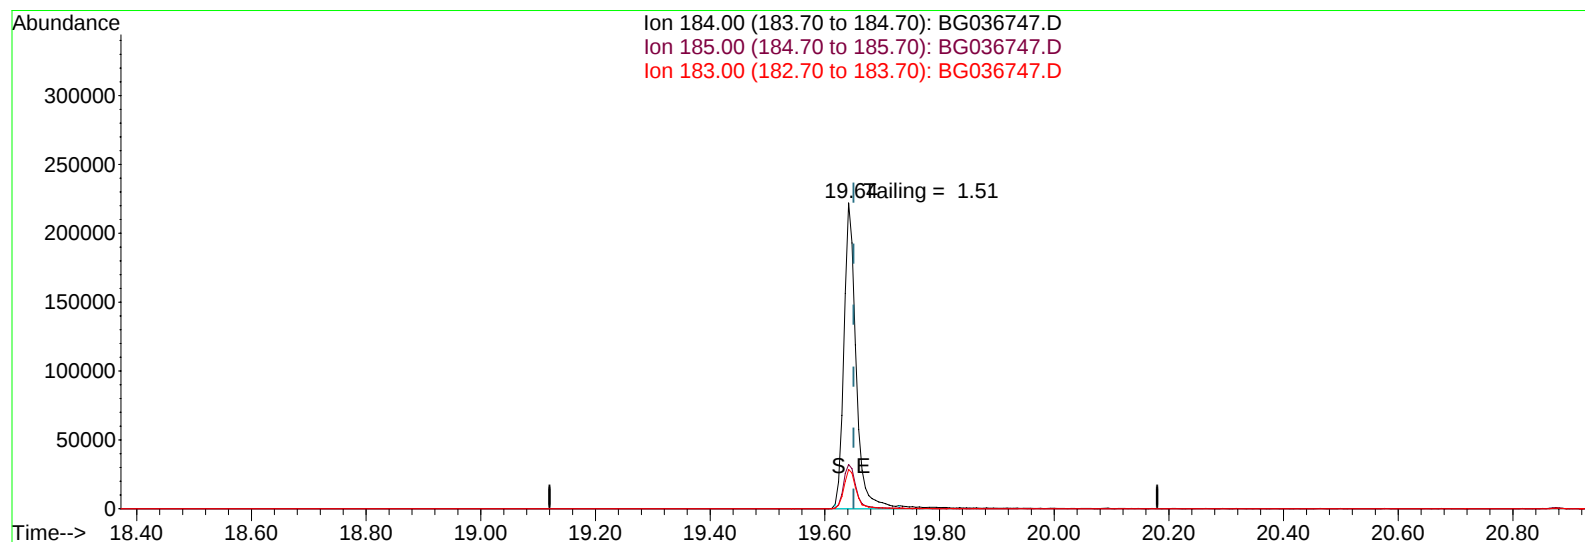

TIC: BG036747.D

(76) Benzidine




19.642min (-0.009) 12927.72ng

response 325837

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 14.48 |
| 183.00 | 13.60 | 12.87 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091718\  
Data File : BG036747.D  
Acq On : 17 Sep 2018 10:12  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 13:30:53 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 31 13:03:20 2018  
Response via : Initial Calibration

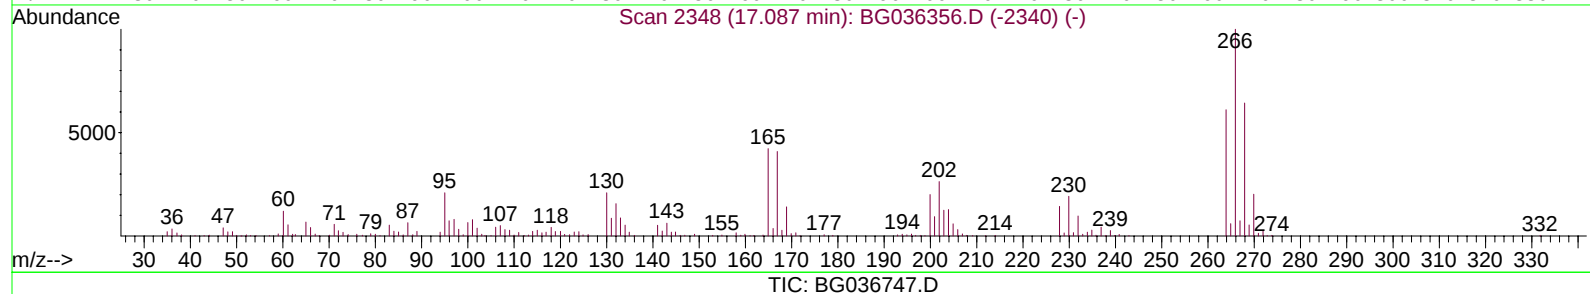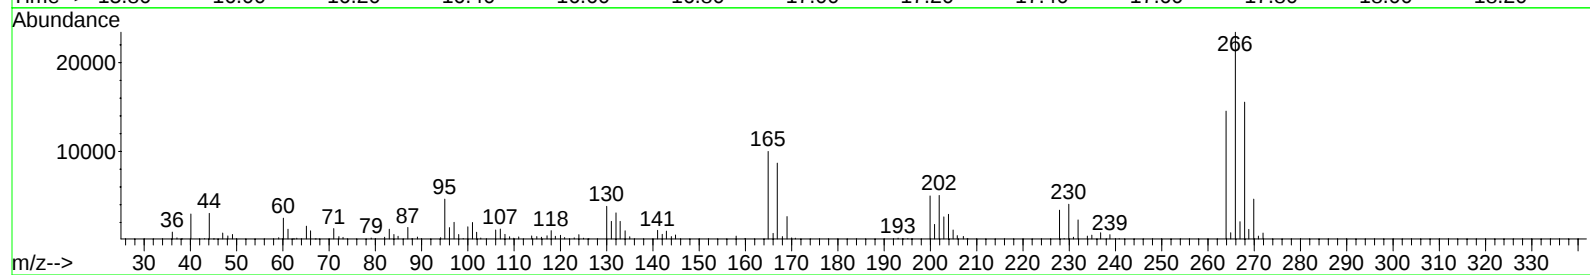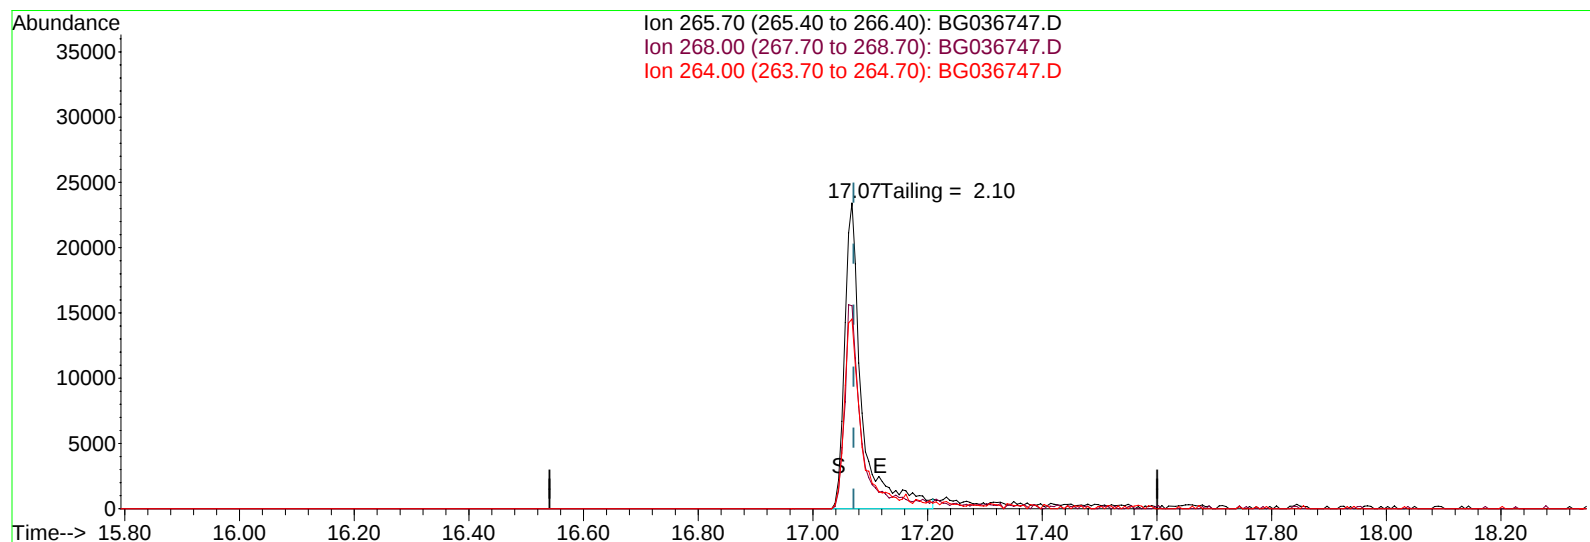

(69) Pentachlorophenol (C)

17.068min (-0.003) 11079.72ng

response 45706

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.30 | 66.39 |
| 264.00 | 61.10 | 62.06 |
| 0.00   | 0.00  | 0.00  |