

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091718\
 Data File : BG036768.D
 Acq On : 18 Sep 2018 1:25
 Operator : JU/SJ
 Sample : J4935-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PHASE-1-CONCRETE

Quant Time: Sep 18 07:22:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 31 13:03:20 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	61306	20.00	ng	-0.01
21) Naphthalene-d8	10.86	136	247513	20.00	ng	-0.01
38) Acenaphthene-d10	14.67	164	157442	20.00	ng	-0.01
63) Phenanthrene-d10	17.42	188	381255	20.00	ng	-0.01
75) Chrysene-d12	21.68	240	371786	20.00	ng	-0.01
86) Perylene-d12	24.89	264	332073	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	273164	70.68	ng	0.00
7) Phenol-d6	7.21	99	435334	78.67	ng	-0.01
23) Nitrobenzene-d5	9.21	82	284441	62.35	ng	-0.01
41) 2,4,6-Tribromophenol	16.16	330	120612	64.20	ng	-0.01
44) 2-Fluorobiphenyl	13.30	172	660909	59.94	ng	-0.01
78) Terphenyl-d14	20.03	244	1013857	63.74	ng	0.00
Target Compounds						
49) Dimethylphthalate	14.12	163	47680	3.709	ng	98
83) Bis(2-ethylhexyl)phthalate	21.57	149	43240	3.396	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091718\
Data File : BG036768.D
Acq On : 18 Sep 2018 1:25
Operator : JU/SJ
Sample : J4935-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PHASE-1-CONCRETE

Quant Time: Sep 18 07:22:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

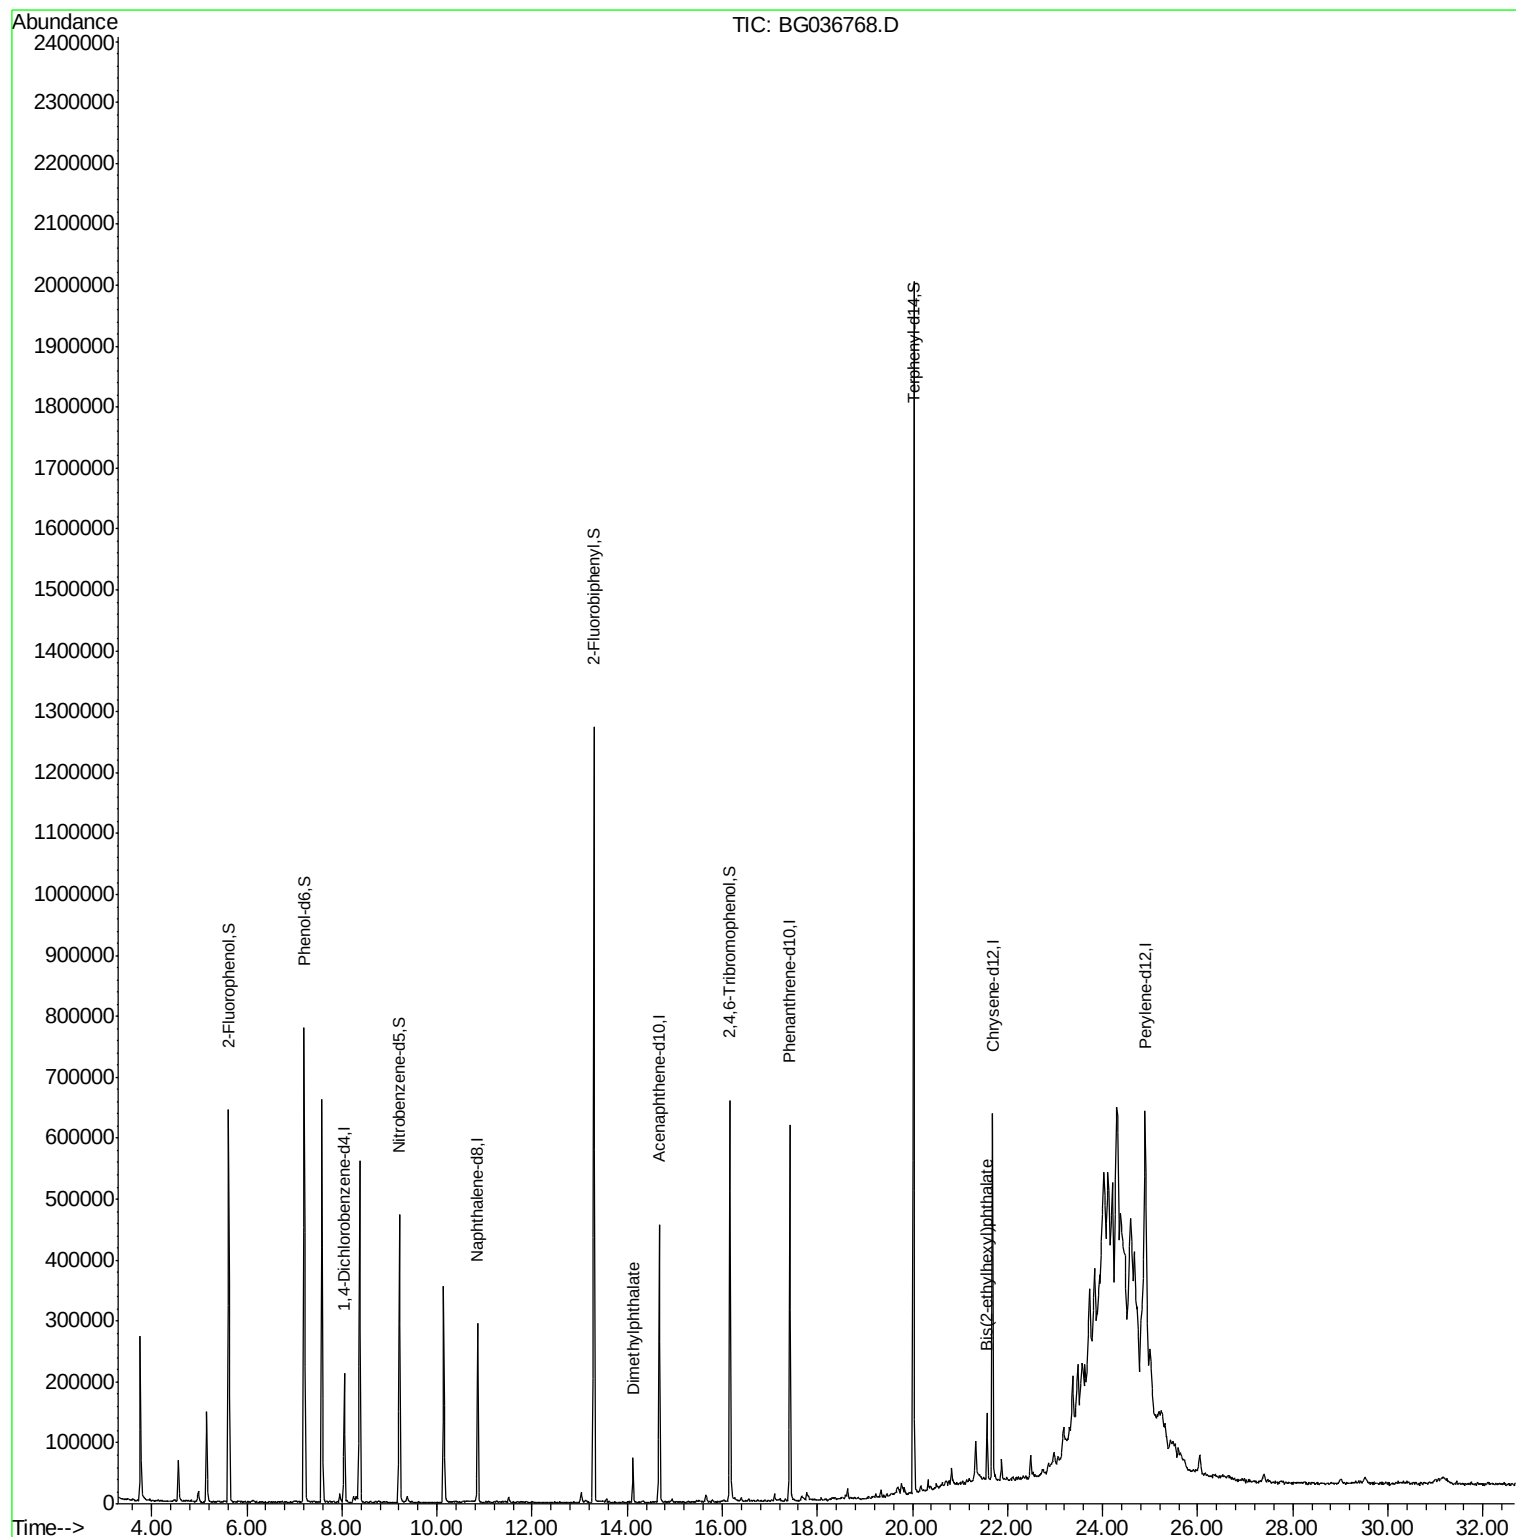

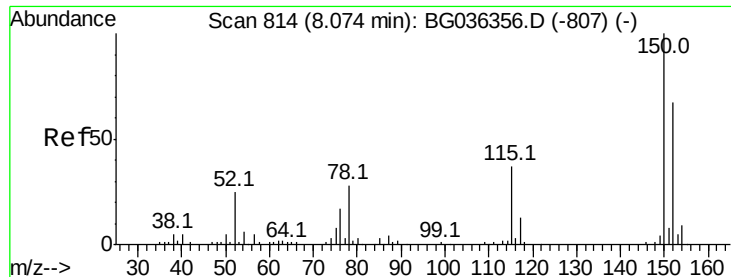


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.05 min Scan# 811
 Delta R.T. -0.01 min
 Lab File: BG036768.D
 Acq: 18 Sep 2018 1:25

Instrument :
 BNA_G
 ClientSampleId :
 PHASE-1-CONCRETE

Tot Ion	Ratio	Lower	Upper
152	100		
150	151.7	119.5	179.3
115	58.7	44.5	66.7

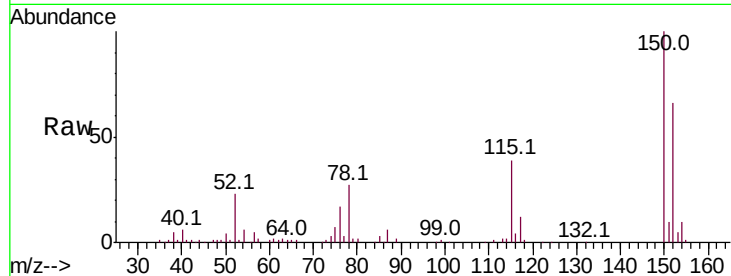


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

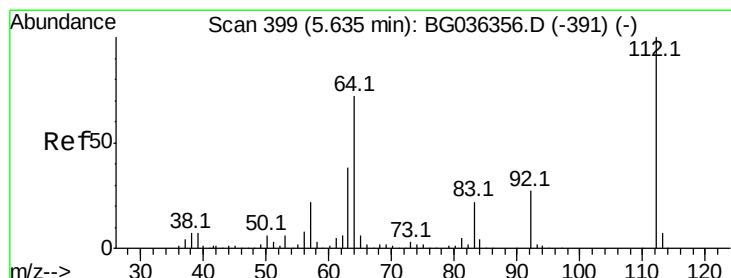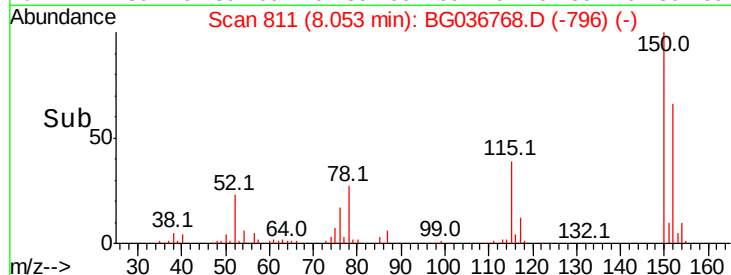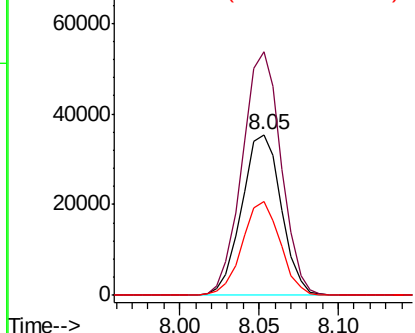



#5


2-Fluorophenol
 Concen: 70.681 ng
 RT: 5.62 min Scan# 397
 Delta R.T. -0.00 min
 Lab File: BG036768.D
 Acq: 18 Sep 2018 1:25

Tgt Ion	Ratio	Lower	Upper
112	100		
64	68.7	57.2	85.8
63	36.3	30.8	46.2

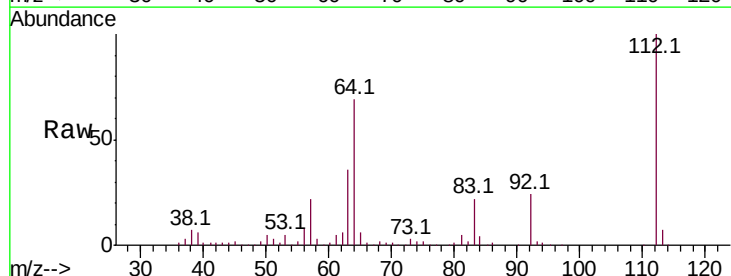

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BG
 Ion 63.00 (62.70 to 63.70): BG

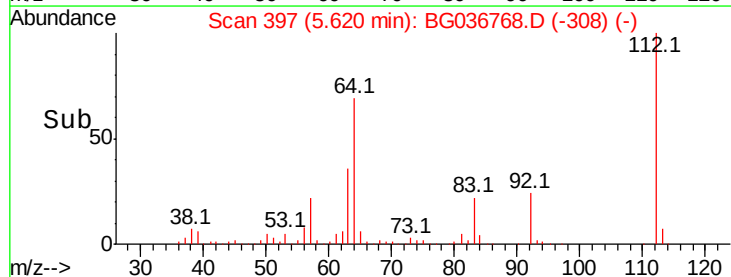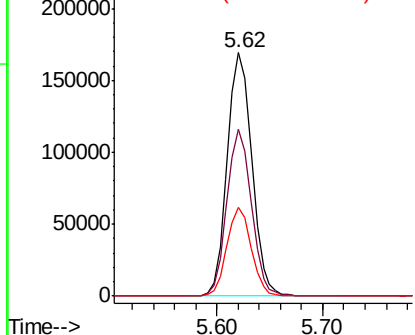

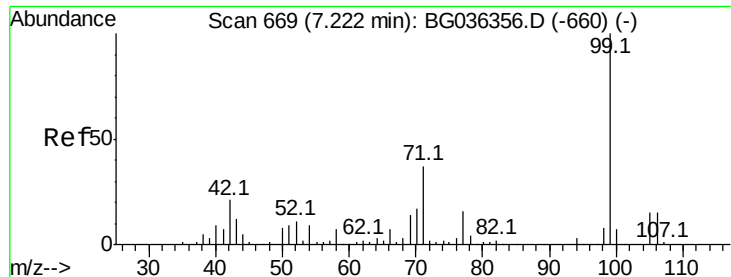

#7

Phenol-d6

Concen: 78.675 ng

RT: 7.21 min Scan# 667

Delta R.T. -0.01 min

Lab File: BG036768.D

Acq: 18 Sep 2018 1:25

Instrument :

BNA_G

ClientSampleId :

PHASE-1-CONCRETE


Tot Ion: 99 Resp: 435334

Ion Ratio Lower Upper




99 100

42 19.8 16.5 24.7

71 36.4 29.4 44.2

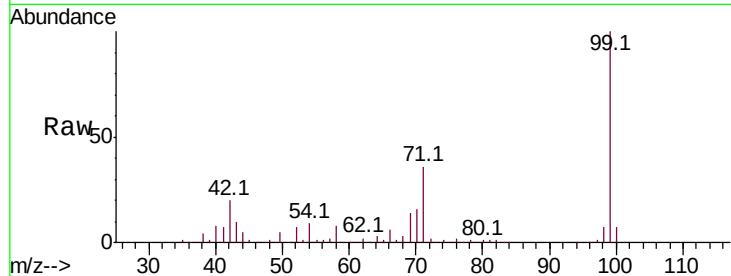

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

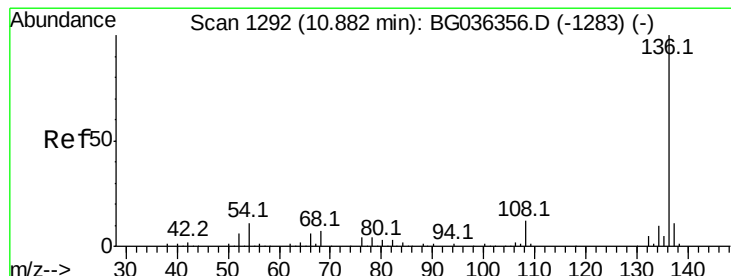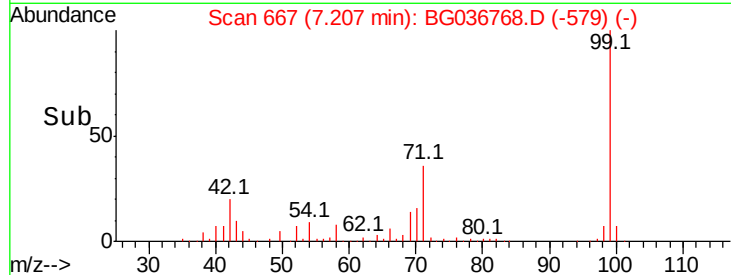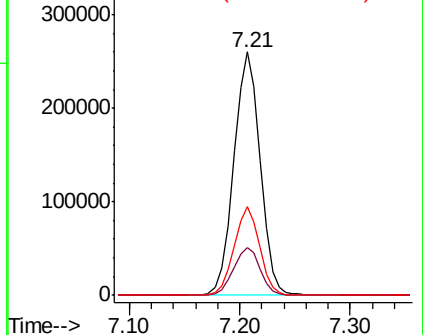

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1288

Delta R.T. -0.01 min

Lab File: BG036768.D

Acq: 18 Sep 2018 1:25

Tgt Ion: 136 Resp: 247513


Ion Ratio Lower Upper

136 100



137 11.0 8.8 13.2


54 11.8 9.2 13.8

68 6.0 5.8 8.6

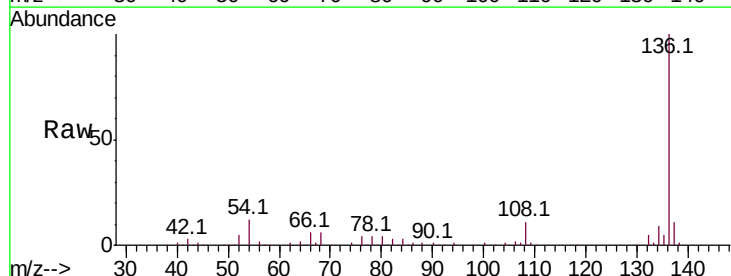

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

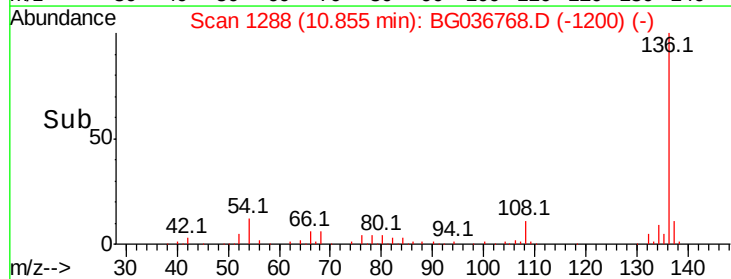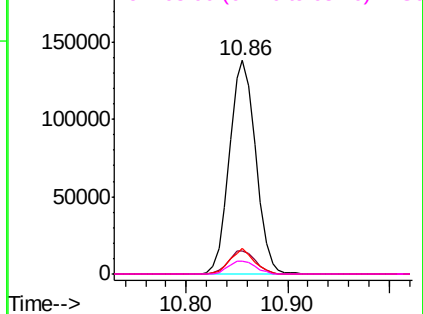


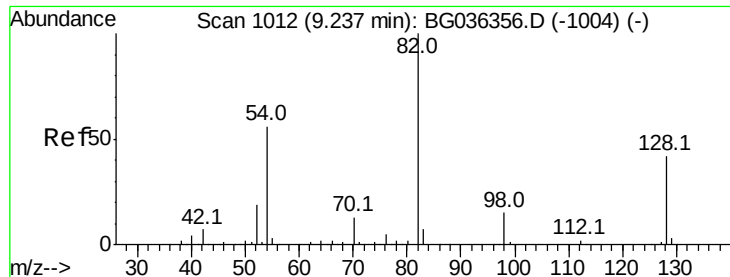




#23
Nitrobenzene-d5
Concen: 62.352 ng
RT: 9.21 min Scan# 1008
Delta R.T. -0.01 min
Lab File: BG036768.D
Acq: 18 Sep 2018 1:25

Instrument :
BNA_G
ClientSampleId :
PHASE-1-CONCRETE

Tot Ion: 82 Resp: 284441
Ion Ratio Lower Upper
82 100
128 41.6 33.3 49.9
54 54.2 45.1 67.7

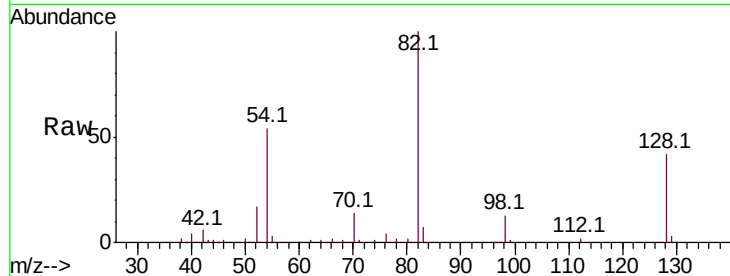


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

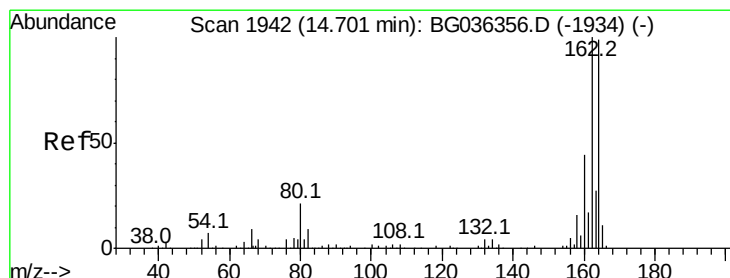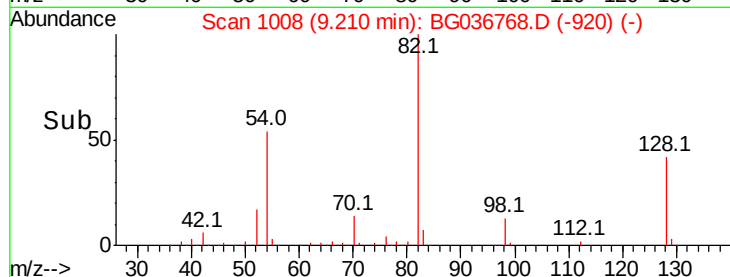
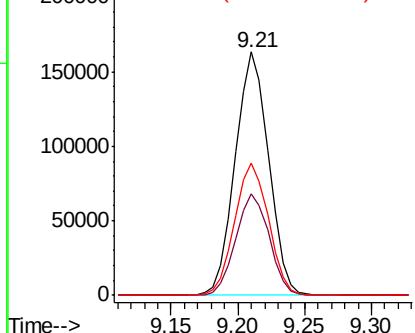



#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.67 min Scan# 1938
Delta R.T. -0.01 min
Lab File: BG036768.D
Acq: 18 Sep 2018 1:25

Tgt Ion:164 Resp: 157442
Ion Ratio Lower Upper
164 100
162 105.2 80.7 121.1
160 45.4 35.3 52.9

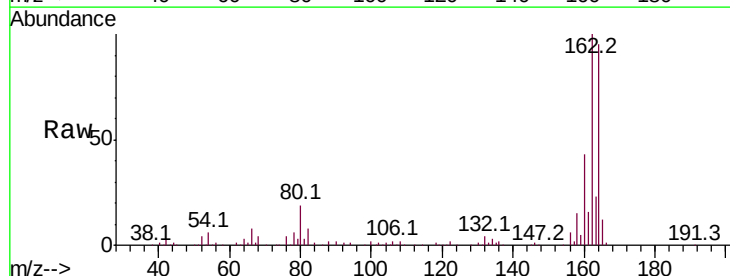

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

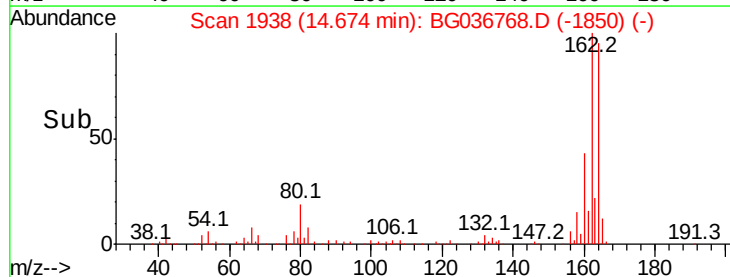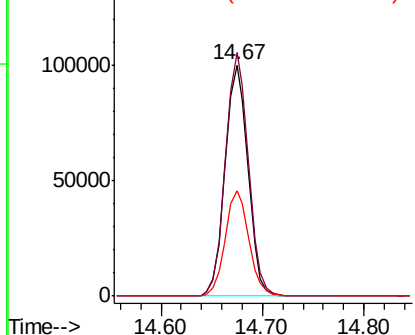


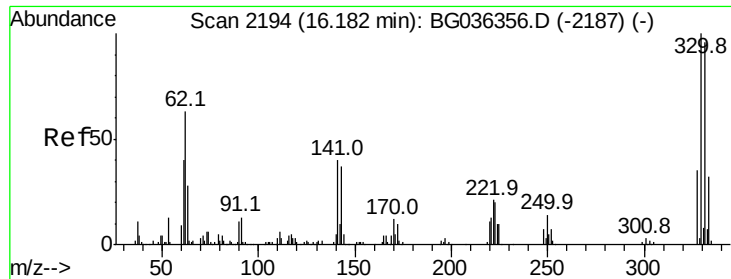




#41
 2,4,6-Tribromophenol
 Concen: 64.202 ng
 RT: 16.16 min Scan# 2191
 Delta R.T. -0.01 min
 Lab File: BG036768.D
 Acq: 18 Sep 2018 1:25

Instrument :
 BNA_G
 ClientSampleId :
 PHASE-1-CONCRETE

Tot Ion:330 Resp: 120612
 Ion Ratio Lower Upper
 330 100
 332 96.1 75.4 113.2
 141 35.7 30.7 46.1

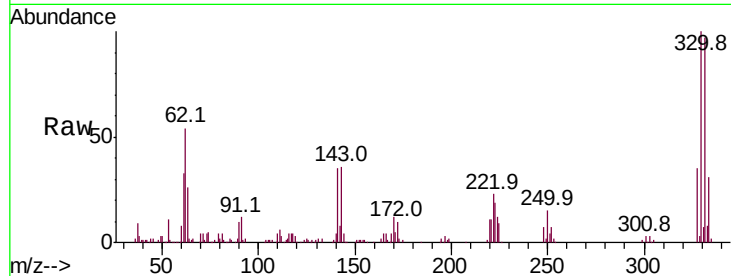


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

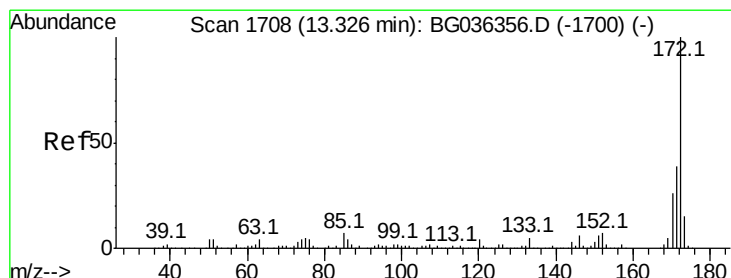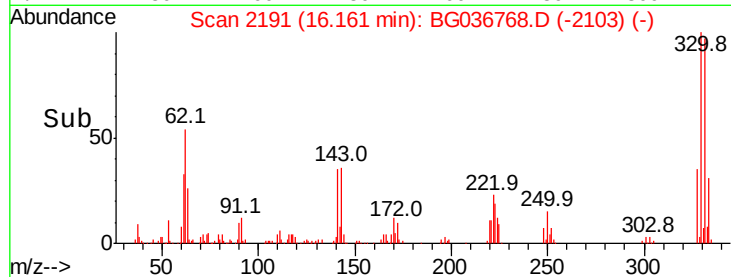
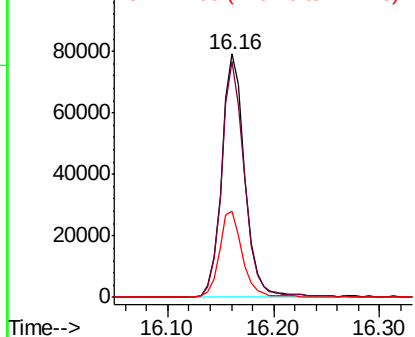



#44
 2-Fluorobiphenyl
 Concen: 59.937 ng
 RT: 13.30 min Scan# 1704
 Delta R.T. -0.01 min
 Lab File: BG036768.D
 Acq: 18 Sep 2018 1:25

Tgt Ion:172 Resp: 660909
 Ion Ratio Lower Upper
 172 100
 171 37.1 31.3 46.9
 170 25.5 21.0 31.6

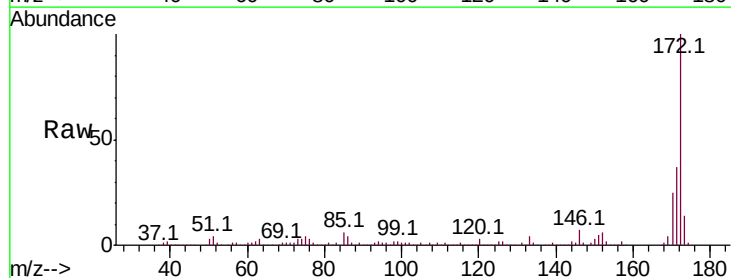

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

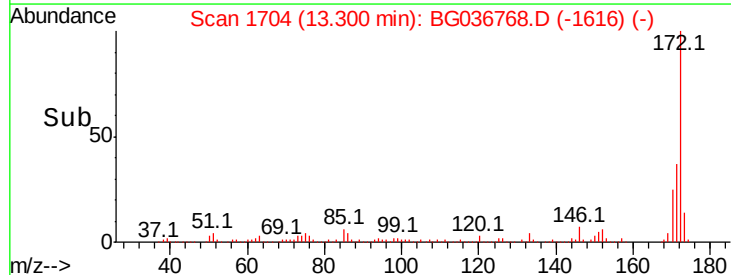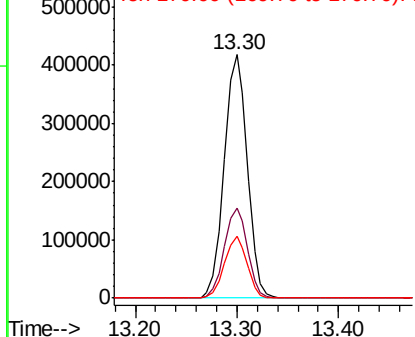


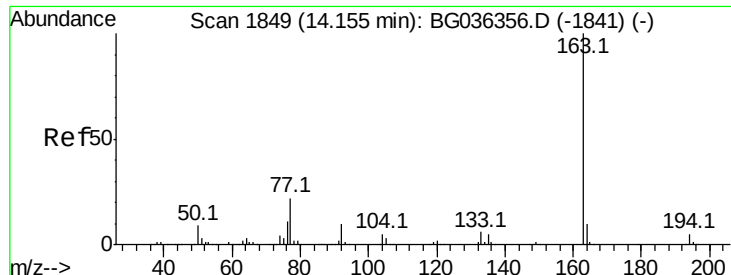




#49
Dimethylphthalate
Concen: 3.709 ng
RT: 14.12 min Scan# 1844
Delta R.T. -0.02 min
Lab File: BG036768.D
Acq: 18 Sep 2018 1:25

Instrument :
BNA_G
ClientSampleId :
PHASE-1-CONCRETE

Tot Ion:163 Resp: 47680
Ion Ratio Lower Upper
163 100
194 5.8 4.0 6.0
164 11.0 8.1 12.1

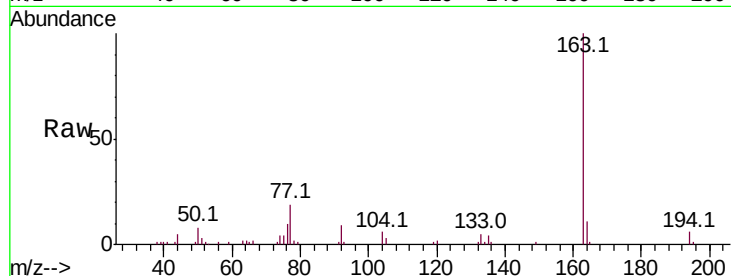


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

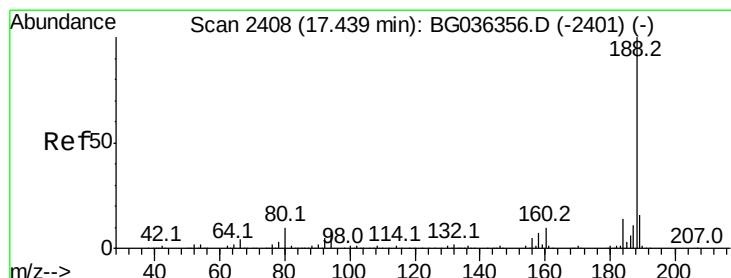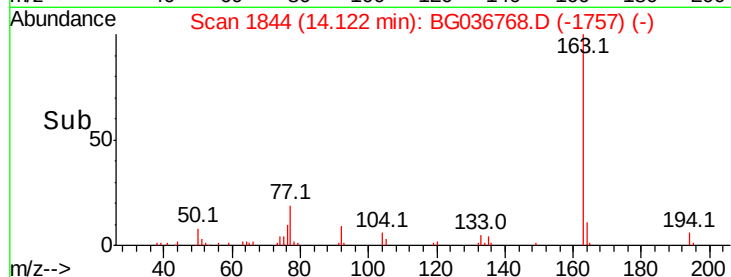
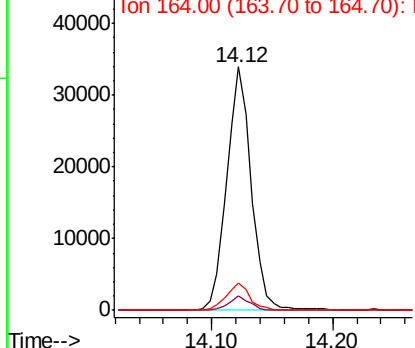



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.42 min Scan# 2405
Delta R.T. -0.01 min
Lab File: BG036768.D
Acq: 18 Sep 2018 1:25

Tgt Ion:188 Resp: 381255
Ion Ratio Lower Upper
188 100
94 7.8 6.7 10.1
80 9.1 8.1 12.1

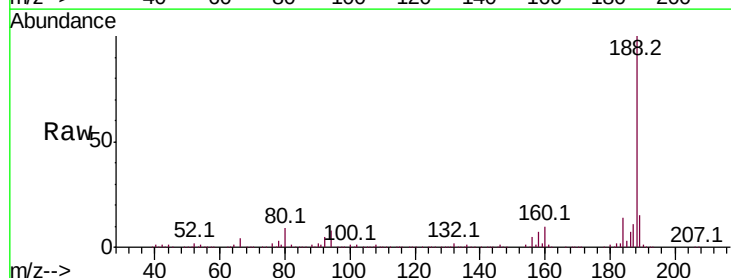

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

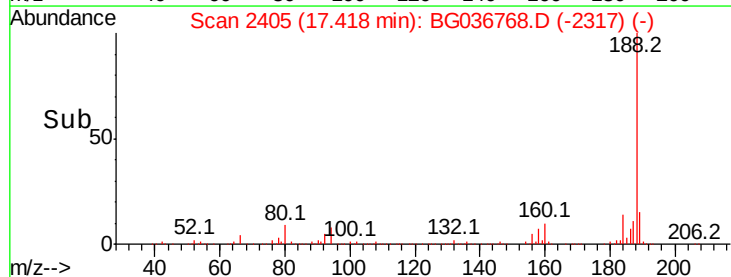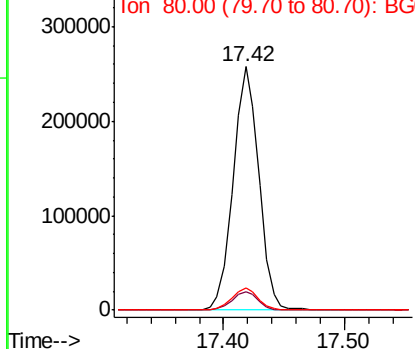

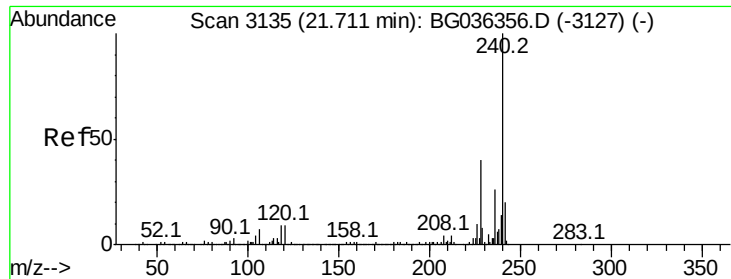

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.68 min Scan# 3131

Delta R.T. -0.01 min

Lab File: BG036768.D

Acq: 18 Sep 2018 1:25

Instrument :

BNA_G

ClientSampleId :

PHASE-1-CONCRETE


Tot Ion:240 Resp: 371786

Ion Ratio Lower Upper

240 100

120 8.1 6.9 10.3




236 26.2 21.2 31.8

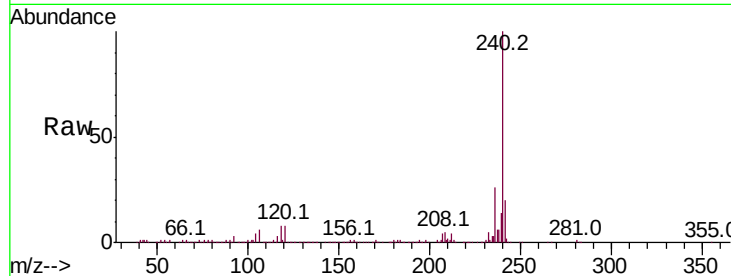

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

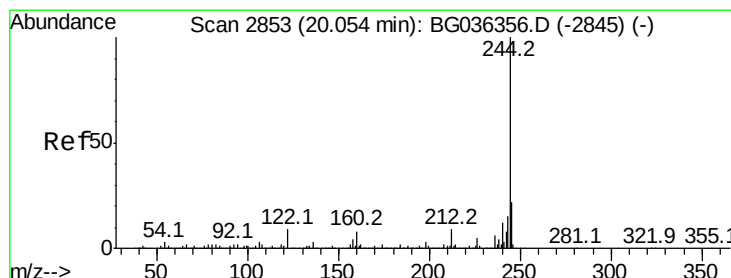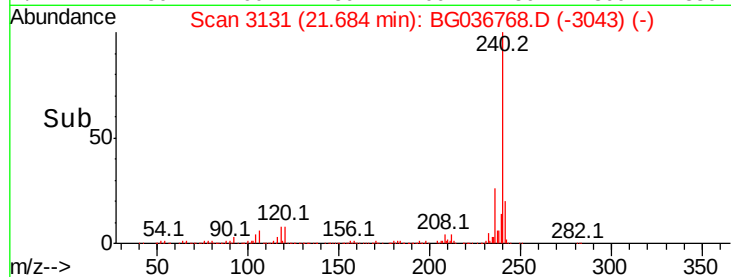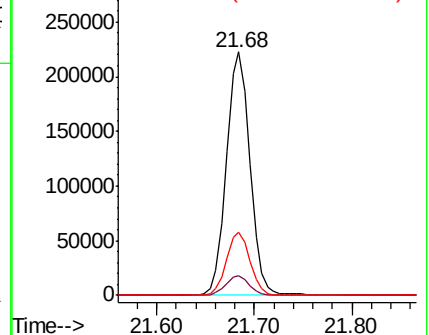

#78

Terphenyl-d14

Concen: 63.739 ng

RT: 20.03 min Scan# 2849

Delta R.T. -0.00 min

Lab File: BG036768.D

Acq: 18 Sep 2018 1:25


Tgt Ion:244 Resp: 1013857

Ion Ratio Lower Upper

244 100

212 8.0 7.0 10.6



122 8.1 7.1 10.7

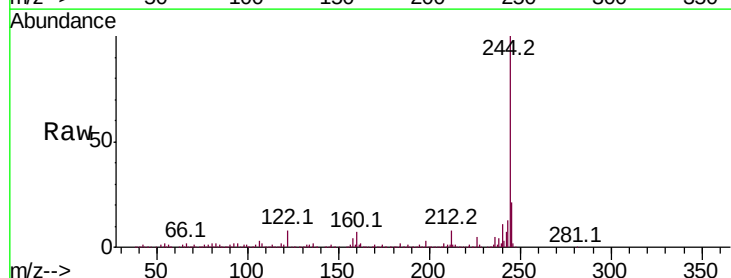


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

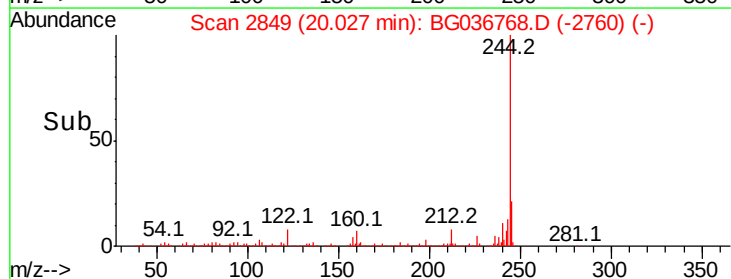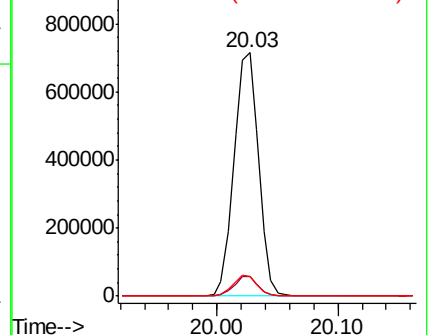

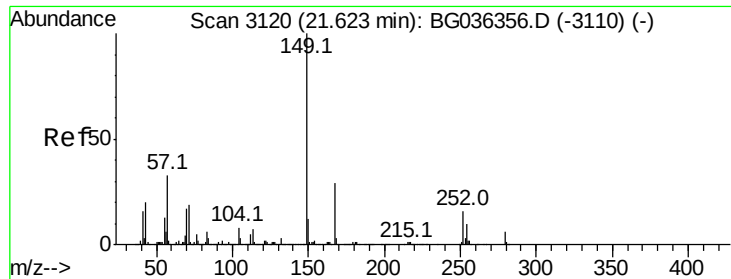

#83

Bis(2-ethylhexyl)phthalate

Concen: 3.396 ng

RT: 21.57 min Scan# 3112

Delta R.T. -0.02 min

Lab File: BG036768.D

Acq: 18 Sep 2018 1:25

Instrument :

BNA_G

ClientSampleId :

PHASE-1-CONCRETE


Tot Ion:149 Resp: 43240

Ion Ratio Lower Upper

149 100

167 26.7 23.4 35.0




279 6.5 4.6 7.0

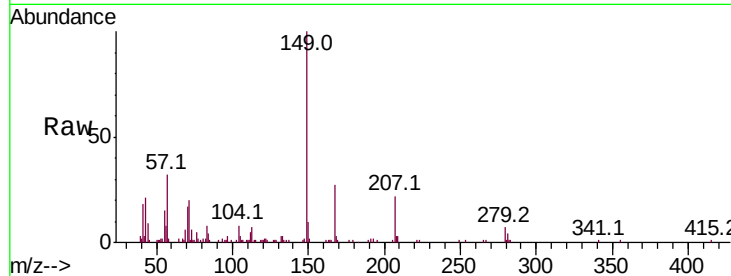

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

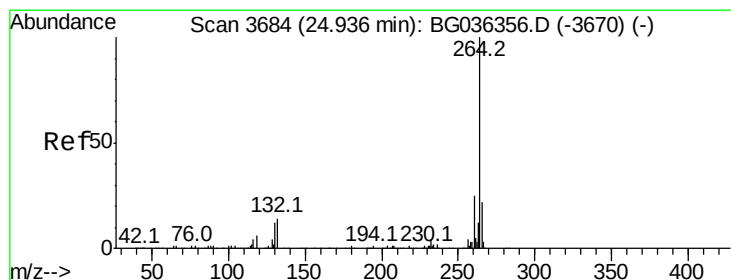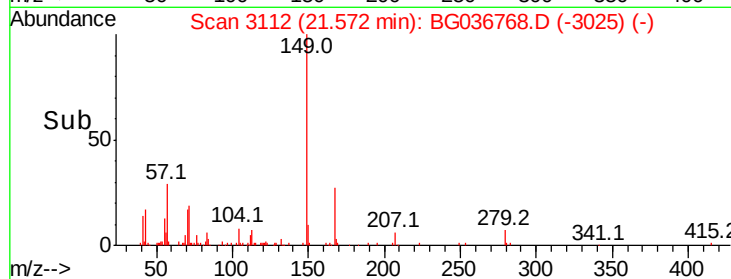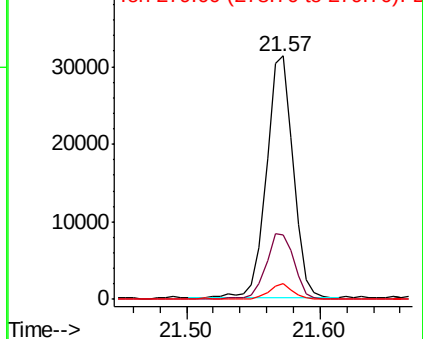

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.89 min Scan# 3677

Delta R.T. -0.01 min

Lab File: BG036768.D

Acq: 18 Sep 2018 1:25


Tgt Ion:264 Resp: 332073

Ion Ratio Lower Upper

264 100

260 24.5 19.6 29.4

265 22.2 17.4 26.0

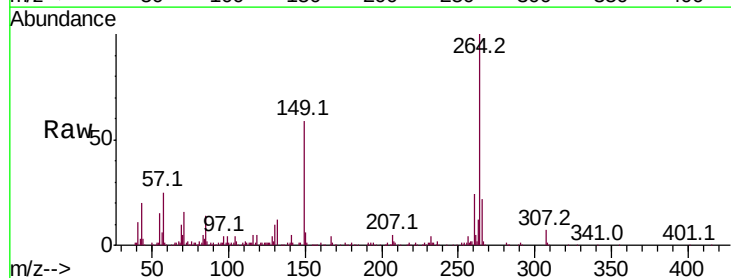

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

