


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091718\
 Data File : BG036766.D
 Acq On : 17 Sep 2018 23:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 31 13:03:20 2018

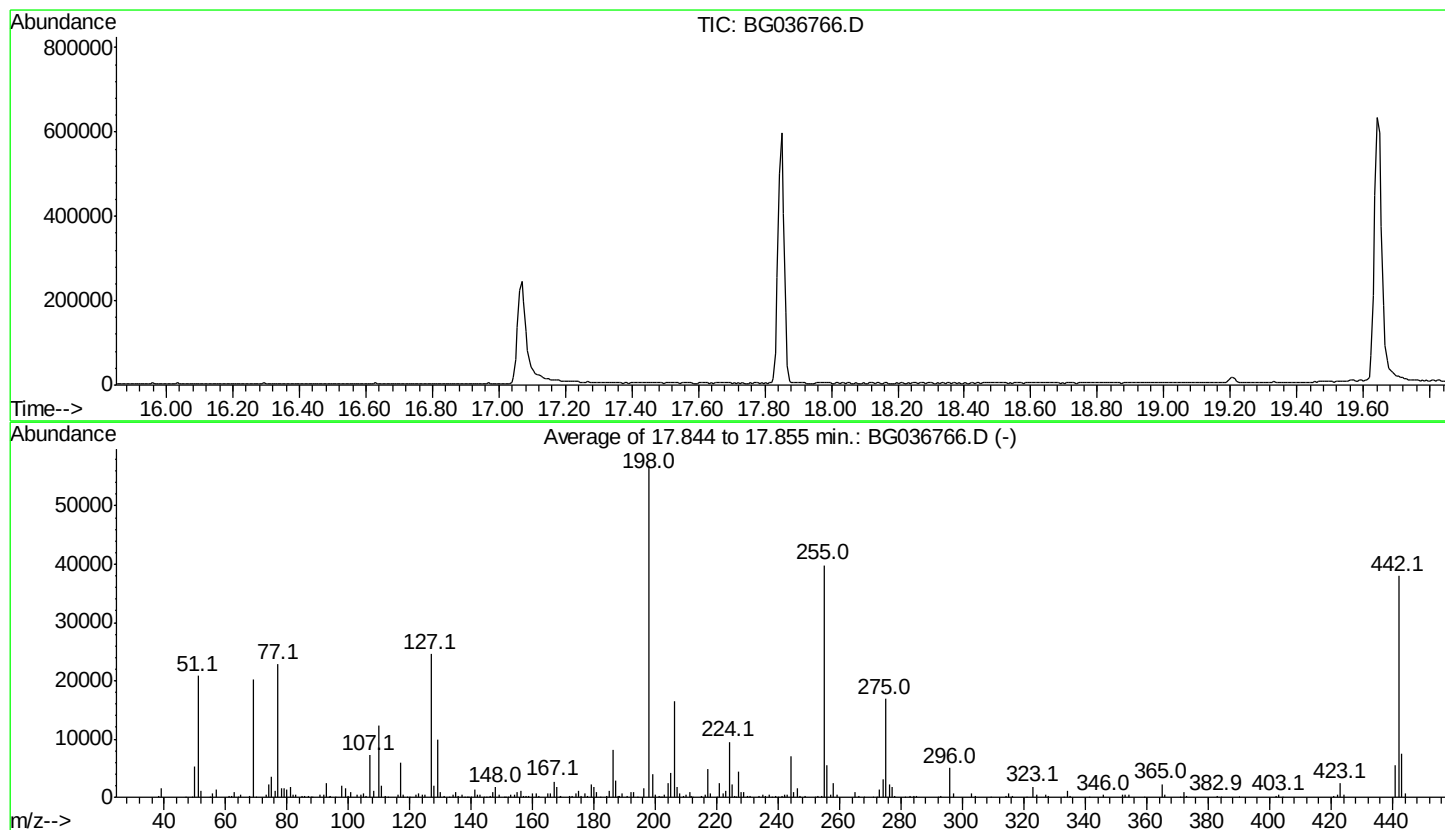

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	20848	PASS
68	69	0.00	2	1.1	215	PASS
69	198	0.00	100	35.7	20332	PASS
70	69	0.00	2	0.4	84	PASS
127	198	10	80	43.2	24578	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56922	PASS
199	198	5	9	7.1	4056	PASS
275	198	10	60	29.6	16832	PASS
365	198	1	100	3.9	2218	PASS
441	198	0.01	100	9.7	5534	PASS
442	198	50	100	66.7	37968	PASS
443	442	15	24	19.9	7574	PASS