
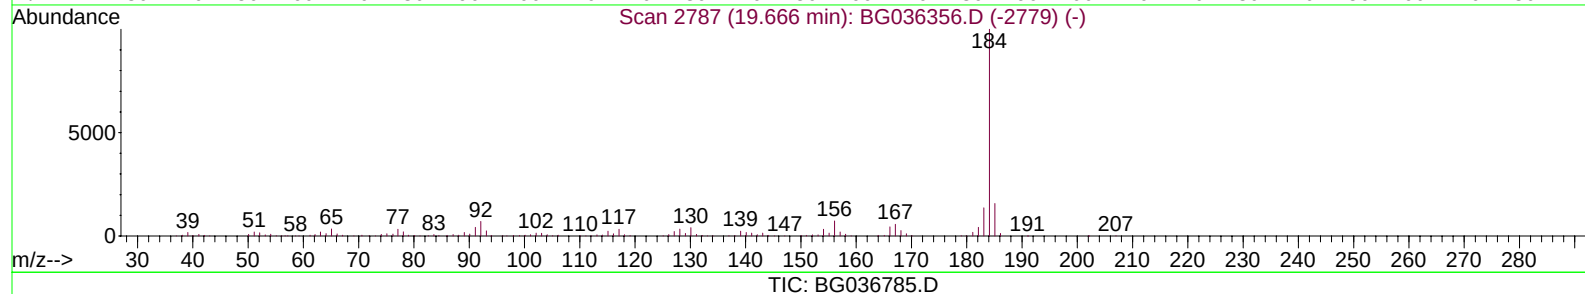
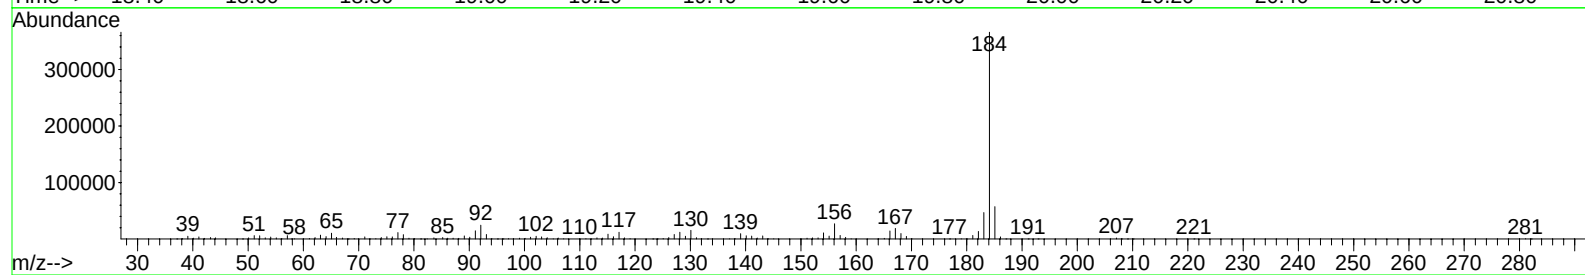


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091818\
Data File : BG036785.D
Acq On : 18 Sep 2018 14:35
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 17:24:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

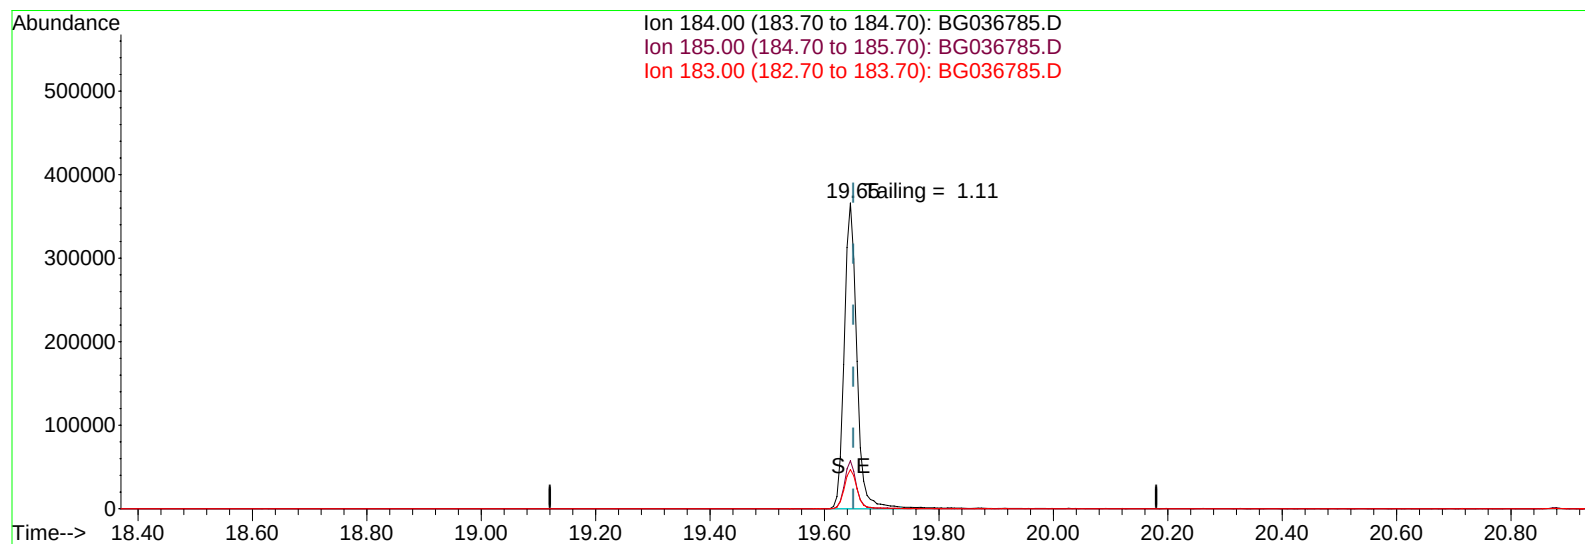

(76) Benzidine




19.645min (-0.005) 8247.44ng

response 563362

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.70
183.00	13.60	12.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091818\
Data File : BG036785.D
Acq On : 18 Sep 2018 14:35
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 17:24:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

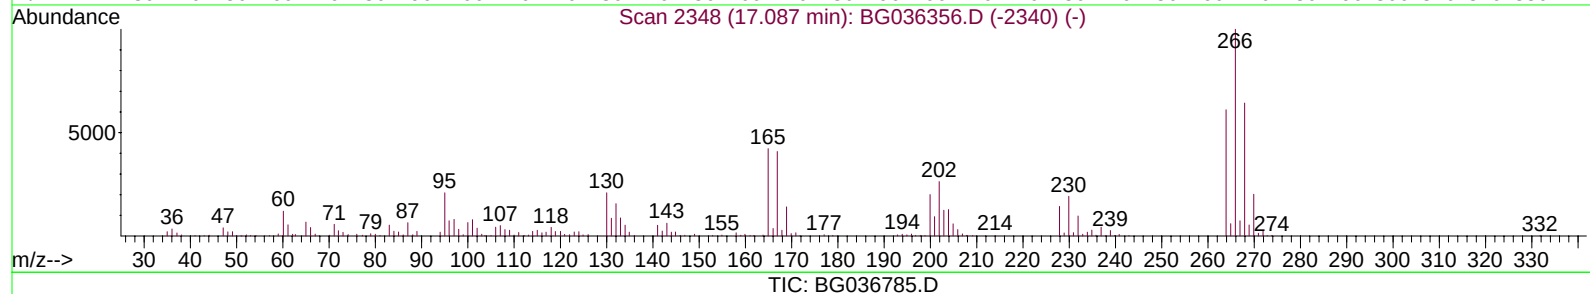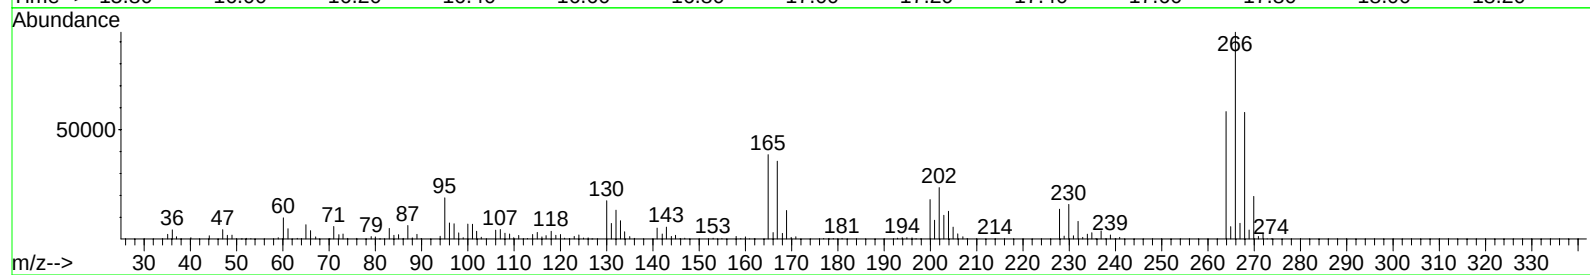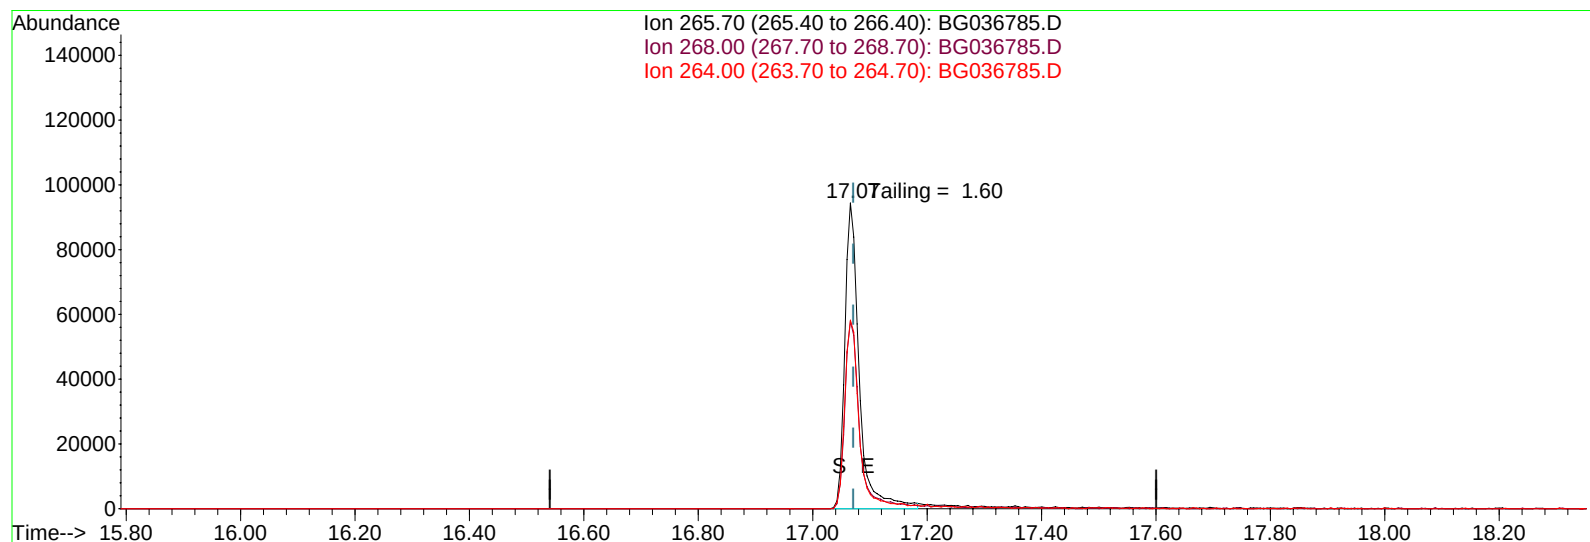

(69) Pentachlorophenol (C)

17.066min (-0.005) 9612.60ng

response 169174

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	61.28
264.00	61.10	61.68
0.00	0.00	0.00