
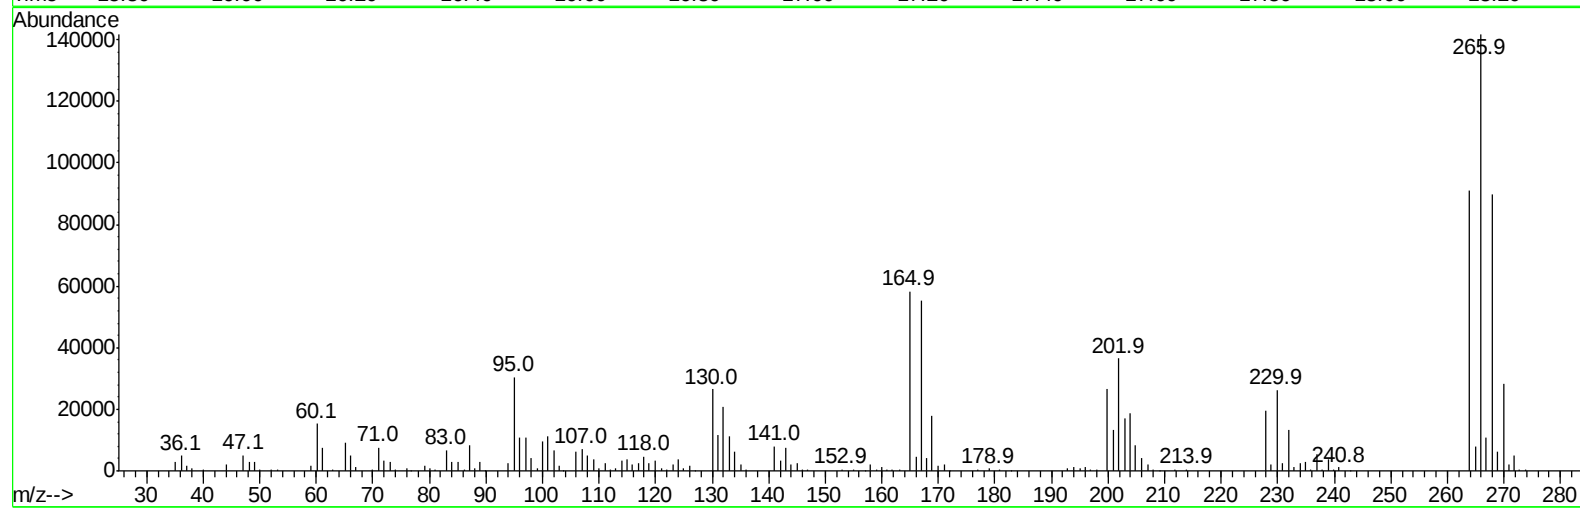


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091818\
Data File : BG036804.D
Acq On : 19 Sep 2018 3:37
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 08:05:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

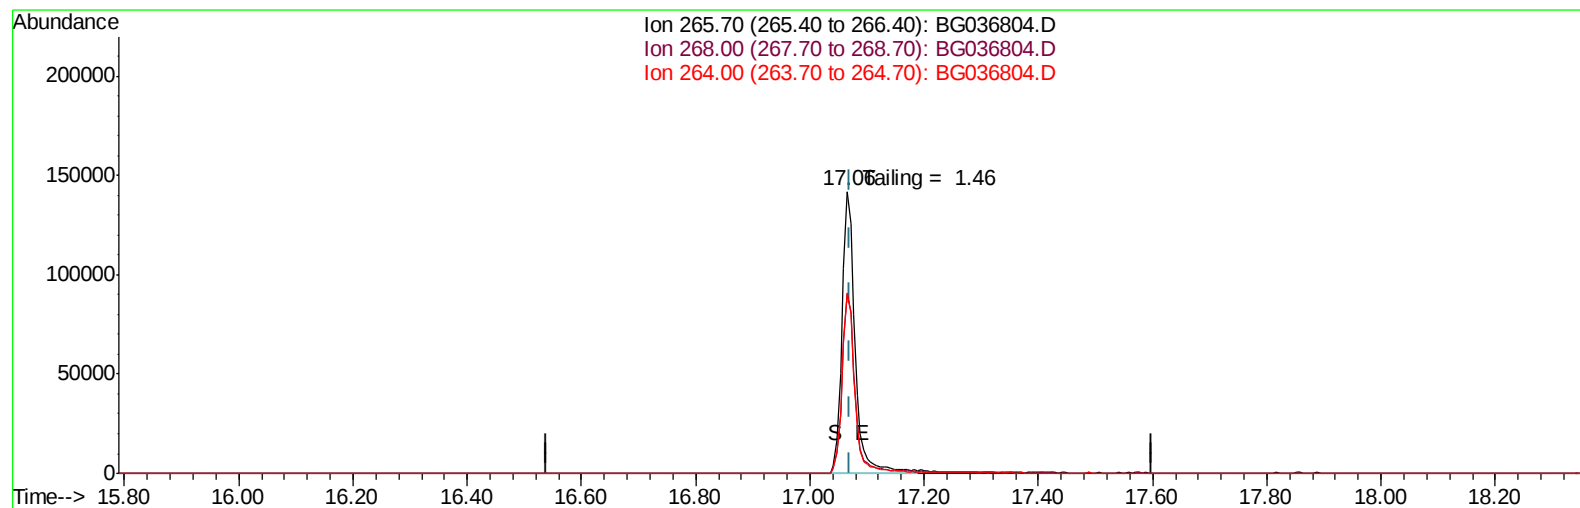

TIC: BG036804.D

(69) Pentachlorophenol (C)



17.065min (-0.006) 12095.21ng

response 224577

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	63.44
264.00	61.10	64.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091818\
Data File : BG036804.D
Acq On : 19 Sep 2018 3:37
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 08:05:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

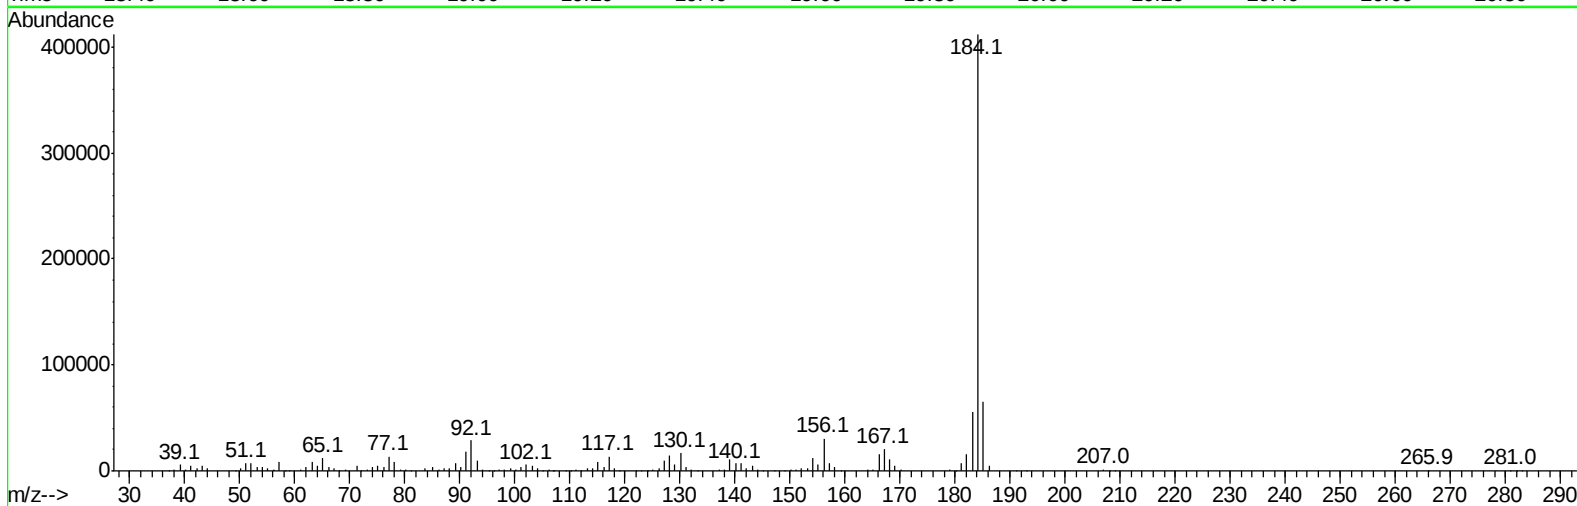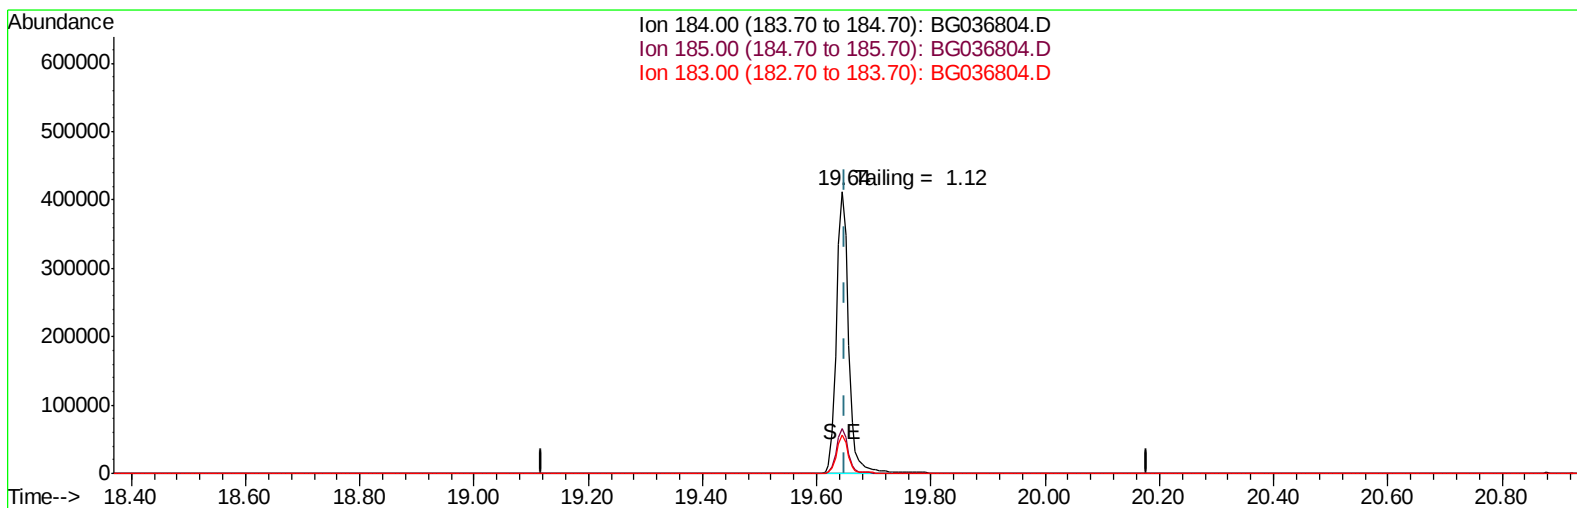

TIC: BG036804.D

(76) Benzidine

19.644min (-0.006) 7973.84ng

response 610308

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.90
183.00	13.60	13.44
0.00	0.00	0.00