


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091819\
 Data File : BG042885.D
 Acq On : 18 Sep 2019 8:40
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG091219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 12 14:06:09 2019

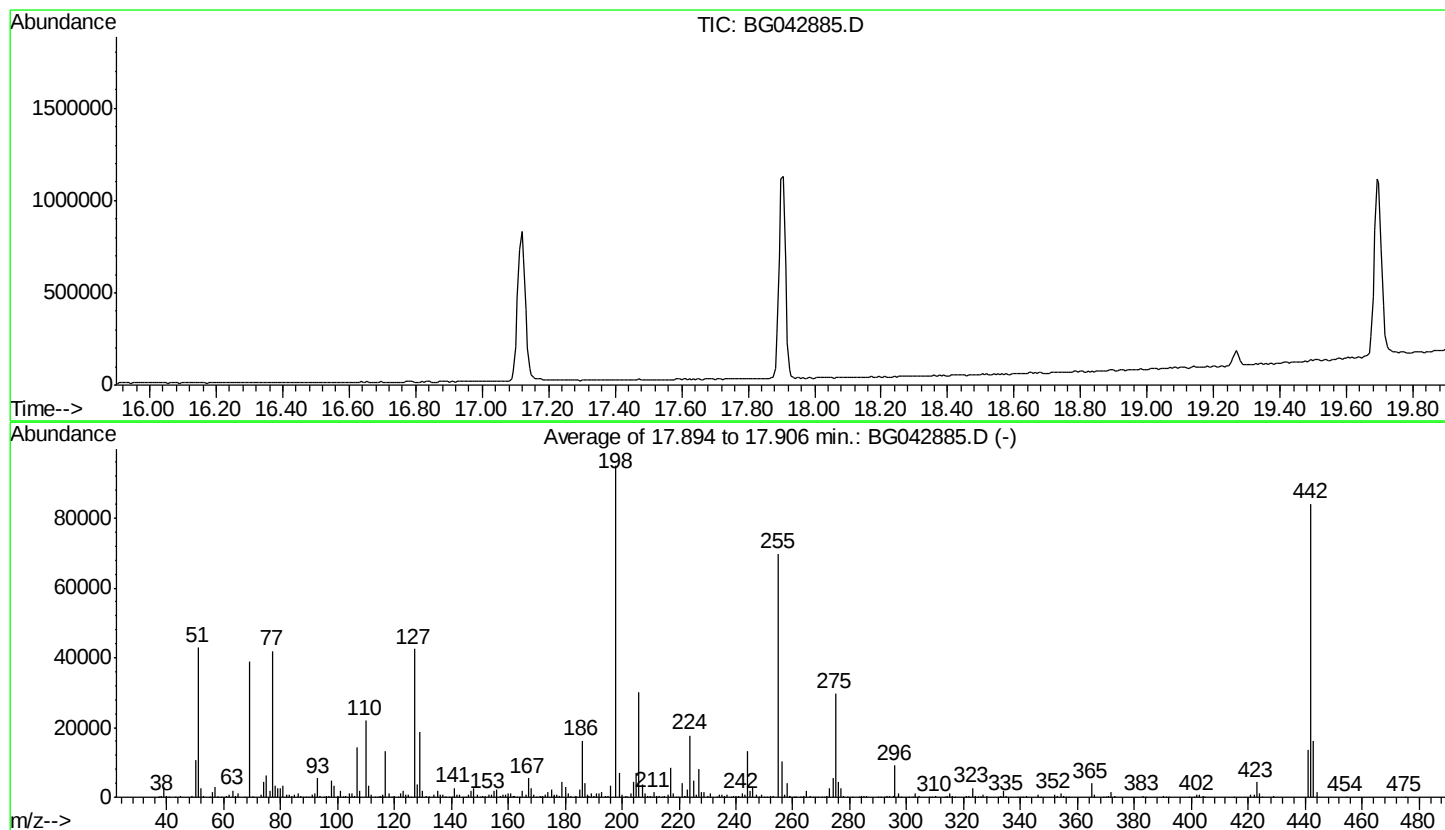

AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	42805	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.8	38754	PASS
70	69	0.00	2	0.3	127	PASS
127	198	10	80	44.7	42533	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	95058	PASS
199	198	5	9	7.4	7000	PASS
275	198	10	60	31.3	29712	PASS
365	198	1	100	4.2	3963	PASS
441	198	0.01	100	14.2	13518	PASS
442	198	50	100	88.5	84144	PASS
443	442	15	24	19.4	16311	PASS