
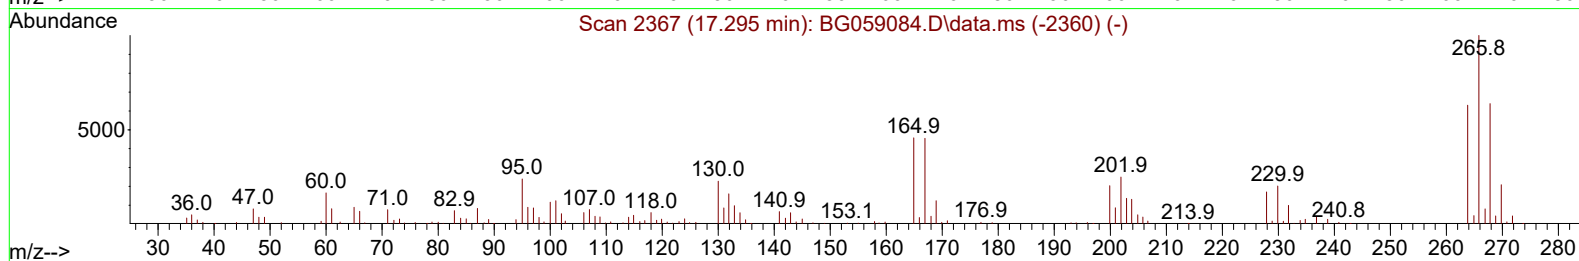
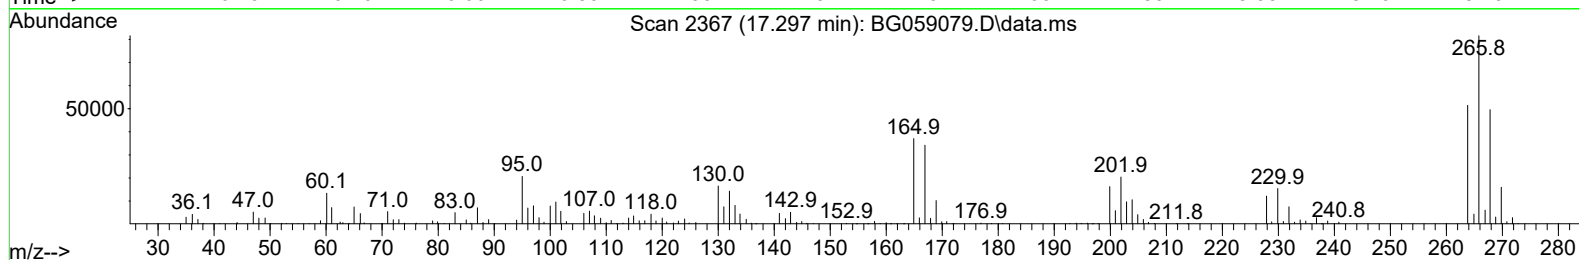


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG091823\  
Data File : BG059079.D  
Acq On : 18 Sep 2023 8:53  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 06:04:19 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG091823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 19 02:12:59 2023  
Response via : Initial Calibration

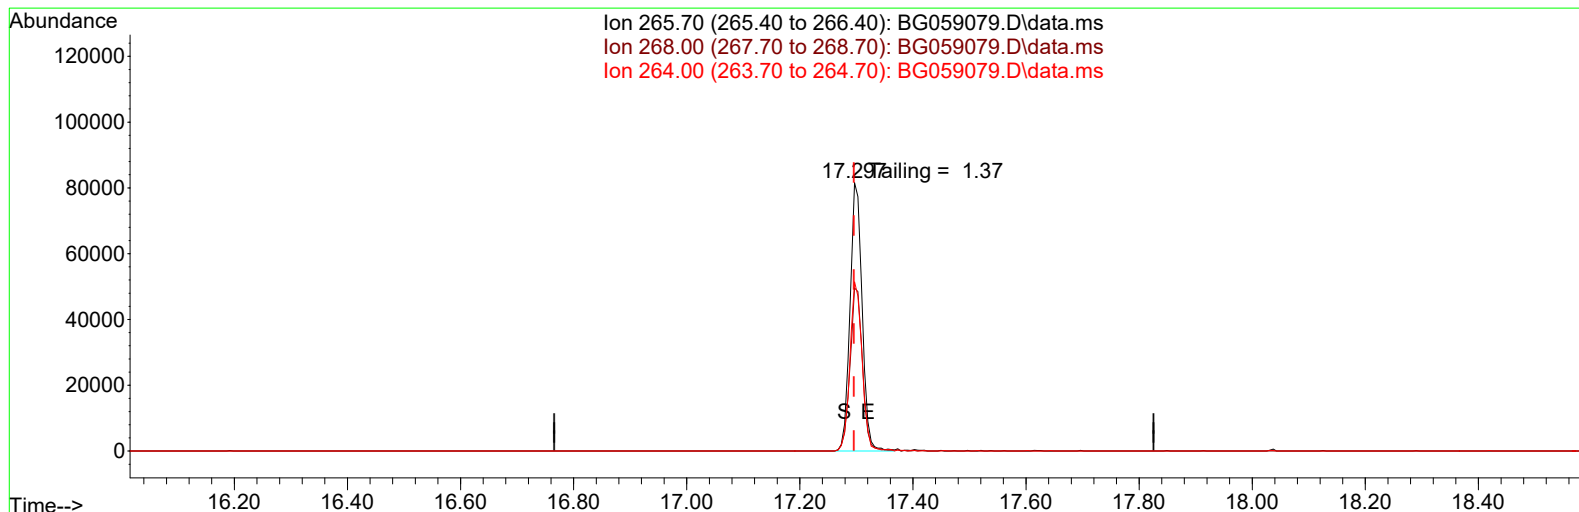

TIC: BG059079.D\data.ms

**(70) Pentachlorophenol (C)**




17.297min (+ 0.001) 276193.39 ng

response 122159

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.90  | 60.73  |
| 264.00 | 63.00  | 63.04  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG091823\  
Data File : BG059079.D  
Acq On : 18 Sep 2023 8:53  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 06:04:19 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG091823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 19 02:12:59 2023  
Response via : Initial Calibration

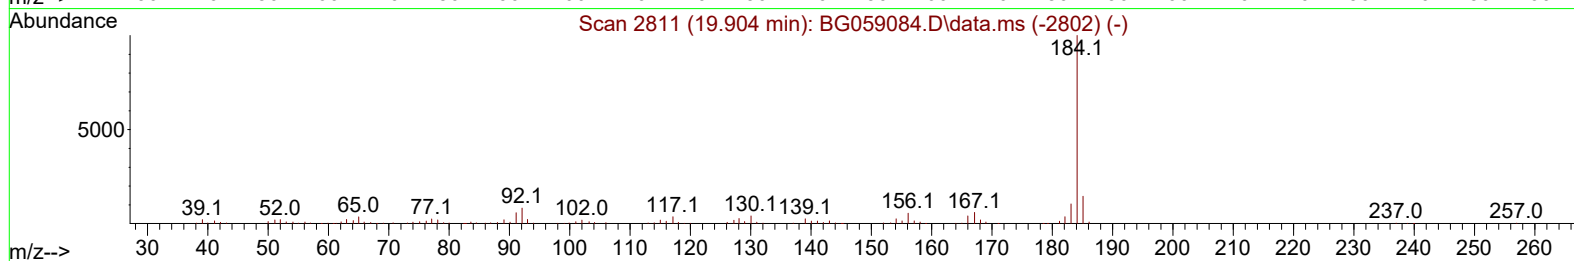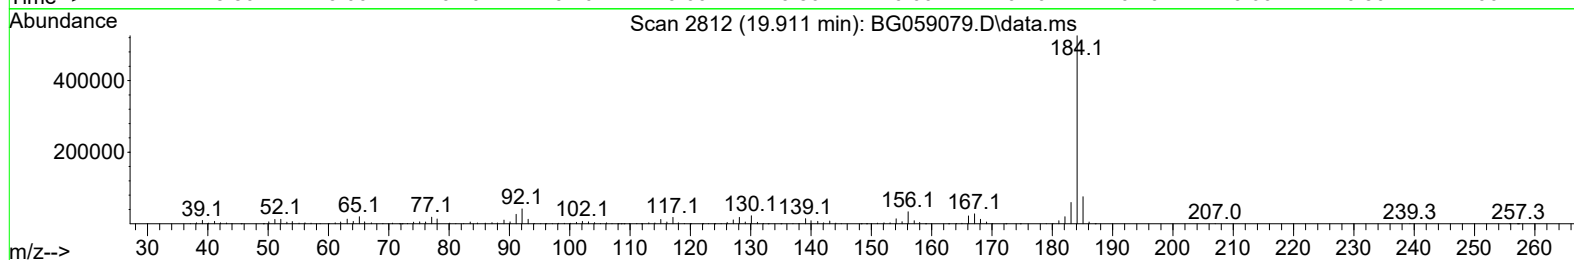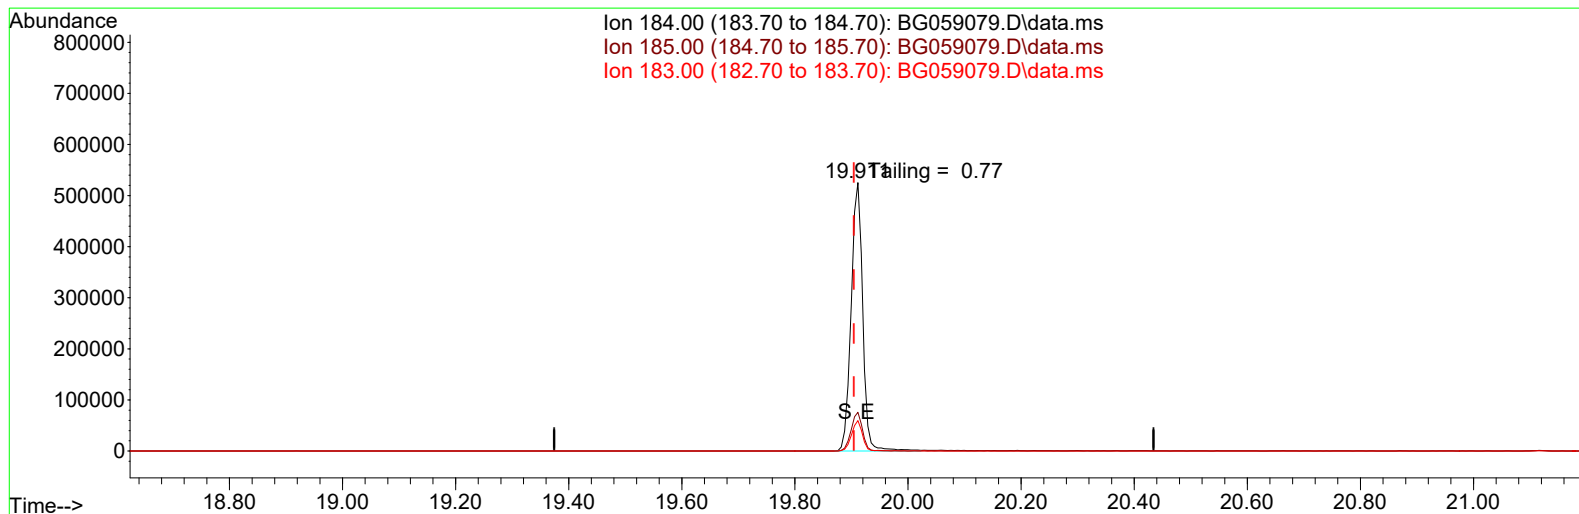

TIC: BG059079.D\data.ms

**(77) Benzidine****19.911min (+ 0.007) 601875.58 ng****response 751824**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.60  | 14.44  |
| 183.00 | 10.50  | 11.32  |
| 0.00   | 0.00   | 0.00   |