
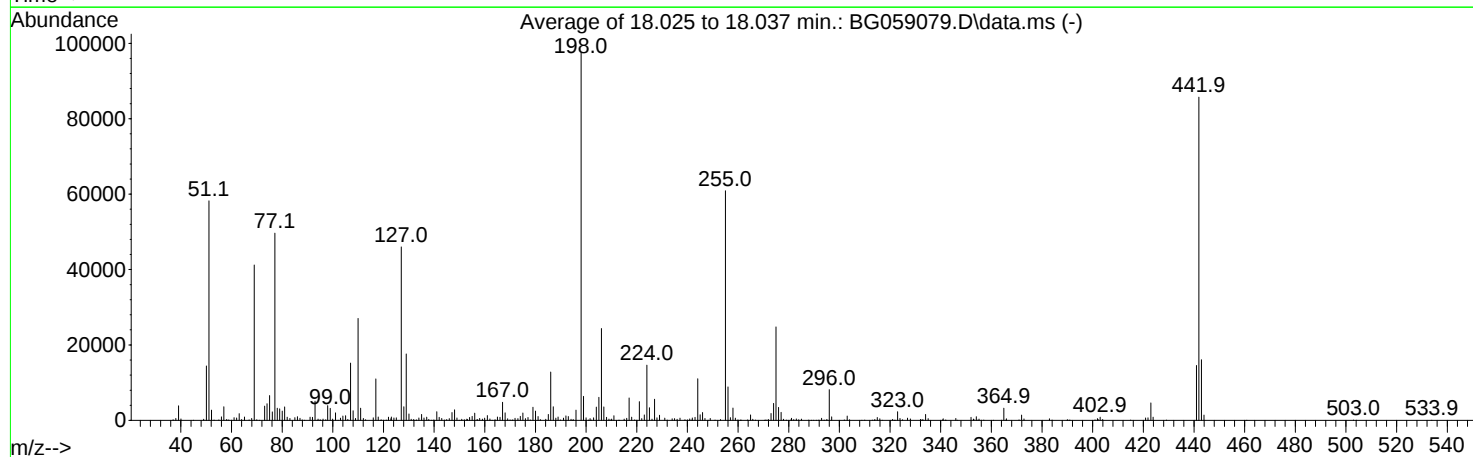


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091823\
Data File : BG059079.D
Acq On : 18 Sep 2023 8:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 19 02:12:59 2023

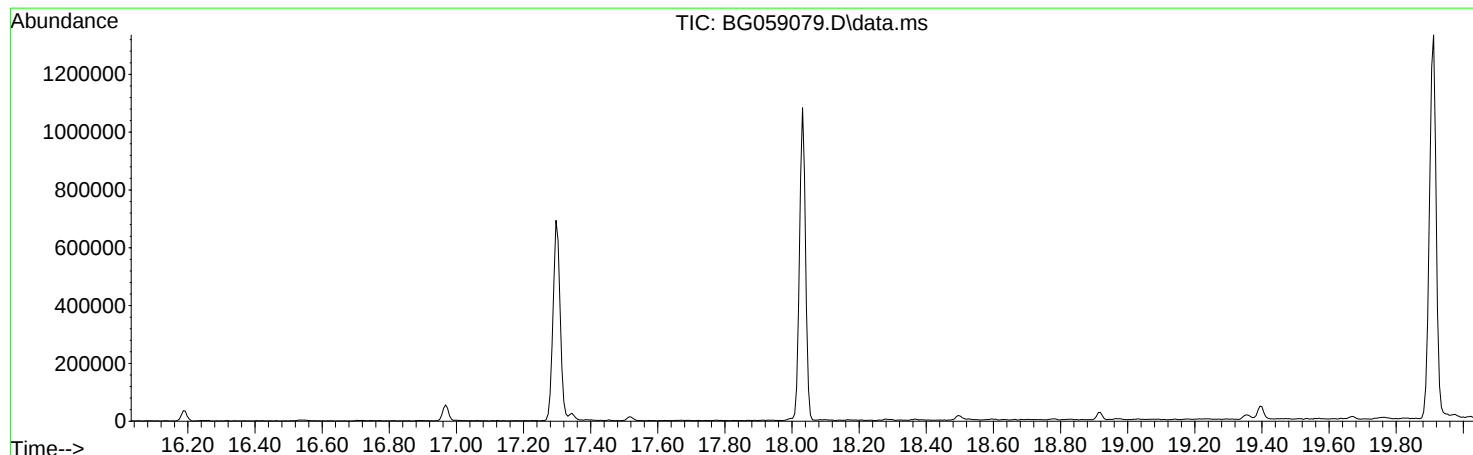




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.7	58237	PASS
68	69	0.00	2	1.3	531	PASS
69	198	0.00	100	42.2	41211	PASS
70	69	0.00	2	0.4	183	PASS
127	198	10	80	47.2	46019	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	97568	PASS
199	198	5	9	6.5	6373	PASS
275	198	10	60	25.4	24776	PASS
365	198	1	100	3.3	3218	PASS
441	198	0.01	100	14.9	14563	PASS
442	442	50	100	100.0	85731	PASS
443	442	15	24	18.8	16078	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091823\
Data File : BG059079.D
Acq On : 18 Sep 2023 8:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 19 06:04:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 19 02:12:59 2023
Response via : Initial Calibration

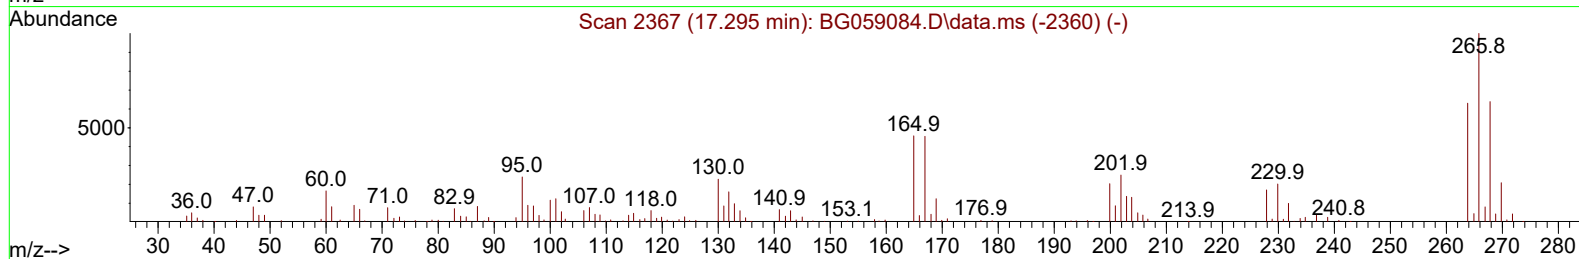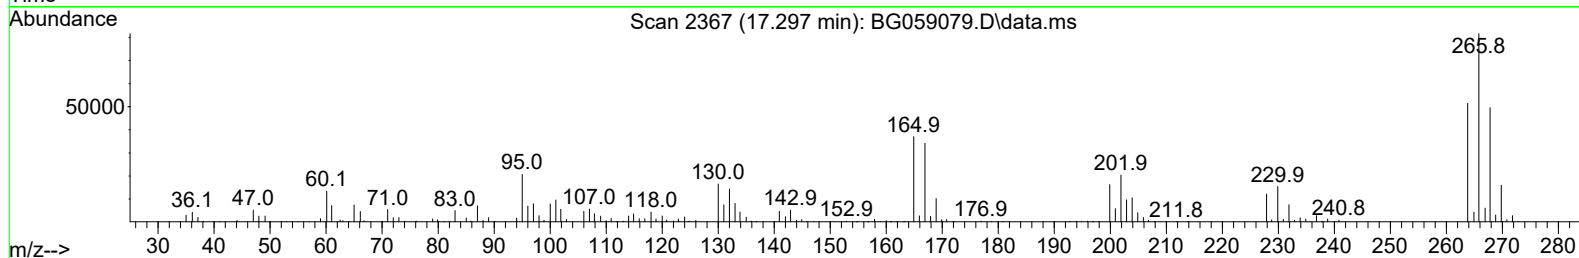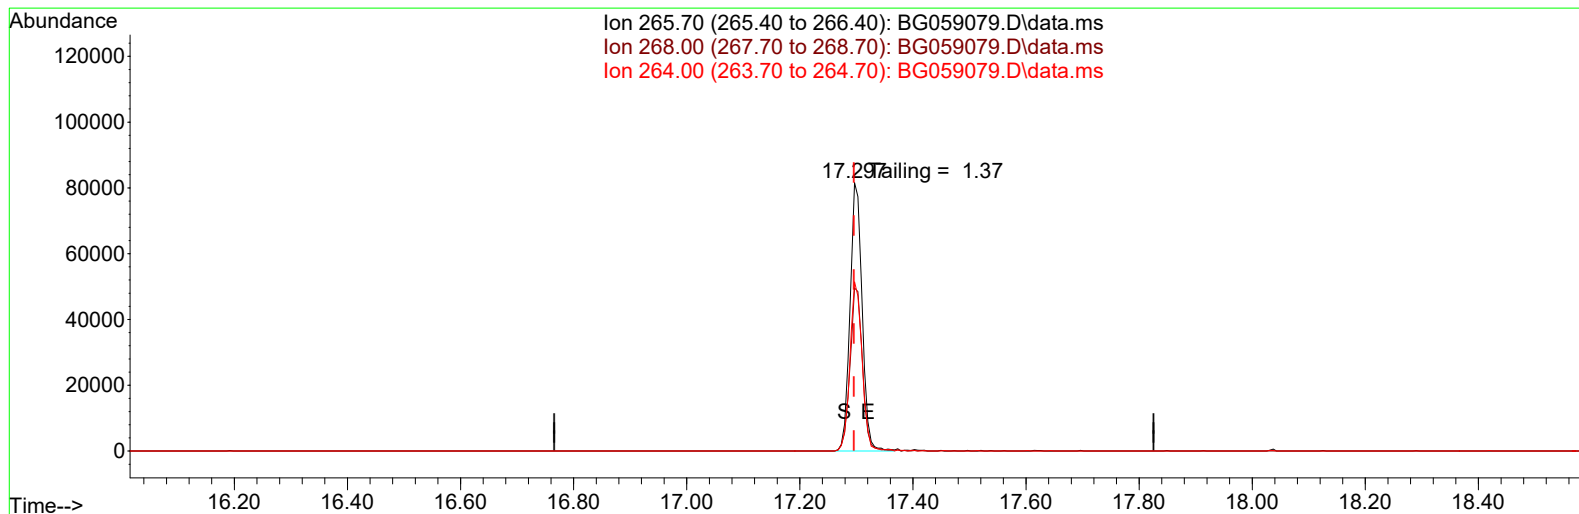

TIC: BG059079.D\data.ms

(70) Pentachlorophenol (C)

17.297min (+ 0.001) 276193.39 ng




response 122159

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	60.73
264.00	63.00	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091823\
Data File : BG059079.D
Acq On : 18 Sep 2023 8:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 19 06:04:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 19 02:12:59 2023
Response via : Initial Calibration

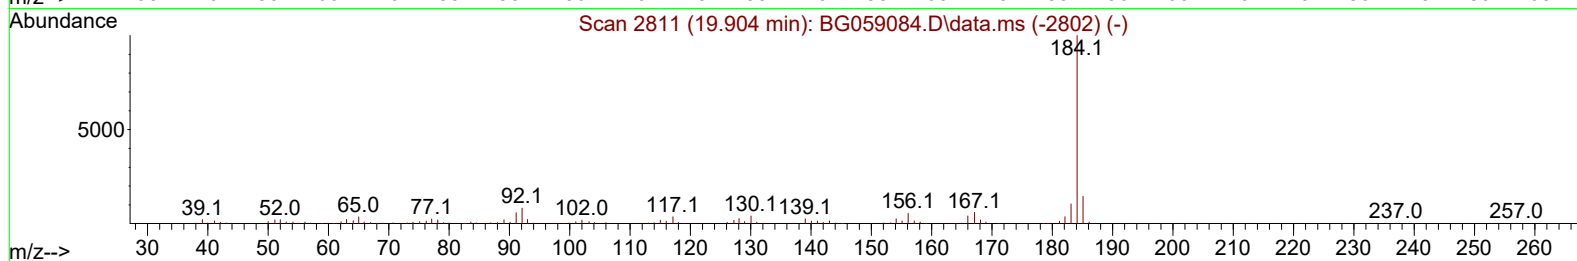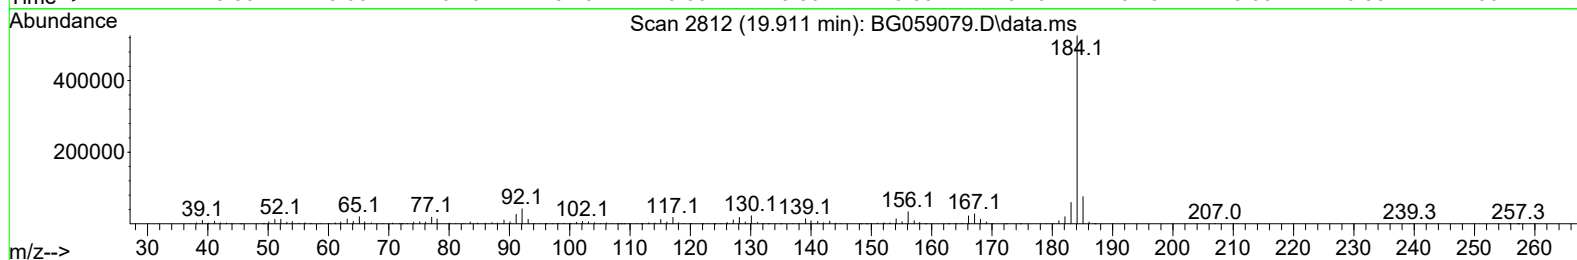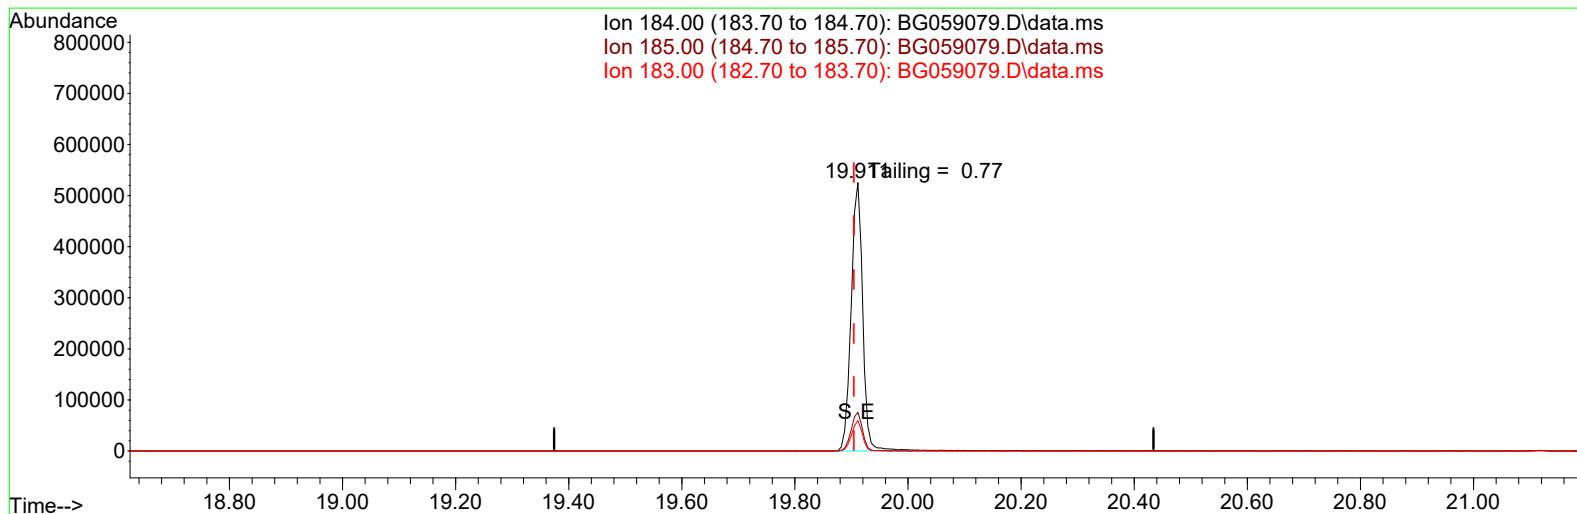

TIC: BG059079.D\data.ms

(77) Benzidine

19.911min (+ 0.007) 601875.58 ng

response 751824

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.44
183.00	10.50	11.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/18/2023	BNA_G	<u>BG059079.D</u>
Compound Name	Response	Retention Time
DDT	333449	21.122
DDD	3361	20.71
DDE	53	20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3414	336863	1.01

Instrument :
BNA_G
ClientSampleId :
DFTPP