

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091923\
 Data File : BG059099.D
 Acq On : 19 Sep 2023 21:47
 Operator : MA/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SICV434

Quant Time: Sep 20 04:26:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 20 04:25:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.299	152	33043	20.000	ng/u1	0.00
20) Naphthalene-d8	11.143	136	157108	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.927	164	105157	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.677	188	240907	20.000	ng/u1	0.00
79) Chrysene-d12	22.001	240	209589	20.000	ng/u1	0.00
88) Perylene-d12	25.544	264	244455	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.605	96	6257	7.412	ng/uL	0.00
4) Pyridine-d5	4.040	84	49617	20.034	ng/u1	0.00
7) Phenol-d5	7.406	99	65579	20.184	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.618	67	40295	20.210	ng/u1	0.00
11) 2-Chlorophenol-d4	7.812	132	49568	20.673	ng/u1	0.00
15) 4-Methylphenol-d8	8.981	113	53358	20.620	ng/u1	0.00
21) Nitrobenzene-d5	9.492	128	27740	22.882	ng/u1	0.00
24) 2-Nitrophenol-d4	10.215	143	28075	22.924	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.738	165	51531	22.164	ng/u1	0.00
31) 4-Chloroaniline-d4	11.284	131	78833	21.724	ng/u1	0.00
46) Dimethylphthalate-d6	14.322	166	176831	21.865	ng/u1	0.00
49) Acenaphthylene-d8	14.627	160	206409	20.961	ng/u1	0.00
54) 4-Nitrophenol-d4	15.097	143	31774	21.534	ng/u1	0.00
60) Fluorene-d10	15.914	176	155432	20.996	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	16.020	200	29498	21.537	ng/u1	0.00
73) Anthracene-d10	17.777	188	236464	21.572	ng/u1	0.00
81) Pyrene-d10	20.045	212	268850	21.946	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.297	264	259041	21.702	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.646	88	7709	8.076	ng/uL	94
5) Pyridine	4.063	79	50588	20.046	ng/u1	92
6) Benzaldehyde	7.442	77	38180	22.663	ng/u1	95
8) Phenol	7.442	94	68488	20.508	ng/u1	95
10) Bis(2-Chloroethyl)ether	7.712	93	56986	21.254	ng/u1	98
12) 2-Chlorophenol	7.847	128	50617	20.691	ng/u1#	94
13) 2-Methylphenol	8.717	108	51509	20.784	ng/u1	92
14) 2,2'-oxybis(1-Chloropr...	8.816	45	114836	20.629	ng/u1	98
16) Acetophenone	9.140	105	81845	20.545	ng/u1	95
17) N-Nitroso-di-n-propyla...	9.104	70	39590	19.659	ng/u1	98
18) 4-Methylphenol	9.046	108	55108	20.749	ng/u1	99
19) Hexachloroethane	9.386	117	20497	21.311	ng/u1	86
22) Nitrobenzene	9.539	77	58641	21.361	ng/u1	94
23) Isophorone	10.044	82	126804	21.540	ng/u1	95
25) 2-Nitrophenol	10.250	139	30087	21.984	ng/u1	98
26) 2,4-Dimethylphenol	10.268	107	55145	21.551	ng/u1	95
27) Bis(2-Chloroethoxy)met...	10.526	93	80033	21.852	ng/u1	98
29) 2,4-Dichlorophenol	10.767	162	52781	22.457	ng/u1	92
30) Naphthalene	11.196	128	184663	21.965	ng/u1	99
32) 4-Chloroaniline	11.308	127	76276	21.353	ng/u1	100
33) Hexachlorobutadiene	11.425	225	34291	22.668	ng/u1	93
34) Caprolactam	12.095	113	3065	3.561	ng/u1#	81
35) 4-Chloro-3-methylphenol	12.377	107	54543	22.032	ng/u1	92
36) 2-Methylnaphthalene	12.771	142	124292	22.136	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091923\
 Data File : BG059099.D
 Acq On : 19 Sep 2023 21:47
 Operator : MA/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SICV434


Quant Time: Sep 20 04:26:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 20 04:25:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.994	142	123540	21.781	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	13.117	216	66798	21.668	ng/ul	97
40) Hexachlorocyclopentadiene	13.070	237	40721	20.719	ng/ul#	91
41) 2,4,6-Trichlorophenol	13.358	196	43161	21.440	ng/ul	96
42) 2,4,5-Trichlorophenol	13.423	196	45239	20.775	ng/ul	96
43) 1,1'-Biphenyl	13.764	154	177262	21.119	ng/ul	94
44) 2-Chloronaphthalene	13.817	162	132057	20.605	ng/ul	95
45) 2-Nitroaniline	14.028	65	43029	21.181	ng/ul	97
47) Dimethylphthalate	14.369	163	175259	21.217	ng/ul	99
48) 2,6-Dinitrotoluene	14.510	165	34963	22.905	ng/ul#	89
50) Acenaphthylene	14.657	152	219600	20.878	ng/ul	98
51) 3-Nitroaniline	14.845	138	36815	21.859	ng/ul	92
52) Acenaphthene	14.992	153	150103	21.044	ng/ul	99
53) 2,4-Dinitrophenol	15.039	184	19942	21.682	ng/ul	90
55) 4-Nitrophenol	15.115	109	21565	22.114	ng/ul	86
56) Dibenzofuran	15.321	168	200826	21.227	ng/ul	100
57) 2,4-Dinitrotoluene	15.285	165	48450	22.016	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	15.526	232	44204	21.931	ng/ul#	89
59) Diethylphthalate	15.714	149	172474	21.190	ng/ul	96
61) Fluorene	15.973	166	169112	20.934	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.955	204	86880	21.669	ng/ul	92
63) 4-Nitroaniline	16.008	138	34322	21.984	ng/ul	89
66) 4,6-Dinitro-2-methylph...	16.037	198	31602	21.407	ng/ul#	97
67) N-Nitrosodiphenylamine	16.173	169	139740	21.787	ng/ul	97
68) 4-Bromophenyl-phenylether	16.854	248	52341	22.331	ng/ul	96
69) Hexachlorobenzene	16.942	284	57695	21.490	ng/ul	96
70) Atrazine	17.107	200	57595	22.568	ng/ul	97
71) Pentachlorophenol	17.295	266	36561	20.966	ng/ul	94
72) Phenanthrene	17.718	178	289114	21.445	ng/ul	98
74) Anthracene	17.812	178	299948	21.775	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.723	216	70967	22.096	ng/ul	89
76) Pentachlorobenzene	15.215	250	63976	21.535	ng/ul	90
77) Carbazole	18.088	167	250164	21.844	ng/ul	98
78) Di-n-butylphthalate	18.593	149	300436	21.295	ng/ul	99
80) Fluoranthene	19.710	202	332387	21.773	ng/ul	99
82) Pyrene	20.080	202	348856	21.908	ng/ul	98
83) Butylbenzylphthalate	20.938	149	123834	21.530	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.884	252	114211	22.550	ng/ul	99
85) Benzo(a)anthracene	21.978	228	326271	21.442	ng/ul	97
86) Bis(2-ethylhexyl)phtha...	21.813	149	189228	21.989	ng/ul	99
87) Chrysene	22.048	228	306040	21.566	ng/ul	98
89) Di-n-octyl phthalate	23.135	149	319950	21.408	ng/ul	100
90) Benzo(b)fluoranthene	24.398	252	326139	21.895	ng/ul	97
91) Benzo(k)fluoranthene	24.475	252	333892	21.619	ng/ul	99
93) Benzo(a)pyrene	25.374	252	312394	21.821	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	29.651	276	340655	20.923	ng/ul	98
95) Dibenzo(a,h)anthracene	29.733	278	268635	20.531	ng/ul	97
96) Benzo(g,h,i)perylene	30.955	276	279131	21.283	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 20 04:26:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 20 04:25:24 2023
Response via : Initial Calibration





#2

1,4-Dioxane

Concen: 8.076 ng/uL

RT: 3.646 min Scan# 44

Delta R.T. -0.006 min

Lab File: BG059099.D


Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :

SICV434

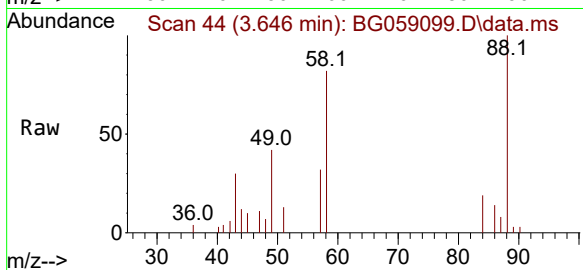




Tgt Ion: 88 Resp: 7709

Ion Ratio Lower Upper

88 100

43 29.6 24.5 36.7

58 82.4 60.6 91.0



#5

Pyridine

Concen: 20.046 ng/uL

RT: 4.063 min Scan# 115

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47




Tgt Ion: 79 Resp: 50588


Ion Ratio Lower Upper

79 100

52 104.0 90.6 135.8

51 53.6 39.6 59.4



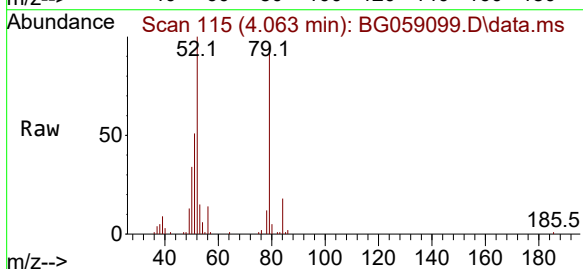





#6
Benzaldehyde
Concen: 22.663 ng/ul
RT: 7.442 min Scan# 690
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion: 77 Resp: 38180
Ion Ratio Lower Upper
77 100
105 101.6 76.9 115.3
106 90.7 69.4 104.0

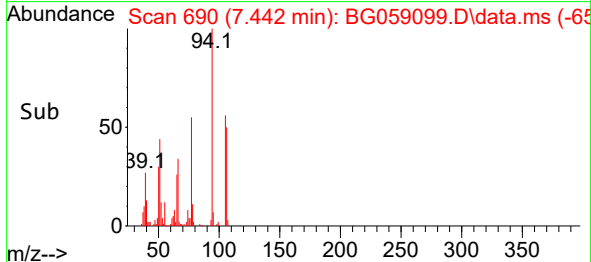

#8
Phenol
Concen: 20.508 ng/ul
RT: 7.442 min Scan# 690
Delta R.T. 0.005 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion: 94 Resp: 68488
Ion Ratio Lower Upper
94 100
65 25.9 24.4 36.6
66 34.4 28.4 42.6









#10
Bis(2-Chloroethyl)ether
Concen: 21.254 ng/ul
RT: 7.712 min Scan# 736
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion: 93 Resp: 56986
Ion Ratio Lower Upper
93 100
63 82.8 68.3 102.5
95 29.7 23.8 35.8



#12
2-Chlorophenol
Concen: 20.691 ng/ul
RT: 7.847 min Scan# 759
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion:128 Resp: 50617
Ion Ratio Lower Upper
128 100
64 48.1 40.3 60.5
130 36.2 24.0 36.0#

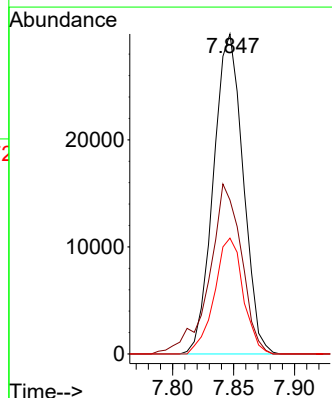



#13

2-Methylphenol

Concen: 20.784 ng/ul

RT: 8.717 min Scan# 907

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :





SICV434

Tgt Ion:108 Resp: 51509

Ion Ratio Lower Upper

108 100

107 85.8 75.1 112.7

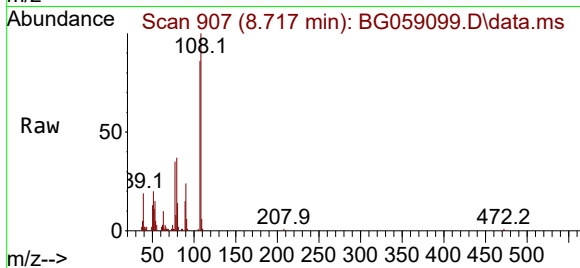

#14

2,2'-oxybis(1-Chloropropane)

Concen: 20.629 ng/ul

RT: 8.816 min Scan# 924

Delta R.T. 0.011 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47




Tgt Ion: 45 Resp: 114836


Ion Ratio Lower Upper

45 100

77 8.2 7.8 11.6

79 7.1 5.6 8.4




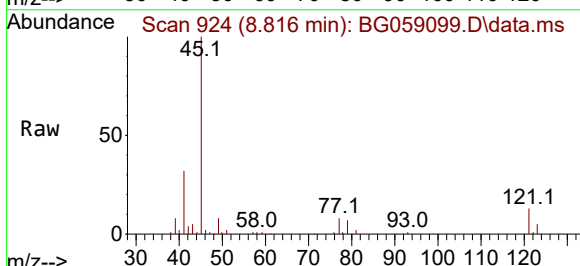




#16
Acetophenone
Concen: 20.545 ng/ul
RT: 9.140 min Scan# 91
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion:105 Resp: 81845
Ion Ratio Lower Upper
105 100
77 76.7 57.2 85.8
51 38.2 31.6 47.4

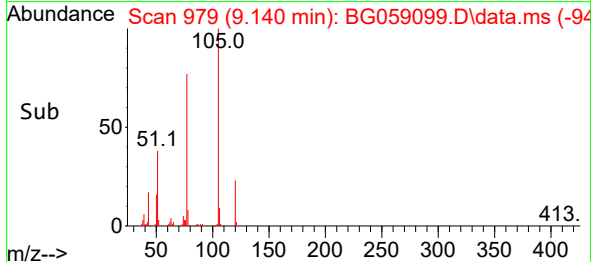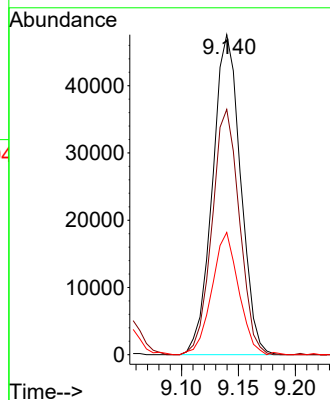

#17
N-Nitroso-di-n-propylamine
Concen: 19.659 ng/ul
RT: 9.104 min Scan# 973
Delta R.T. 0.005 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion: 70 Resp: 39590
Ion Ratio Lower Upper
70 100
42 86.0 67.1 100.7
101 7.8 7.6 11.4
130 19.9 15.9 23.9



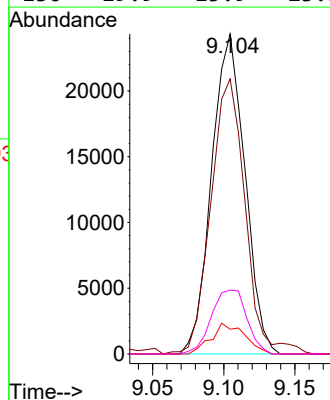





#18
4-Methylphenol
Concen: 20.749 ng/ul
RT: 9.046 min Scan# 90
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion:108 Resp: 55108
Ion Ratio Lower Upper
108 100
107 117.4 94.4 141.6

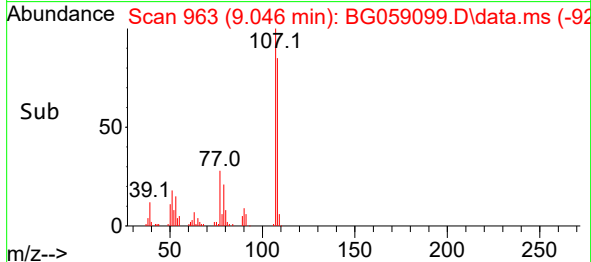

#19
Hexachloroethane
Concen: 21.311 ng/ul
RT: 9.386 min Scan# 1021
Delta R.T. 0.005 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion:117 Resp: 20497
Ion Ratio Lower Upper
117 100
201 129.5 86.4 129.6
199 73.4 56.2 84.2









#22
Nitrobenzene
Concen: 21.361 ng/ul
RT: 9.539 min Scan# 1047
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion: 77 Resp: 58641
Ion Ratio Lower Upper
77 100
123 46.9 41.8 62.8
65 14.7 12.3 18.5

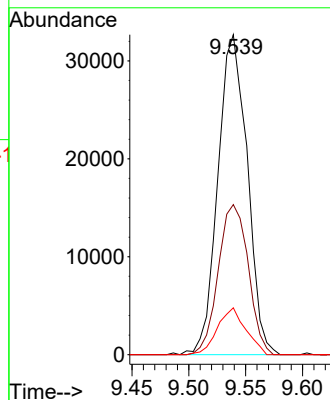

#23
Isophorone
Concen: 21.540 ng/ul
RT: 10.044 min Scan# 1133
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion: 82 Resp: 126804
Ion Ratio Lower Upper
82 100
95 6.5 5.4 8.2
138 18.7 12.7 19.1

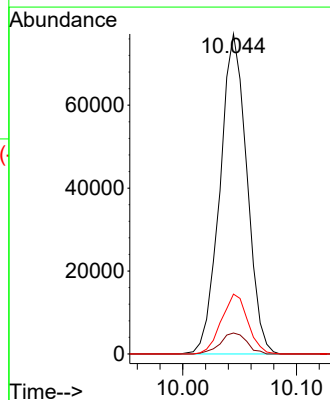



#25

2-Nitrophenol

Concen: 21.984 ng/ul

RT: 10.250 min Scan# 1168

Delta R.T. 0.005 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :

SICV434





Tgt Ion:139 Resp: 30087

Ion Ratio Lower Upper

139 100

65 58.5 46.4 69.6

109 24.8 21.6 32.4

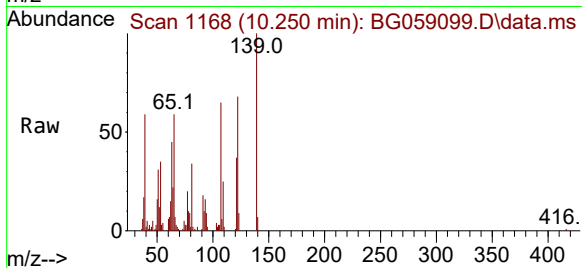

#26

2,4-Dimethylphenol

Concen: 21.551 ng/ul

RT: 10.268 min Scan# 1171

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47




Tgt Ion:107 Resp: 55145


Ion Ratio Lower Upper

107 100

121 51.5 41.4 62.0

122 93.8 80.6 120.8

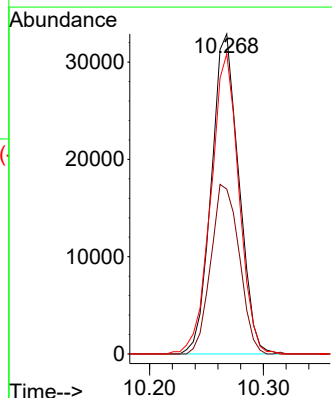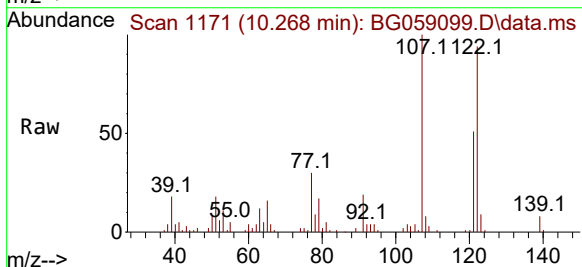



#27

Bis(2-Chloroethoxy)methane

Concen: 21.852 ng/ul

RT: 10.526 min Scan# 1215

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :

SICV434





Tgt Ion: 93 Resp: 80033

Ion Ratio Lower Upper

93 100

95 32.9 26.1 39.1

123 8.9 8.7 13.1



#29

2,4-Dichlorophenol

Concen: 22.457 ng/ul

RT: 10.767 min Scan# 1256

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47




Tgt Ion:162 Resp: 52781


Ion Ratio Lower Upper

162 100

164 70.9 49.8 74.8

98 32.2 25.9 38.9









#30
Naphthalene
Concen: 21.965 ng/ul
RT: 11.196 min Scan# 11
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion:128 Resp: 184663
Ion Ratio Lower Upper
128 100
129 10.9 8.4 12.6
127 12.7 10.2 15.4



#32
4-Chloroaniline
Concen: 21.353 ng/ul
RT: 11.308 min Scan# 1348
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion:127 Resp: 76276
Ion Ratio Lower Upper
127 100
129 33.9 27.2 40.8





#33

Hexachlorobutadiene

Concen: 22.668 ng/ul

RT: 11.425 min Scan# 1368

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :

SICV434





Tgt Ion:225 Resp: 34291

Ion Ratio Lower Upper

225 100

223 55.4 39.0 58.4

227 60.7 45.7 68.5



#34

Caprolactam

Concen: 3.561 ng/ul

RT: 12.095 min Scan# 1482

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47




Tgt Ion:113 Resp: 3065


Ion Ratio Lower Upper

113 100

55 220.0 157.6 236.4

56 170.4 112.3 168.5#









#35
 4-Chloro-3-methylphenol
 Concen: 22.032 ng/ul
 RT: 12.377 min Scan# 1530
 Delta R.T. -0.001 min
 Lab File: BG059099.D
 Acq: 19 Sep 2023 21:47




Instrument :
 BNA_G
 ClientSampleId :
 SICV434


Tgt Ion:	107	Resp:	54543
Ion	Ratio	Lower	Upper
107	100		
144	28.1	20.1	30.1
142	85.5	62.7	94.1



#36
 2-Methylnaphthalene
 Concen: 22.136 ng/ul
 RT: 12.771 min Scan# 1597
 Delta R.T. -0.006 min
 Lab File: BG059099.D
 Acq: 19 Sep 2023 21:47

Tgt Ion:	142	Resp:	124292
Ion	Ratio	Lower	Upper
142	100		
141	89.0	70.6	106.0





#37

1-Methylnaphthalene

Concen: 21.781 ng/ul

RT: 12.994 min Scan# 1

Delta R.T. 0.005 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :

SICV434





Tgt Ion:142 Resp: 123540

Ion Ratio Lower Upper

142 100

141 91.5 72.0 108.0

116 3.1 2.7 4.1



#39

1,2,4,5-Tetrachlorobenzene

Concen: 21.668 ng/ul

RT: 13.117 min Scan# 1656

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Tgt Ion:216 Resp: 66798




Ion Ratio Lower Upper


216 100

214 76.1 62.6 94.0

179 20.3 16.0 24.0

108 12.8 12.0 18.0



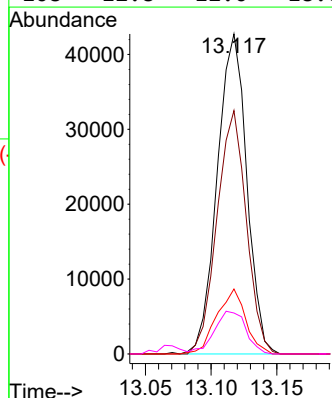





#40
Hexachlorocyclopentadiene
Concen: 20.719 ng/ul
RT: 13.070 min Scan# 1648
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion:237 Resp: 40721
Ion Ratio Lower Upper
237 100
235 58.2 51.6 77.4
272 17.8 10.6 15.8#



#41
2,4,6-Trichlorophenol
Concen: 21.440 ng/ul
RT: 13.358 min Scan# 1697
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion:196 Resp: 43161
Ion Ratio Lower Upper
196 100
198 93.2 78.5 117.7
200 31.9 24.4 36.6





#42

2,4,5-Trichlorophenol

Concen: 20.775 ng/ul

RT: 13.423 min Scan# 1708

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :

SICV434





Tgt Ion:196 Resp: 45239

Ion Ratio Lower Upper

196 100

198 106.5 81.0 121.6

200 34.8 27.1 40.7



#43

1,1'-Biphenyl

Concen: 21.119 ng/ul

RT: 13.764 min Scan# 1766

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47




Tgt Ion:154 Resp: 177262


Ion Ratio Lower Upper

154 100

153 36.8 33.2 49.8

76 11.6 9.8 14.8





#44

2-Chloronaphthalene

Concen: 20.605 ng/ul

RT: 13.817 min Scan# 11

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :

SICV434





Tgt Ion:162 Resp: 132057

Ion Ratio Lower Upper

162 100

164 30.1 27.2 40.8

127 36.1 27.4 41.2



#45

2-Nitroaniline

Concen: 21.181 ng/ul

RT: 14.028 min Scan# 1811

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47




Tgt Ion: 65 Resp: 43029


Ion Ratio Lower Upper

65 100

92 61.9 53.6 80.4

138 99.1 79.8 119.6









#47
Dimethylphthalate
Concen: 21.217 ng/ul
RT: 14.369 min Scan# 1869
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion:163 Resp: 175259
Ion Ratio Lower Upper
163 100
194 3.3 2.8 4.2
164 9.7 7.6 11.4

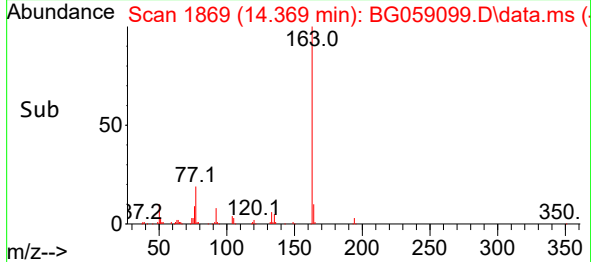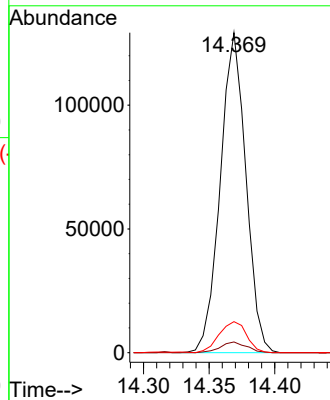

#48
2,6-Dinitrotoluene
Concen: 22.905 ng/ul
RT: 14.510 min Scan# 1893
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion:165 Resp: 34963
Ion Ratio Lower Upper
165 100
89 55.2 38.7 58.1
121 23.5 13.4 20.0#



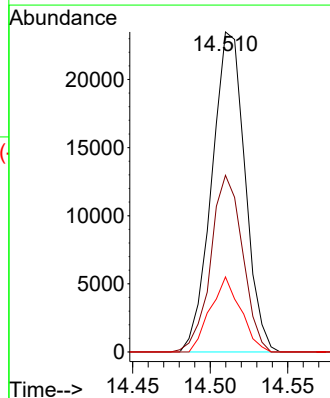





#50
Acenaphthylene
Concen: 20.878 ng/ul
RT: 14.657 min Scan# 1918
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion:152 Resp: 219600
Ion Ratio Lower Upper
152 100
151 18.6 15.8 23.6
153 13.9 11.3 16.9



#51
3-Nitroaniline
Concen: 21.859 ng/ul
RT: 14.845 min Scan# 1950
Delta R.T. -0.006 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion:138 Resp: 36815
Ion Ratio Lower Upper
138 100
108 8.4 7.4 11.2
92 107.7 93.4 140.0









#52
Acenaphthene
Concen: 21.044 ng/ul
RT: 14.992 min Scan# 1975
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion:153 Resp: 150103
Ion Ratio Lower Upper
153 100
152 44.8 36.0 54.0
154 89.9 71.3 106.9



#53
2,4-Dinitrophenol
Concen: 21.682 ng/ul
RT: 15.039 min Scan# 1983
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion:184 Resp: 19942
Ion Ratio Lower Upper
184 100
63 60.7 53.5 80.3
154 57.8 54.6 81.8









#55
4-Nitrophenol
Concen: 22.114 ng/ul
RT: 15.115 min Scan# 1996
Delta R.T. 0.005 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion:109 Resp: 21565
Ion Ratio Lower Upper
109 100
139 159.0 114.5 171.7
65 185.0 132.1 198.1



#56
Dibenzofuran
Concen: 21.227 ng/ul
RT: 15.321 min Scan# 2031
Delta R.T. -0.006 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion:168 Resp: 200826
Ion Ratio Lower Upper
168 100
139 32.7 26.3 39.5









#57
2,4-Dinitrotoluene
Concen: 22.016 ng/ul
RT: 15.285 min Scan# 2025
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion:165 Resp: 48450
Ion Ratio Lower Upper
165 100
63 49.8 40.0 60.0
182 2.5 2.1 3.1



#58
2,3,4,6-Tetrachlorophenol
Concen: 21.931 ng/ul
RT: 15.526 min Scan# 2066
Delta R.T. -0.006 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion:232 Resp: 44204
Ion Ratio Lower Upper
232 100
131 39.1 25.8 38.8#
130 3.0 1.8 2.6#
166 28.0 18.4 27.6#





#59

Diethylphthalate

Concen: 21.190 ng/ul

RT: 15.714 min Scan# 2098

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :

SICV434





Tgt Ion:149 Resp: 172474

Ion Ratio Lower Upper

149 100

177 26.9 19.4 29.2

150 12.4 9.8 14.8



#61

Fluorene

Concen: 20.934 ng/ul

RT: 15.973 min Scan# 2142

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47




Tgt Ion:166 Resp: 169112


Ion Ratio Lower Upper

166 100

165 101.9 81.6 122.4

167 12.4 12.1 18.1





#62

4-Chlorophenyl-phenylether

Concen: 21.669 ng/ul

RT: 15.955 min Scan# 2139

Delta R.T. -0.001 min

Lab File: BG059099.D


Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :

SICV434






Tgt Ion:204 Resp: 86880

Ion Ratio Lower Upper

204 100

206 32.5 28.2 42.2

141 47.3 43.4 65.0



#63

4-Nitroaniline

Concen: 21.984 ng/ul

RT: 16.008 min Scan# 2148

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47




Tgt Ion:138 Resp: 34322


Ion Ratio Lower Upper

138 100

92 52.0 39.0 58.6

108 79.8 53.5 80.3









#66
 4,6-Dinitro-2-methylphenol
 Concen: 21.407 ng/ul
 RT: 16.037 min Scan# 2153
 Delta R.T. -0.001 min
 Lab File: BG059099.D
 Acq: 19 Sep 2023 21:47




Instrument :
 BNA_G
 ClientSampleId :
 SICV434


Tgt Ion:198 Resp: 31602
 Ion Ratio Lower Upper
 198 100
 182 2.6 3.5 5.3#
 77 23.0 17.3 25.9

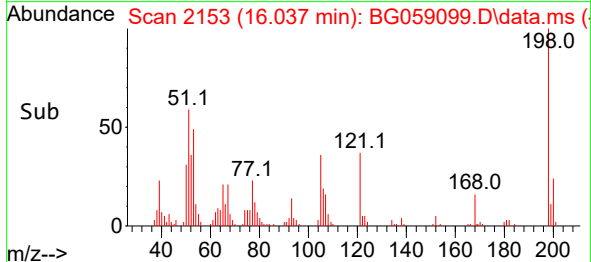

#67
 N-Nitrosodiphenylamine
 Concen: 21.787 ng/ul
 RT: 16.173 min Scan# 2176
 Delta R.T. -0.001 min
 Lab File: BG059099.D
 Acq: 19 Sep 2023 21:47

Tgt Ion:169 Resp: 139740
 Ion Ratio Lower Upper
 169 100
 168 67.3 52.1 78.1
 167 36.0 30.5 45.7









#68
4-Bromophenyl-phenylether
Concen: 22.331 ng/ul
RT: 16.854 min Scan# 21
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion:	248	Resp:	52341
Ion Ratio	Lower	Upper	
248	100		
250	98.3	81.8	122.8
141	58.8	50.0	75.0

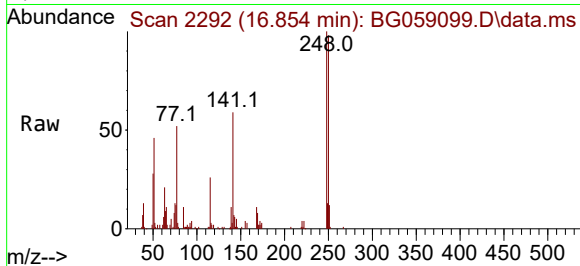

#69
Hexachlorobenzene
Concen: 21.490 ng/ul
RT: 16.942 min Scan# 2307
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion:	284	Resp:	57695
Ion Ratio	Lower	Upper	
284	100		
142	31.9	23.2	34.8
249	32.8	27.8	41.8




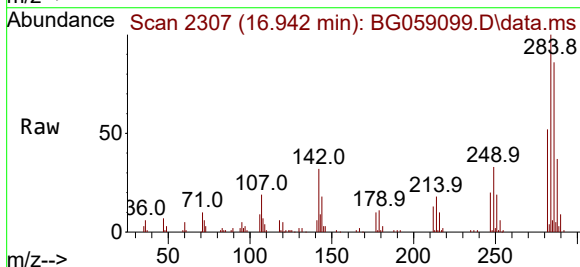




#70
Atrazine
Concen: 22.568 ng/ul
RT: 17.107 min Scan# 21
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion:200 Resp: 57595
Ion Ratio Lower Upper
200 100
173 21.9 19.4 29.0
215 46.4 38.5 57.7

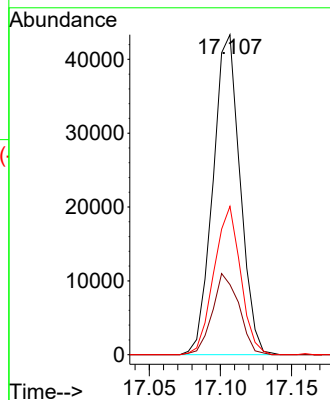

#71
Pentachlorophenol
Concen: 20.966 ng/ul
RT: 17.295 min Scan# 2367
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion:266 Resp: 36561
Ion Ratio Lower Upper
266 100
264 65.2 50.6 76.0
268 63.5 56.4 84.6



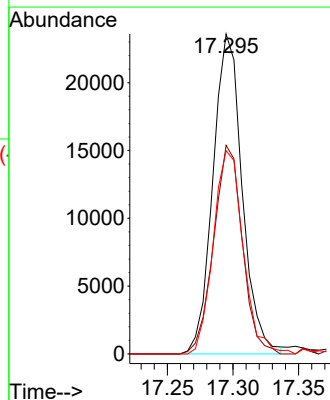





#72
Phenanthrene
Concen: 21.445 ng/ul
RT: 17.718 min Scan# 2439
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion:178 Resp: 289114
Ion Ratio Lower Upper
178 100
179 15.3 11.8 17.8
176 18.9 14.6 21.8



#74
Anthracene
Concen: 21.775 ng/ul
RT: 17.812 min Scan# 2455
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion:178 Resp: 299948
Ion Ratio Lower Upper
178 100
179 15.5 12.4 18.6
176 18.0 14.8 22.2









#75
1,2,3,4-Tetrachlorobenzene
Concen: 22.096 ng/uL
RT: 13.723 min Scan# 1
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion:216 Resp: 70967
Ion Ratio Lower Upper
216 100
214 74.4 69.9 104.9
218 46.2 39.4 59.0

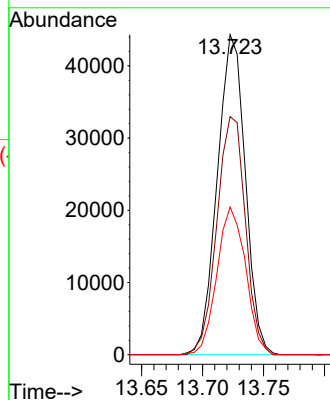

#76
Pentachlorobenzene
Concen: 21.535 ng/uL
RT: 15.215 min Scan# 2013
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion:250 Resp: 63976
Ion Ratio Lower Upper
250 100
248 61.6 52.5 78.7
252 61.8 59.4 89.2

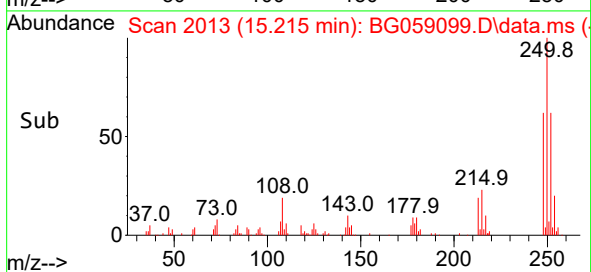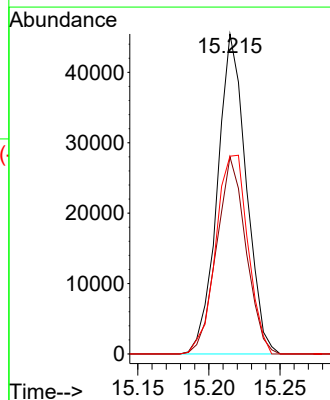



#77

Carbazole

Concen: 21.844 ng/ul

RT: 18.088 min Scan# 2502

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :

SICV434





Tgt Ion:167 Resp: 250164

Ion Ratio Lower Upper

167 100

166 22.0 16.7 25.1

139 12.0 9.4 14.0

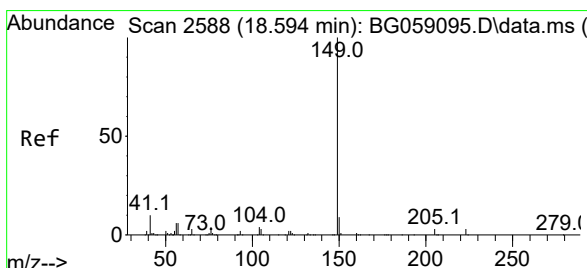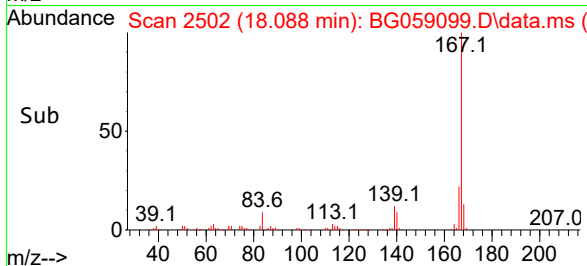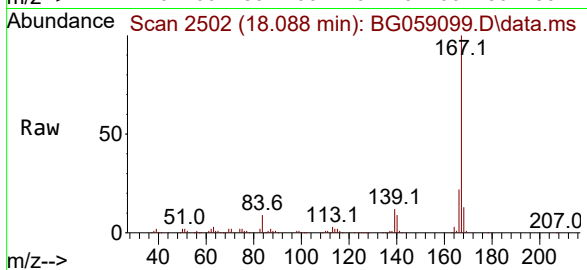

#78

Di-n-butylphthalate

Concen: 21.295 ng/ul

RT: 18.593 min Scan# 2588

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47




Tgt Ion:149 Resp: 300436


Ion Ratio Lower Upper

149 100

150 9.0 7.4 11.2

104 4.4 3.5 5.3

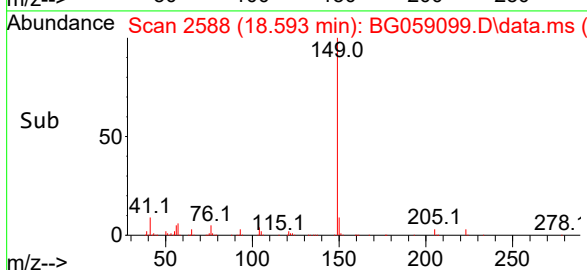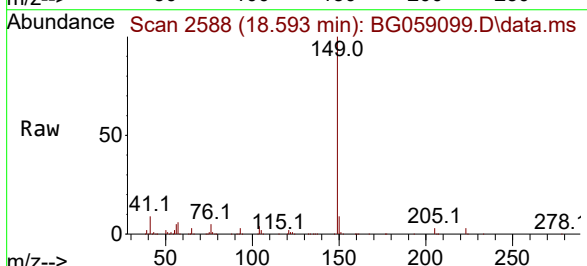



#80

Fluoranthene

Concen: 21.773 ng/ul

RT: 19.710 min Scan# 21

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :

SICV434





Tgt Ion:202 Resp: 332387

Ion Ratio Lower Upper

202 100

101 10.9 9.2 13.8

100 9.1 7.7 11.5



#82

Pyrene

Concen: 21.908 ng/ul

RT: 20.080 min Scan# 2841

Delta R.T. 0.005 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47




Tgt Ion:202 Resp: 348856


Ion Ratio Lower Upper

202 100

101 13.0 11.0 16.4

100 11.4 10.1 15.1





#83

Butylbenzylphthalate

Concen: 21.530 ng/ul

RT: 20.938 min Scan# 2987

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :

SICV434





Tgt Ion:149 Resp: 123834

Ion Ratio Lower Upper

149 100

91 77.1 61.2 91.8

206 21.5 15.8 23.6



#84

3,3'-Dichlorobenzidine

Concen: 22.550 ng/ul

RT: 21.884 min Scan# 3148

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47




Tgt Ion:252 Resp: 114211


Ion Ratio Lower Upper

252 100

254 66.0 52.4 78.6

126 10.6 8.2 12.2





#85

Benzo(a)anthracene

Concen: 21.442 ng/ul

RT: 21.978 min Scan# 3163

Delta R.T. 0.005 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :

SICV434





Tgt Ion:228 Resp: 326271

Ion Ratio Lower Upper

228 100

229 19.4 16.1 24.1

226 27.4 20.6 30.8



#86

Bis(2-ethylhexyl)phthalate

Concen: 21.989 ng/ul

RT: 21.813 min Scan# 3136

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47




Tgt Ion:149 Resp: 189228


Ion Ratio Lower Upper

149 100

167 25.0 20.2 30.4

279 3.4 3.2 4.8









#87
Chrysene
Concen: 21.566 ng/ul
RT: 22.048 min Scan# 3176
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion:228 Resp: 306040
Ion Ratio Lower Upper
228 100
226 30.6 23.3 34.9
229 19.2 15.6 23.4



#89
Di-n-octyl phthalate
Concen: 21.408 ng/ul
RT: 23.135 min Scan# 3361
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion:149 Resp: 319950









#90
Benzo(b)fluoranthene
Concen: 21.895 ng/ul
RT: 24.398 min Scan# 3575
Delta R.T. 0.005 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47




Instrument :
BNA_G
ClientSampleId :
SICV434


Tgt Ion:252 Resp: 326139
Ion Ratio Lower Upper
252 100
253 20.5 17.1 25.7
125 9.1 8.6 13.0

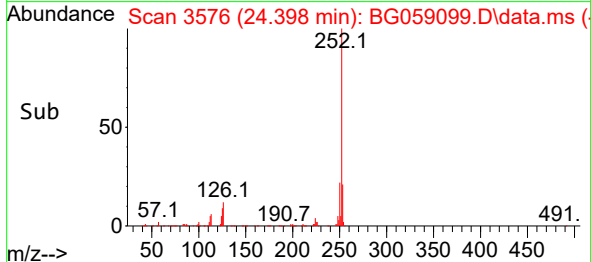

#91
Benzo(k)fluoranthene
Concen: 21.619 ng/ul
RT: 24.475 min Scan# 3589
Delta R.T. -0.001 min
Lab File: BG059099.D
Acq: 19 Sep 2023 21:47

Tgt Ion:252 Resp: 333892
Ion Ratio Lower Upper
252 100
253 21.1 16.5 24.7
125 10.3 7.9 11.9





#93

Benzo(a)pyrene

Concen: 21.821 ng/ul

RT: 25.374 min Scan# 31

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :

SICV434





Tgt Ion:252 Resp: 312394

Ion Ratio Lower Upper

252 100

253 21.6 17.6 26.4

125 9.8 8.3 12.5



#94

Indeno(1,2,3-cd)pyrene

Concen: 20.923 ng/ul

RT: 29.651 min Scan# 4470

Delta R.T. 0.011 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47




Tgt Ion:276 Resp: 340655


Ion Ratio Lower Upper

276 100

138 22.3 17.1 25.7

277 24.2 20.4 30.6





#95

Dibenzo(a,h)anthracene

Concen: 20.531 ng/ul

RT: 29.733 min Scan# 4484

Delta R.T. -0.001 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Instrument :

BNA_G

ClientSampleId :

SICV434





Tgt Ion:278 Resp: 268635

Ion Ratio Lower Upper

278 100

139 15.5 13.8 20.6

279 24.5 19.0 28.4



#96

Benzo(g,h,i)perylene

Concen: 21.283 ng/ul

RT: 30.955 min Scan# 4692

Delta R.T. -0.006 min

Lab File: BG059099.D

Acq: 19 Sep 2023 21:47

Tgt Ion:276 Resp: 279131

Ion Ratio Lower Upper

276 100

138 22.4 16.9 25.3

277 22.4 19.3 28.9

